

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019885.D
Acq On : 26 Feb 2024 18:37
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	398	405	421	rBV	1674331	2599095	30.88%	7.896%
2	7.075	670	678	691	rBV	1537526	2474024	29.39%	7.516%
3	7.899	808	818	834	rBV	288709	466155	5.54%	1.416%
4	9.069	1009	1017	1027	rBV	893806	1599057	19.00%	4.858%
5	10.699	1285	1294	1315	rBV	333704	632124	7.51%	1.920%
6	13.169	1706	1714	1728	rBV	3680753	5742810	68.23%	17.447%
7	14.540	1940	1947	1958	rBV	851183	1353494	16.08%	4.112%
8	16.039	2194	2202	2222	rBV	3315442	4934094	58.62%	14.990%
9	17.304	2409	2417	2431	rBV	1034073	1575199	18.71%	4.785%
10	19.875	2848	2854	2864	rBV	6862663	8417300	100.00%	25.572%
11	21.404	3108	3114	3122	rBV	1116766	1578485	18.75%	4.795%
12	23.827	3519	3526	3535	rVB	730713	1544516	18.35%	4.692%




Sum of corrected areas: 32916353

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019885.D
Acq On : 26 Feb 2024 18:37
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

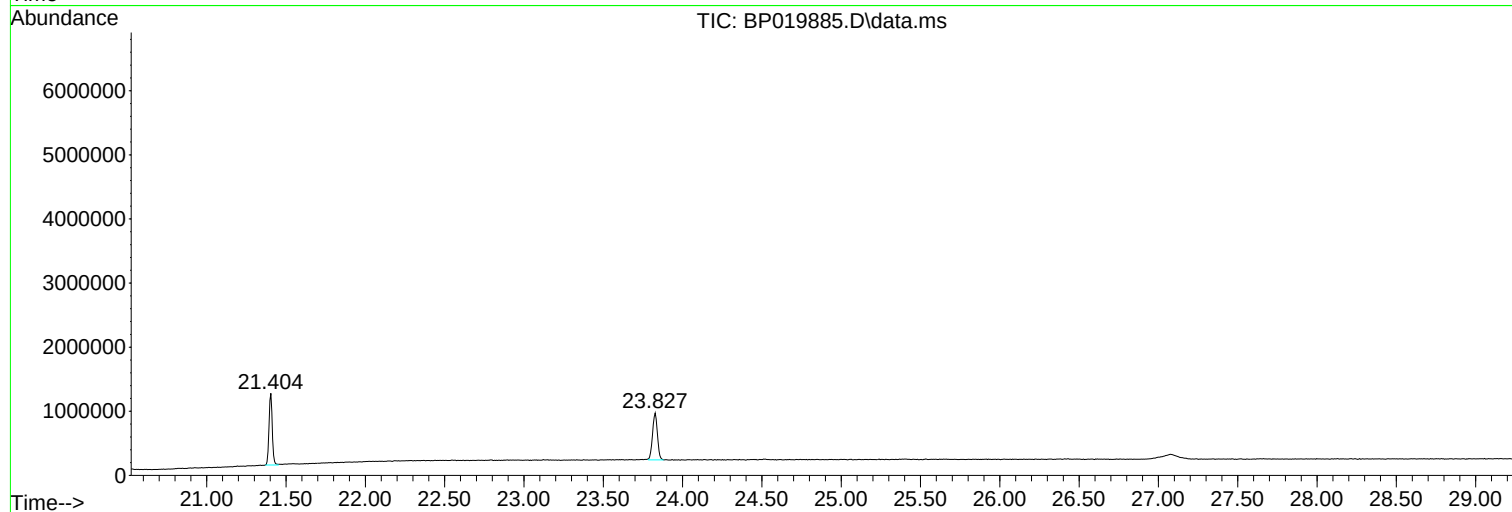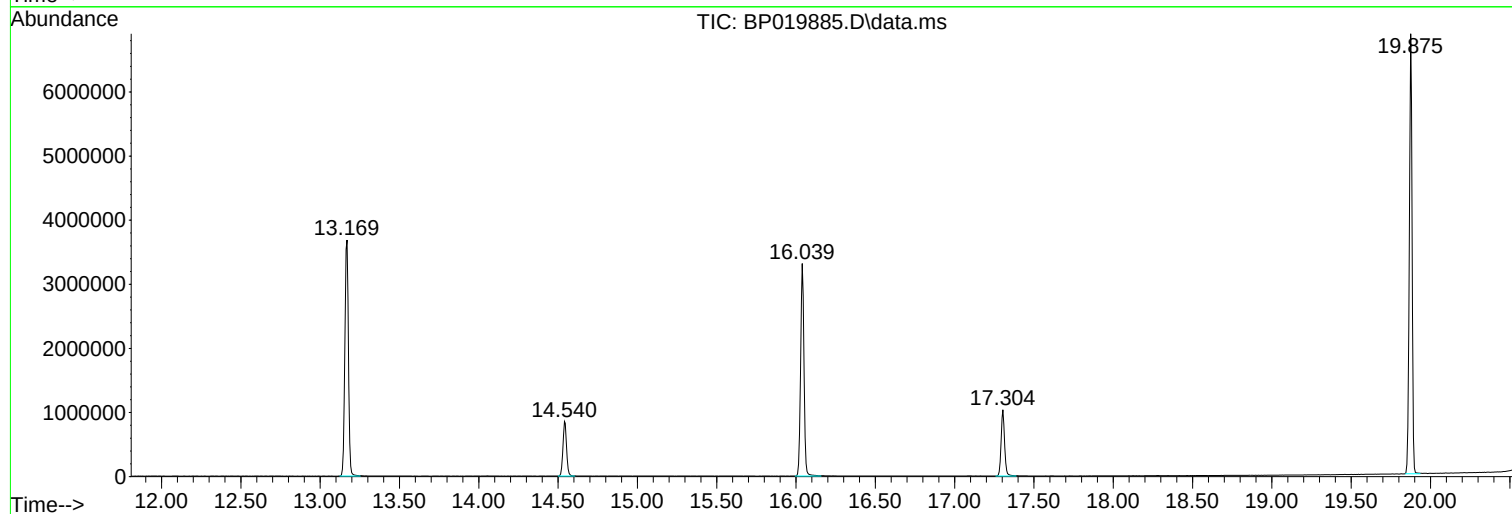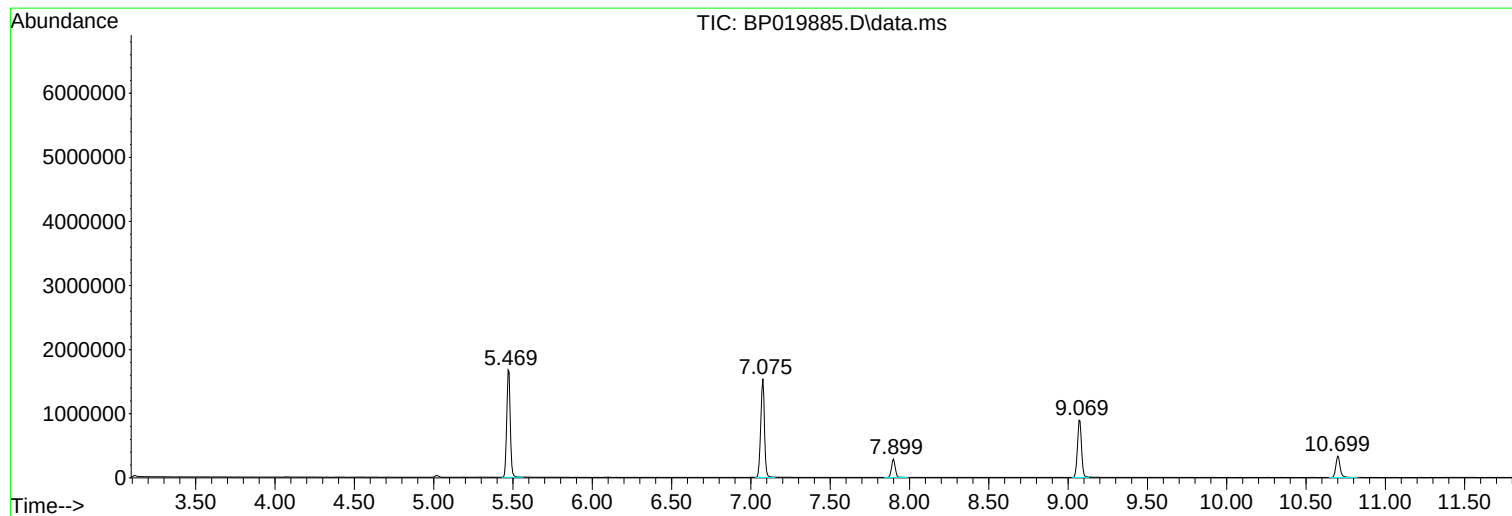

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019885.D
Acq On : 26 Feb 2024 18:37
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019885.D
Acq On : 26 Feb 2024 18:37
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------