
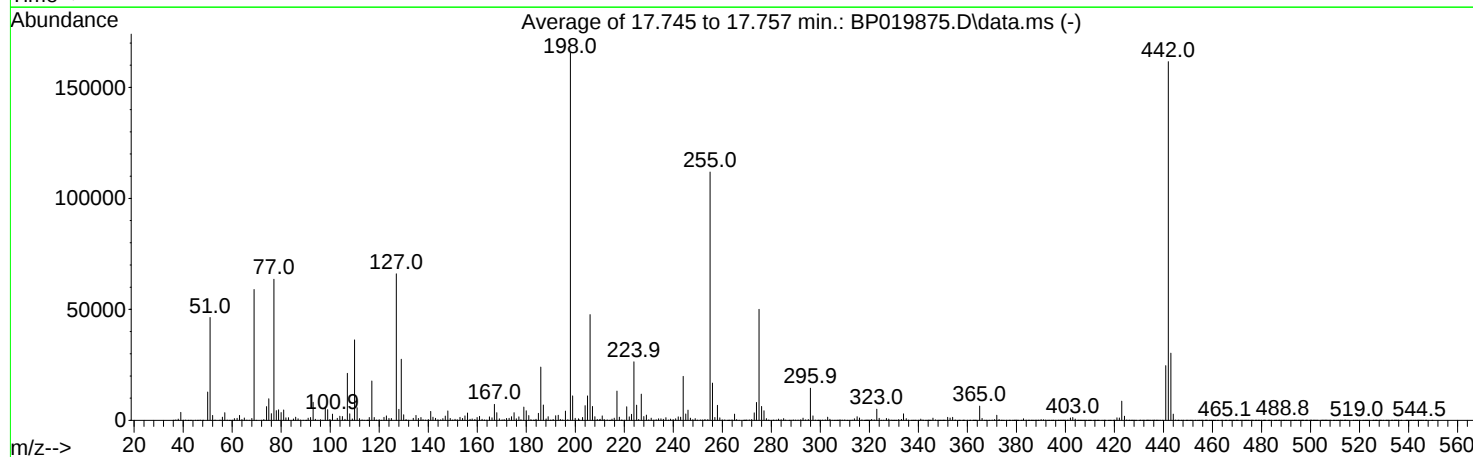


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019875.D
Acq On : 26 Feb 2024 12:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 27 02:05:05 2024

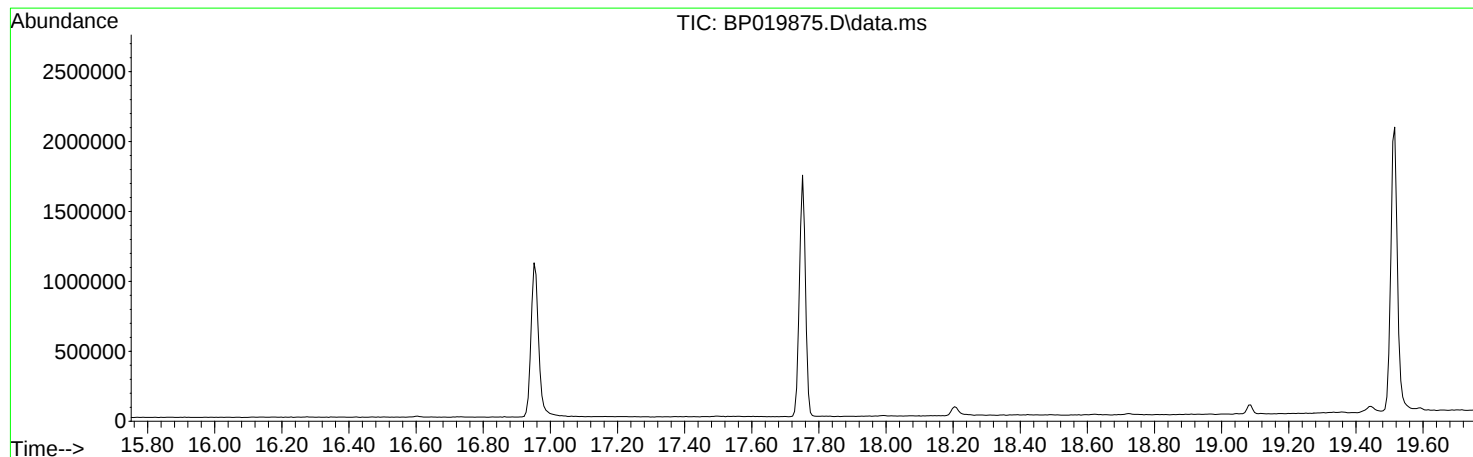




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	46390	PASS
68	69	0.00	2	1.5	871	PASS
69	198	0.00	100	35.6	58940	PASS
70	69	0.00	2	0.1	77	PASS
127	198	10	80	39.9	66068	PASS
197	198	0.00	2	0.2	283	PASS
198	198	100	100	100.0	165722	PASS
199	198	5	9	6.7	11034	PASS
275	198	10	60	30.2	50050	PASS
365	198	1	100	3.9	6434	PASS
441	198	0.01	100	14.9	24679	PASS
442	442	100	100	100.0	161576	PASS
443	442	15	24	18.7	30293	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019875.D
Acq On : 26 Feb 2024 12:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 27 02:10:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

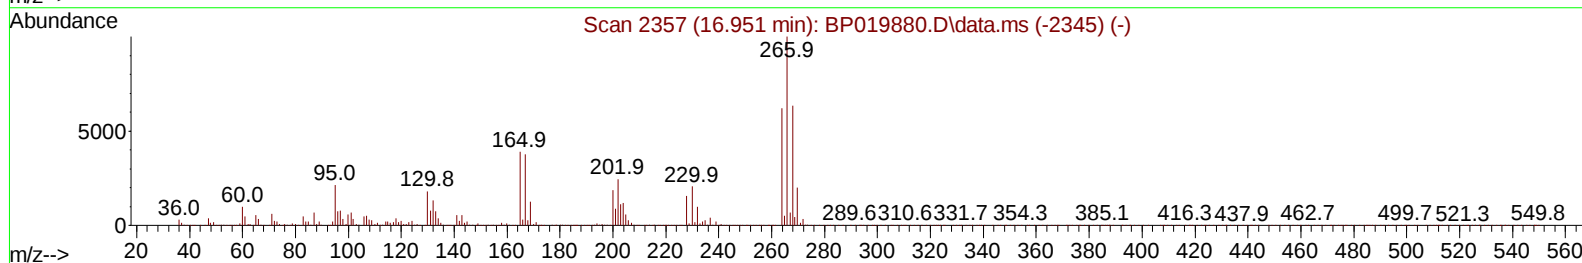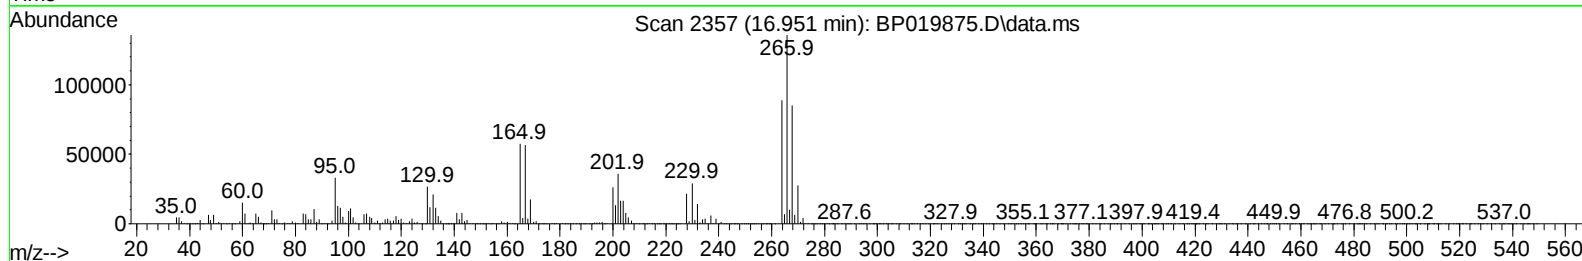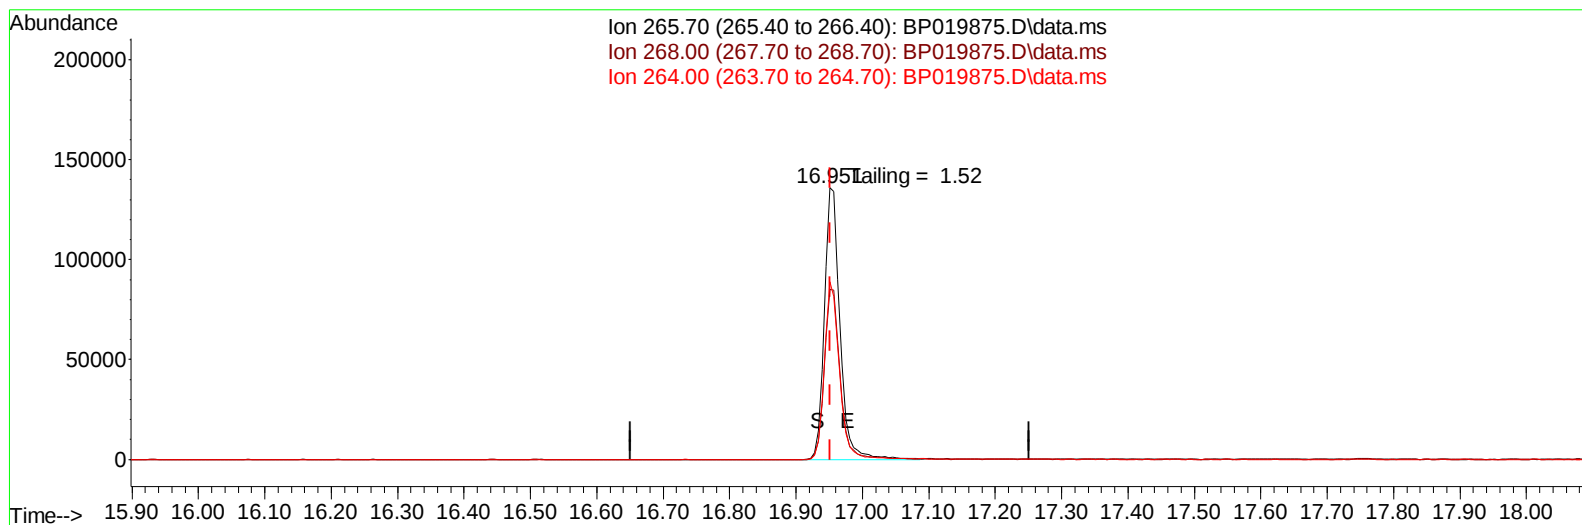

TIC: BP019875.D\data.ms

(70) Pentachlorophenol (C)

16.951min (+ 0.000) 748974.56 ng




response 221468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.58
264.00	62.10	65.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019875.D
Acq On : 26 Feb 2024 12:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 27 02:10:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

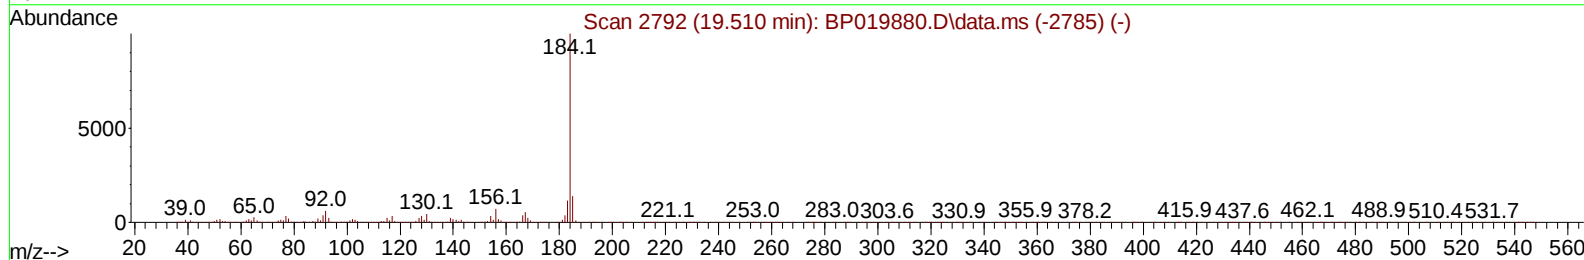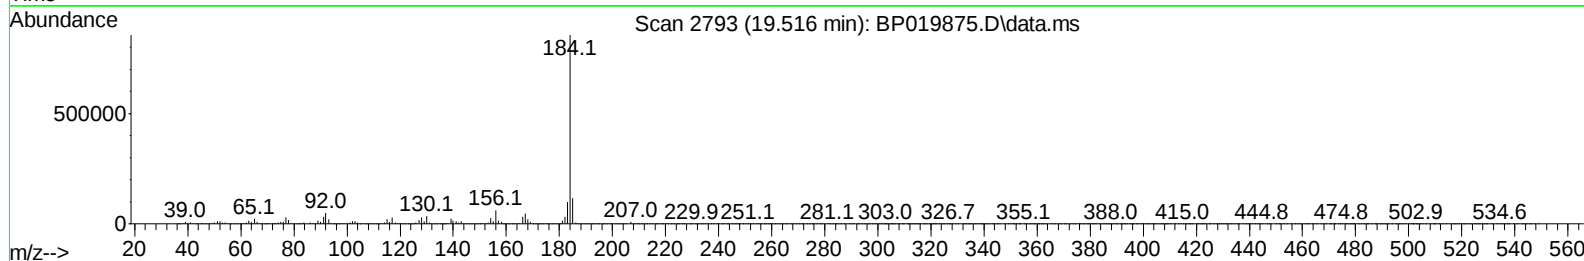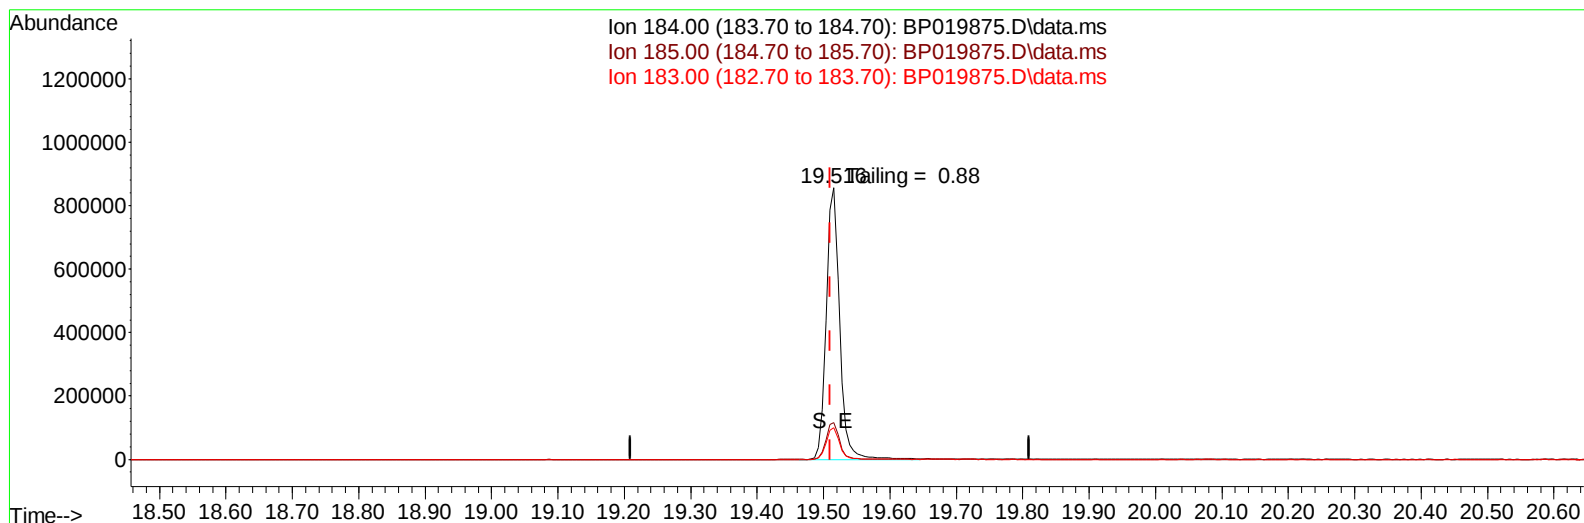

TIC: BP019875.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 572536.29 ng

response 1184118

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.55
183.00	11.60	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2024	BNA_P	<u>BP019875.D</u>
Compound Name	Response	Retention Time
DDT	662085	20.71
DDD	8573	20.327
DDE	224	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8797	670882	1.31

Instrument :
BNA_P
ClientSampleId :
DFTPP