
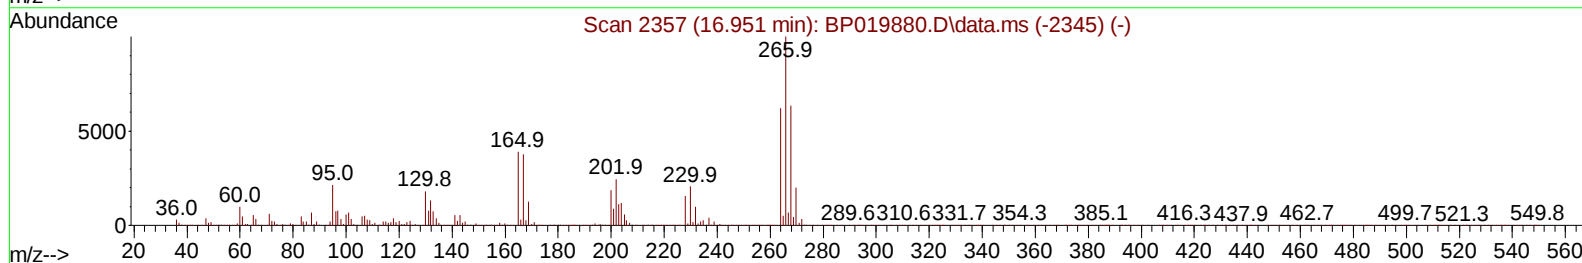
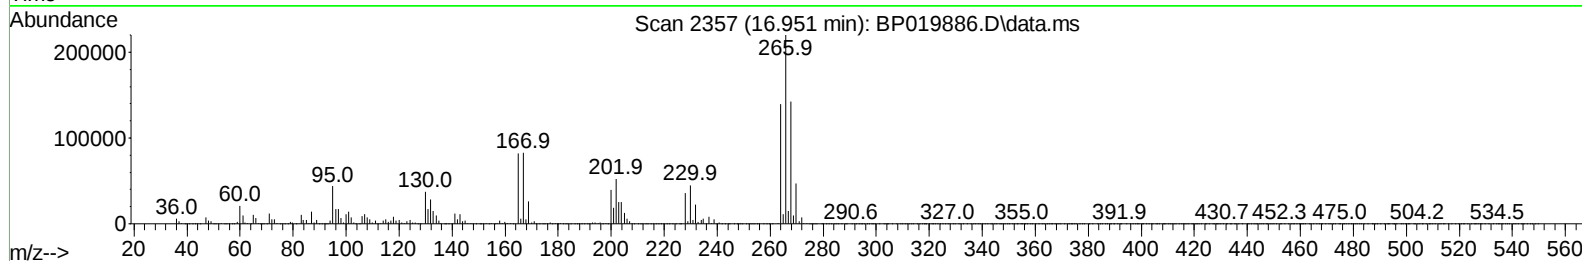


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019886.D
Acq On : 27 Feb 2024 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 02:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

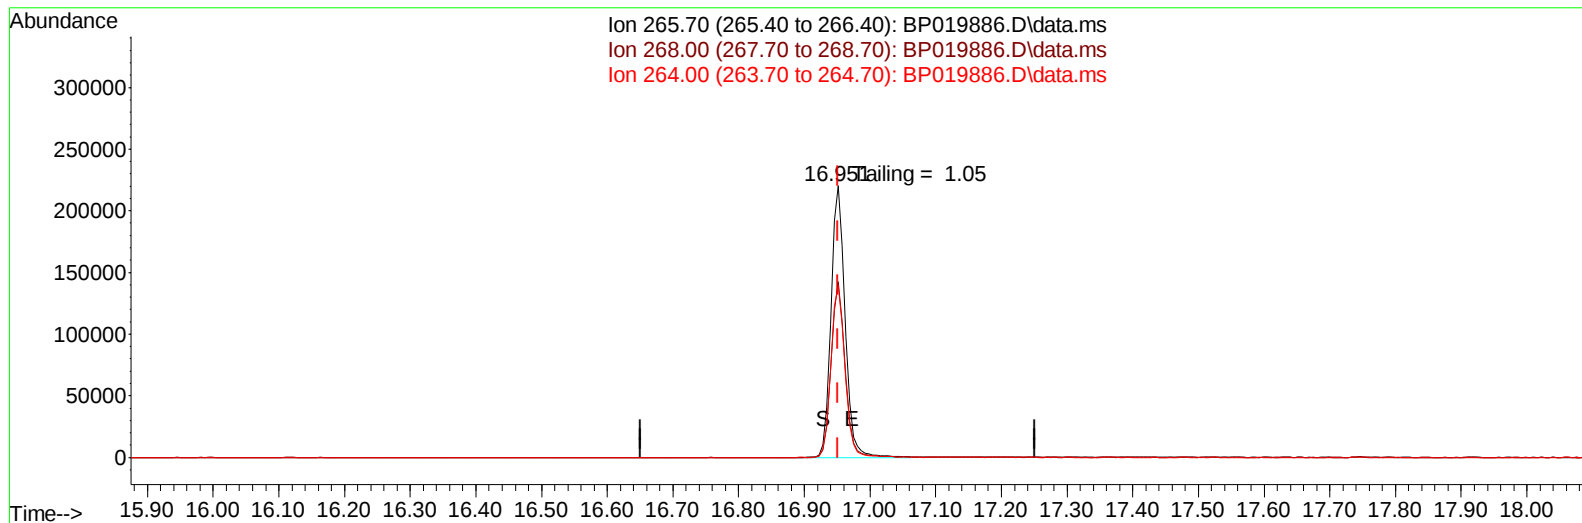




TIC: BP019886.D\data.ms

(70) Pentachlorophenol (C)**16.951min (+ 0.000) 35680.49 ng****response 331287**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.74
264.00	62.10	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019886.D
Acq On : 27 Feb 2024 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 02:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

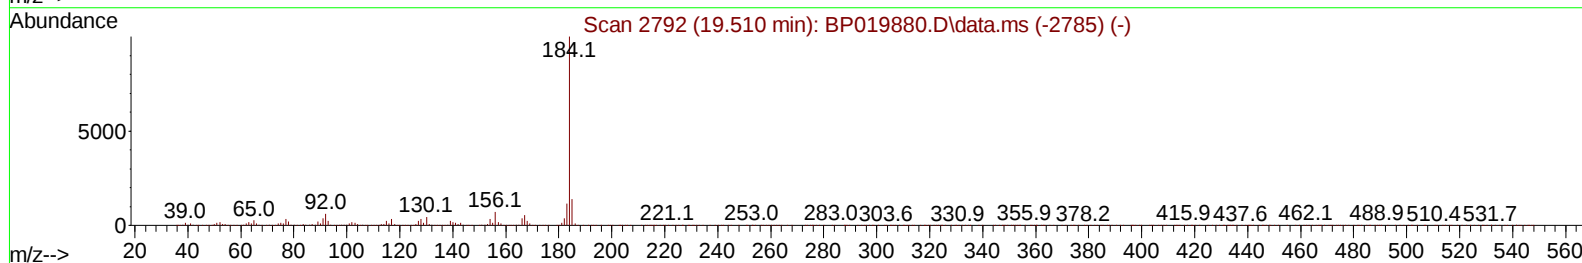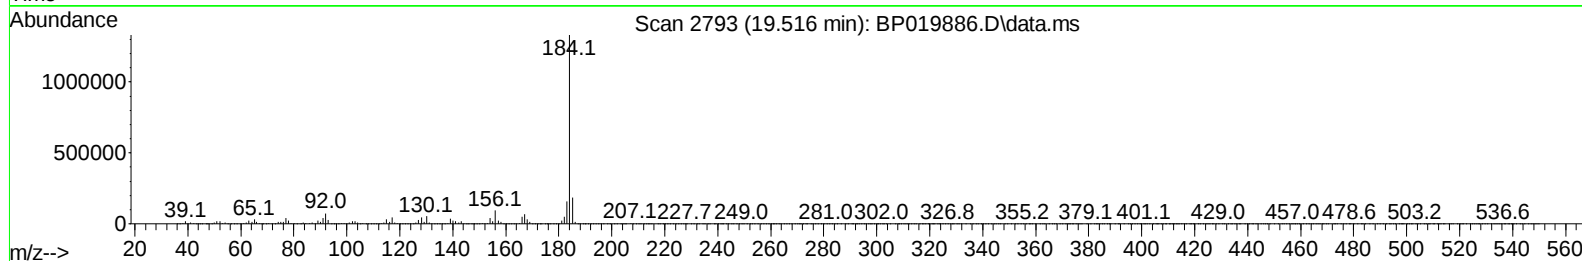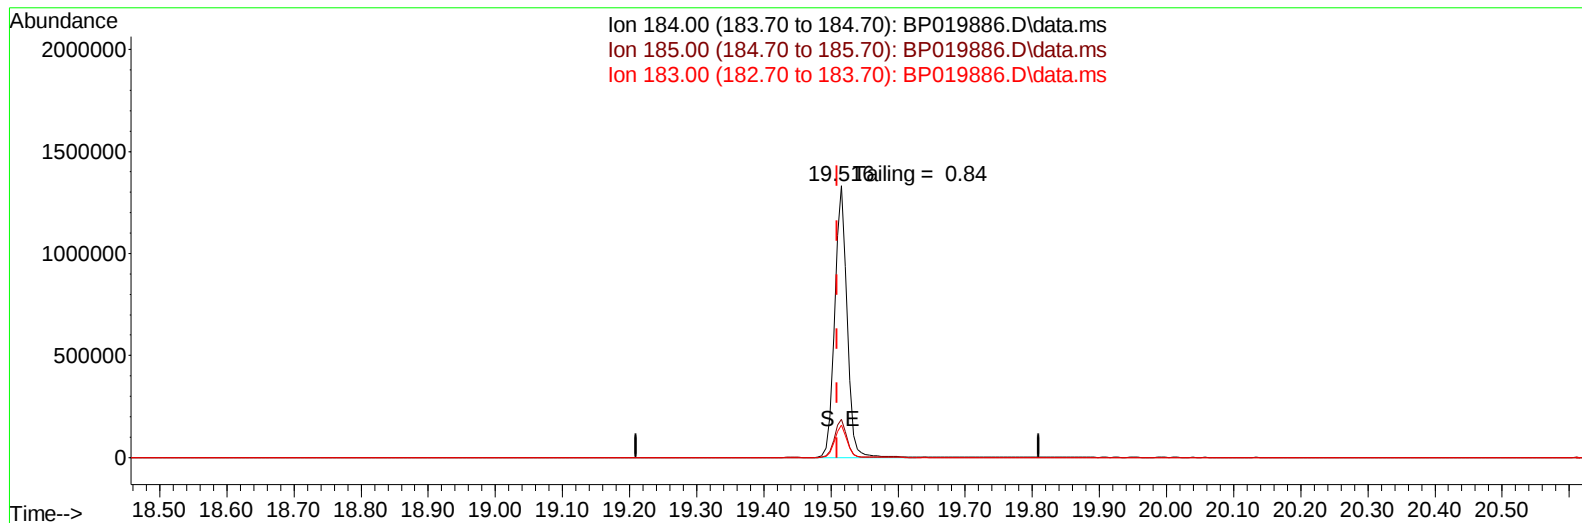

TIC: BP019886.D\data.ms

(77) Benzidine**19.516min (+ 0.006) 21101.25 ng****response 1703839**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.60	11.92
0.00	0.00	0.00