

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
 Data File : BP019893.D
 Acq On : 27 Feb 2024 13:11
 Operator : MA/JU
 Sample : P1564-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-16

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.017	323	328	336	rVB	24728	37615	1.30%	0.227%
2	5.470	398	405	418	rBV	754504	1158708	39.98%	7.001%
3	7.069	669	677	689	rBV	905169	1493458	51.53%	9.023%
4	7.899	811	818	828	rVB	299972	498956	17.22%	3.015%
5	9.069	1009	1017	1032	rBV	483771	876532	30.25%	5.296%
6	10.699	1284	1294	1306	rBV	366150	678895	23.43%	4.102%
7	11.475	1416	1426	1435	rBV2	13421	34866	1.20%	0.211%
8	13.163	1704	1713	1727	rBV	1429171	2213146	76.37%	13.372%
9	14.540	1939	1947	1964	rBV	622166	973981	33.61%	5.885%
10	14.763	1978	1985	1992	rVB6	14775	34927	1.21%	0.211%
11	16.040	2194	2202	2223	rBV	1118659	1787575	61.68%	10.800%
12	17.298	2409	2416	2425	rBV	714458	1122897	38.75%	6.784%
13	18.198	2563	2569	2579	rBV	264806	431584	14.89%	2.608%
14	19.439	2775	2780	2787	rBV	103476	167853	5.79%	1.014%
15	19.869	2848	2853	2862	rBV	2307425	2897970	100.00%	17.509%
16	21.122	3063	3066	3072	rBV	124239	168375	5.81%	1.017%
17	21.398	3108	3113	3121	rBV	702983	989969	34.16%	5.981%
18	23.821	3519	3525	3536	rVB	455022	983873	33.95%	5.944%




Sum of corrected areas: 16551180

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019893.D
Acq On : 27 Feb 2024 13:11
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

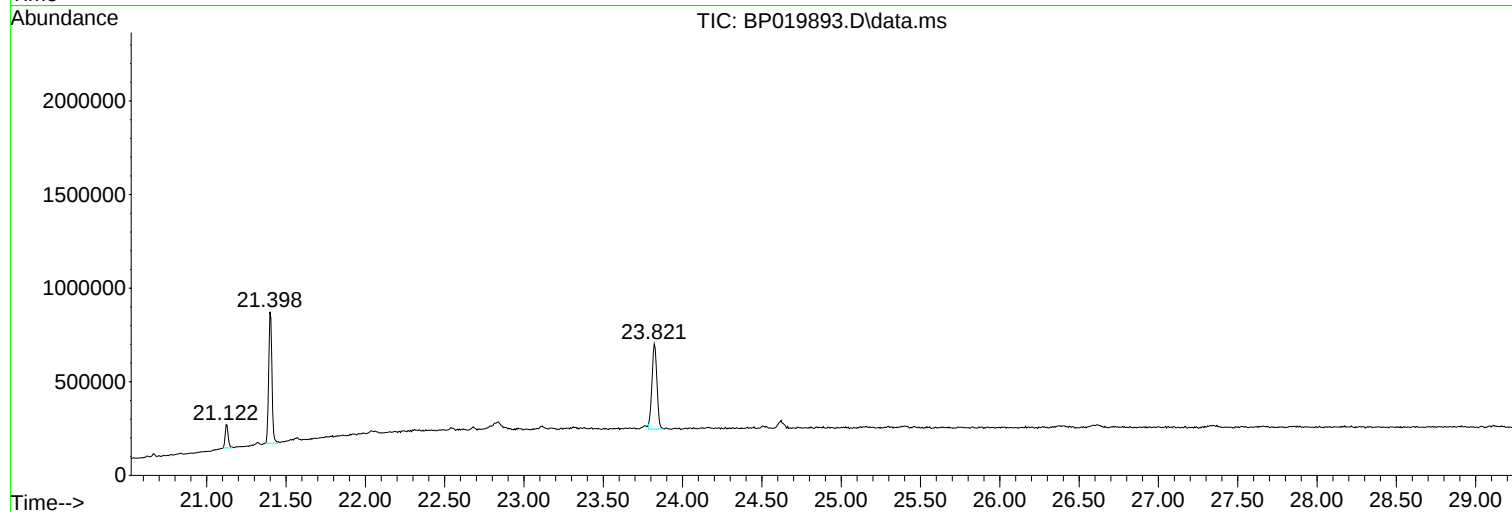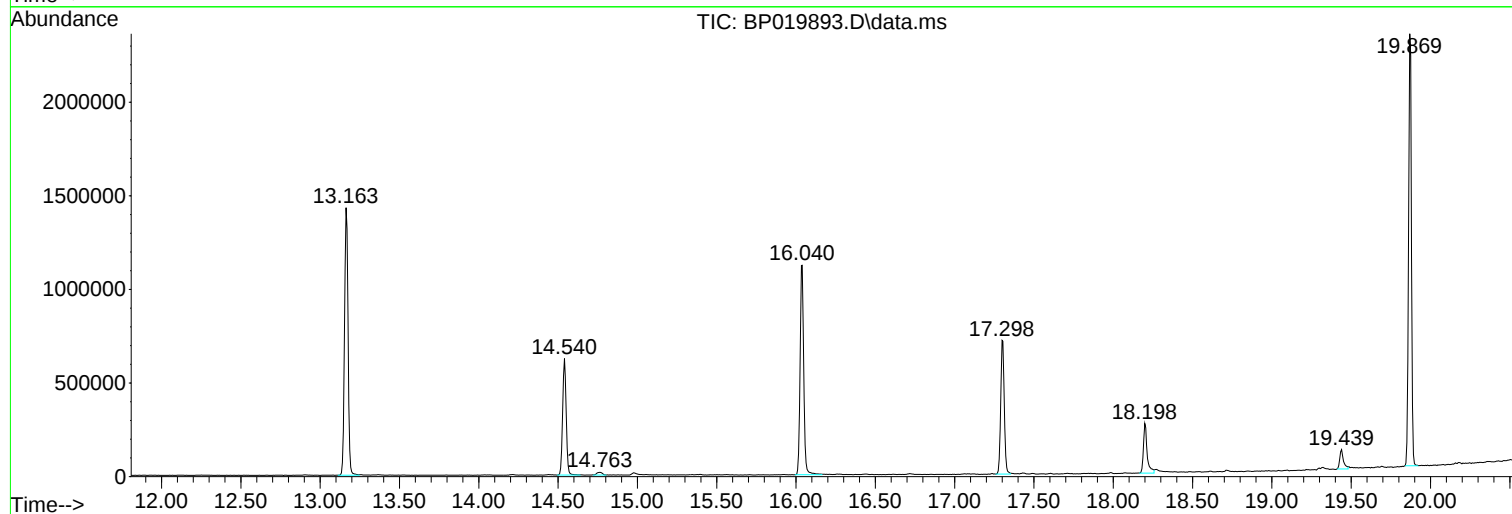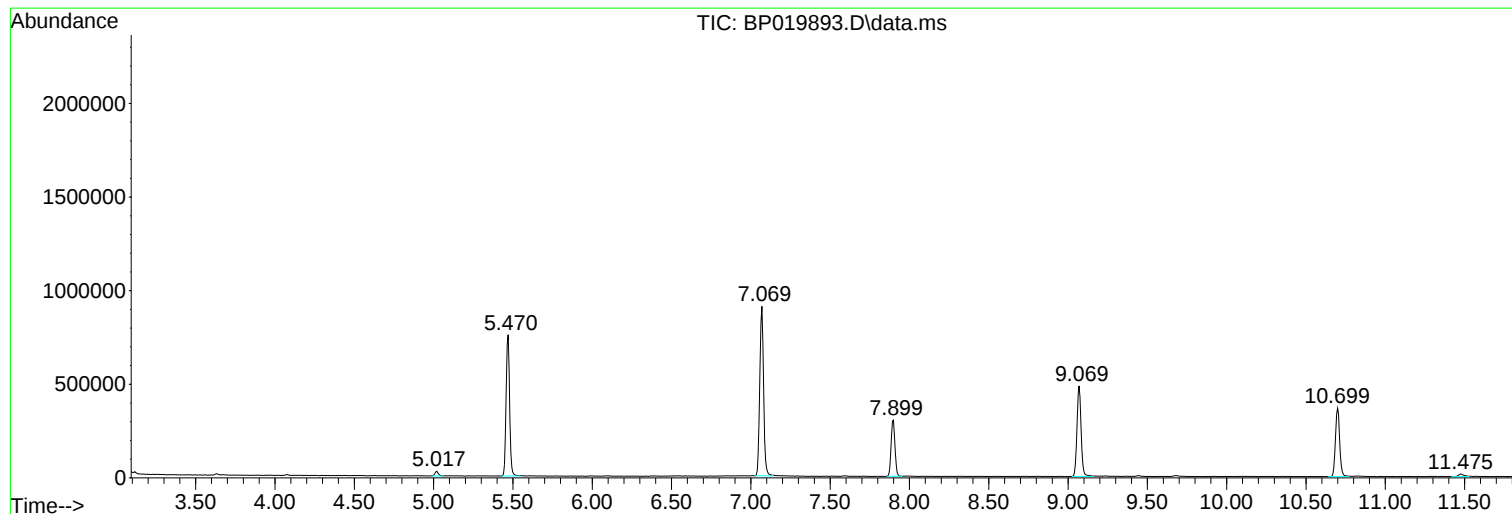

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019893.D
Acq On : 27 Feb 2024 13:11
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019893.D
Acq On : 27 Feb 2024 13:11
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------