
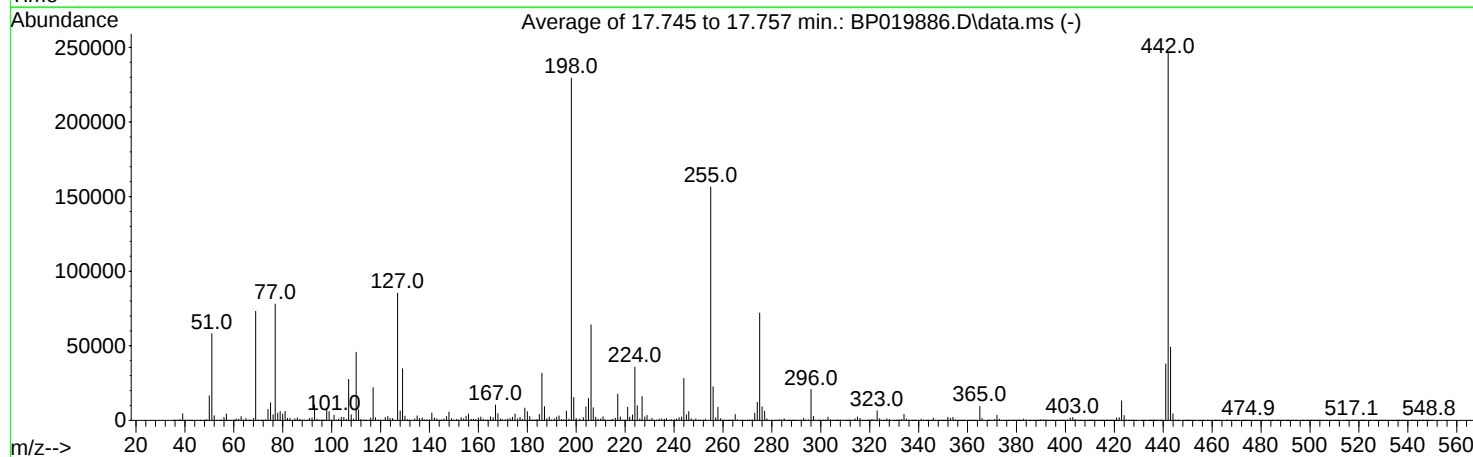


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019886.D
Acq On : 27 Feb 2024 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 27 02:05:05 2024

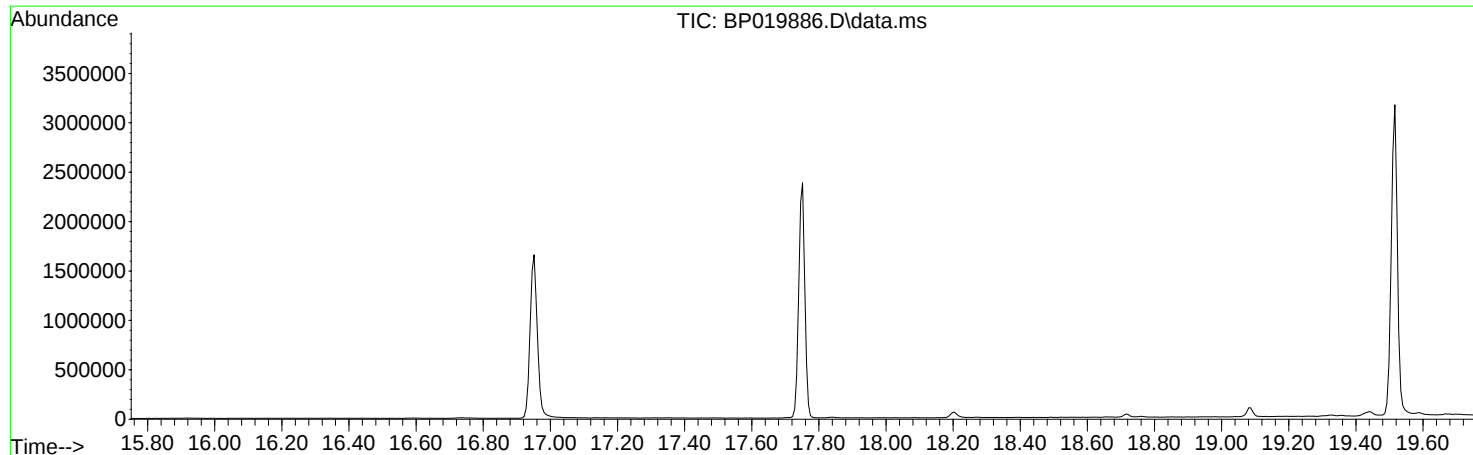




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	58128	PASS
68	69	0.00	2	1.8	1285	PASS
69	198	0.00	100	31.9	73143	PASS
70	69	0.00	2	0.5	330	PASS
127	198	10	80	37.2	85280	PASS
197	198	0.00	2	0.4	866	PASS
198	198	100	100	100.0	229487	PASS
199	198	5	9	6.7	15357	PASS
275	198	10	60	31.4	71952	PASS
365	198	1	100	4.1	9361	PASS
441	198	0.01	100	16.5	37827	PASS
442	442	100	100	100.0	246602	PASS
443	442	15	24	19.9	49042	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019886.D
Acq On : 27 Feb 2024 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 28 02:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

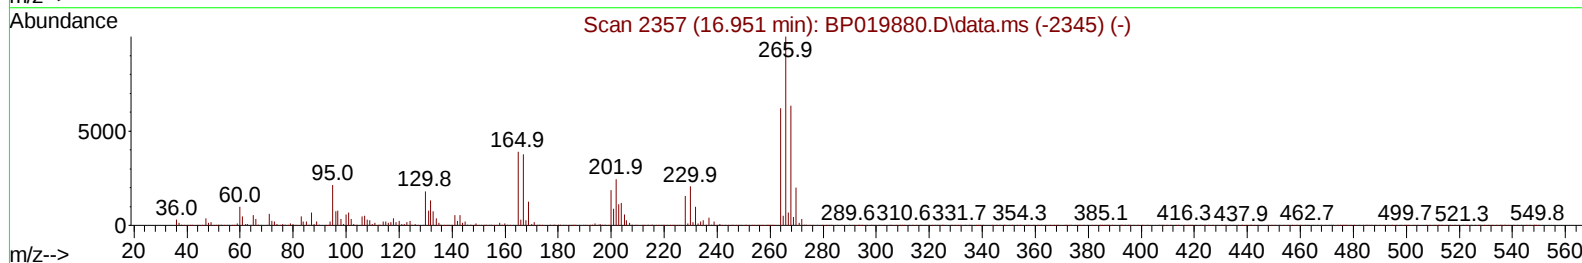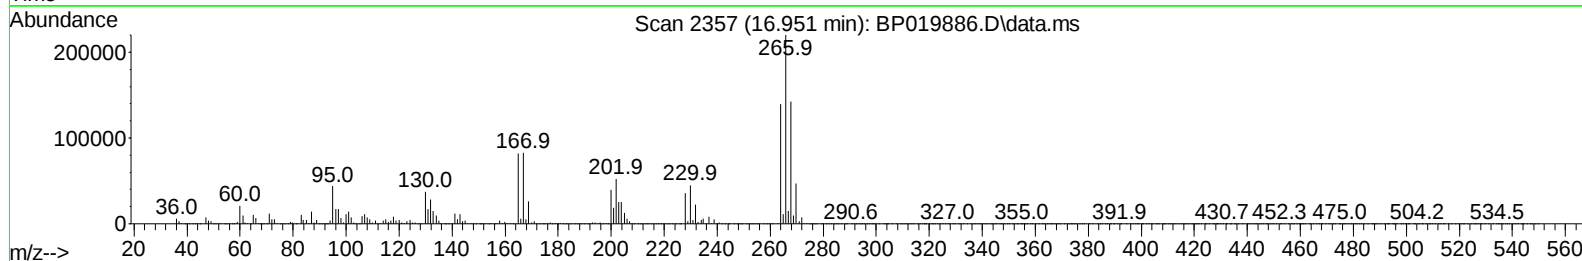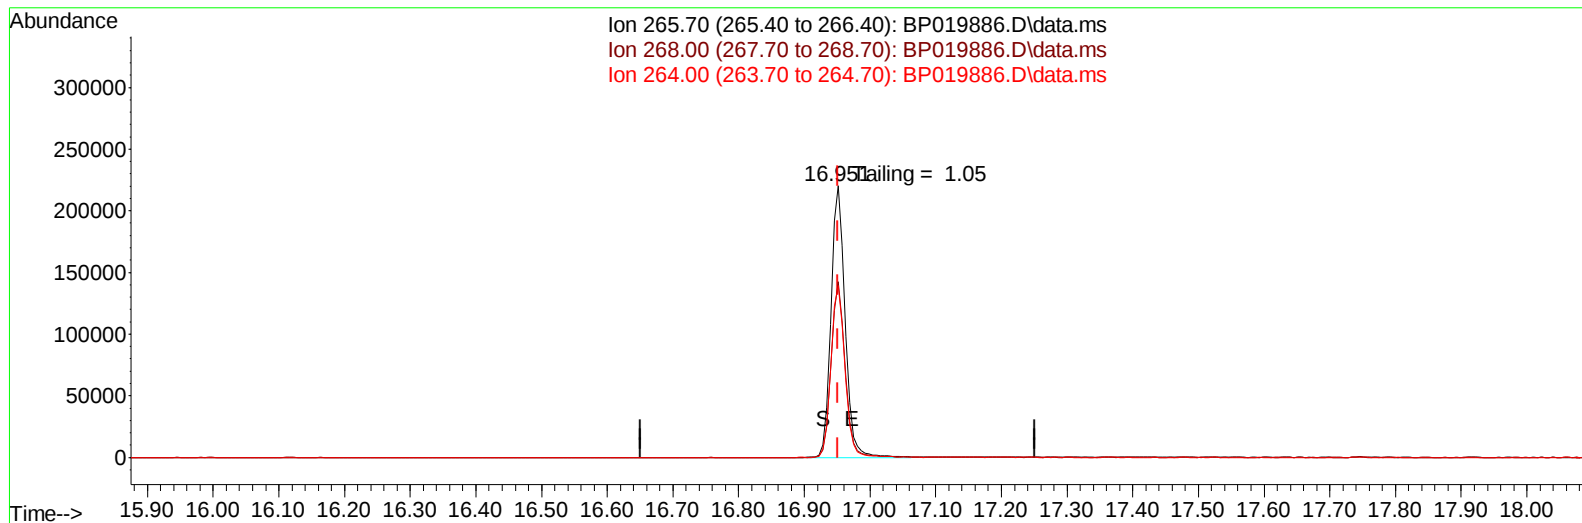

TIC: BP019886.D\data.ms

(70) Pentachlorophenol (C)

16.951min (+ 0.000) 35680.49 ng




response 331287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.74
264.00	62.10	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022724\
Data File : BP019886.D
Acq On : 27 Feb 2024 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 28 02:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

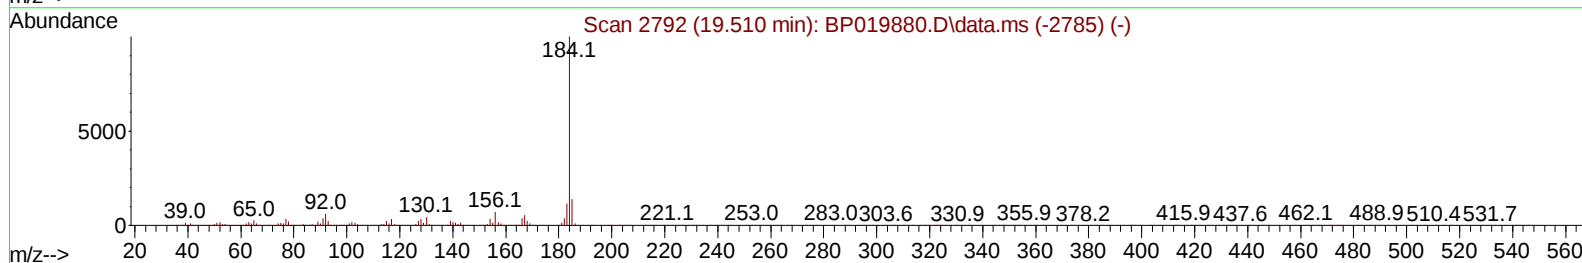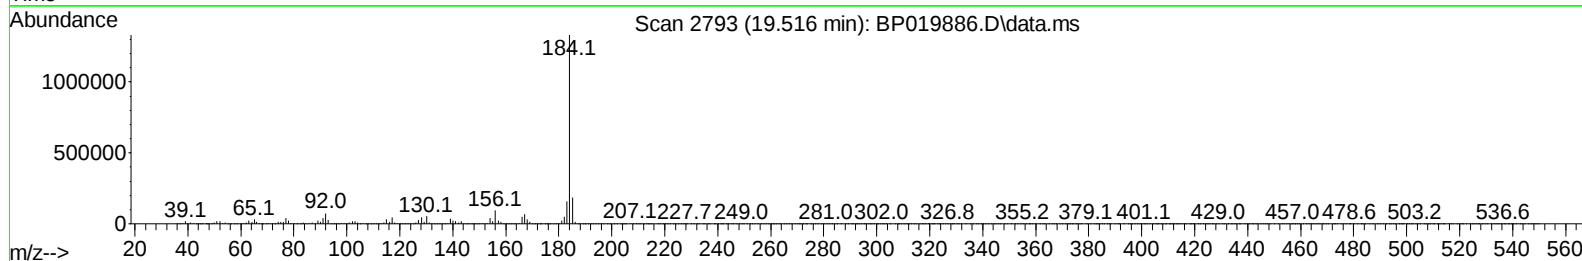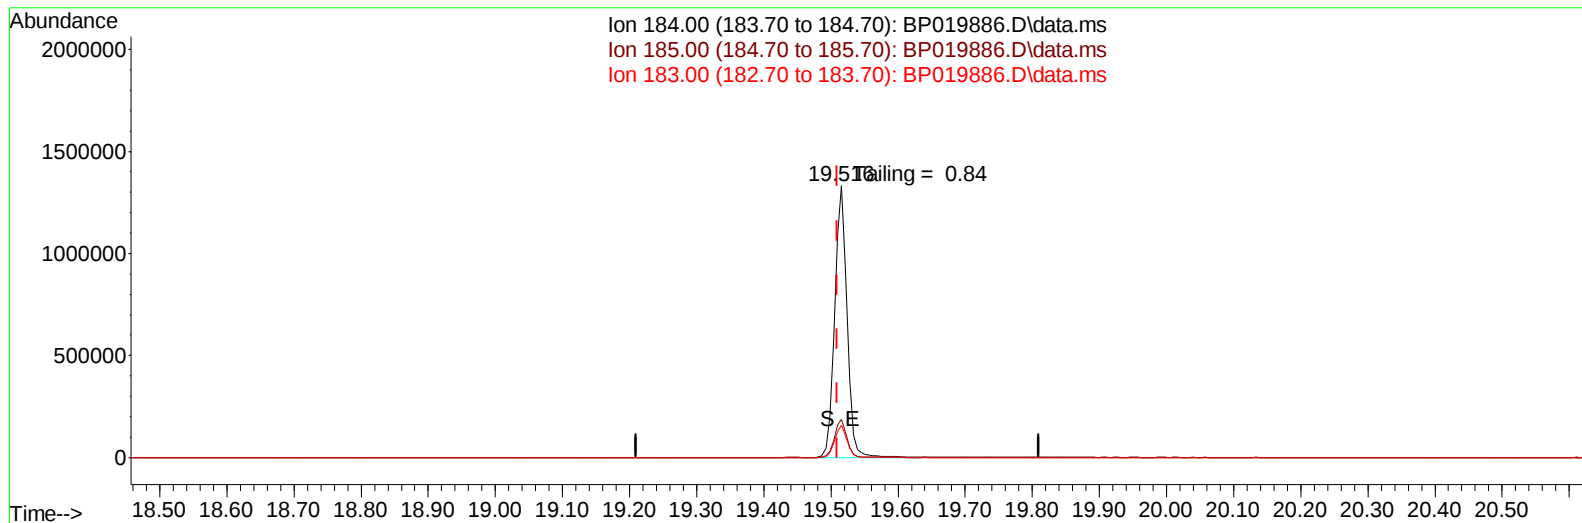

TIC: BP019886.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 21101.25 ng

response 1703839

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.60	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/27/2024	BNA_P	<u>BP019886.D</u>
Compound Name	Response	Retention Time
DDT	964958	20.71
DDD	14177	20.328
DDE	670	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14847	979805	1.52

Instrument :
BNA_P
ClientSampleId :
DFTPP