
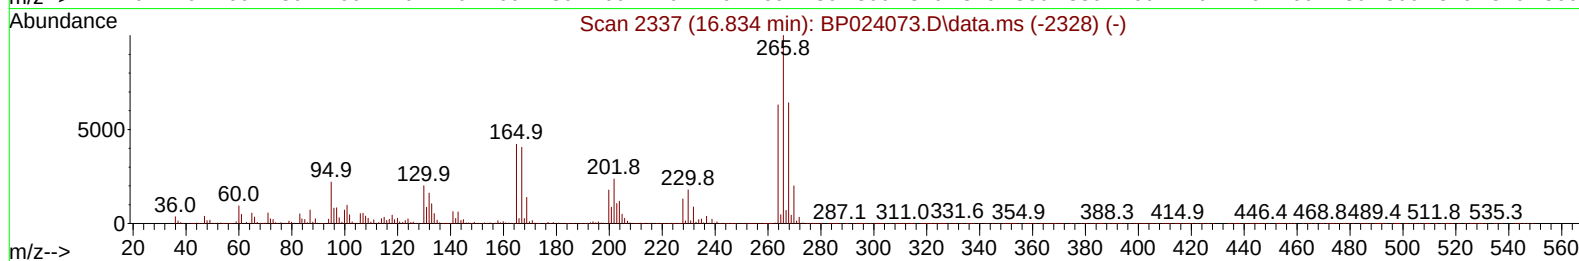
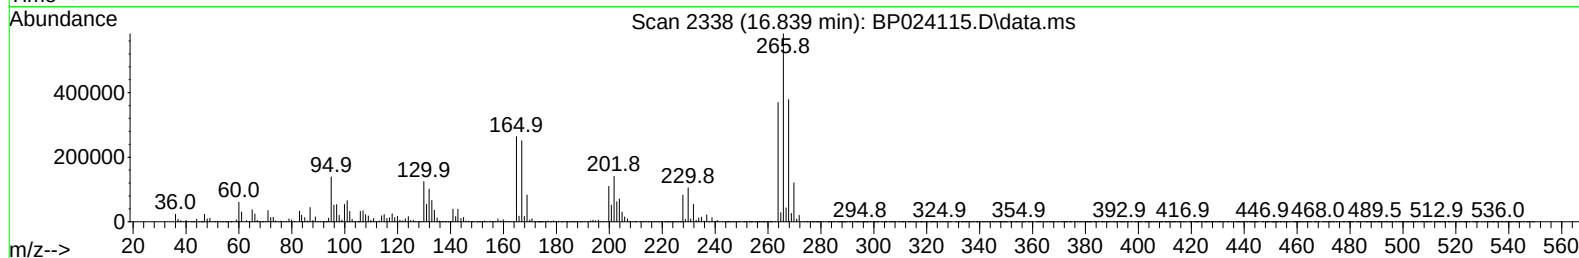


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024115.D
Acq On : 27 Feb 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 13:56:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

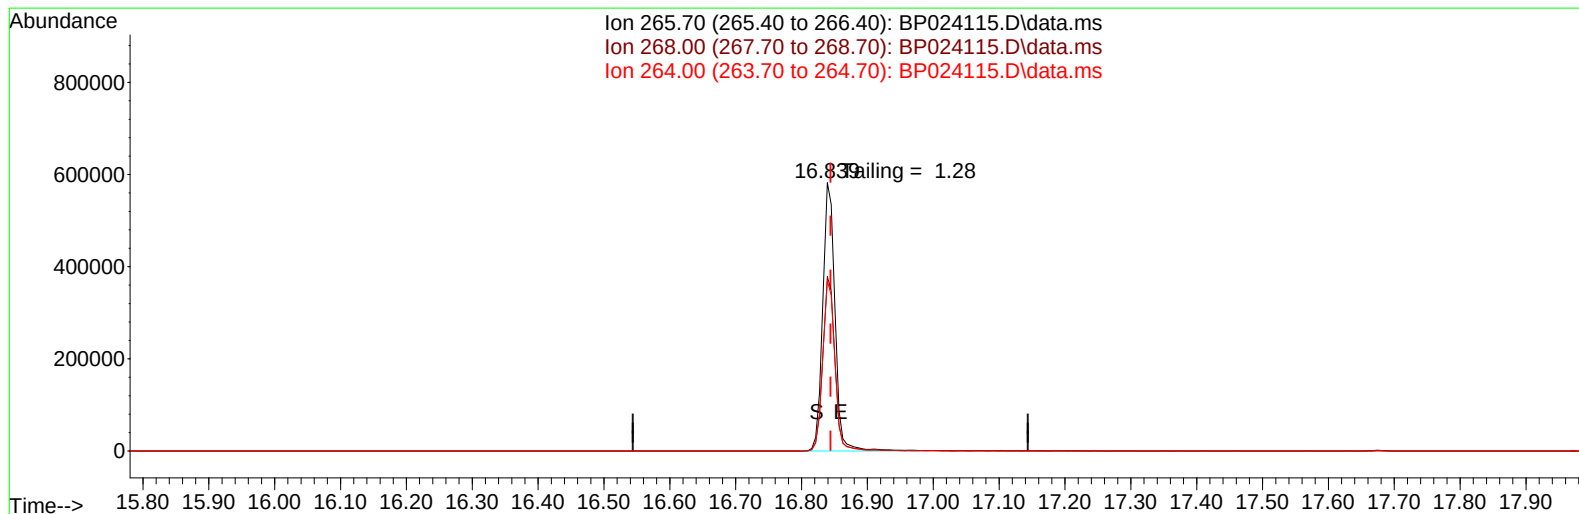

TIC: BP024115.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.005) 446010.46 ng

response 754050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.97
264.00	63.10	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024115.D
Acq On : 27 Feb 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 13:58:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

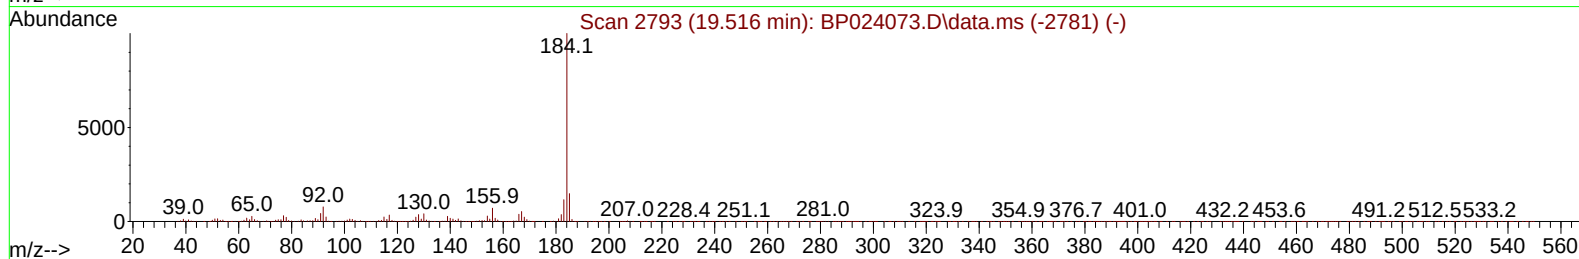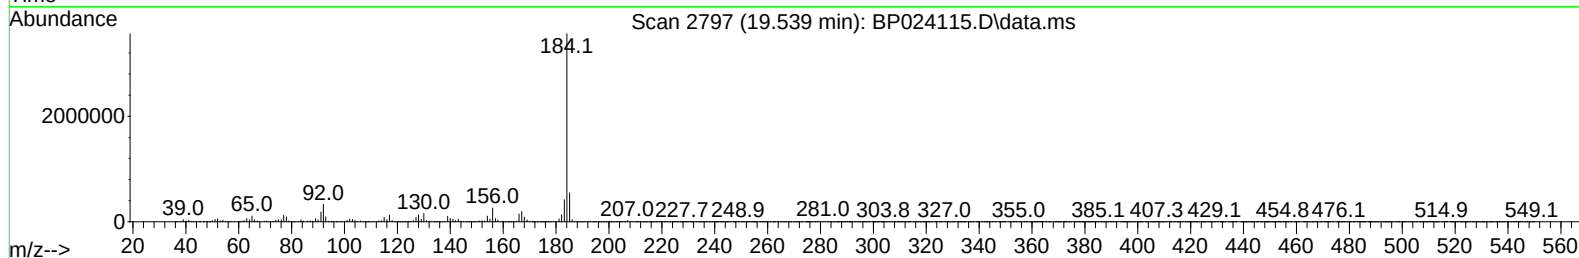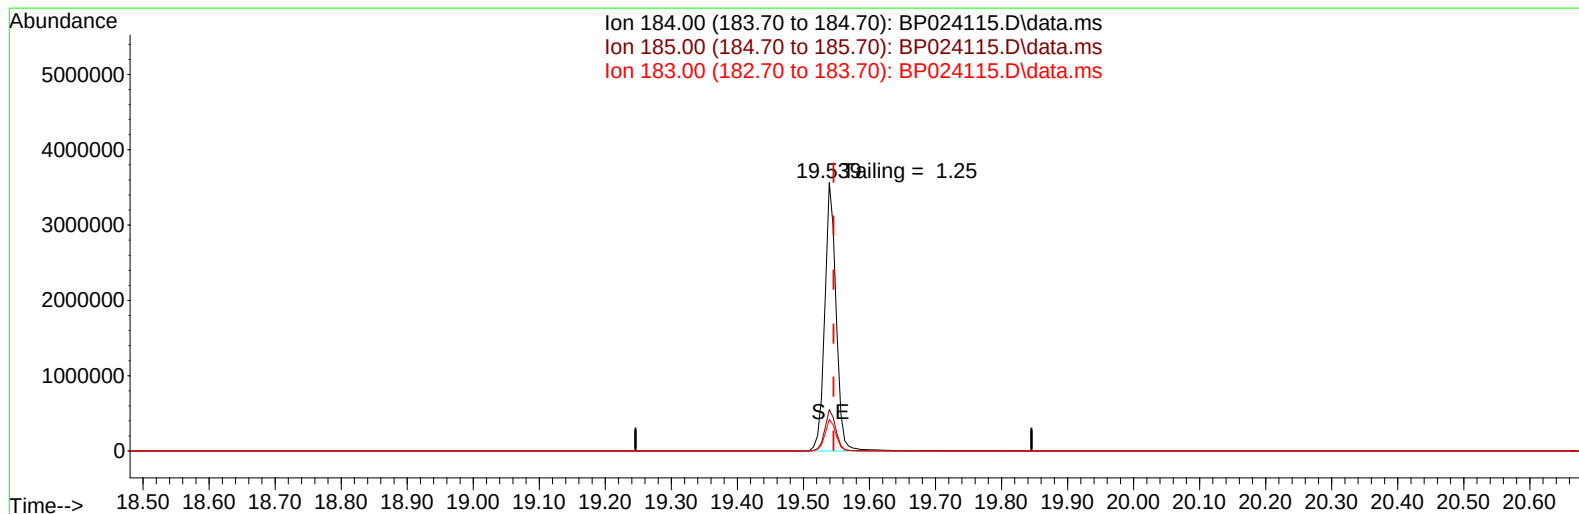

TIC: BP024115.D\data.ms

(77) Benzidine**19.539min (-0.007) 57911.67 ng****response 4286338**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.37
183.00	11.60	11.77
0.00	0.00	0.00