

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
 Data File : BP024117.D
 Acq On : 27 Feb 2025 11:47
 Operator : RC/JU
 Sample : PB166894BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB166894BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.346	377	384	400	rBV	9462387	13418772	59.41%	12.033%
2	6.917	642	651	675	rBV	8677231	13286844	58.82%	11.915%
3	7.734	782	790	799	rBV	1554536	2432401	10.77%	2.181%
4	8.881	977	985	1003	rBV	4839793	8459877	37.45%	7.586%
5	10.516	1252	1263	1281	rBV	2103633	3290089	14.57%	2.950%
6	12.993	1676	1684	1694	rBV	13069034	19773207	87.54%	17.731%
7	14.393	1914	1922	1937	rBV	2439142	4062251	17.98%	3.643%
8	15.916	2171	2181	2206	rBV	9121766	12626286	55.90%	11.322%
9	17.210	2394	2401	2413	rBV2	2809261	4259322	18.86%	3.819%
10	19.939	2859	2865	2873	rBV	19185594	22587304	100.00%	20.255%
11	21.663	3152	3158	3167	rVB	2343248	3753867	16.62%	3.366%
12	25.063	3727	3736	3754	rVB2	1203184	3565980	15.79%	3.198%




Sum of corrected areas: 111516200

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024117.D
Acq On : 27 Feb 2025 11:47
Operator : RC/JU
Sample : PB166894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

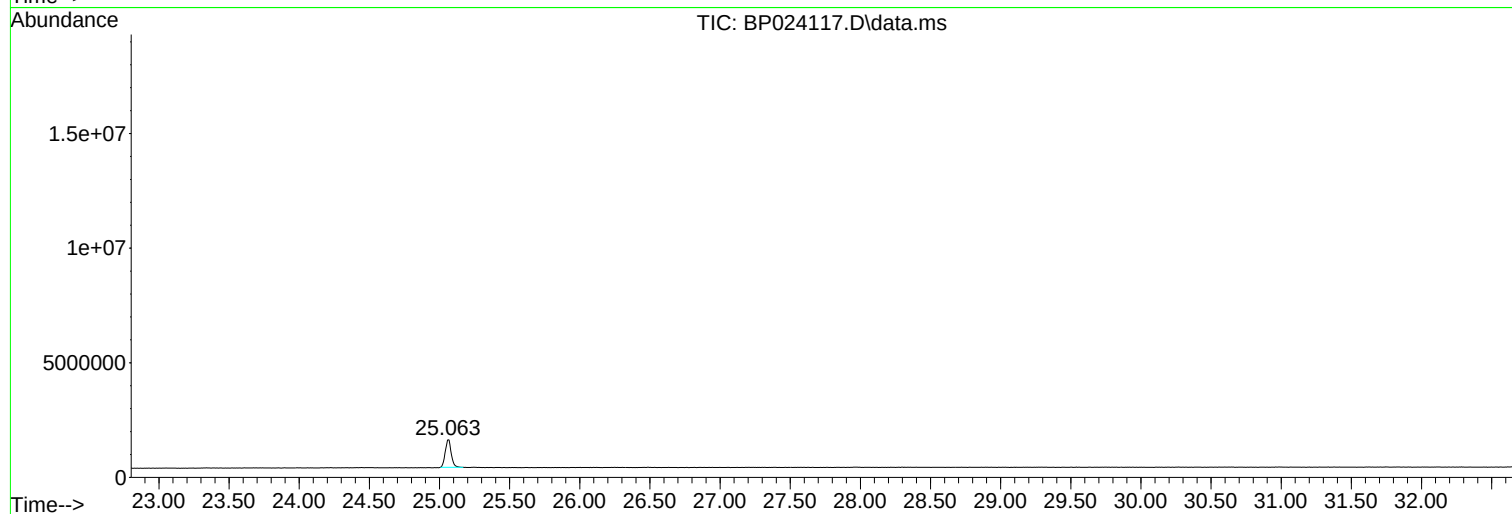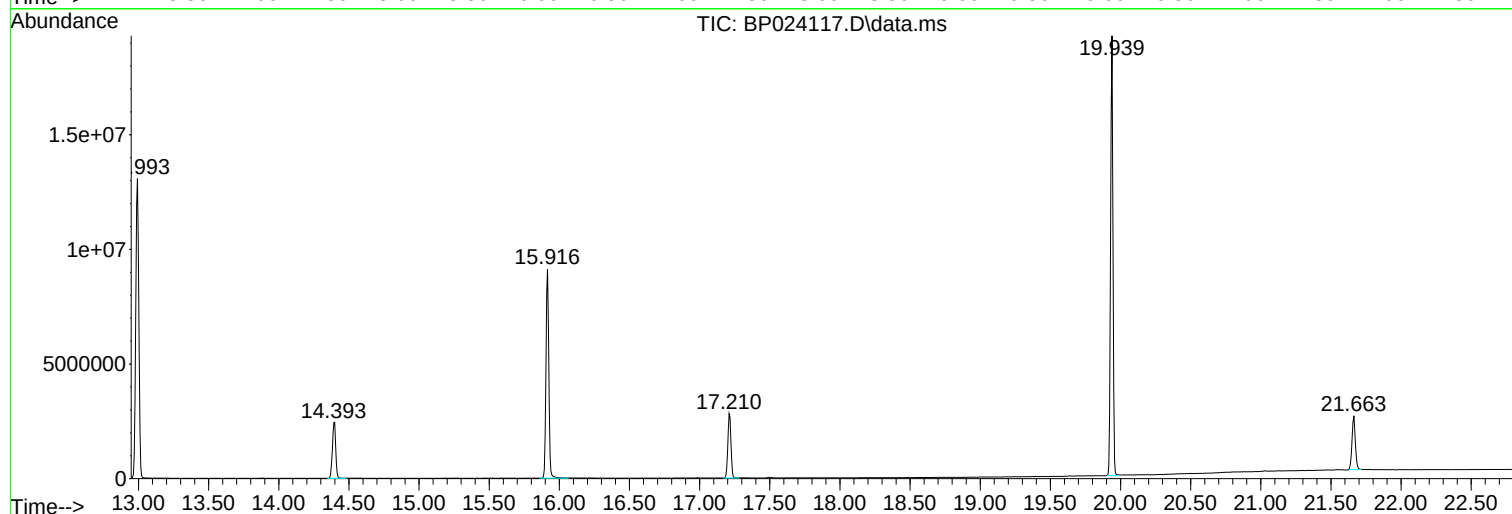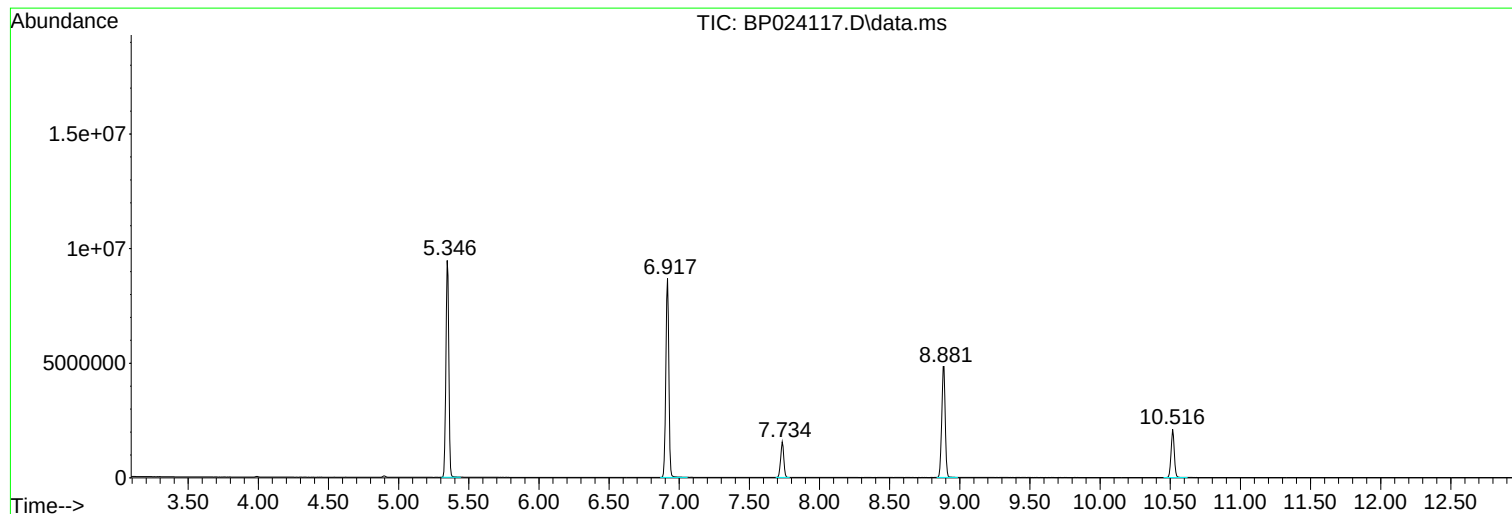

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024117.D
Acq On : 27 Feb 2025 11:47
Operator : RC/JU
Sample : PB166894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024117.D
Acq On : 27 Feb 2025 11:47
Operator : RC/JU
Sample : PB166894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------