
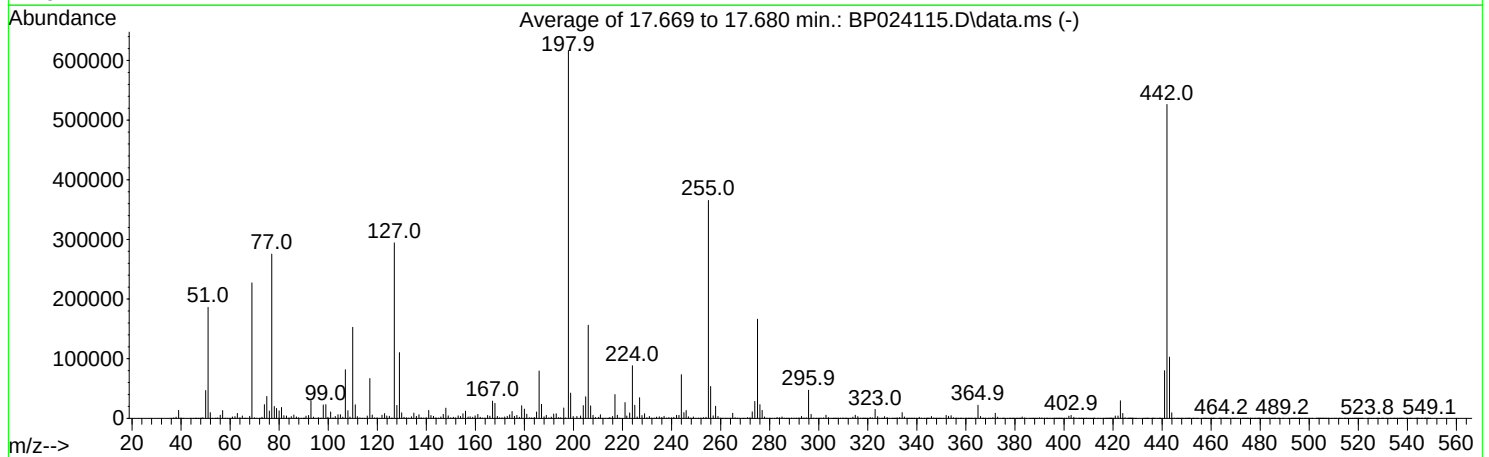


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024115.D
Acq On : 27 Feb 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

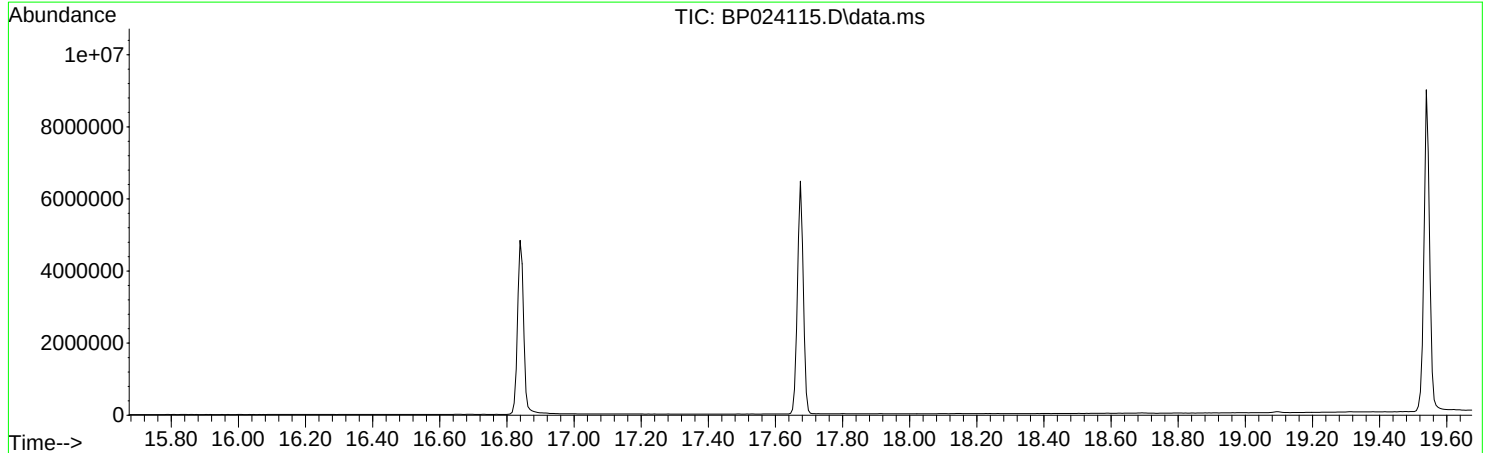

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	186291	PASS
68	69	0.00	2	1.5	3448	PASS
69	198	0.00	100	36.8	227157	PASS
70	69	0.00	2	0.4	979	PASS
127	198	10	80	47.7	294192	PASS
197	198	0.00	2	0.1	902	PASS
198	198	100	100	100.0	616770	PASS
199	198	5	9	6.9	42328	PASS
275	198	10	60	26.9	166208	PASS
365	198	1	100	3.5	21889	PASS
441	198	0.01	100	13.0	79905	PASS
442	442	100	100	100.0	526208	PASS
443	442	15	24	19.5	102666	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/27/2025	BNA_P	<u>BP024115.D</u>
Compound Name	Response	Retention Time
DDT	2101982	20.827
DDD	18091	20.421
DDE	803	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18894	2120876	0.89

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024115.D
Acq On : 27 Feb 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 27 13:56:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

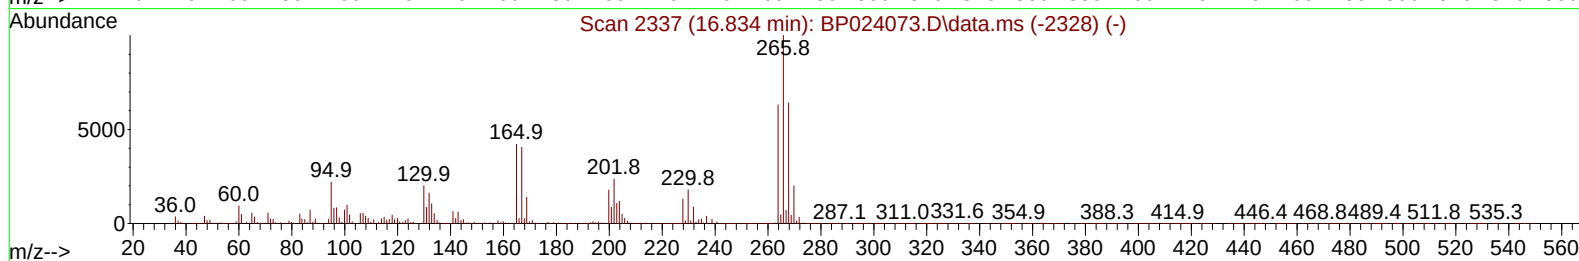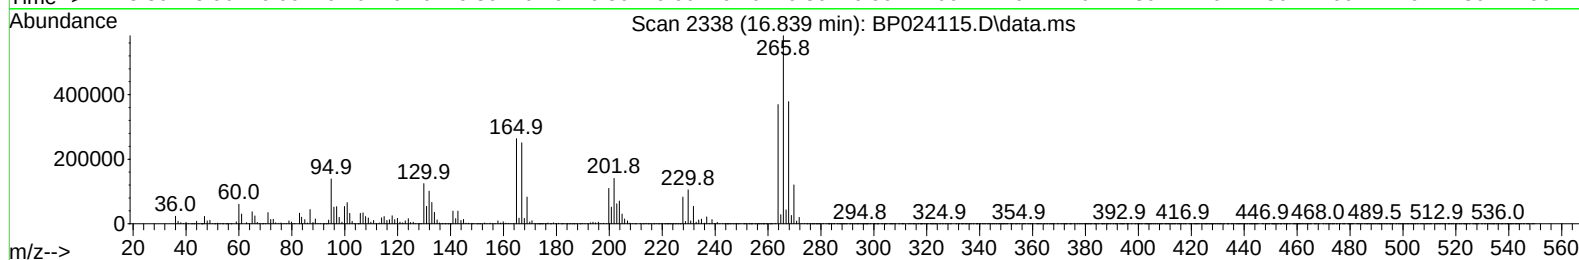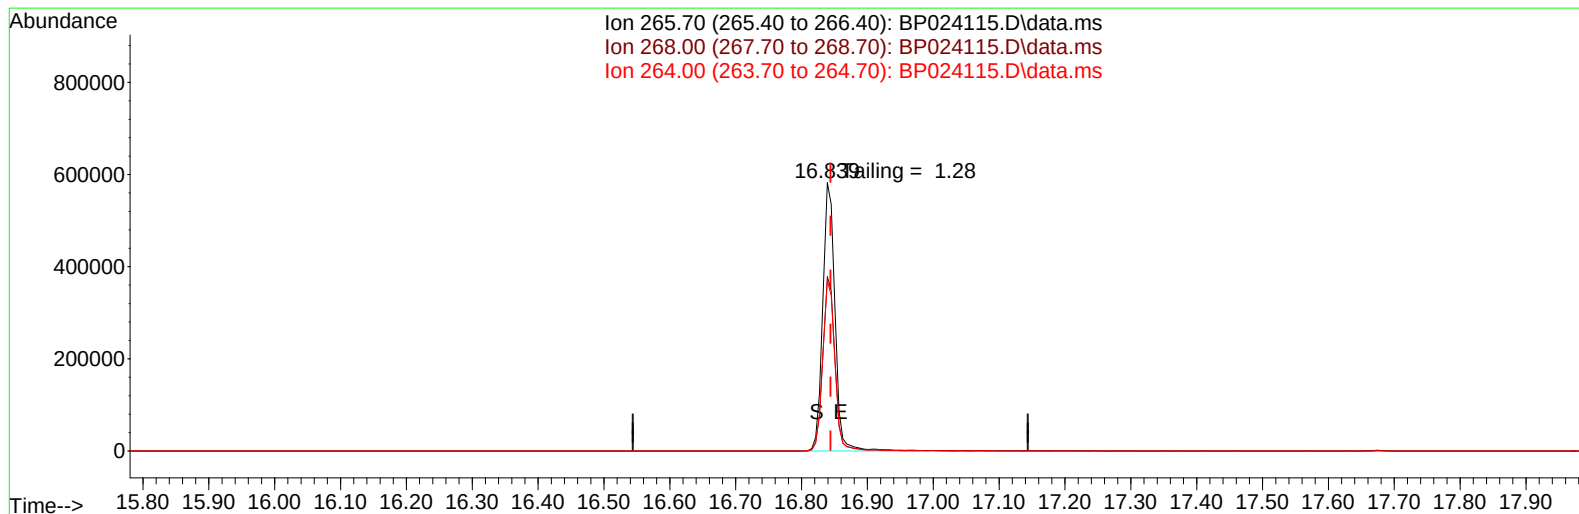

TIC: BP024115.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.005) 446010.46 ng




response 754050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.97
264.00	63.10	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022725\
Data File : BP024115.D
Acq On : 27 Feb 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 27 13:58:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

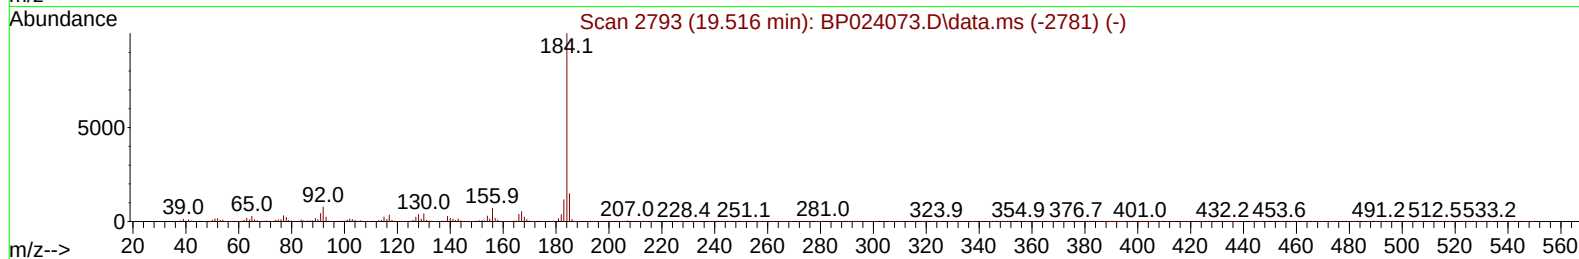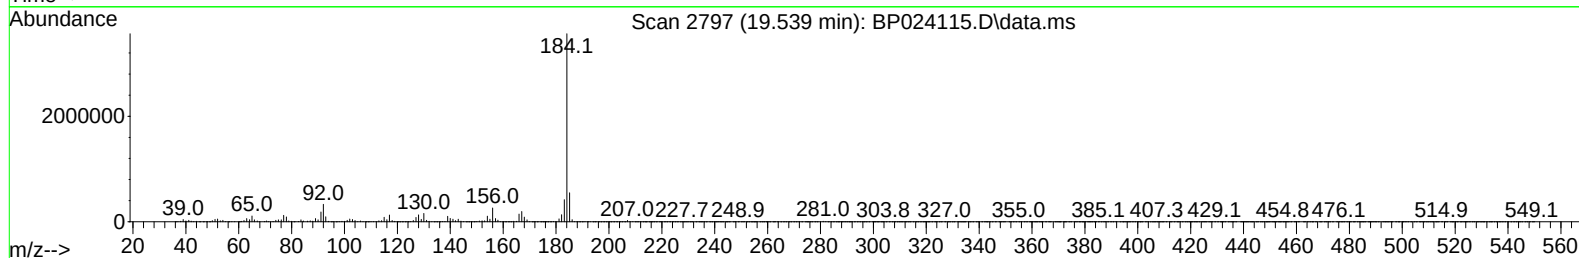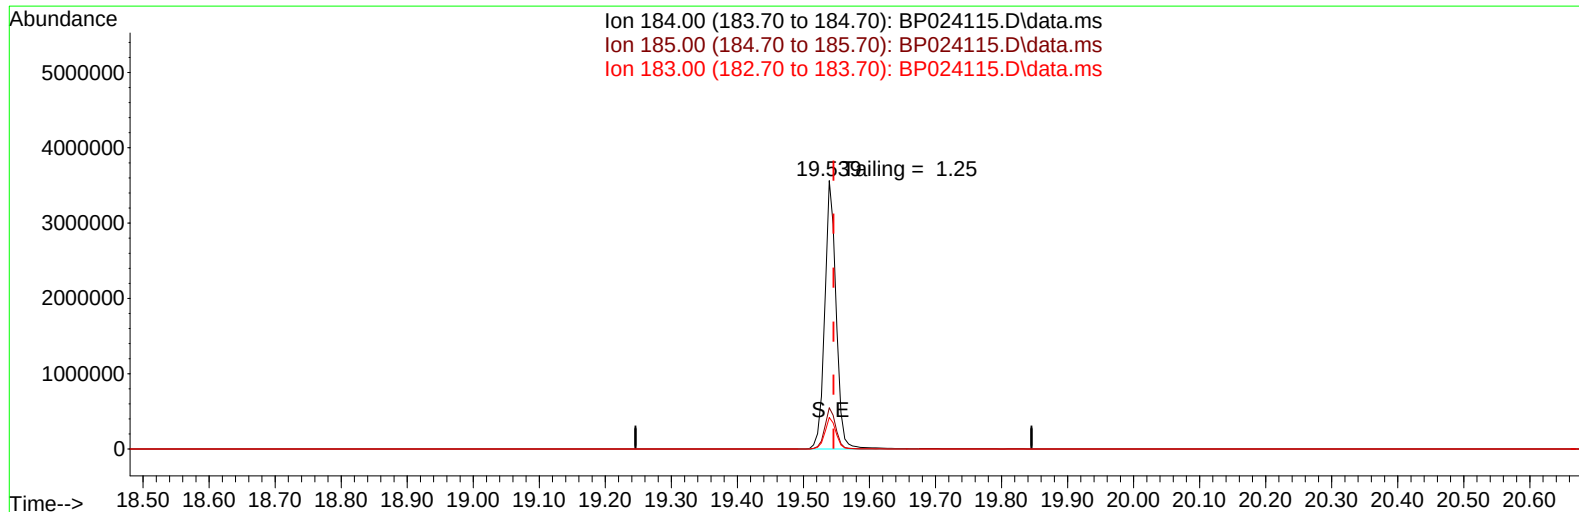

TIC: BP024115.D\data.ms

(77) Benzidine

19.539min (-0.007) 57911.67 ng

response 4286338

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.37
183.00	11.60	11.77
0.00	0.00	0.00