
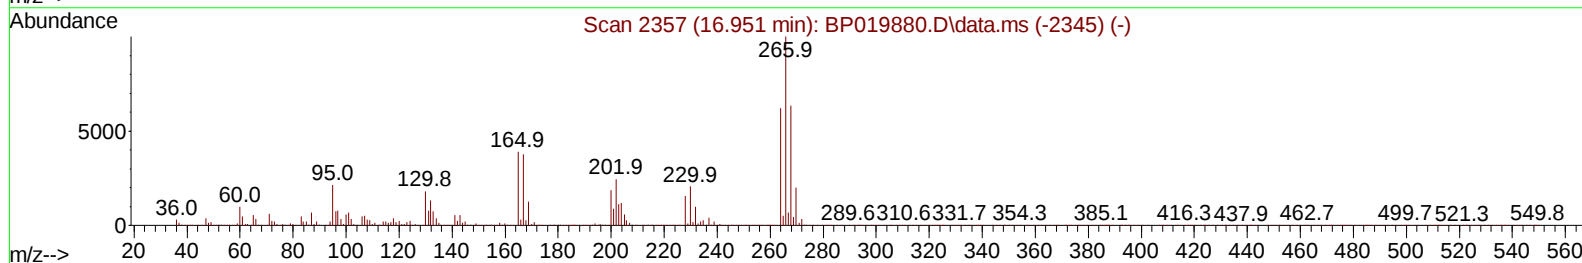
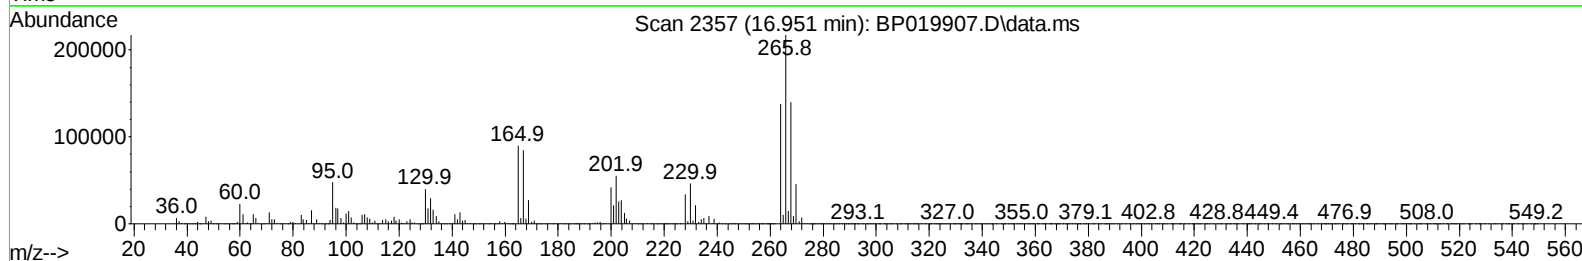


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022824\
Data File : BP019907.D
Acq On : 28 Feb 2024 09:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 01:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

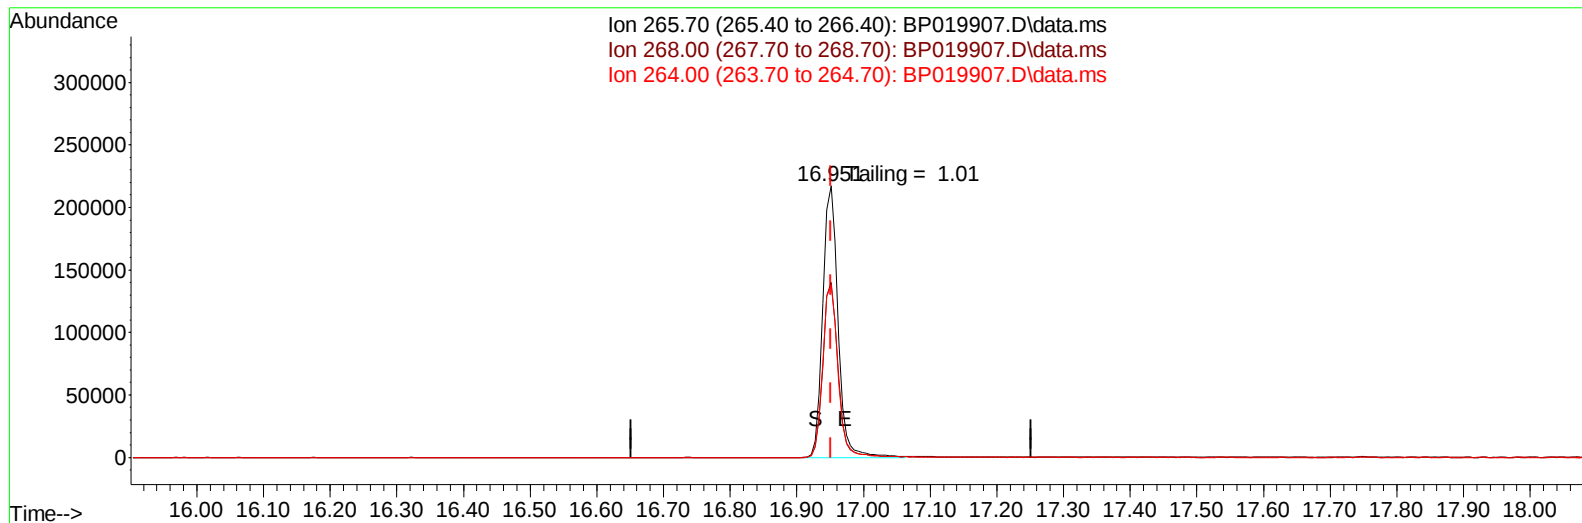

TIC: BP019907.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.000) 1738994.83 ng

response 342808

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.53
264.00	62.10	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022824\
Data File : BP019907.D
Acq On : 28 Feb 2024 09:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 01:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

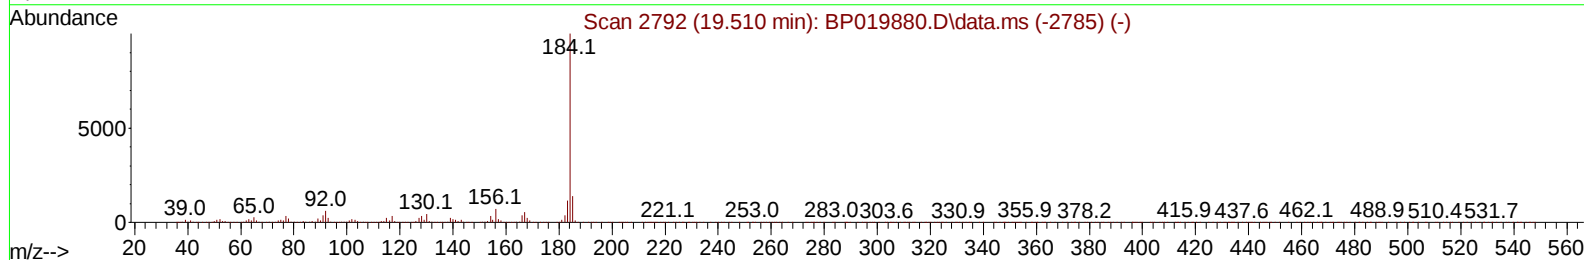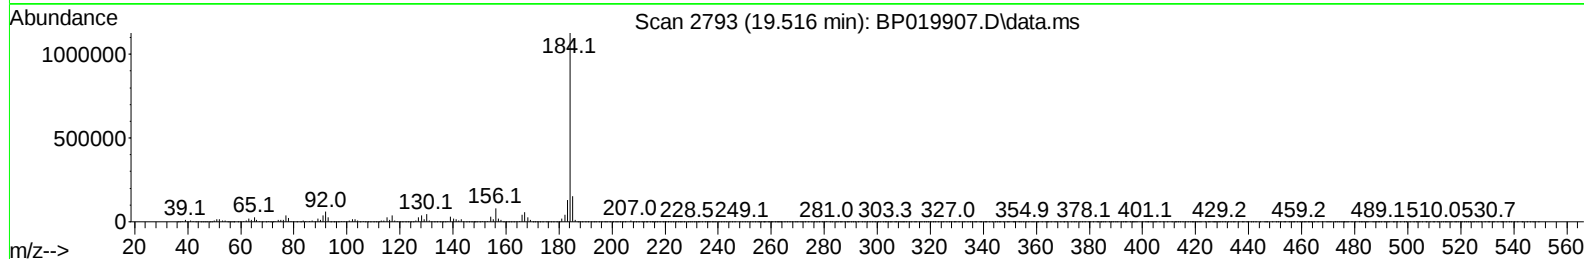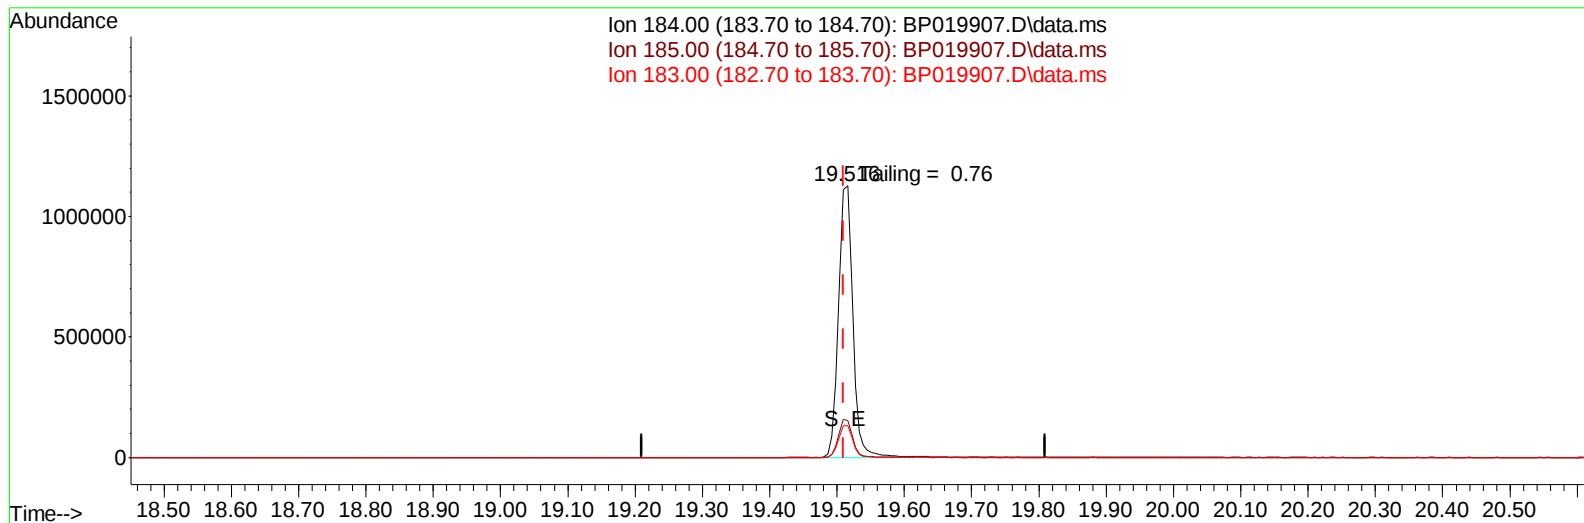

TIC: BP019907.D\data.ms

(77) Benzidine**19.516min (+ 0.006) 435399.25 ng****response 1663408**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.47
183.00	11.60	11.68
0.00	0.00	0.00