

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022824\  
 Data File : BP019909.D  
 Acq On : 28 Feb 2024 10:50  
 Operator : MA/JU  
 Sample : PB159054BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB159054BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP022624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019909.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.475       | 399           | 406         | 417          | rBV      | 1794465        | 2693655       | 22.24%          | 6.325%        |
| 2         | 7.075       | 671           | 678         | 696          | rBV      | 1694997        | 2871975       | 23.71%          | 6.743%        |
| 3         | 7.905       | 810           | 819         | 829          | rBV      | 344665         | 580202        | 4.79%           | 1.362%        |
| 4         | 9.075       | 1008          | 1018        | 1033         | rBV      | 1095495        | 1886938       | 15.58%          | 4.431%        |
| 5         | 10.704      | 1287          | 1295        | 1313         | rBV      | 424533         | 783886        | 6.47%           | 1.841%        |
| 6         | 13.169      | 1706          | 1714        | 1737         | rBV      | 4373714        | 6639131       | 54.80%          | 15.589%       |
| 7         | 14.545      | 1940          | 1948        | 1962         | rBV      | 1070148        | 1675407       | 13.83%          | 3.934%        |
| 8         | 16.039      | 2195          | 2202        | 2223         | rBV      | 3979985        | 6230328       | 51.43%          | 14.629%       |
| 9         | 17.304      | 2410          | 2417        | 2432         | rBV      | 1537606        | 2310452       | 19.07%          | 5.425%        |
| 10        | 19.586      | 2801          | 2805        | 2809         | rBV      | 173834         | 194497        | 1.61%           | 0.457%        |
| 11        | 19.880      | 2848          | 2855        | 2864         | rBV      | 9093881        | 12114145      | 100.00%         | 28.444%       |
| 12        | 20.610      | 2975          | 2979        | 2984         | rVB      | 134944         | 146669        | 1.21%           | 0.344%        |
| 13        | 21.404      | 3109          | 3114        | 3124         | rBV      | 1761823        | 2383939       | 19.68%          | 5.598%        |
| 14        | 23.827      | 3520          | 3526        | 3538         | rVB      | 1019499        | 2077779       | 17.15%          | 4.879%        |




Sum of corrected areas: 42589003

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022824\  
Data File : BP019909.D  
Acq On : 28 Feb 2024 10:50  
Operator : MA/JU  
Sample : PB159054BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB159054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP022624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

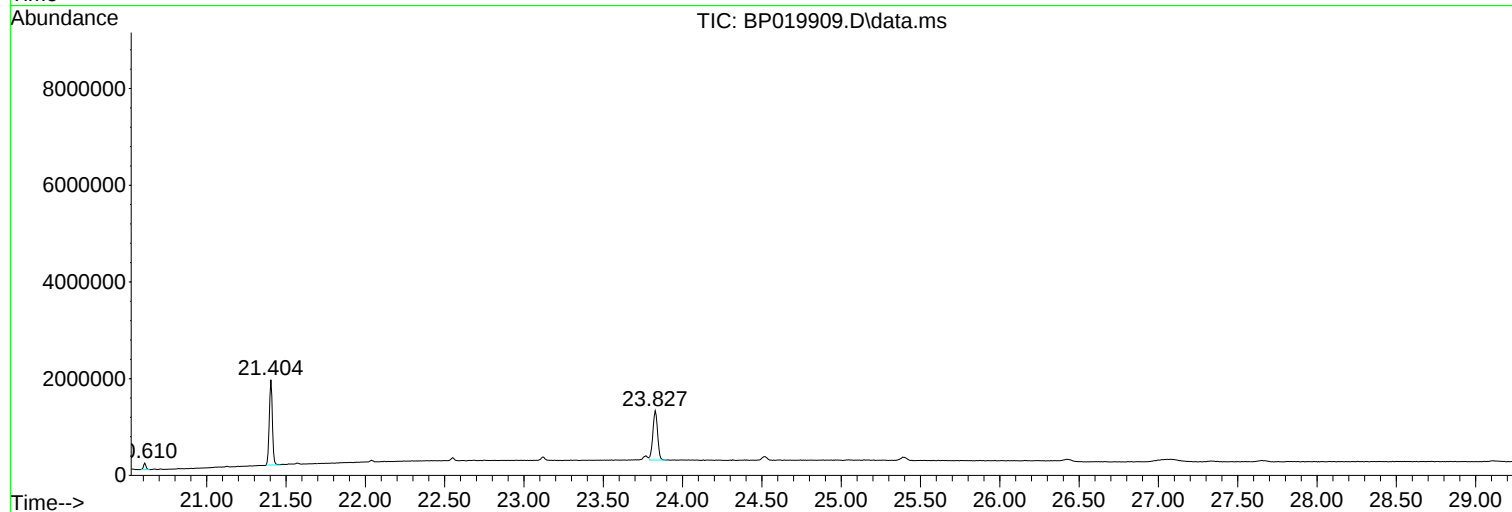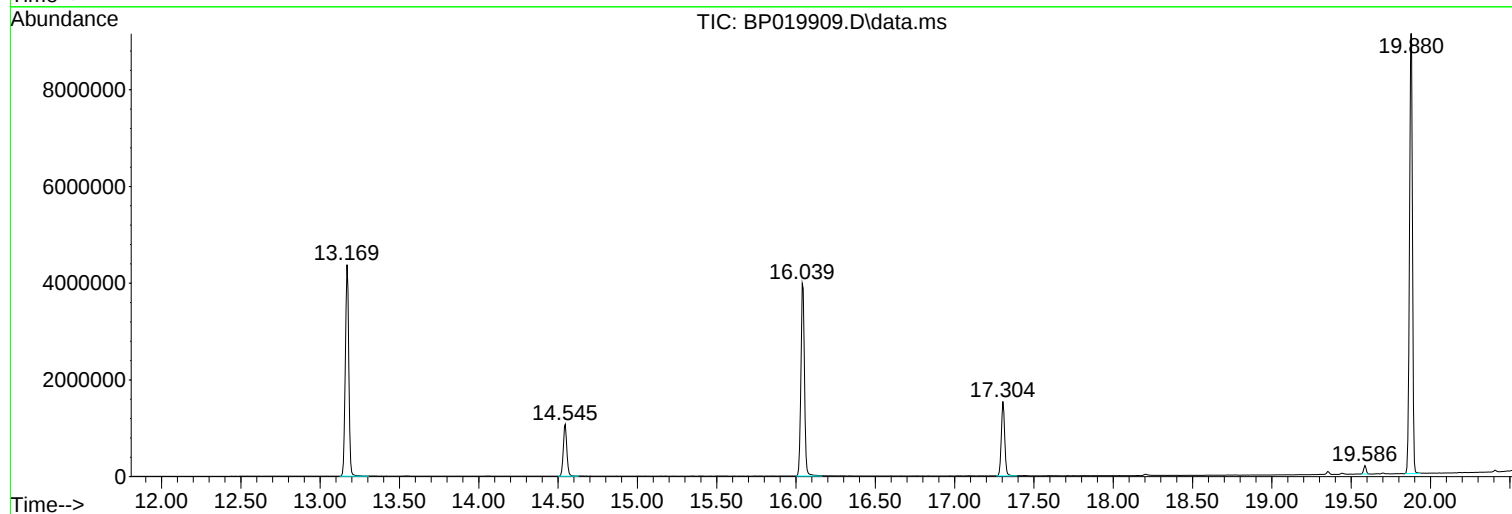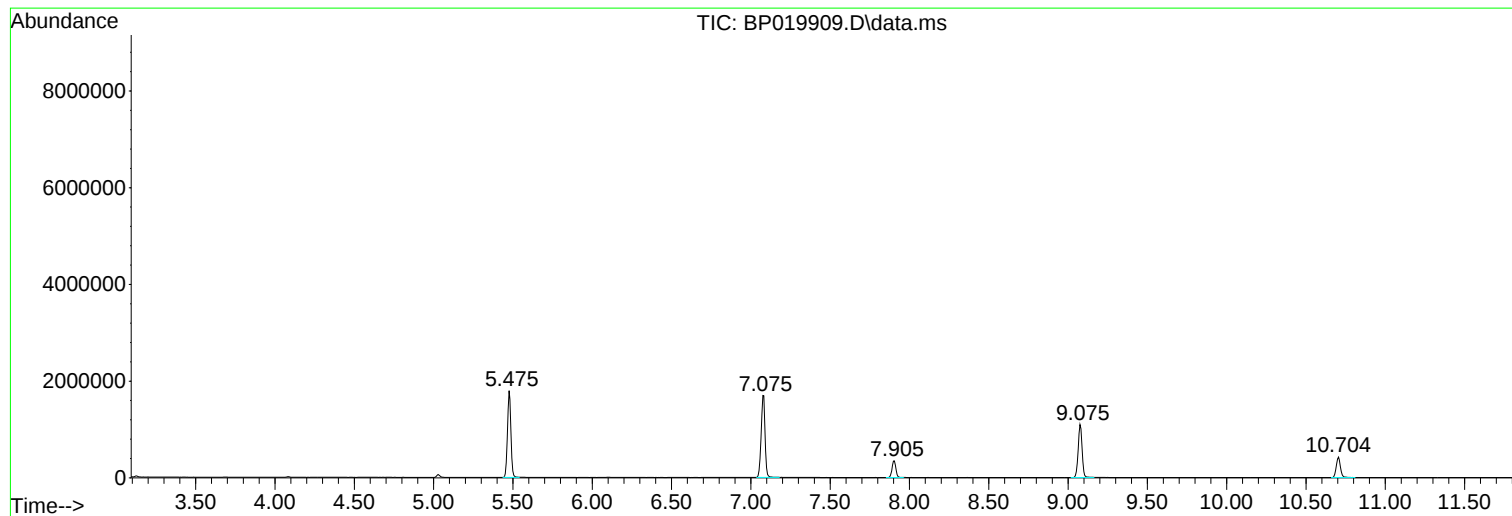

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022824\  
Data File : BP019909.D  
Acq On : 28 Feb 2024 10:50  
Operator : MA/JU  
Sample : PB159054BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB159054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP022624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022824\  
Data File : BP019909.D  
Acq On : 28 Feb 2024 10:50  
Operator : MA/JU  
Sample : PB159054BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB159054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP022624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|