
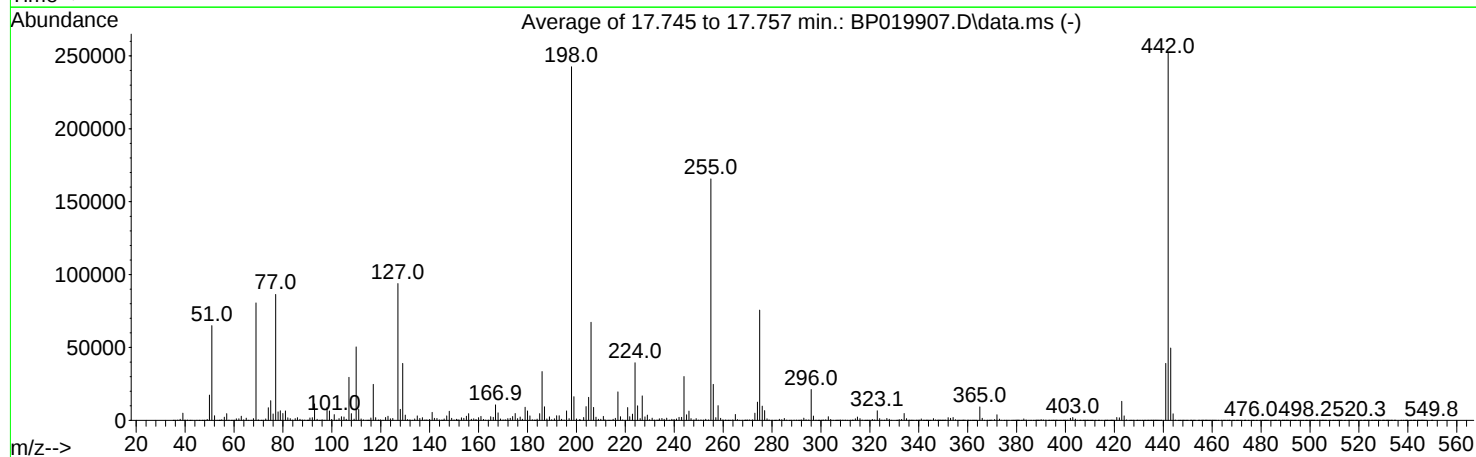


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022824\
Data File : BP019907.D
Acq On : 28 Feb 2024 09:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 27 02:05:05 2024

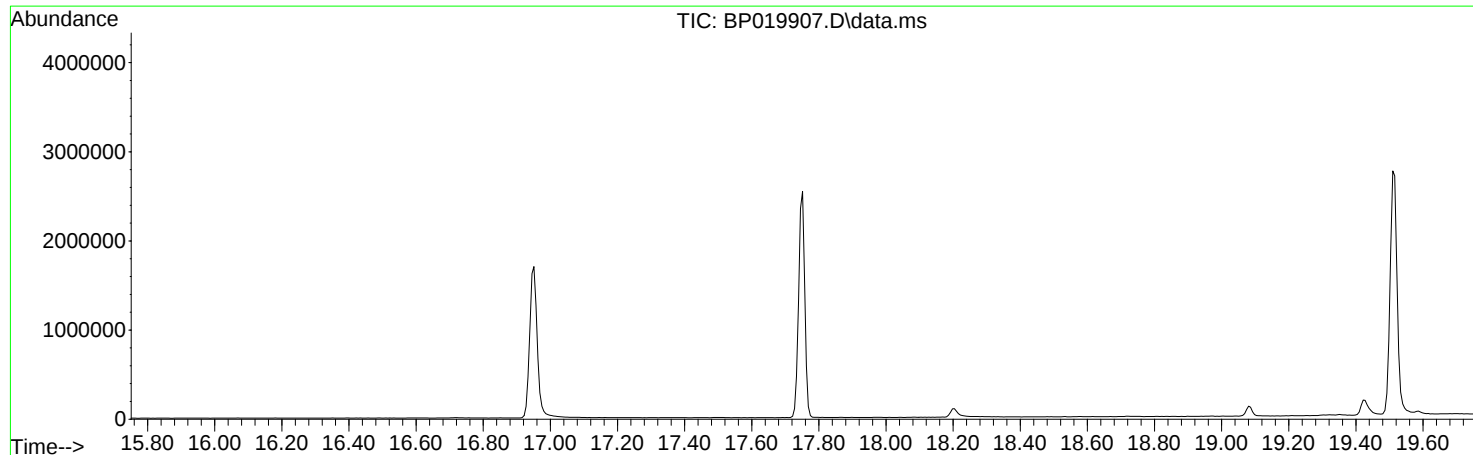




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	65036	PASS
68	69	0.00	2	1.5	1240	PASS
69	198	0.00	100	33.2	80556	PASS
70	69	0.00	2	0.5	392	PASS
127	198	10	80	38.7	93832	PASS
197	198	0.00	2	0.5	1259	PASS
198	198	100	100	100.0	242631	PASS
199	198	5	9	6.7	16256	PASS
275	198	10	60	31.2	75660	PASS
365	198	1	100	3.8	9273	PASS
441	198	0.01	100	16.1	39056	PASS
442	442	100	100	100.0	252352	PASS
443	442	15	24	19.6	49579	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022824\
Data File : BP019907.D
Acq On : 28 Feb 2024 09:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 29 01:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

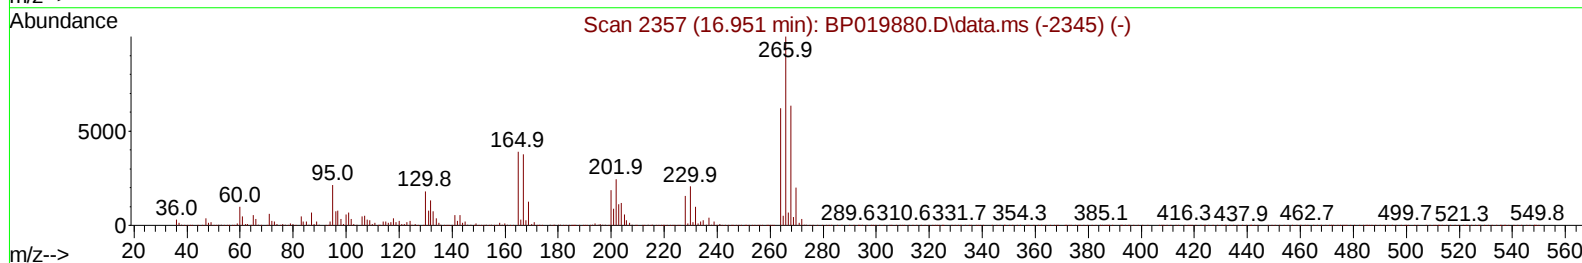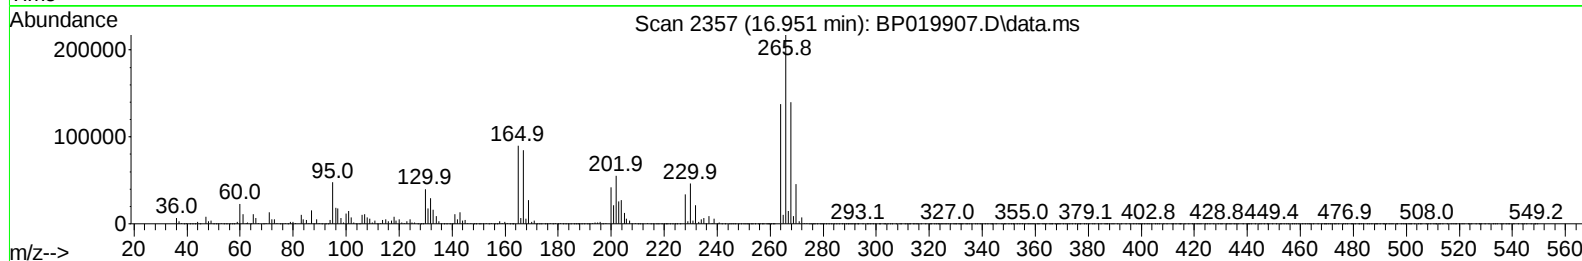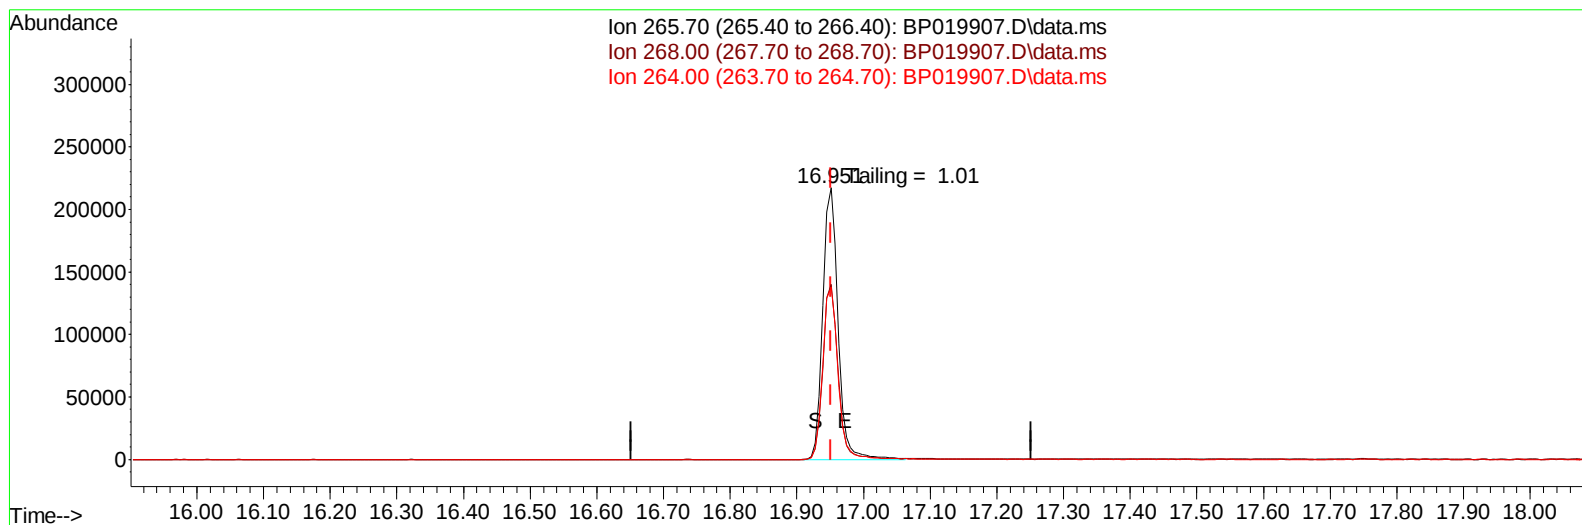

TIC: BP019907.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 1738994.83 ng




response 342808

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.53
264.00	62.10	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022824\
Data File : BP019907.D
Acq On : 28 Feb 2024 09:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 29 01:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

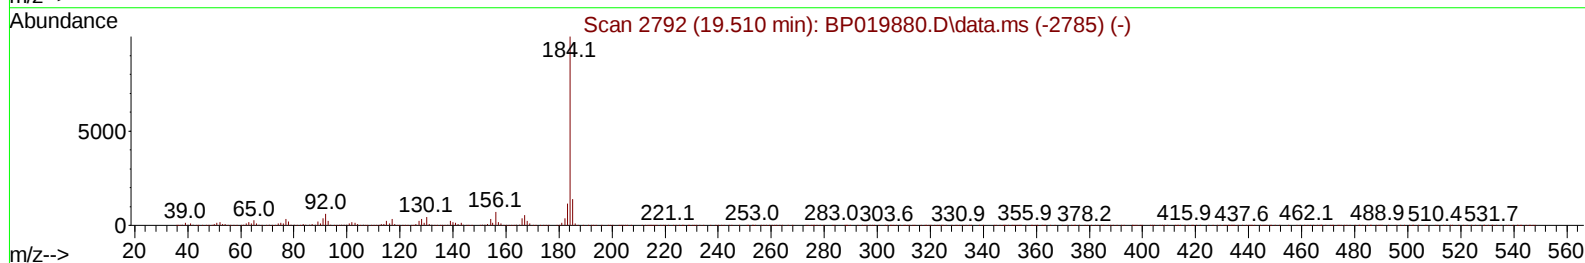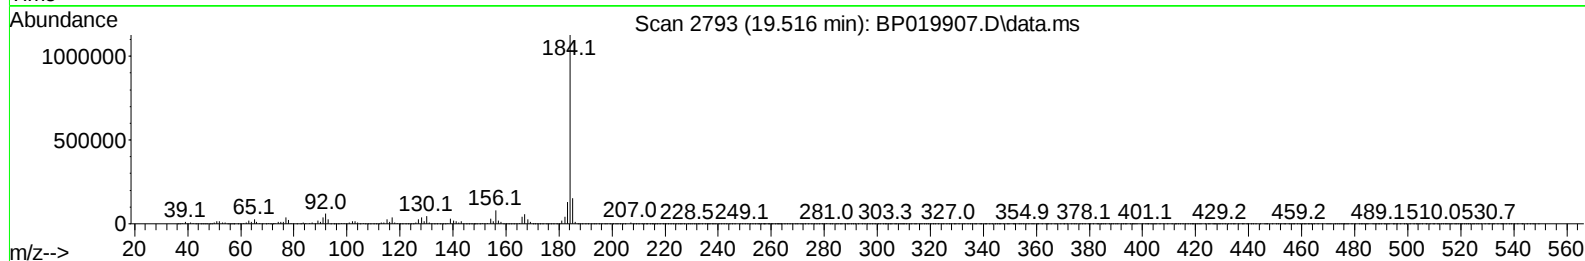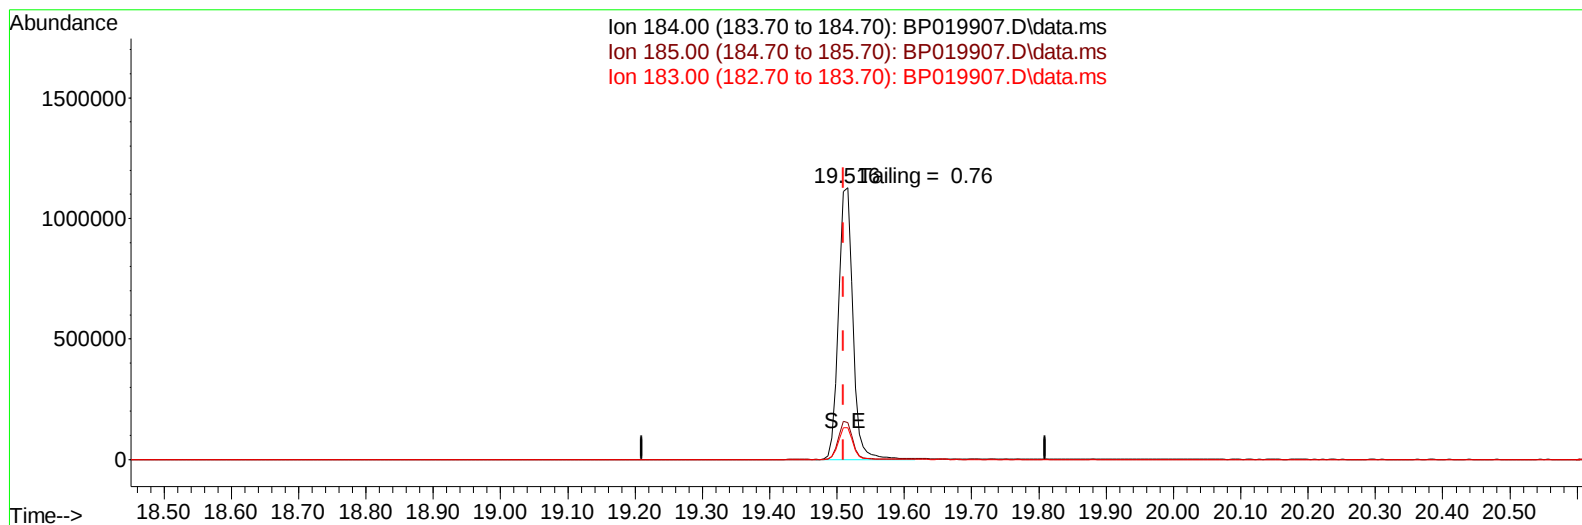

TIC: BP019907.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 435399.25 ng

response 1663408

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.47
183.00	11.60	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/28/2024	BNA_P	<u>BP019907.D</u>
Compound Name	Response	Retention Time
DDT	1025335	20.71
DDD	22041	20.28
DDE	1154	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23195	1048530	2.21

Instrument :
BNA_P
ClientSampleId :
DFTPP