
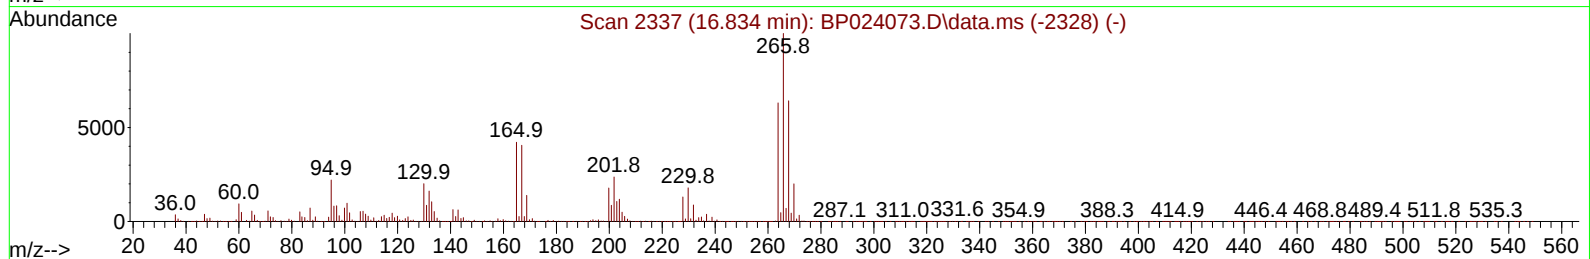
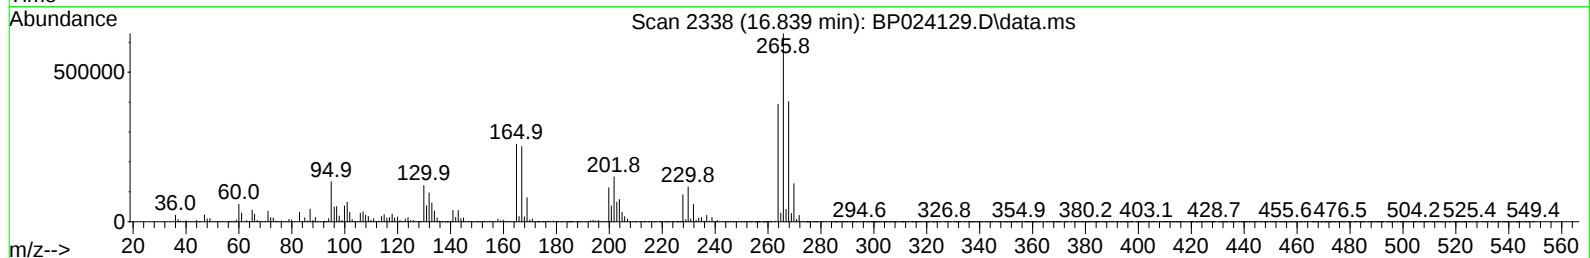


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024129.D
Acq On : 28 Feb 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 11:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

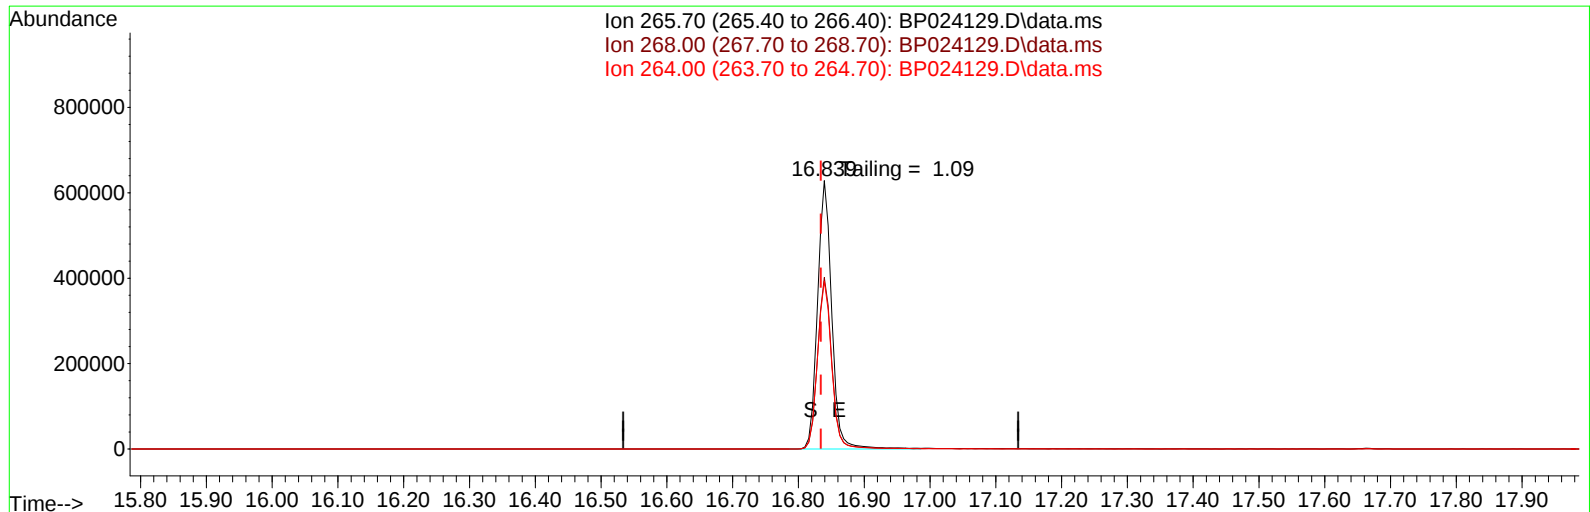

TIC: BP024129.D\data.ms

(70) Pentachlorophenol (C)




16.839min (+ 0.005) 478876.88 ng

response 941127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.91
264.00	63.10	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024129.D
Acq On : 28 Feb 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 11:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

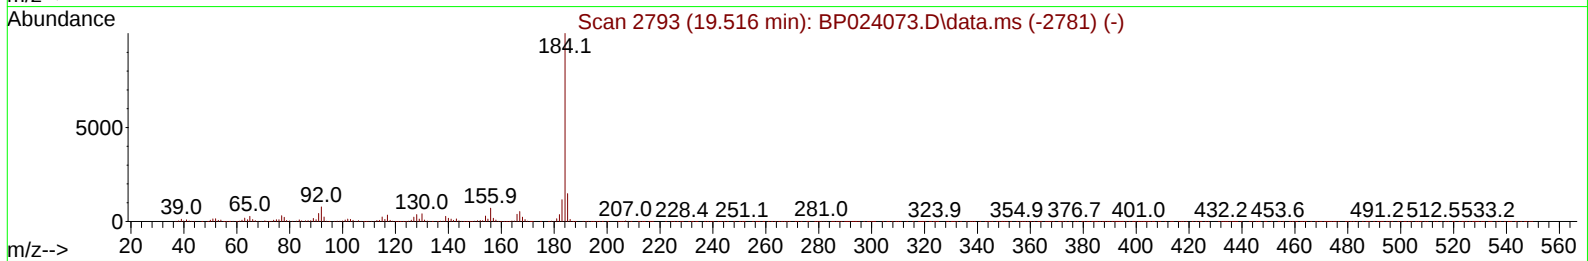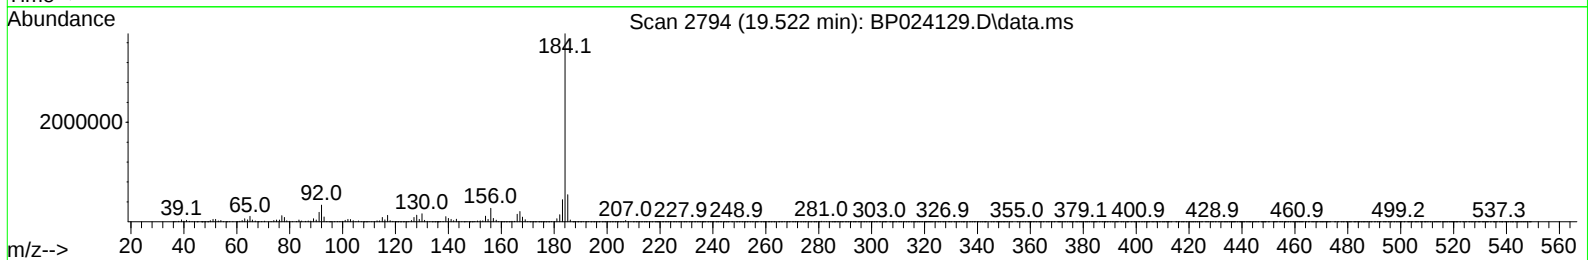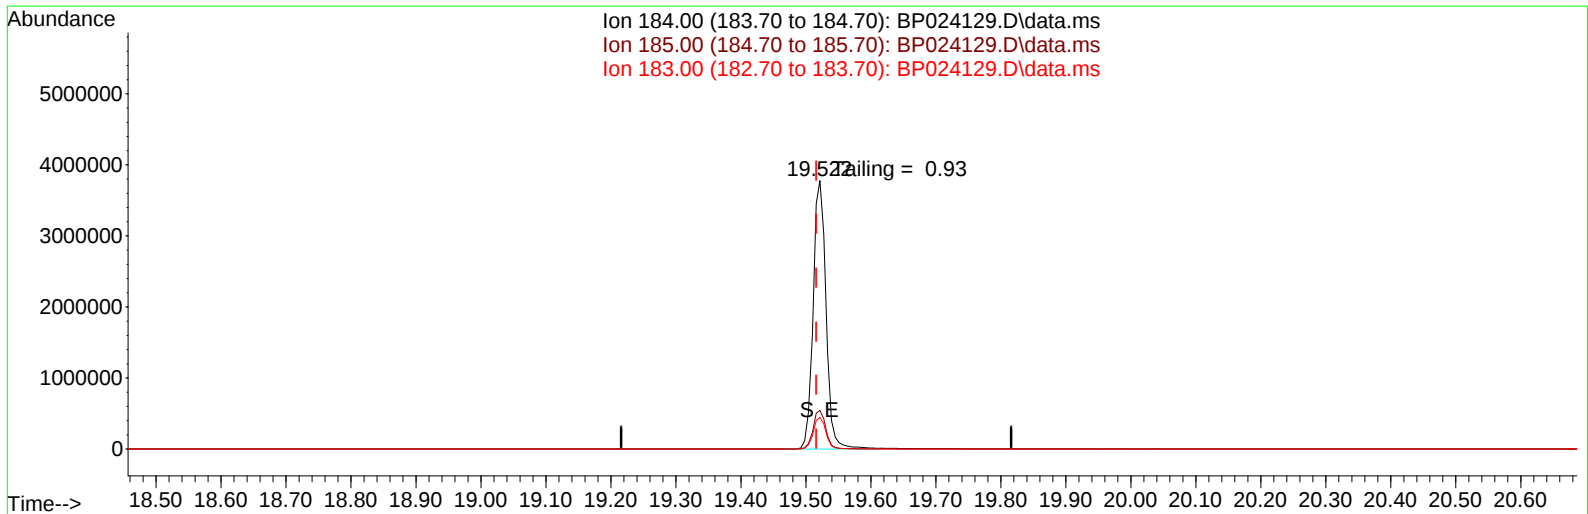

TIC: BP024129.D\data.ms

(77) Benzidine

19.522min (+ 0.006) 649183.29 ng

response 5260591

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.38
183.00	11.60	11.78
0.00	0.00	0.00