

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024133.D
Acq On : 28 Feb 2025 13:31
Operator : RC/JU
Sample : PB166890BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166890BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	383	390	405	rBV	7691549	10778760	44.86%	10.543%
2	6.946	648	656	676	rBV	6762157	10683712	44.46%	10.450%
3	7.763	788	795	804	rBV	1299652	2054502	8.55%	2.009%
4	8.910	982	990	1008	rBV	4186266	6802815	28.31%	6.654%
5	10.540	1258	1267	1278	rBV	1626863	2753367	11.46%	2.693%
6	12.998	1679	1685	1705	rBV	10841565	15815847	65.82%	15.469%
7	14.393	1911	1922	1933	rBV	2357369	3537272	14.72%	3.460%
8	15.904	2172	2179	2203	rBV	8171142	12127784	50.47%	11.862%
9	17.192	2391	2398	2411	rBV2	2886320	4136767	17.22%	4.046%
10	19.922	2855	2862	2874	rBV	18797511	24028690	100.00%	23.502%
11	21.651	3150	3156	3168	rVB	3150161	4647648	19.34%	4.546%
12	25.051	3726	3734	3744	rVB	1903703	4873443	20.28%	4.767%




Sum of corrected areas: 102240607

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024133.D
Acq On : 28 Feb 2025 13:31
Operator : RC/JU
Sample : PB166890BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

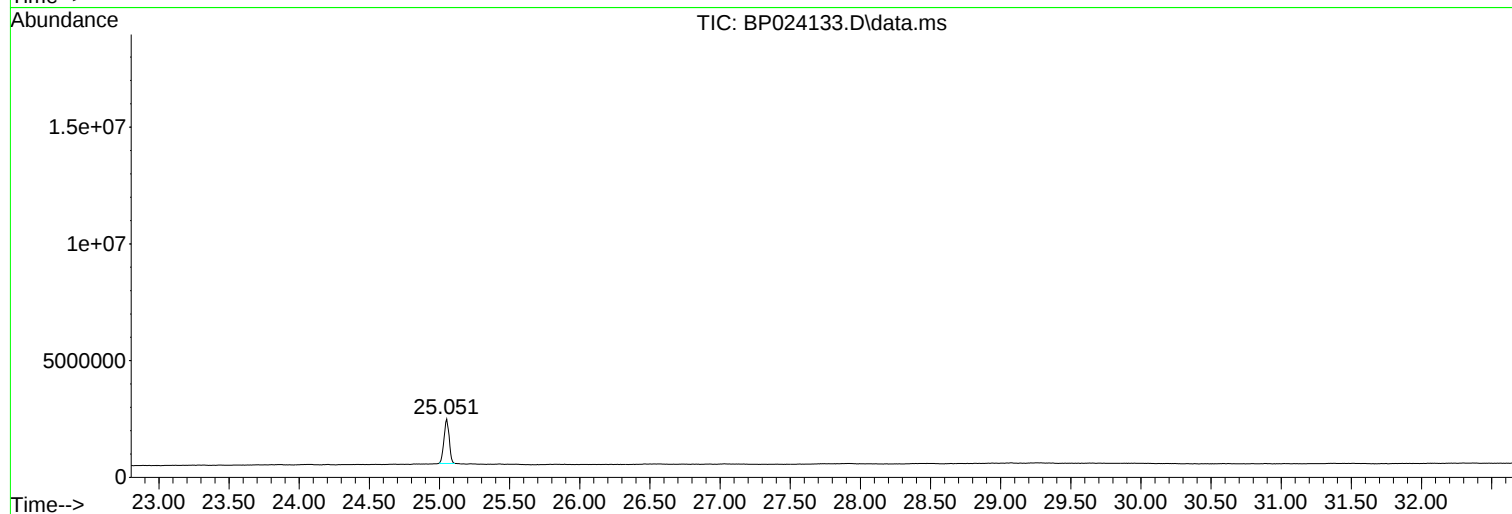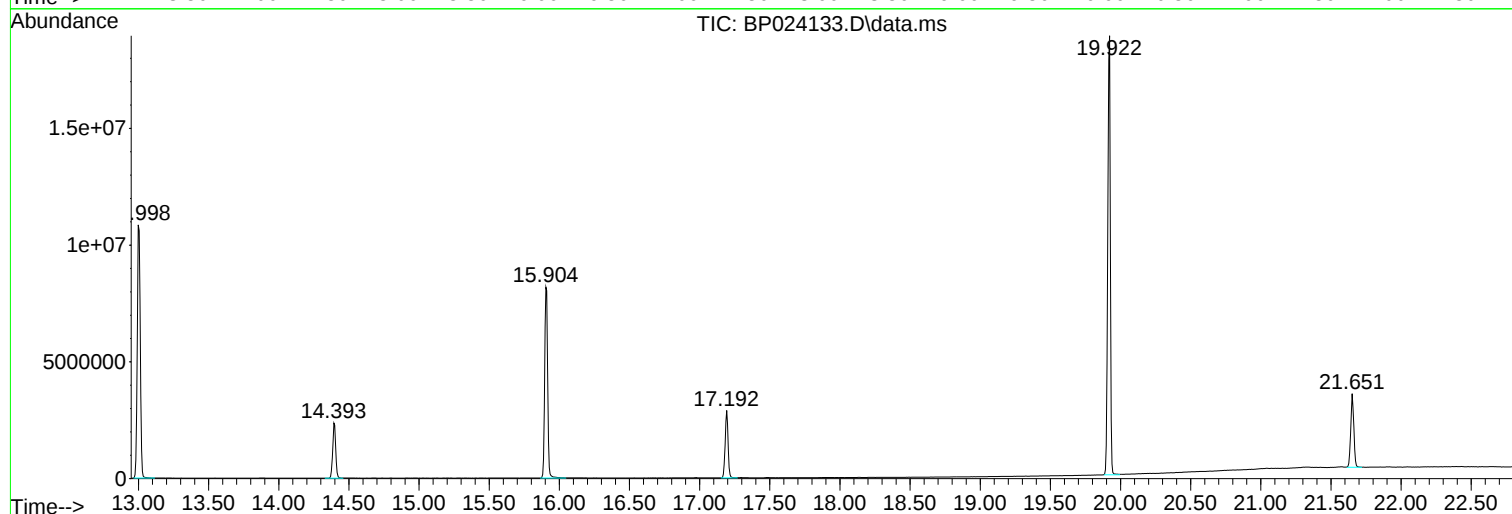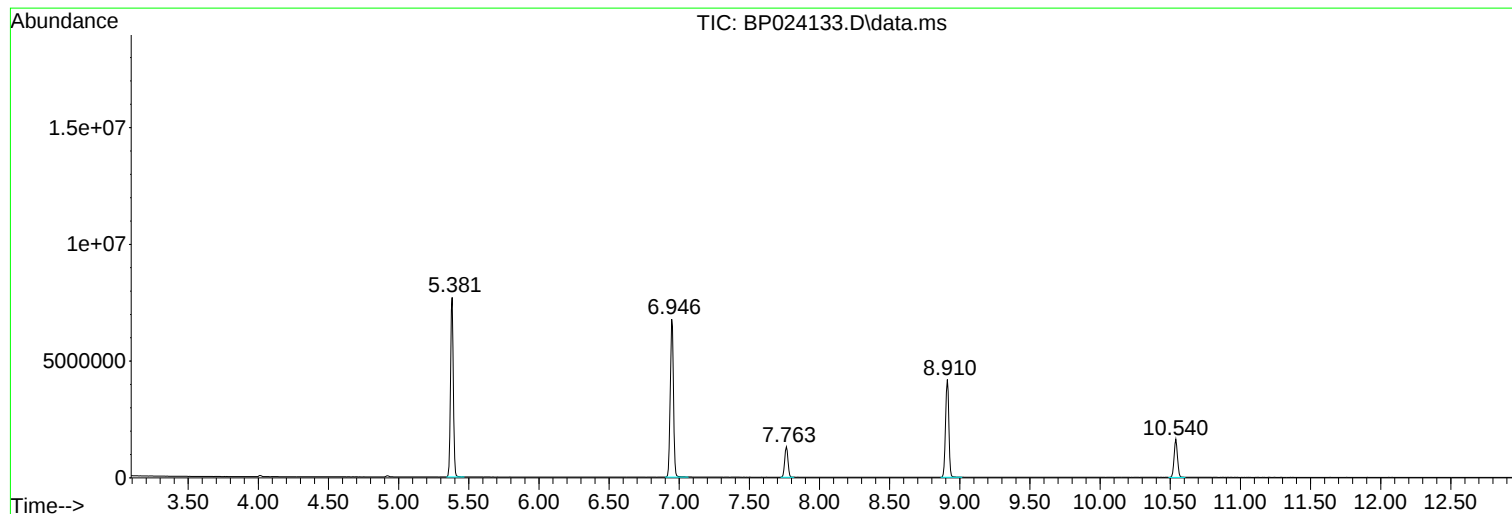

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024133.D
Acq On : 28 Feb 2025 13:31
Operator : RC/JU
Sample : PB166890BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024133.D
Acq On : 28 Feb 2025 13:31
Operator : RC/JU
Sample : PB166890BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc