
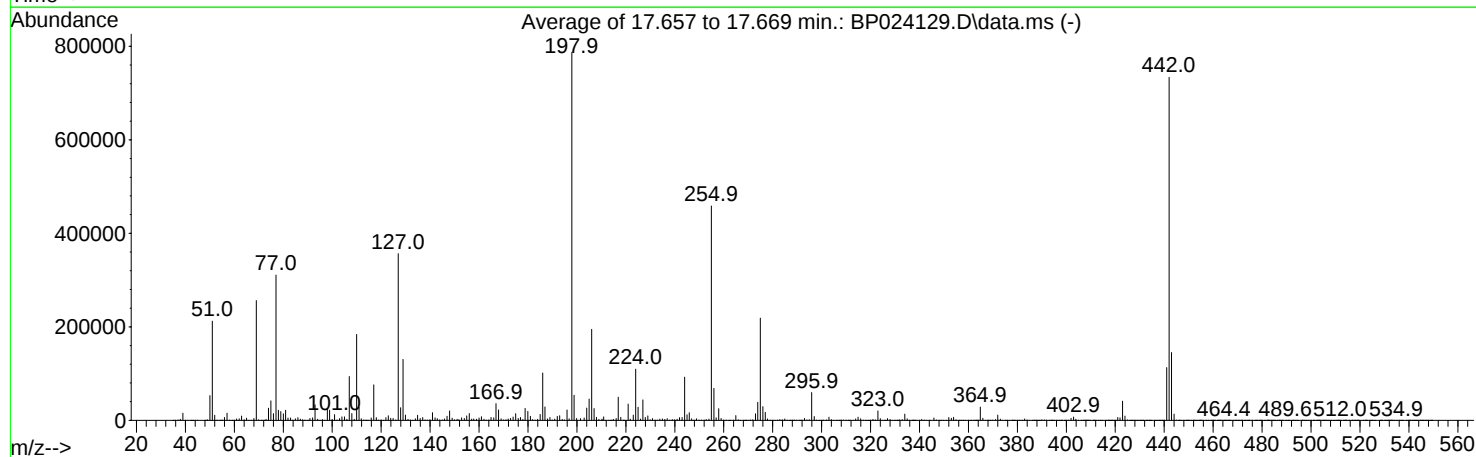


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024129.D
Acq On : 28 Feb 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

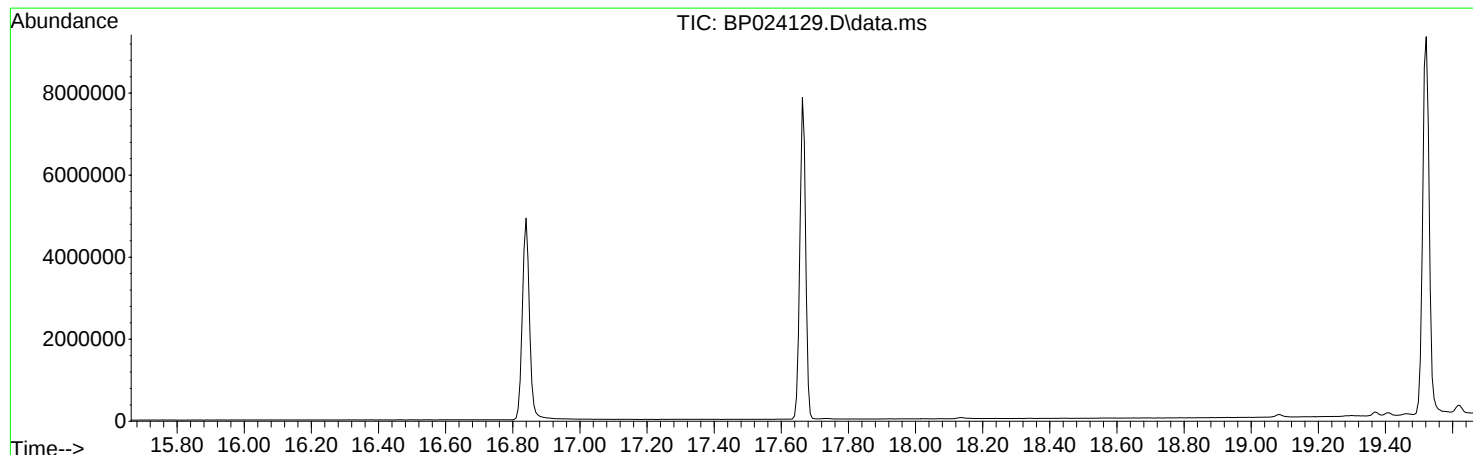

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	212374	PASS
68	69	0.00	2	1.6	3991	PASS
69	198	0.00	100	32.6	256196	PASS
70	69	0.00	2	0.5	1220	PASS
127	198	10	80	45.3	356583	PASS
197	198	0.00	2	0.4	3383	PASS
198	198	100	100	100.0	786813	PASS
199	198	5	9	6.8	53668	PASS
275	198	10	60	27.8	218791	PASS
365	198	1	100	3.6	28439	PASS
441	198	0.01	100	14.3	112841	PASS
442	442	100	100	100.0	733906	PASS
443	442	15	24	19.8	145213	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/28/2025	BNA_P	<u>BP024129.D</u>
Compound Name	Response	Retention Time
DDT	2195452	20.816
DDD	267269	20.351
DDE	2080	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
269349	2464801	10.93

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024129.D
Acq On : 28 Feb 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 28 11:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

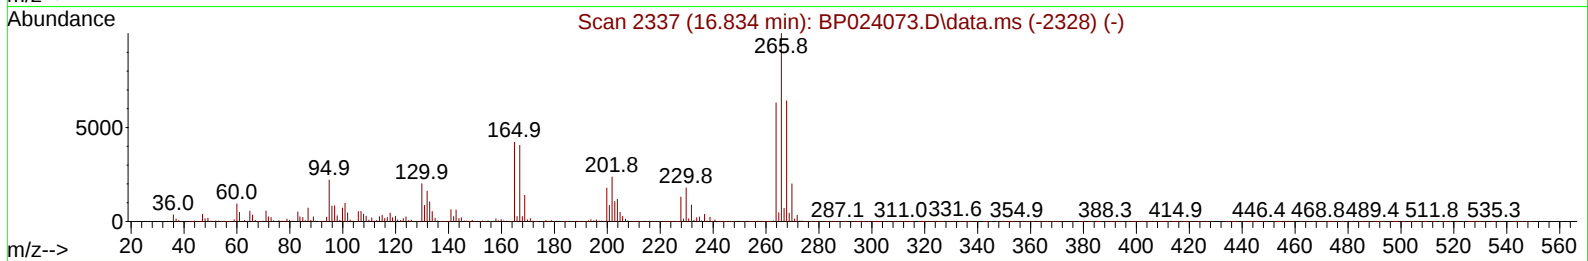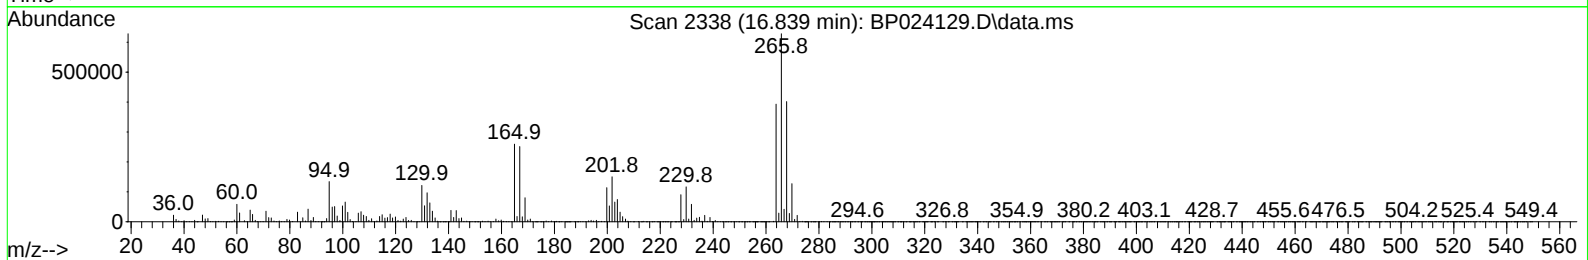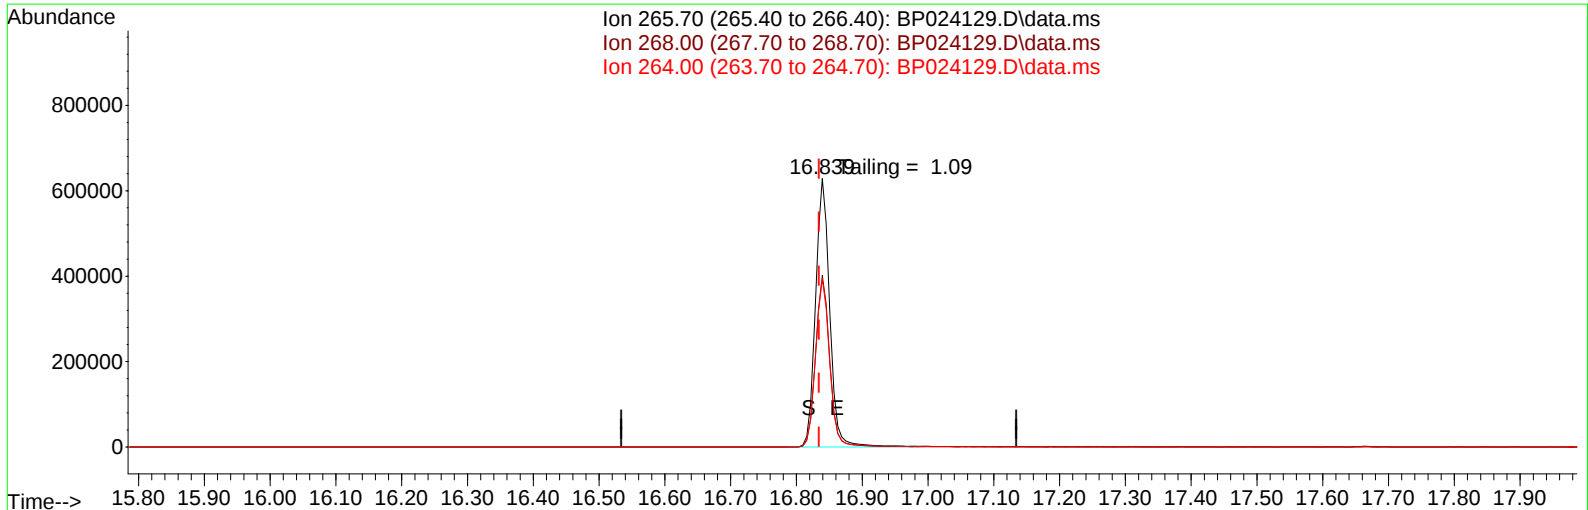

TIC: BP024129.D\data.ms

(70) Pentachlorophenol (C)

16.839min (+ 0.005) 478876.88 ng




response 941127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.91
264.00	63.10	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022825\
Data File : BP024129.D
Acq On : 28 Feb 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 28 11:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

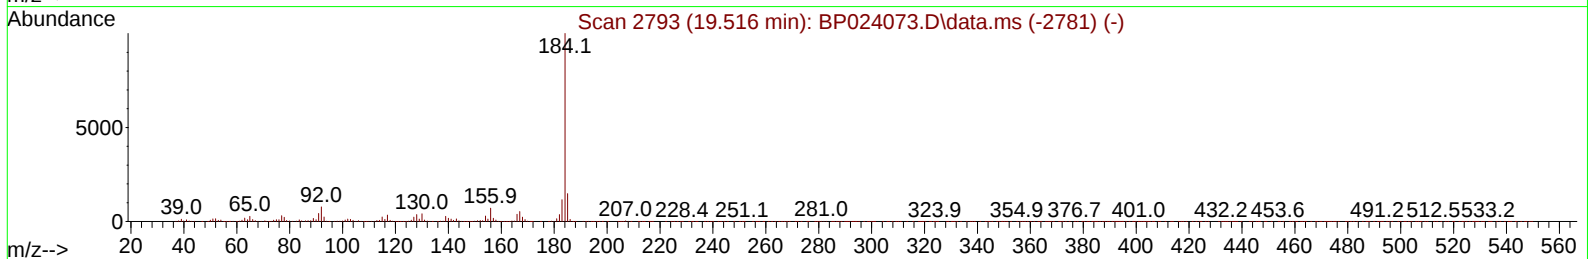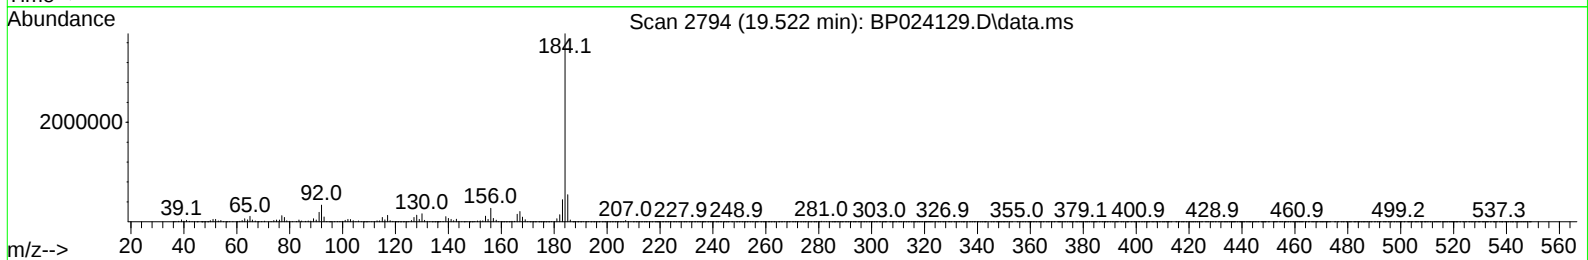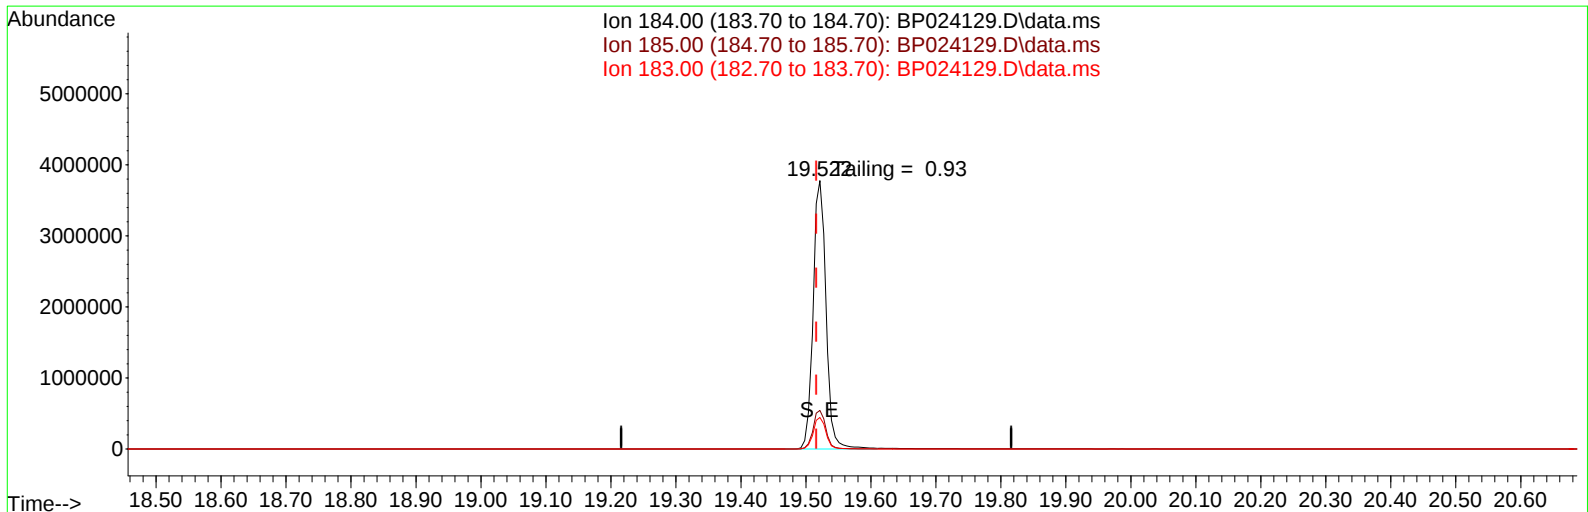

TIC: BP024129.D\data.ms

(77) Benzidine

19.522min (+ 0.006) 649183.29 ng

response 5260591

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.38
183.00	11.60	11.78
0.00	0.00	0.00