

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001956.D
 Acq On : 29 Feb 2020 13:27
 Operator : CG/JU
 Sample : L1708-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 02 00:29:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	272420	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1100450	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	701492	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1531122	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1564304	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1782255	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	36005	5.68	ng/uL	0.00
5) Phenol-d5	6.82	99	130178	6.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	370983	33.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	457116	25.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	265627	15.55	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	267363	31.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	294357	30.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	541700	29.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	38484	1.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1979671	37.29	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2276691	35.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	36791	3.63	ng/ul	0.00
58) Fluorene-d10	15.27	176	1698543	36.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	237953	28.19	ng/ul	0.00
71) Anthracene-d10	17.13	188	2725160	39.60	ng/ul	0.00
79) Pyrene-d10	19.37	212	3220779	39.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3616383	39.66	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.74	163	84613	1.544	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001956.D
Acq On : 29 Feb 2020 13:27
Operator : CG/JU
Sample : L1708-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Mar 02 00:29:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

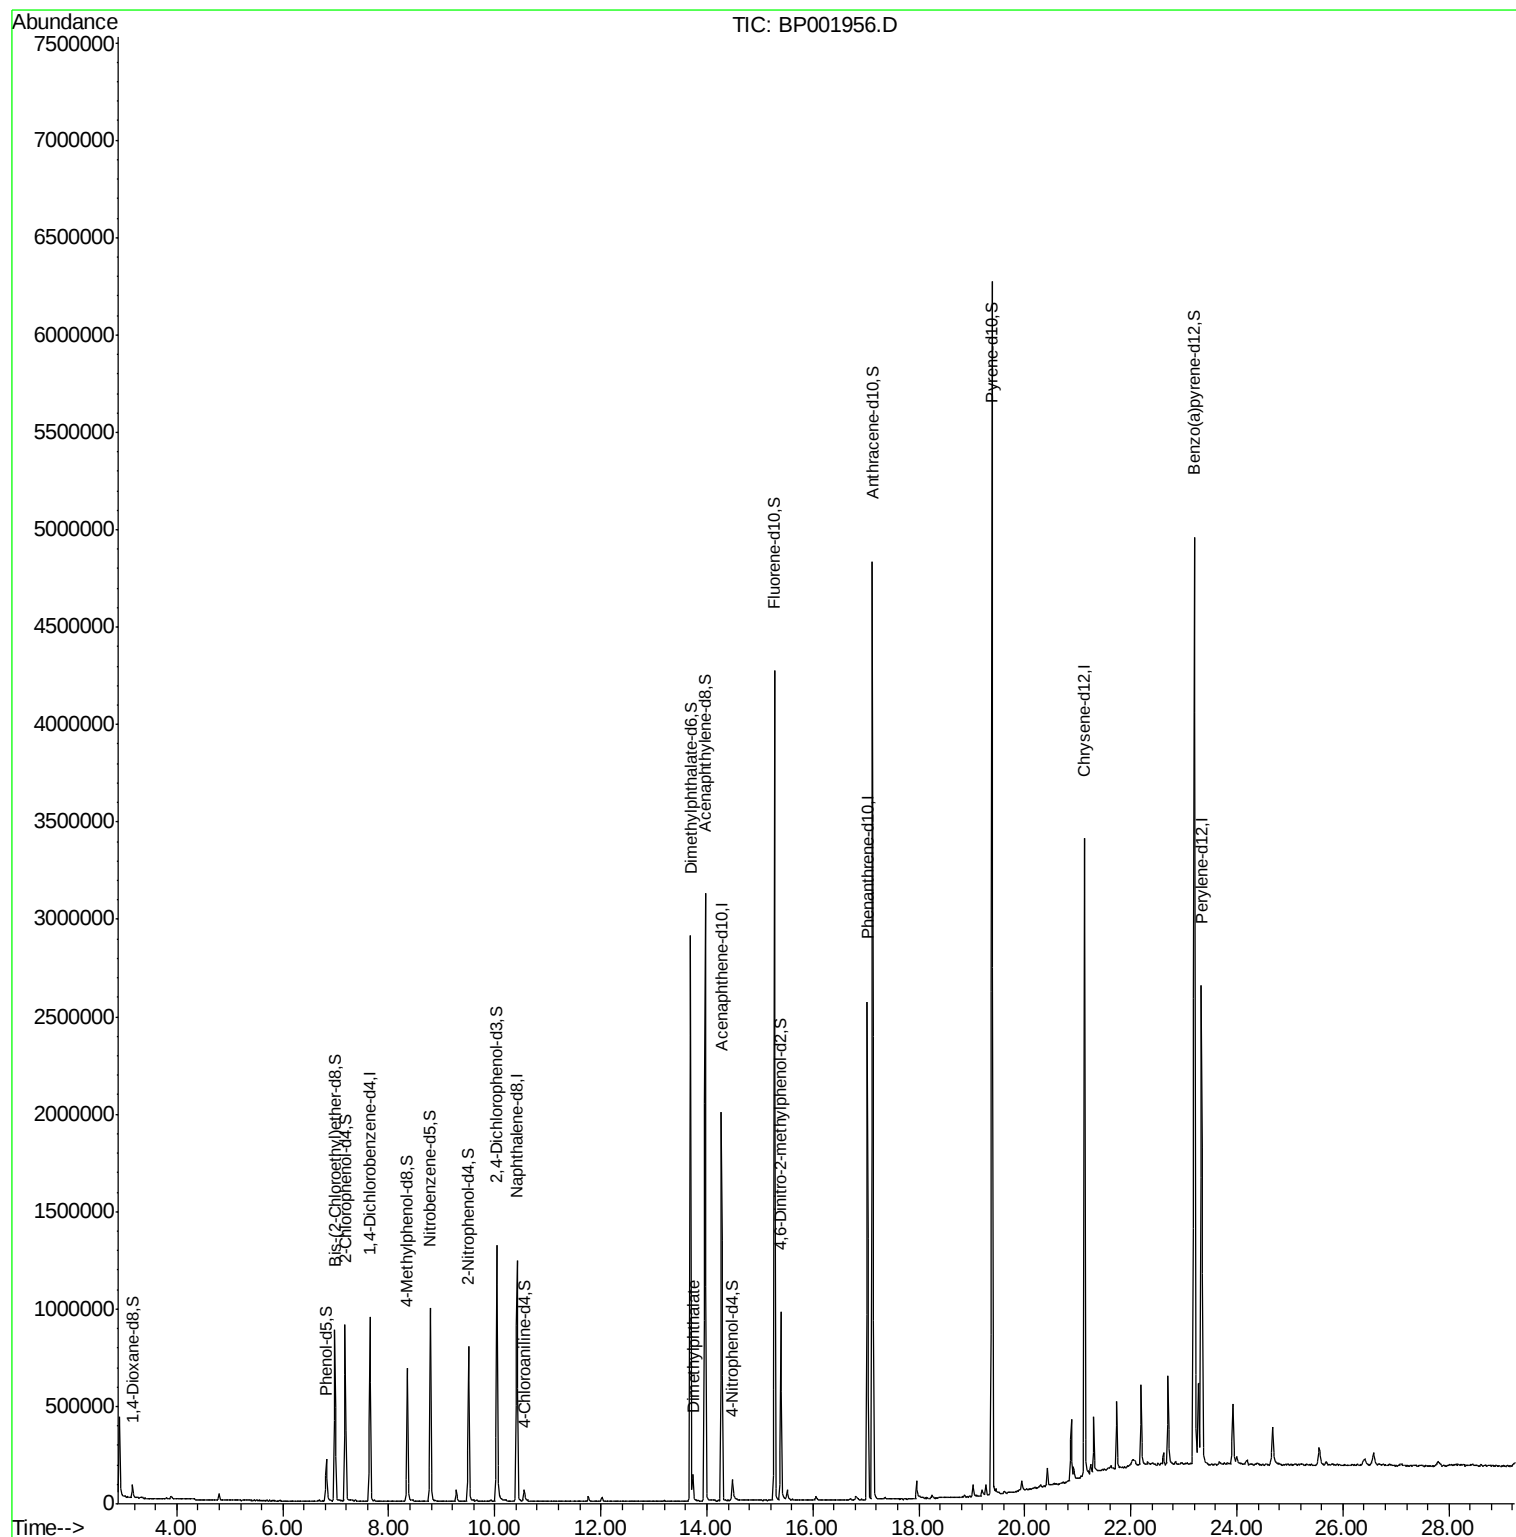

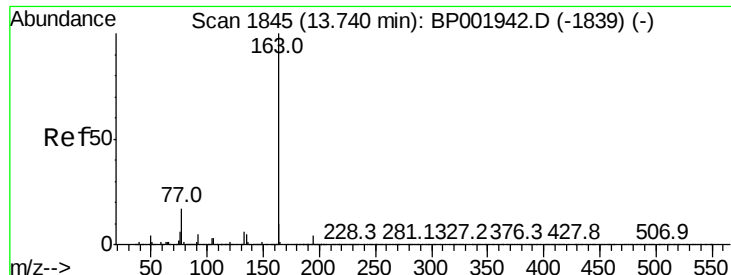

#45

Dimethylphthalate

Concen: 1.544 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. 0.00 min

Lab File: BP001956.D

Acq: 29 Feb 2020 13:27

Instrument :

BNA_P

ClientSampleId :

Tot Ion:163 Resp: 84613

Ion Ratio Lower Upper

163 100

194 4.9 3.6 5.4

164 10.8 8.2 12.4

