

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001957.D
 Acq On : 29 Feb 2020 14:00
 Operator : CG/JU
 Sample : L1708-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 02 00:29:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	259071	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1044317	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	663347	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1459118	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1467769	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1684059	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	36048	5.98	ng/uL	0.00
5) Phenol-d5	6.82	99	126991	6.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	365186	34.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	449137	26.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	262599	16.17	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	261885	32.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	288137	31.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	535814	30.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	32377	1.70	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	1911496	38.08	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2211222	36.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	35428	3.69	ng/ul	0.00
58) Fluorene-d10	15.27	176	1690956	38.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	226015	28.10	ng/ul	0.00
71) Anthracene-d10	17.13	188	2663156	40.61	ng/ul	0.00
79) Pyrene-d10	19.37	212	3100609	40.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3478039	40.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	80207	1.548	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001957.D
Acq On : 29 Feb 2020 14:00
Operator : CG/JU
Sample : L1708-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Mar 02 00:29:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

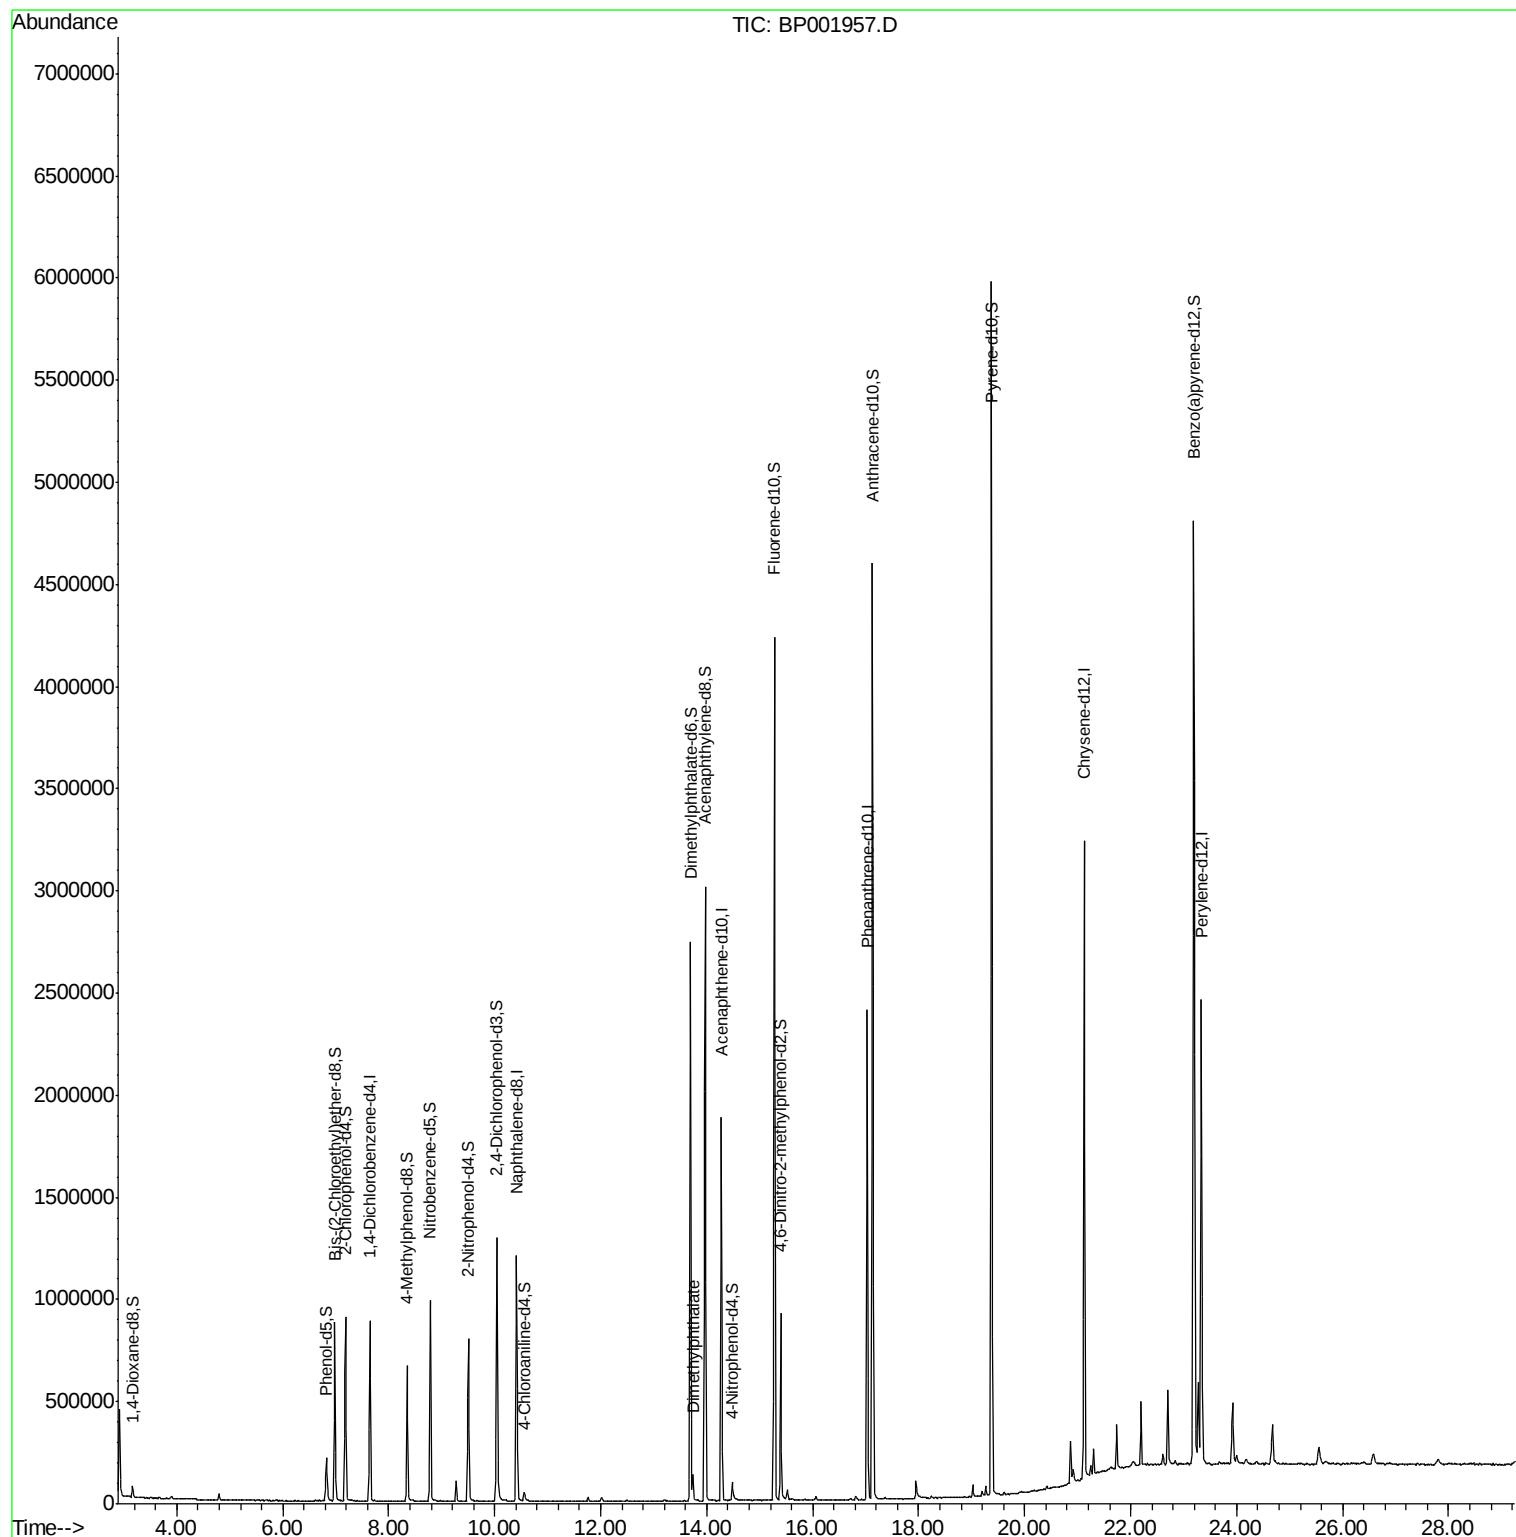

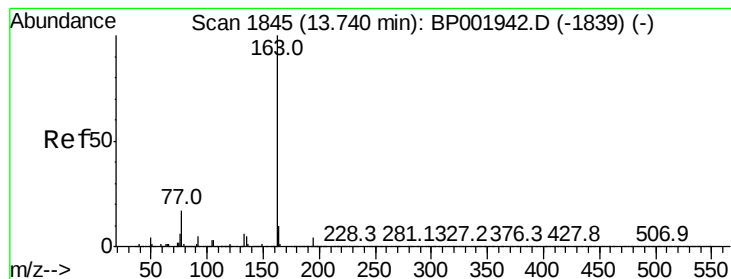

#45

Dimethylphthalate

Concen: 1.548 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001957.D

Acq: 29 Feb 2020 14:00

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 80207

Ion Ratio Lower Upper

163 100

194 3.9 3.6 5.4

164 9.8 8.2 12.4

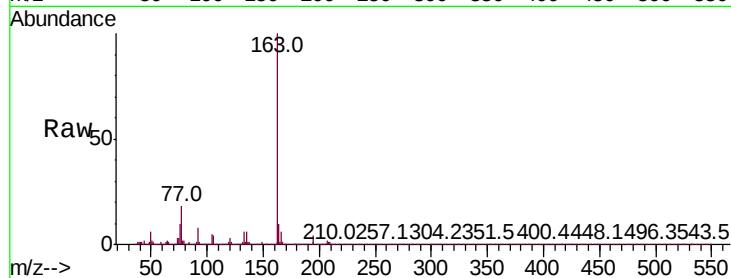

Abundance Ion 163.00 (162.70 to 163.70): E

80000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

