

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001959.D
 Acq On : 29 Feb 2020 15:08
 Operator : CG/JU
 Sample : L1708-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 02 00:29:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	318582	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1278918	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	818517	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1801273	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1789186	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	2031411	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	37785	5.10	ng/uL	0.00
5) Phenol-d5	6.82	99	133027	5.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	379620	29.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	465228	22.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	269074	13.47	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	273545	27.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	300158	27.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	533902	25.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	35113	1.50	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	1881271	30.37	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2257686	30.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	33316	2.81	ng/ul	0.00
58) Fluorene-d10	15.27	176	1706096	31.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	214235	21.57	ng/ul	0.00
71) Anthracene-d10	17.13	188	2636728	32.57	ng/ul	0.00
79) Pyrene-d10	19.37	212	3046062	32.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3332914	32.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	145026	2.268	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001959.D
Acq On : 29 Feb 2020 15:08
Operator : CG/JU
Sample : L1708-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Mar 02 00:29:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

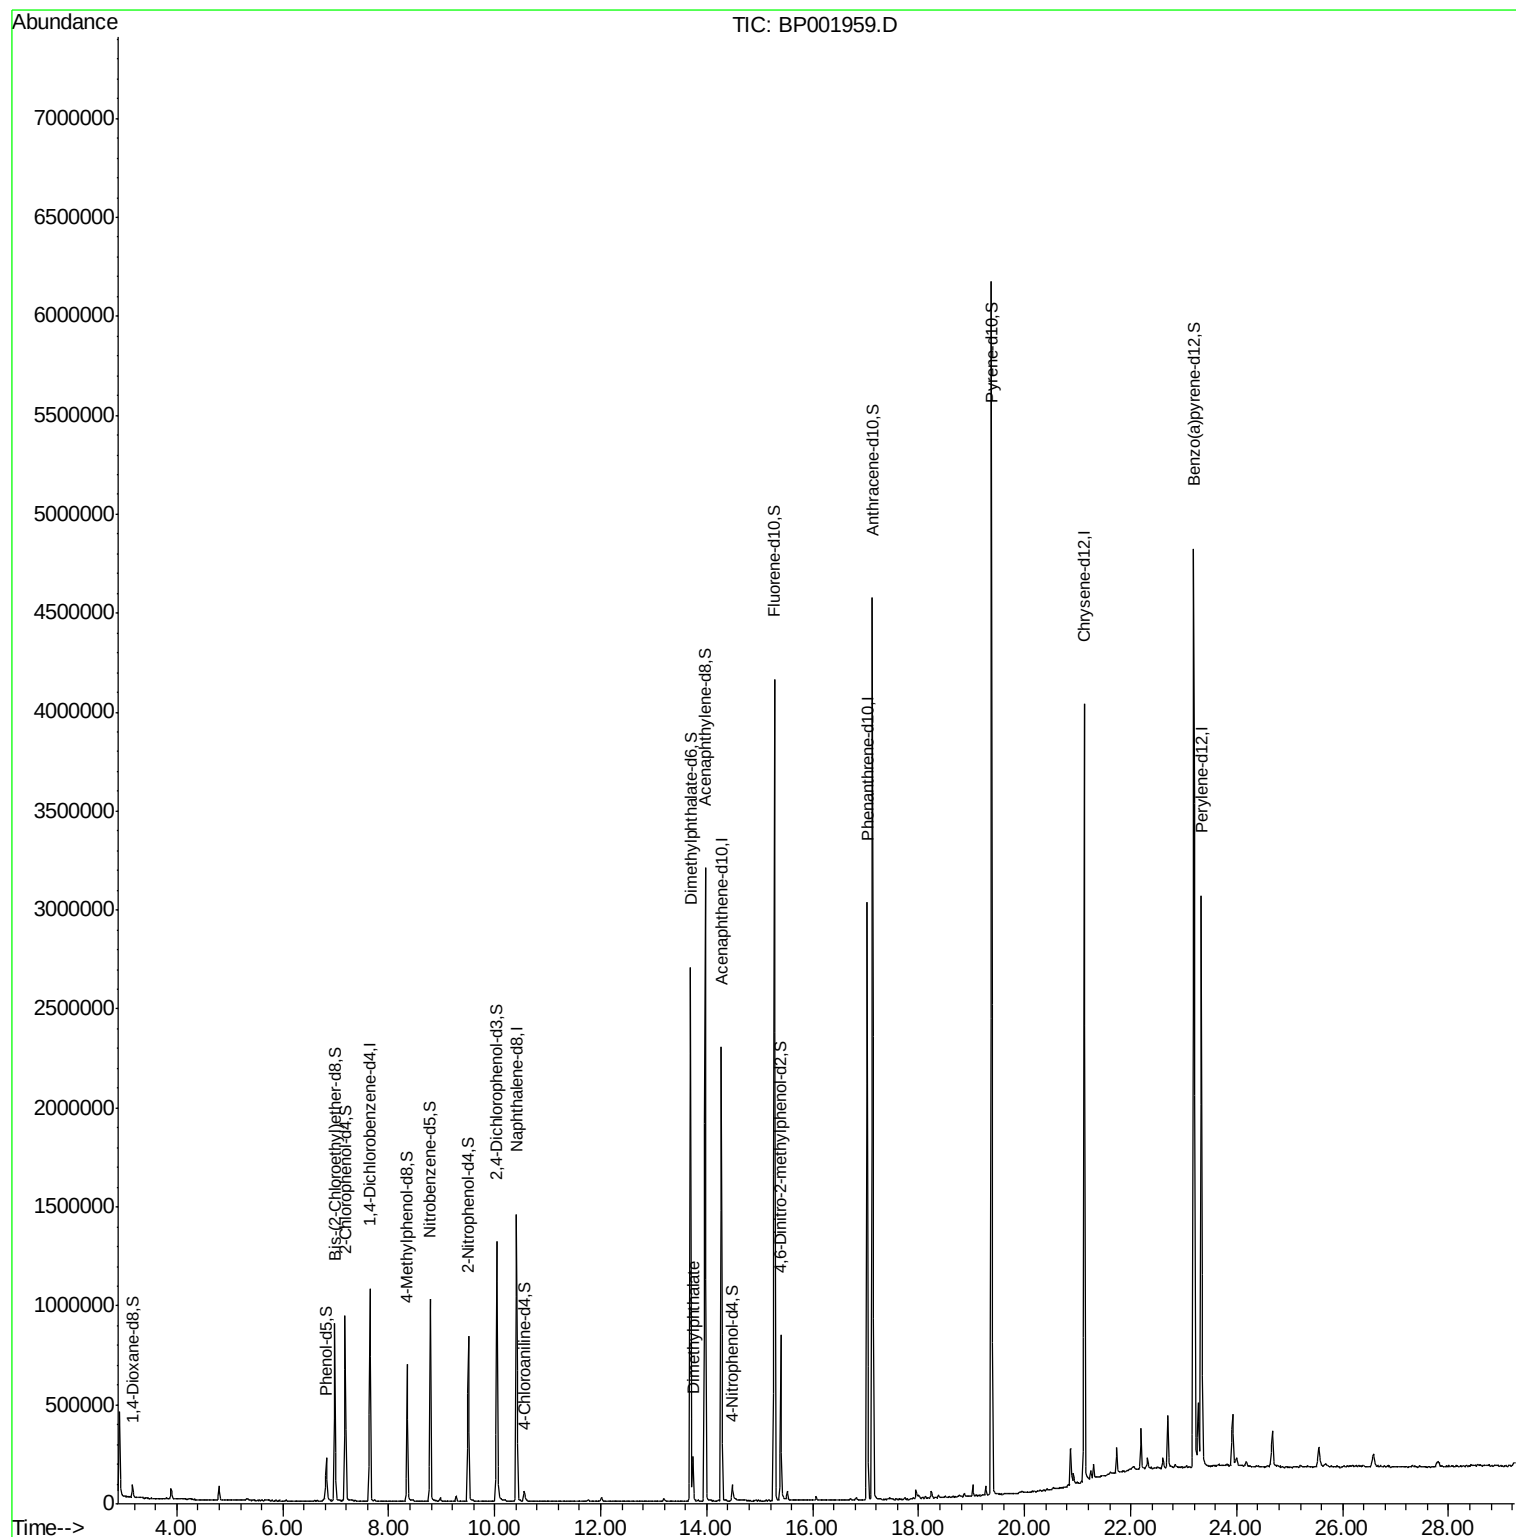

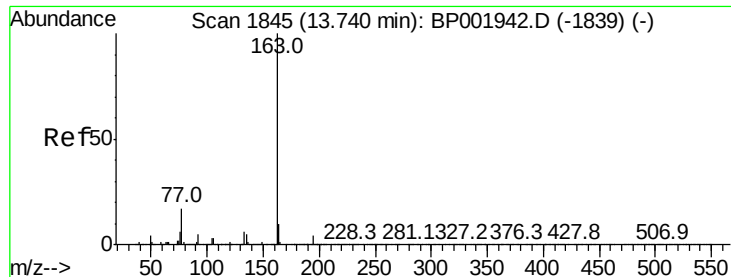

#45
 Dimethylphthalate
 Concen: 2.268 ng/ul
 RT: 13.74 min Scan# 1845
 Delta R.T. -0.00 min
 Lab File: BP001959.D
 Acq: 29 Feb 2020 15:08

Instrument :
 BNA_P
 ClientSampleId :

Tot Ion:	163	Resp:	145026
Ion Ratio	Lower	Upper	
163	100		
194	4.4	3.6	5.4
164	9.7	8.2	12.4

