

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001980.D
 Acq On : 01 Mar 2020 03:32
 Operator : CG/JU
 Sample : L1732-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 02 00:33:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	277249	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1103229	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	705540	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1540044	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1513833	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1751549	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	34779	5.39	ng/uL	0.00
5) Phenol-d5	6.82	99	129843	6.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	369703	33.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	467689	25.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	258091	14.85	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	271118	31.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	291098	30.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	523770	28.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	33850	1.68	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	1837901	34.42	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2178386	34.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	31683	3.10	ng/ul	0.00
58) Fluorene-d10	15.27	176	1642368	35.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	206300	24.30	ng/ul	0.00
71) Anthracene-d10	17.13	188	2694960	38.94	ng/ul	0.00
79) Pyrene-d10	19.37	212	3097589	39.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3438954	38.38	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	133538	2.423	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001980.D
Acq On : 01 Mar 2020 03:32
Operator : CG/JU
Sample : L1732-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Mar 02 00:33:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

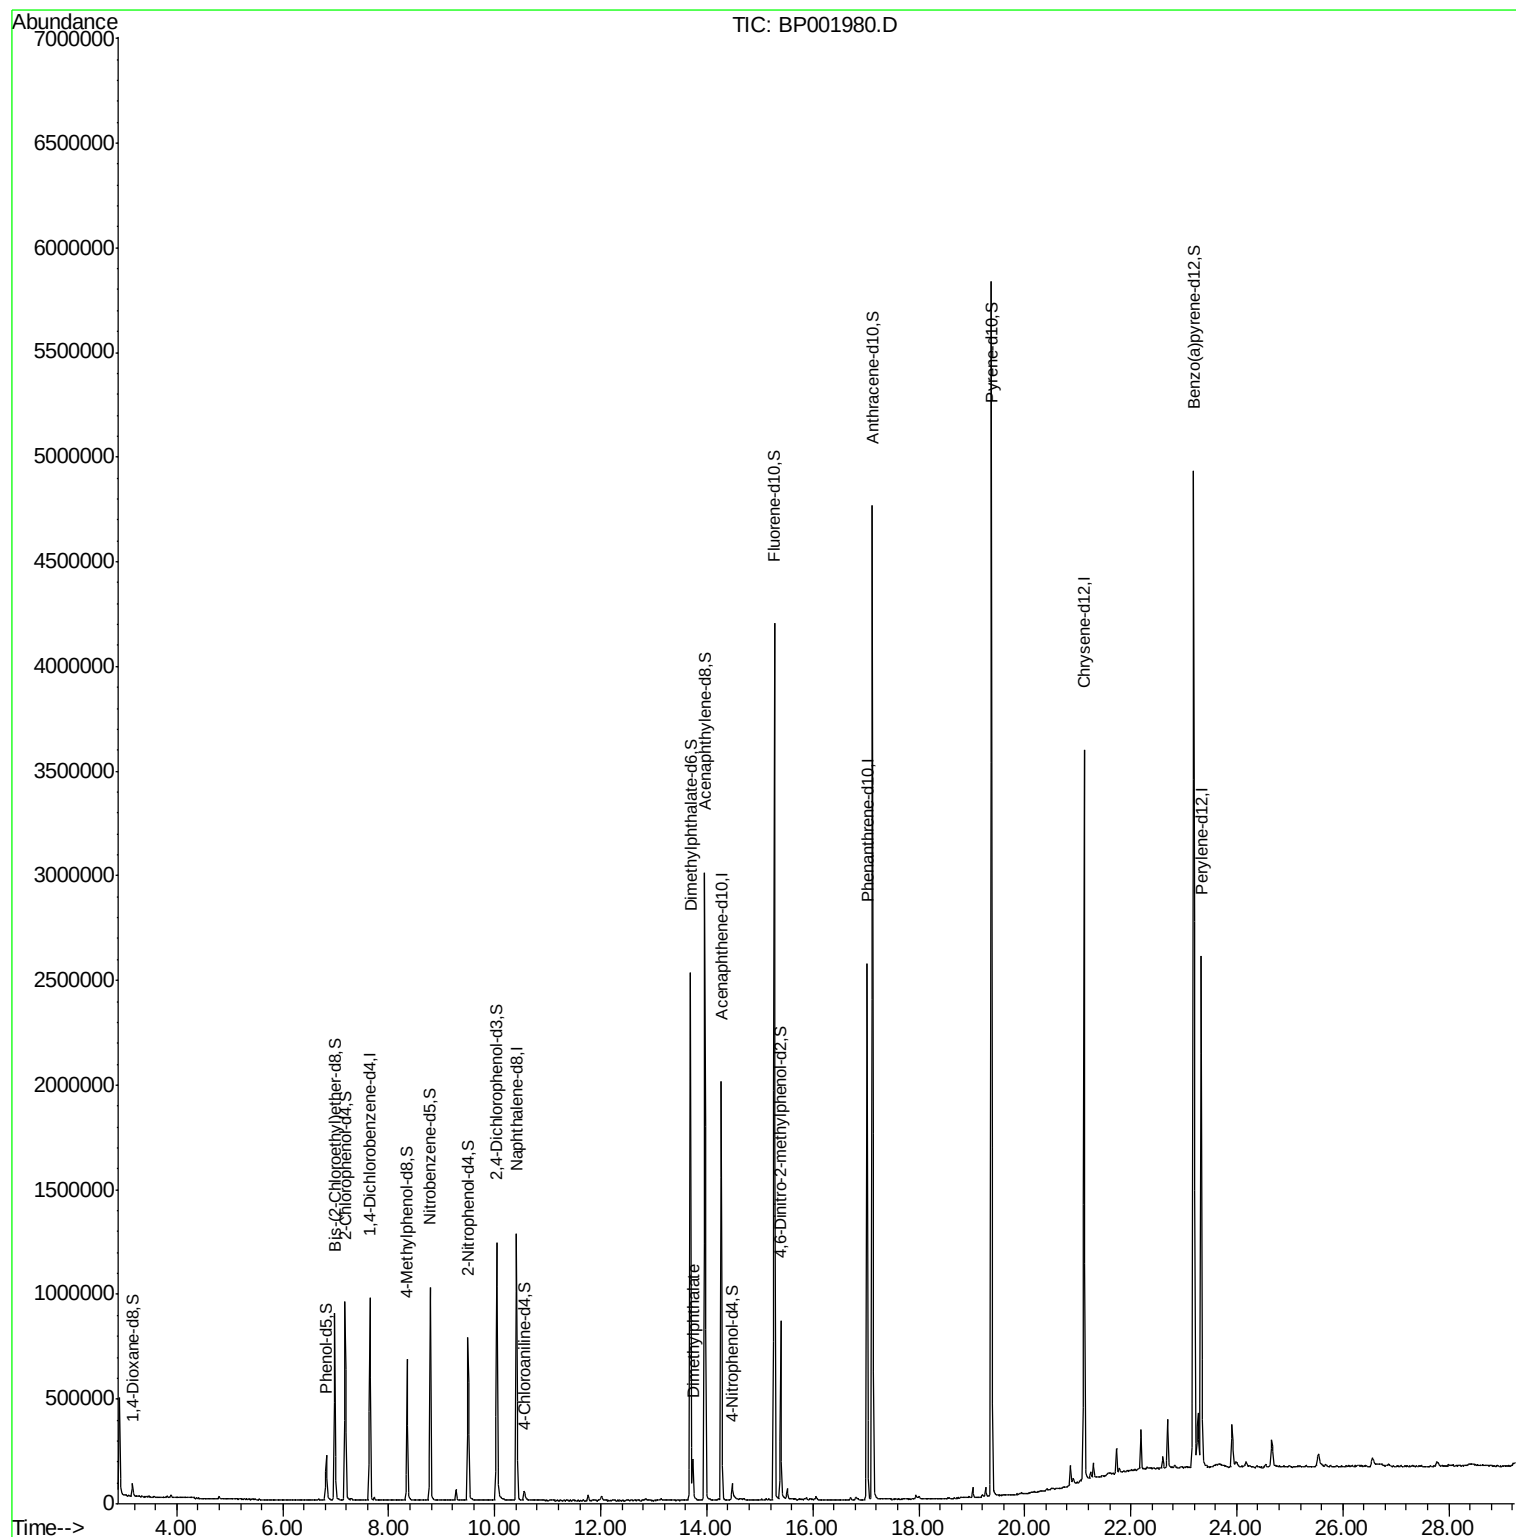

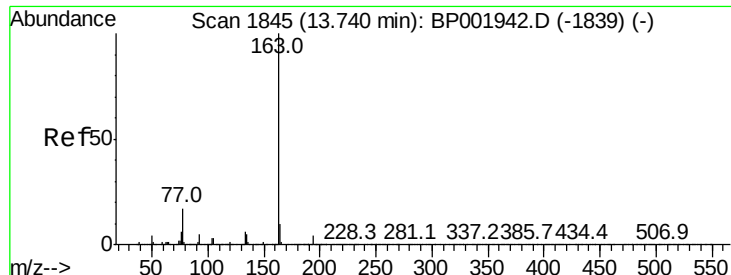

#45

Dimethylphthalate

Concen: 2.423 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001980.D

Acq: 01 Mar 2020 03:32

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 133538

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4

164 9.7 8.2 12.4

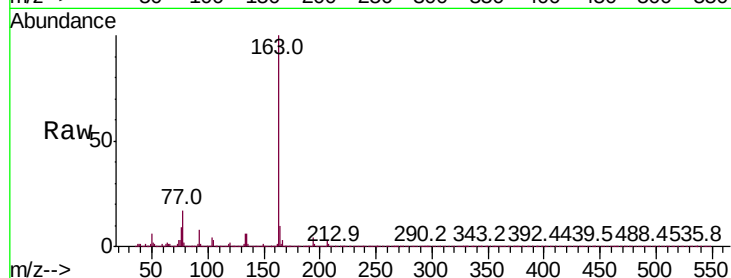

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

