

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001958.D
 Acq On : 29 Feb 2020 14:34
 Operator : CG/JU
 Sample : L1708-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE0

Quant Time: Mar 02 00:29:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	285220	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1153292	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	734556	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1620564	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1597699	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1813189	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	40722	6.14	ng/uL	0.00
5) Phenol-d5	6.82	99	156748	7.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	427404	37.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	529688	28.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	314306	17.58	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	311990	35.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	341431	34.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	622539	32.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	44057	2.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2148766	38.65	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2539819	38.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	45890	4.32	ng/ul	0.00
58) Fluorene-d10	15.27	176	1900208	39.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	266318	29.81	ng/ul	0.00
71) Anthracene-d10	17.13	188	3038495	41.72	ng/ul	0.00
79) Pyrene-d10	19.37	212	3484046	41.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3853254	41.54	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.74	163	113943	1.986	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001958.D
Acq On : 29 Feb 2020 14:34
Operator : CG/JU
Sample : L1708-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE0

Quant Time: Mar 02 00:29:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

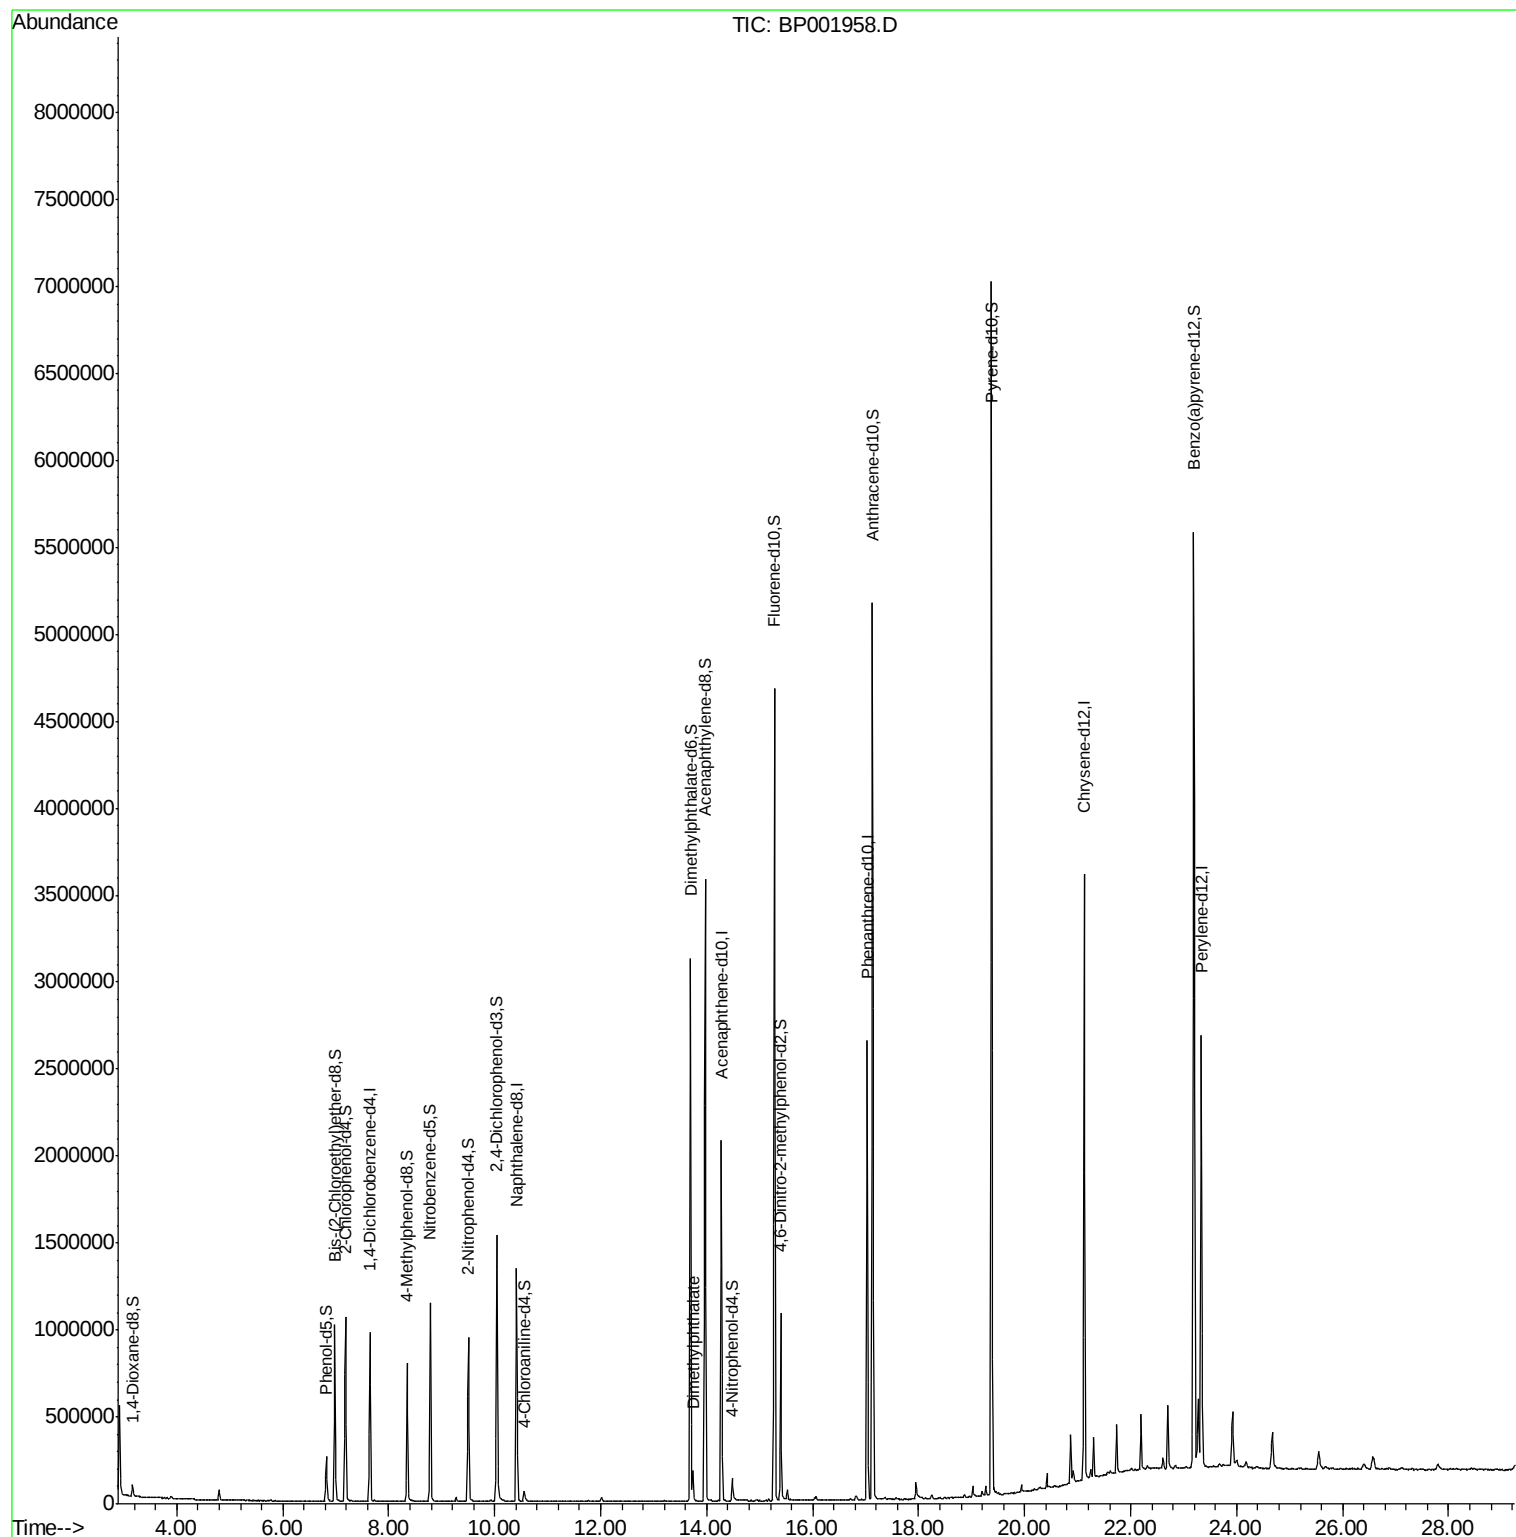

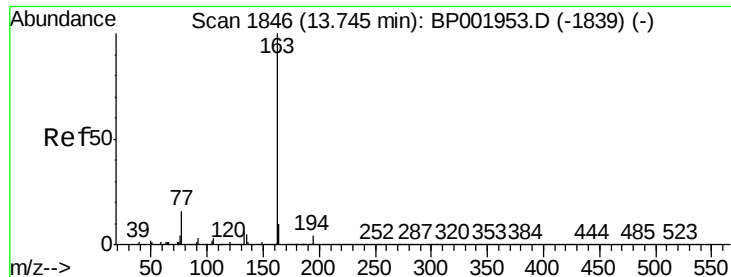

#45

Dimethylphthalate

Concen: 1.986 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001958.D

Acq: 29 Feb 2020 14:34

Instrument :

BNA_P

ClientSampleId :

C0CE0


Tot Ion:163 Resp: 113943

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 10.1 8.2 12.4

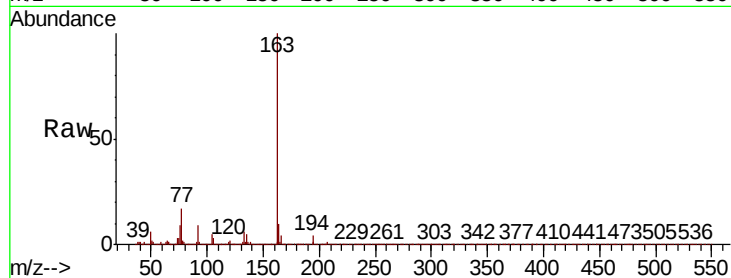

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

