

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001960.D
 Acq On : 29 Feb 2020 15:42
 Operator : CG/JU
 Sample : L1708-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CD6

Quant Time: Mar 02 01:52:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	306894	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1235622	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	792064	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1717630	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1714251	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1935221	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	38521	5.40	ng/uL	0.00
5) Phenol-d5	6.82	99	131066	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	363613	29.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	456932	22.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	258717	13.45	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	261236	27.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	286816	26.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	520639	25.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	33310	1.48	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	1825388	30.45	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2155205	30.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	28979	2.53	ng/ul	0.00
58) Fluorene-d10	15.27	176	1631057	31.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	203604	21.50	ng/ul	0.00
71) Anthracene-d10	17.13	188	2533972	32.82	ng/ul	0.00
79) Pyrene-d10	19.37	212	2934617	32.70	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3210246	32.42	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.74	163	114454	1.850	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001960.D
Acq On : 29 Feb 2020 15:42
Operator : CG/JU
Sample : L1708-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD6

Quant Time: Mar 02 01:52:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

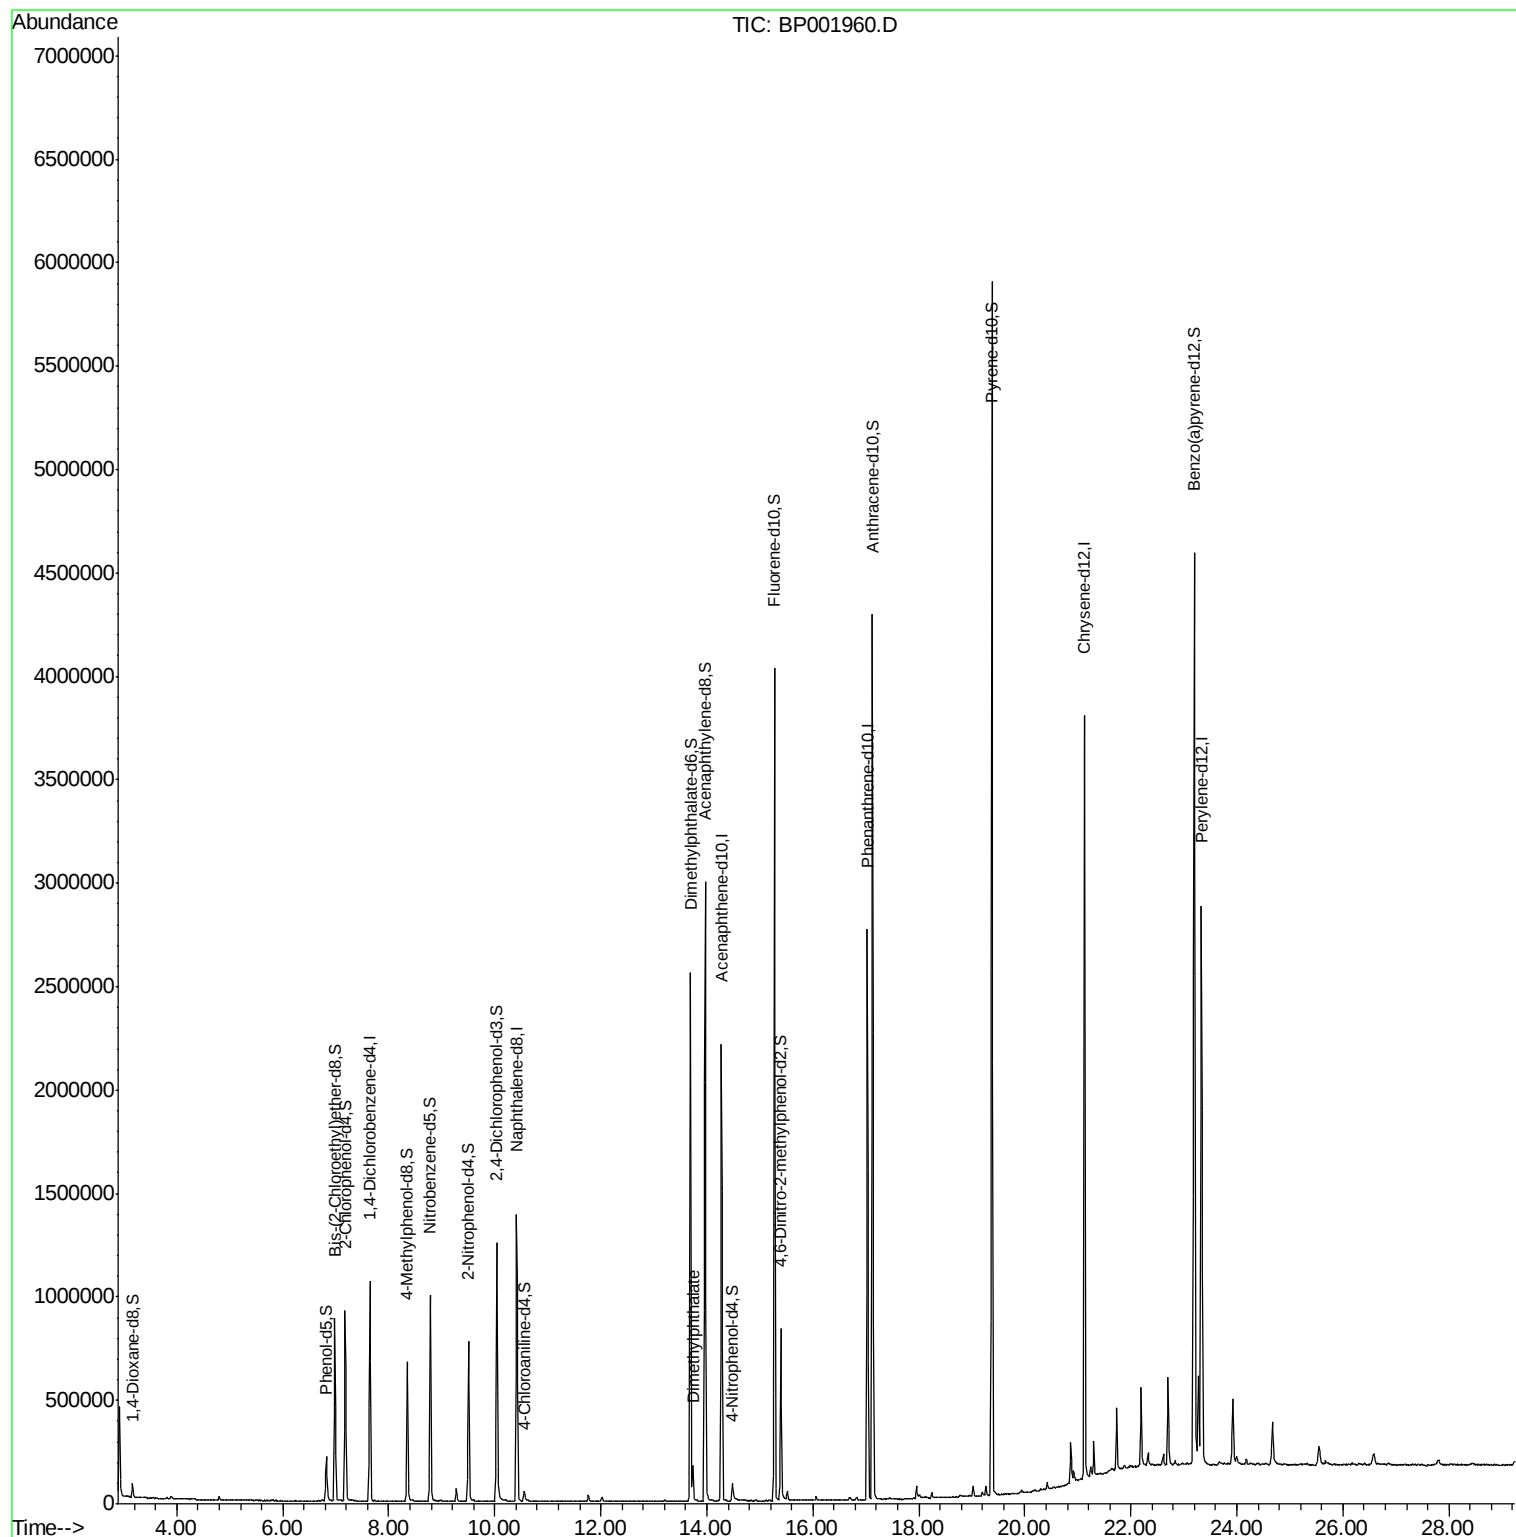

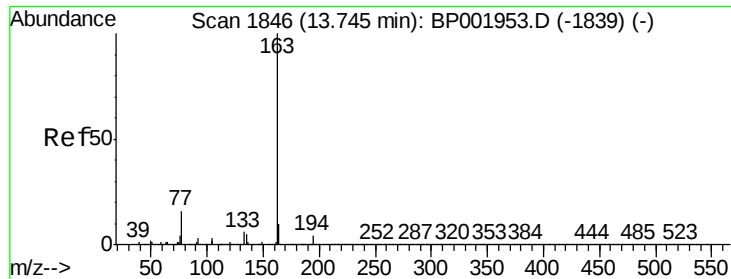

#45

Dimethylphthalate

Concen: 1.850 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. 0.00 min

Lab File: BP001960.D

Acq: 29 Feb 2020 15:42

Instrument :

BNA_P

ClientSampleId :

C0CD6


Tot Ion:163 Resp: 114454

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.2 8.2 12.4

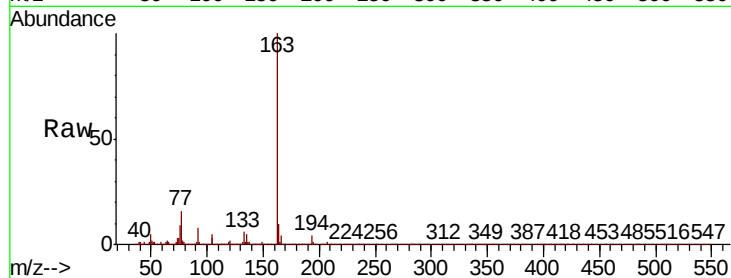

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

