

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001963.D
 Acq On : 29 Feb 2020 17:23
 Operator : CG/JU
 Sample : L1615-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDN6

Quant Time: Mar 02 02:05:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	288399	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1168921	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	739444	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1624673	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1650323	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1886159	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	31294	4.66	ng/uL	0.00
5) Phenol-d5	6.82	99	508041	23.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	305390	26.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	458684	24.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	379096	20.97	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	214146	23.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	233077	23.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	447081	22.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	584724	27.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1483641	26.51	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1757297	26.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	184031	17.20	ng/ul	0.00
58) Fluorene-d10	15.27	176	1326469	27.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	155629	17.38	ng/ul	0.00
71) Anthracene-d10	17.13	188	2026451	27.75	ng/ul	0.00
79) Pyrene-d10	19.37	212	2367472	27.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2591000	26.85	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.74	163	146589	2.538	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001963.D
Acq On : 29 Feb 2020 17:23
Operator : CG/JU
Sample : L1615-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDN6

Quant Time: Mar 02 02:05:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

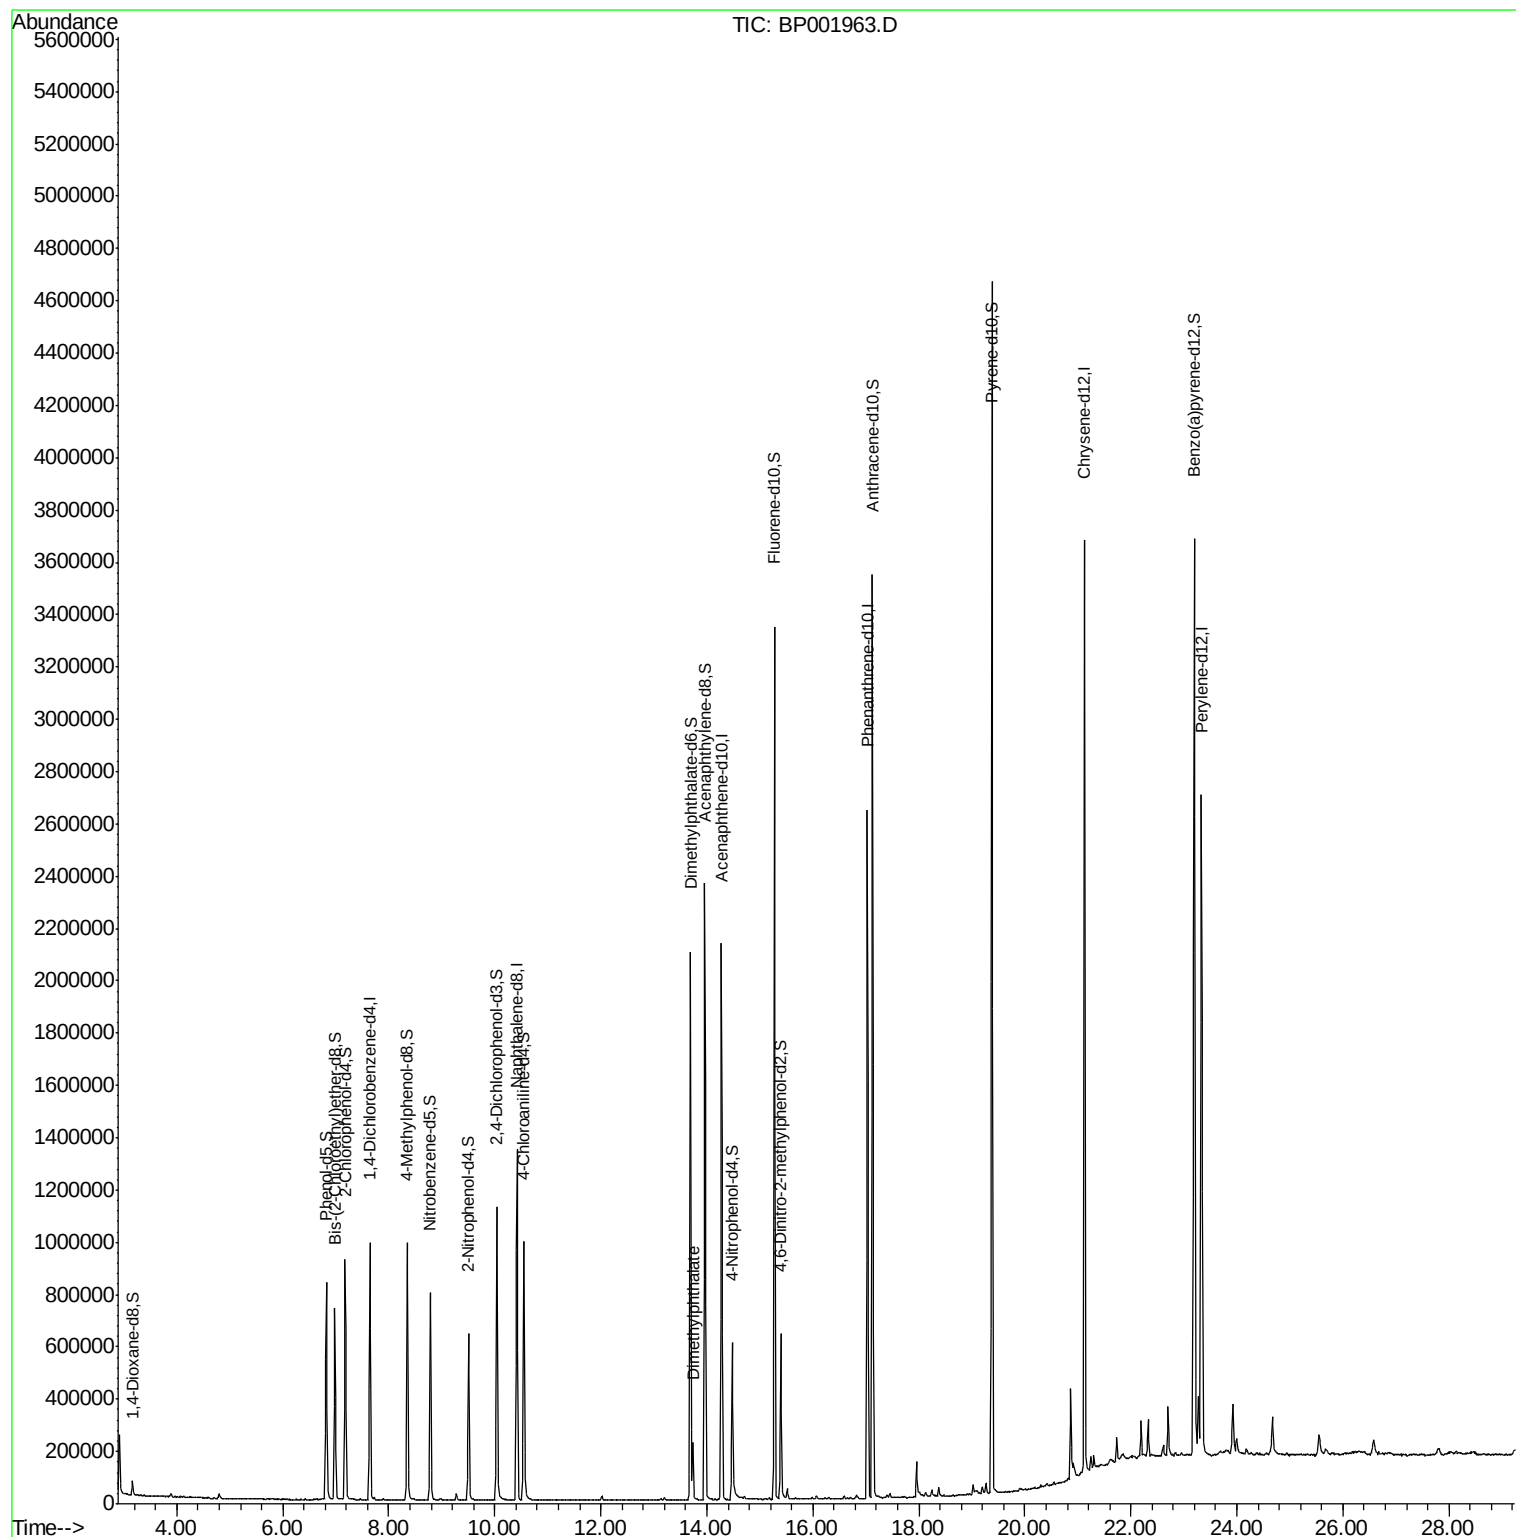

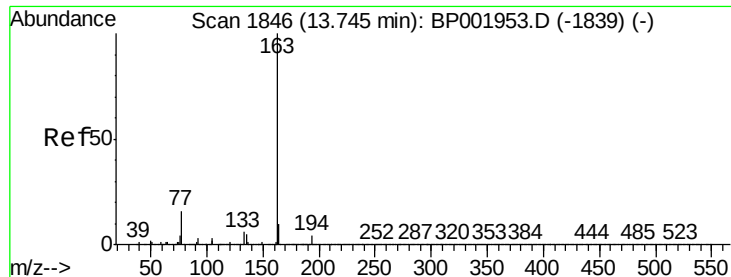

#45

Dimethylphthalate

Concen: 2.538 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. 0.00 min

Lab File: BP001963.D

Acq: 29 Feb 2020 17:23

Instrument :

BNA_P

ClientSampleId :

DBDN6


Tot Ion:163 Resp: 146589

Ion Ratio Lower Upper

163 100

194 4.9 3.6 5.4

164 10.7 8.2 12.4

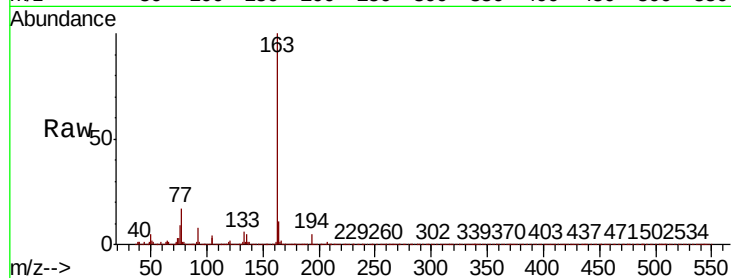

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

