

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001972.D
 Acq On : 29 Feb 2020 23:01
 Operator : CG/JU
 Sample : L1615-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDP4

Quant Time: Mar 02 03:54:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	245934	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	989982	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	614261	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1333279	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1309635	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1482155	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	46799	8.18	ng/uL	0.00
5) Phenol-d5	6.82	99	921823	49.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	502869	50.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	800581	49.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	757841	49.16	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	366776	48.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	410671	48.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	782655	47.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	919984	50.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2272830	48.89	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2741287	49.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	351003	39.50	ng/ul	0.00
58) Fluorene-d10	15.27	176	2008211	49.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	267442	36.39	ng/ul	0.00
71) Anthracene-d10	17.13	188	2994836	49.98	ng/ul	0.00
79) Pyrene-d10	19.37	212	3444495	50.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3781822	49.87	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.85	94	39065	2.006	ng/ul 96
45) Dimethylphthalate	13.74	163	229708	4.787	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001972.D
Acq On : 29 Feb 2020 23:01
Operator : CG/JU
Sample : L1615-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDP4

Quant Time: Mar 02 03:54:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

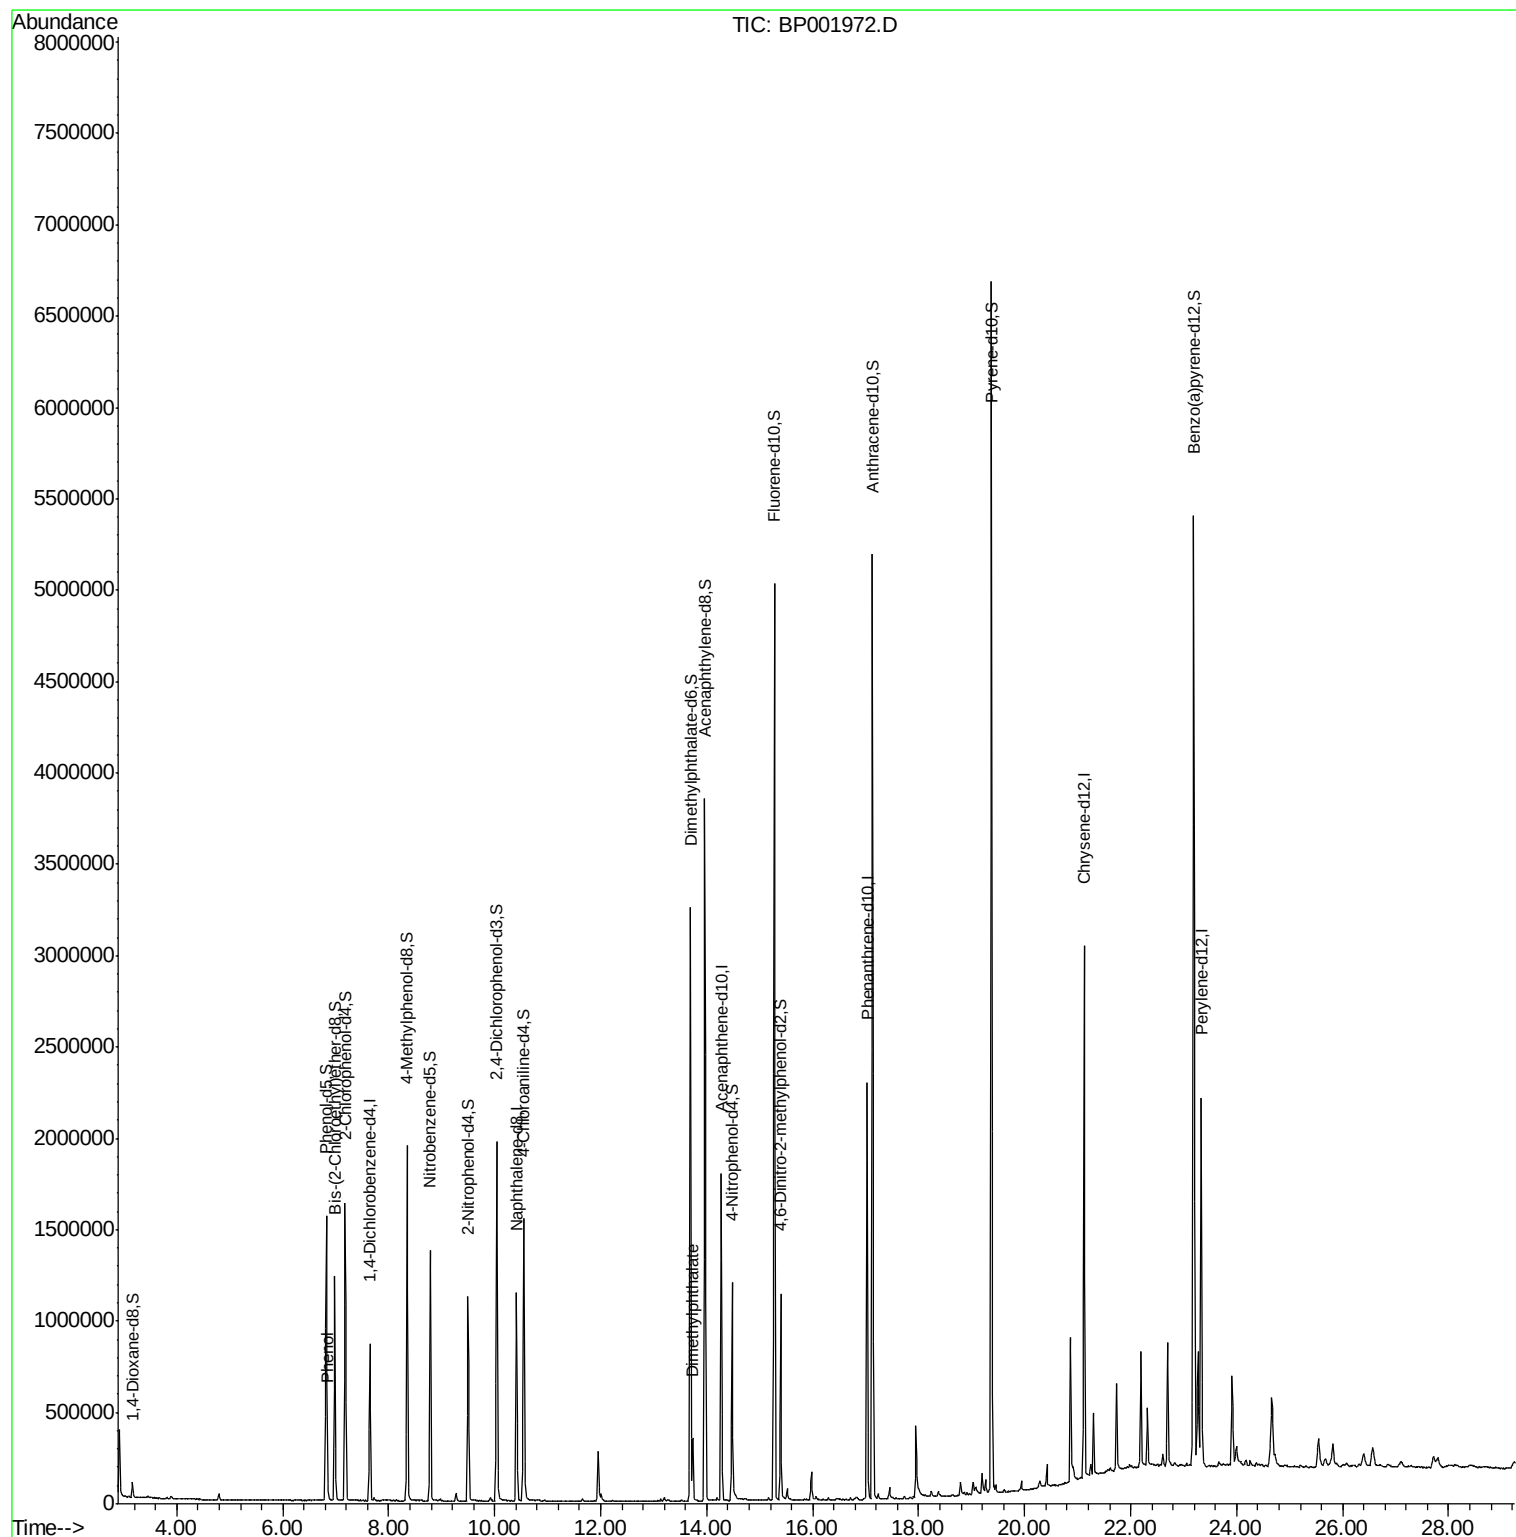

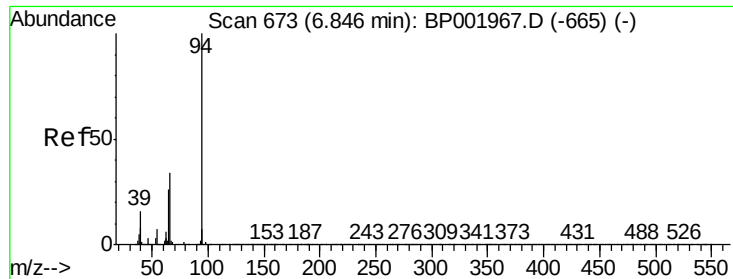

#6

Phenol

Concen: 2.006 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. -0.00 min

Lab File: BP001972.D

Acq: 29 Feb 2020 23:01

Instrument :

BNA_P

ClientSampleId :

DBDP4





Tot Ion: 94 Resp: 39065

Ion Ratio Lower Upper

94 100

65 26.6 20.6 30.8

66 38.1 28.2 42.2

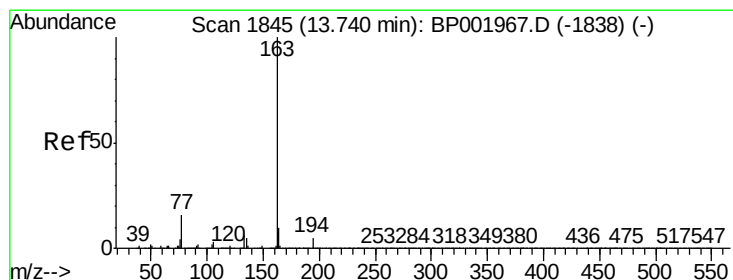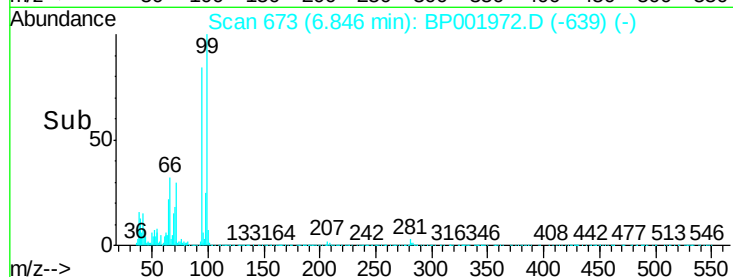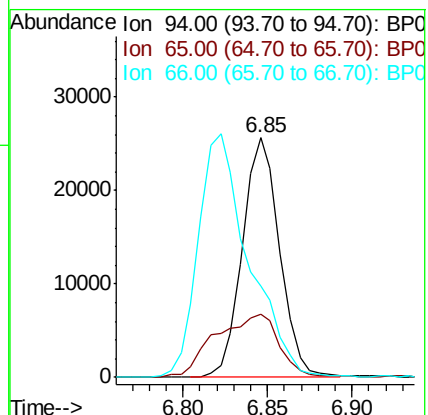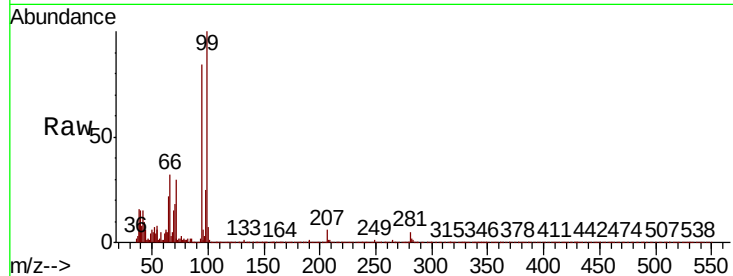

#45

Dimethylphthalate

Concen: 4.787 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001972.D

Acq: 29 Feb 2020 23:01

Tgt Ion: 163 Resp: 229708

Ion Ratio Lower Upper

163 100

194 4.4 3.6 5.4

164 10.5 8.2 12.4

