

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001974.D
 Acq On : 01 Mar 2020 00:09
 Operator : CG/JU
 Sample : L1615-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDP6

Quant Time: Mar 02 04:04:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	272376	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1107248	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	698298	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1518319	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1512110	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1712067	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	32291	5.10	ng/uL	0.00
5) Phenol-d5	6.82	99	573650	27.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	331116	30.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	508847	28.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	486455	28.49	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	236081	27.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	261239	27.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	502379	27.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	680338	33.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1631274	30.87	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1923697	30.44	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	204864	20.28	ng/ul	0.00
58) Fluorene-d10	15.27	176	1432337	31.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	164467	19.65	ng/ul	0.00
71) Anthracene-d10	17.13	188	2181665	31.97	ng/ul	0.00
79) Pyrene-d10	19.37	212	2521411	31.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2745309	31.34	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.85	94	22672	1.051	ng/ul 97
45) Dimethylphthalate	13.74	163	201116	3.687	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001974.D
Acq On : 01 Mar 2020 00:09
Operator : CG/JU
Sample : L1615-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDP6

Quant Time: Mar 02 04:04:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

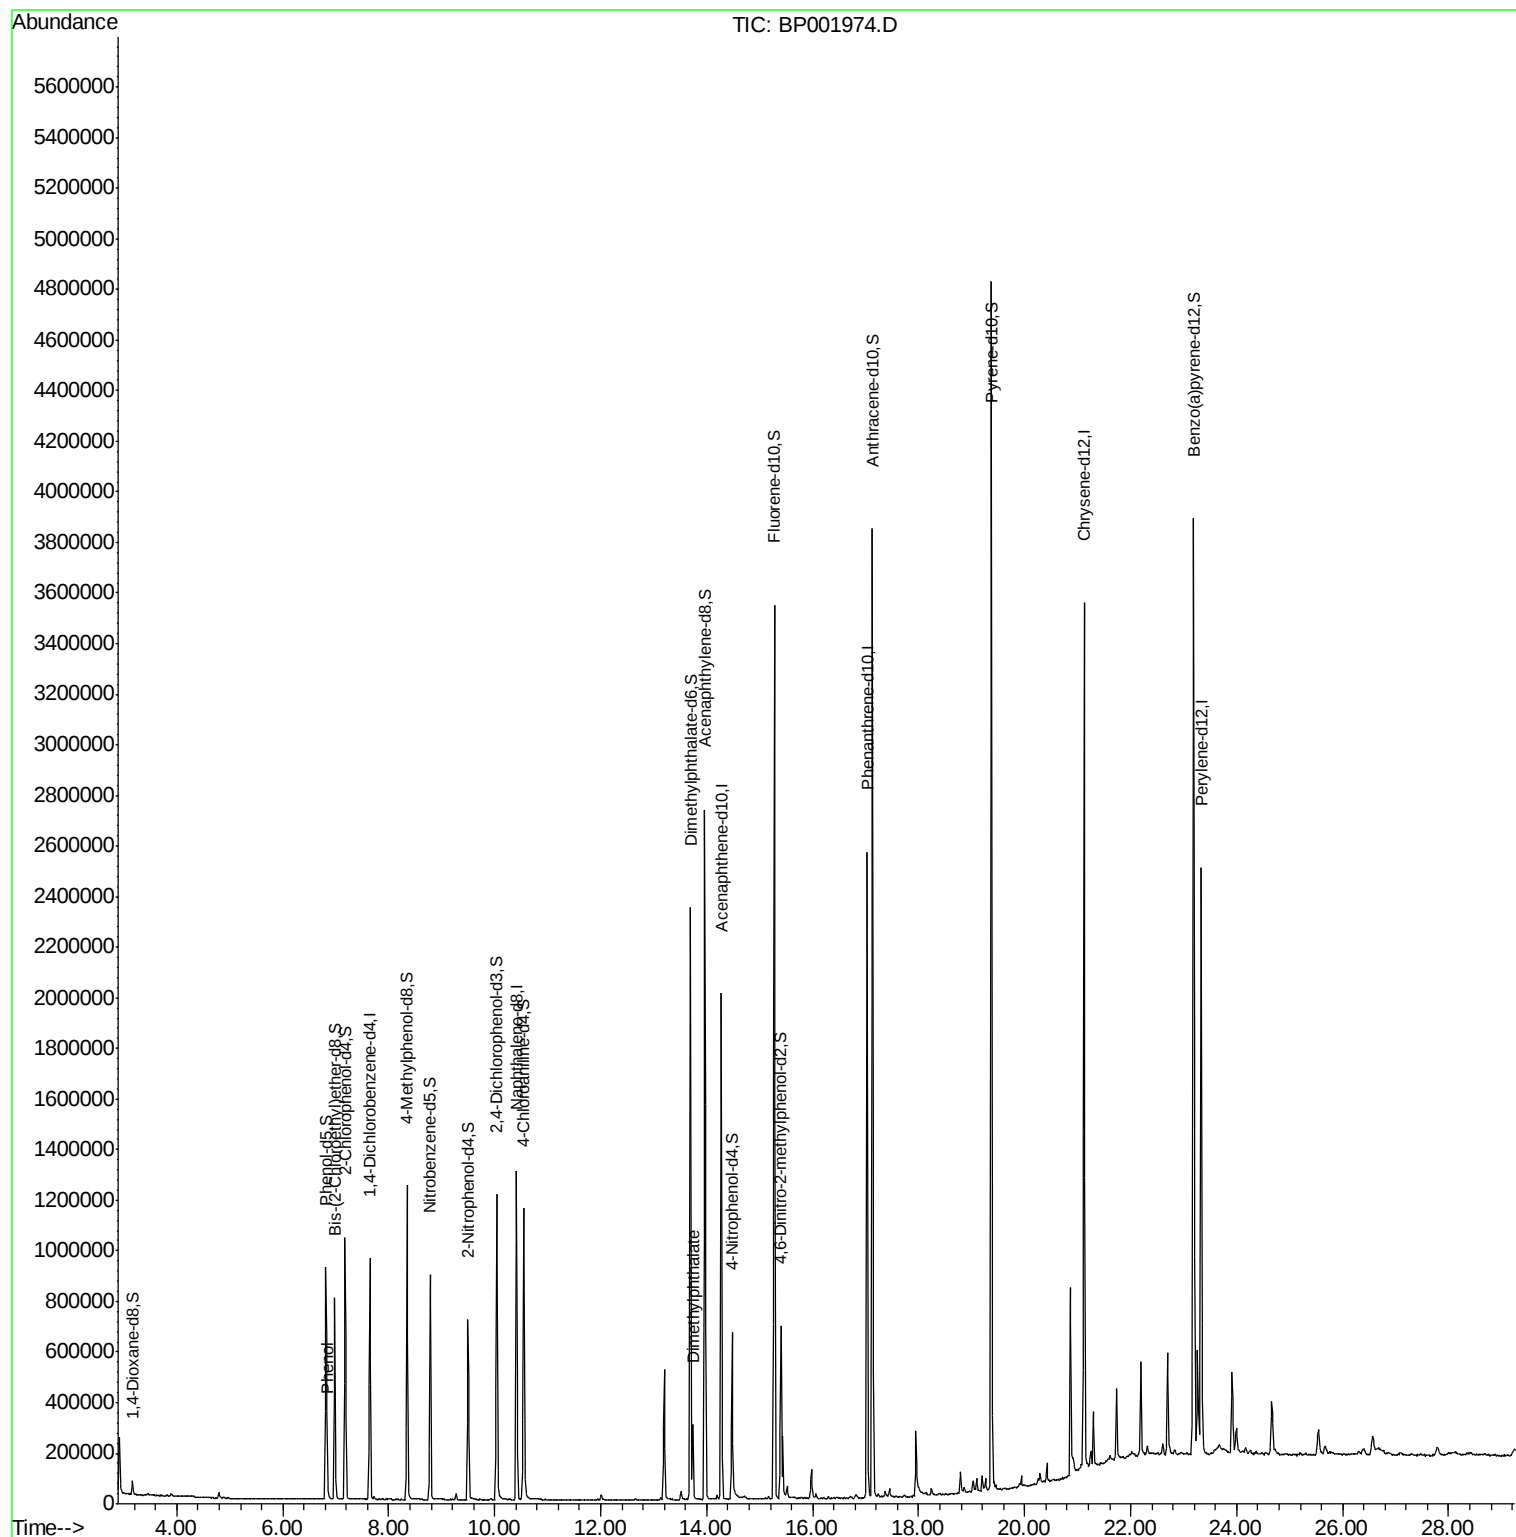

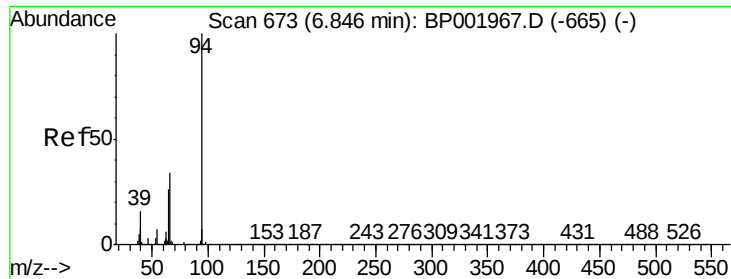

#6

Phenol

Concen: 1.051 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. -0.00 min

Lab File: BP001974.D

Acq: 01 Mar 2020 00:09

Instrument :

BNA_P

ClientSampleId :

DBDP6


Tot Ion: 94 Resp: 22672

Ion Ratio Lower Upper

94 100

65 25.5 20.6 30.8




66 38.1 28.2 42.2

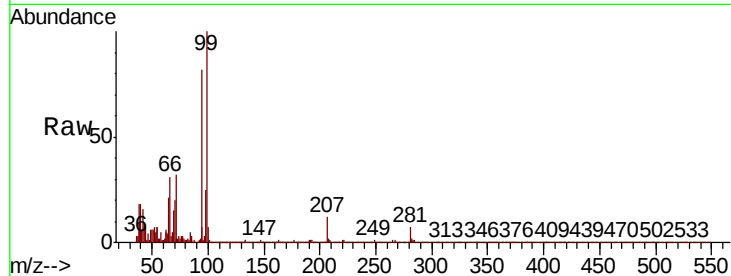

Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

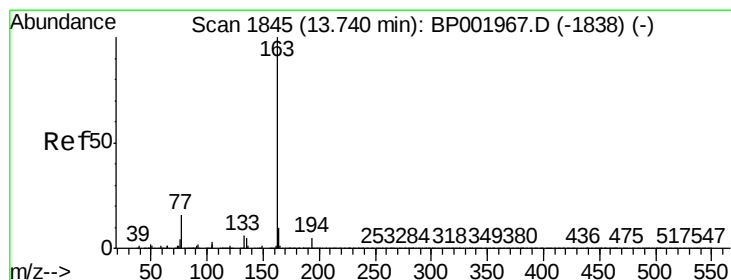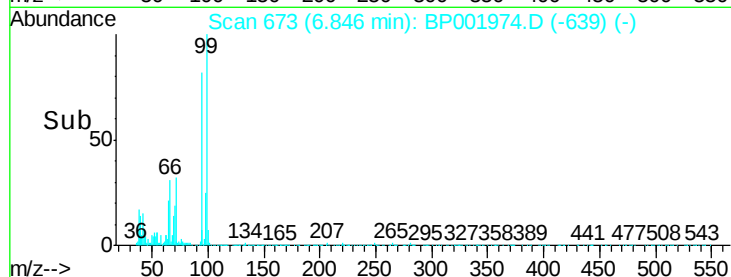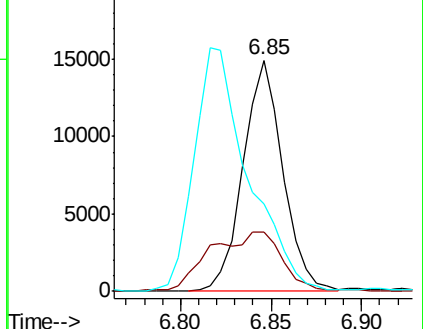

#45

Dimethylphthalate

Concen: 3.687 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001974.D

Acq: 01 Mar 2020 00:09


Tgt Ion: 163 Resp: 201116

Ion Ratio Lower Upper

163 100

194 4.7 3.6 5.4

164 10.4 8.2 12.4

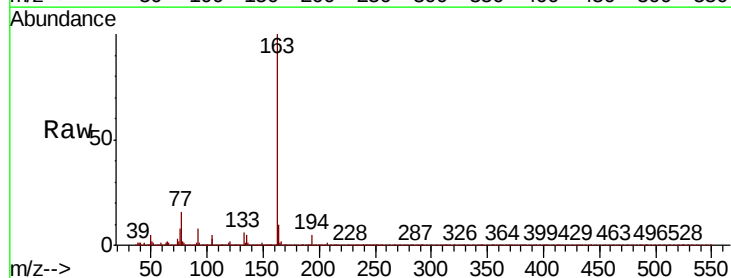

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

