

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001978.D
 Acq On : 01 Mar 2020 02:24
 Operator : CG/JU
 Sample : L1732-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EG9

Quant Time: Mar 02 04:22:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	254163	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1012900	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	641064	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1390158	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1374285	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1599321	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	33224	5.62	ng/uL	0.00
5) Phenol-d5	6.82	99	125329	6.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	346773	33.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	434327	25.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	247067	15.51	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	255703	32.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	275433	31.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	489668	29.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	30594	1.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1844453	38.02	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2098835	36.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	35207	3.80	ng/ul	0.00
58) Fluorene-d10	15.27	176	1641806	39.11	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	228054	29.76	ng/ul	0.00
71) Anthracene-d10	17.13	188	2836411	45.40	ng/ul	0.00
79) Pyrene-d10	19.37	212	3249072	45.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3659311	44.72	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	108535	2.167	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001978.D
Acq On : 01 Mar 2020 02:24
Operator : CG/JU
Sample : L1732-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EG9

Quant Time: Mar 02 04:22:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

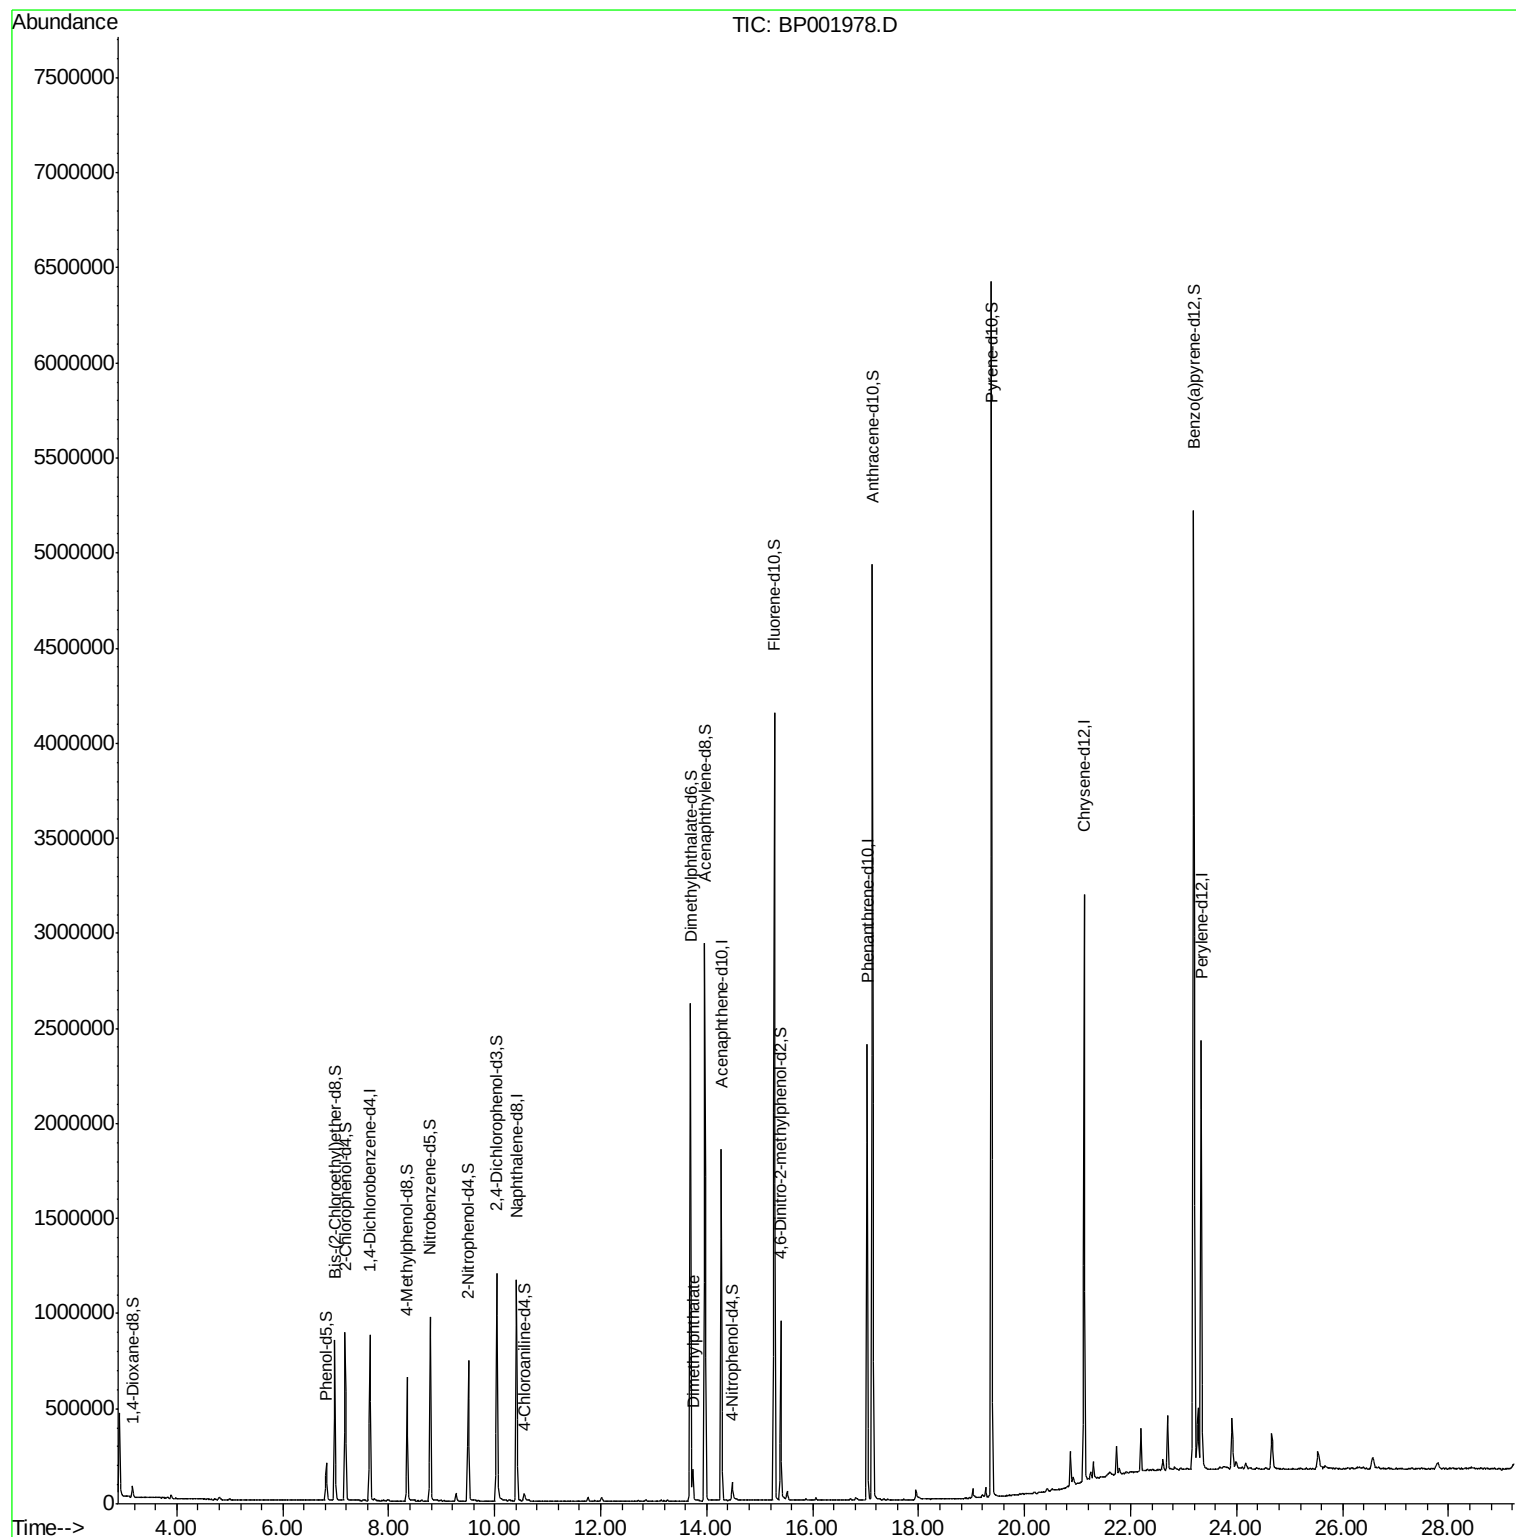

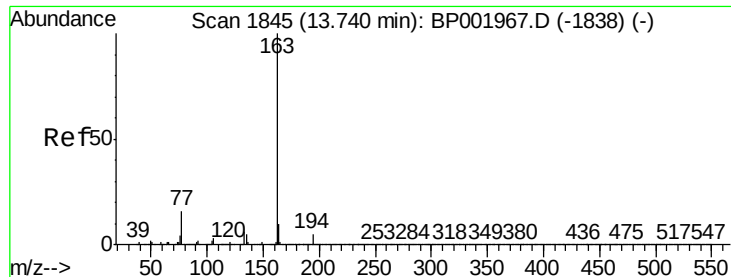

#45

Dimethylphthalate

Concen: 2.167 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001978.D

Acq: 01 Mar 2020 02:24

Instrument :

BNA_P

ClientSampleId :

C0EG9


Tot Ion:163 Resp: 108535

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 9.9 8.2 12.4

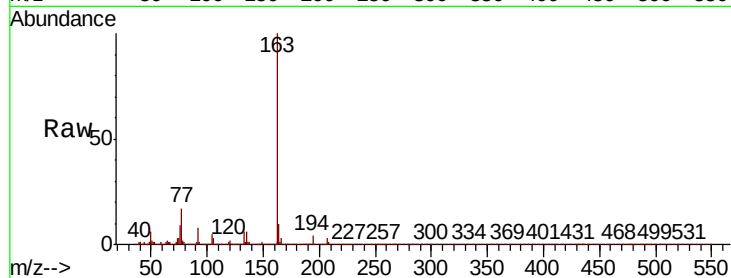

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

