

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022920\
 Data File : BP001979.D
 Acq On : 01 Mar 2020 02:58
 Operator : CG/JU
 Sample : L1732-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EH0

Quant Time: Mar 02 04:27:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 14:59:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	248893	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	997096	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	626913	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1381836	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1372767	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1564627	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	32454	5.61	ng/uL	0.00
5) Phenol-d5	6.82	99	134692	7.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	352590	35.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	446669	27.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	260328	16.68	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	254233	33.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	271627	31.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	500733	30.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	34411	1.89	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	1848974	38.97	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2120403	37.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	36967	4.08	ng/ul	0.00
58) Fluorene-d10	15.27	176	1648802	40.16	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	212492	27.89	ng/ul	0.00
71) Anthracene-d10	17.13	188	2729441	43.95	ng/ul	0.00
79) Pyrene-d10	19.37	212	3157695	43.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3516917	43.93	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.74	163	70215	1.434	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022920\
Data File : BP001979.D
Acq On : 01 Mar 2020 02:58
Operator : CG/JU
Sample : L1732-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EH0

Quant Time: Mar 02 04:27:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 14:59:37 2020
Response via : Initial Calibration

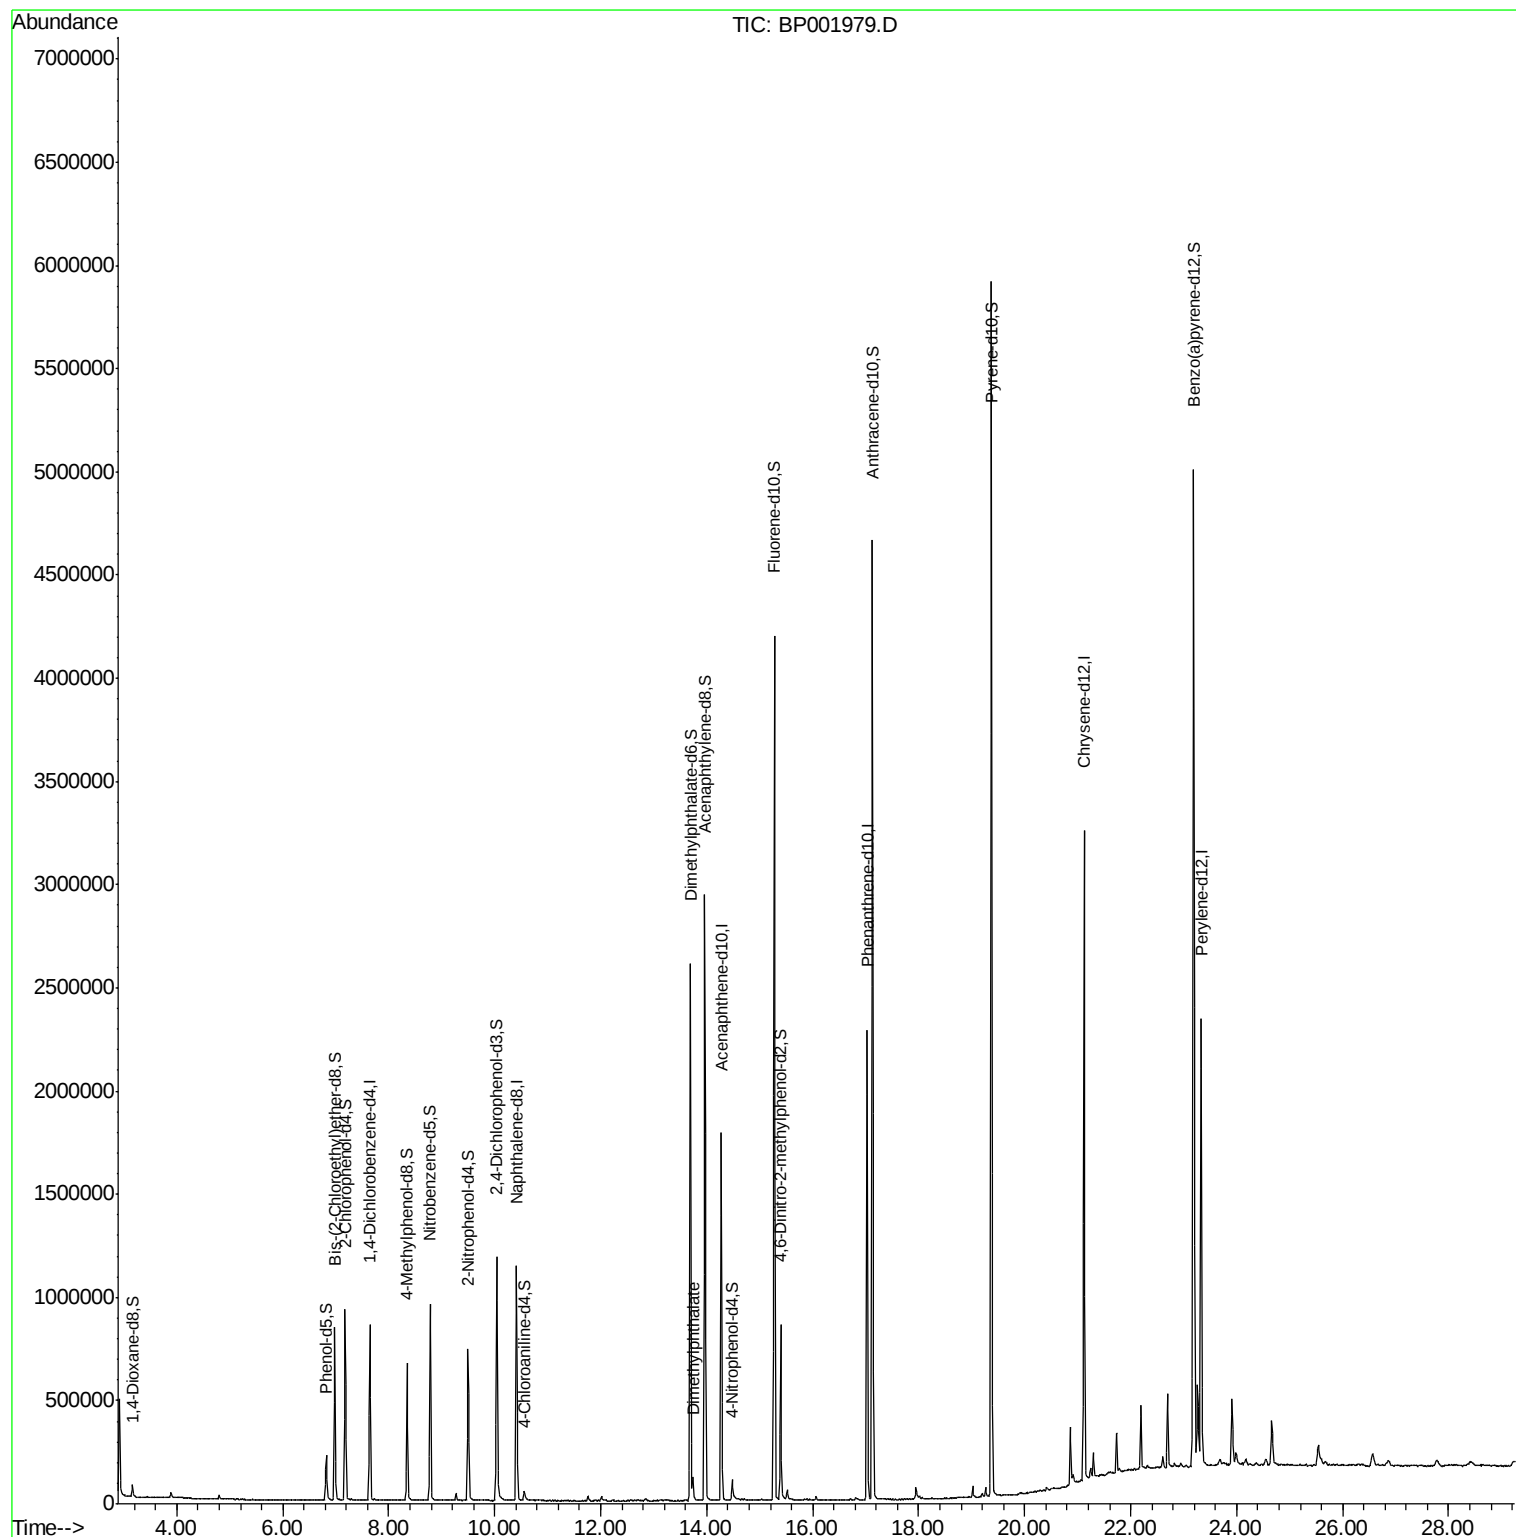

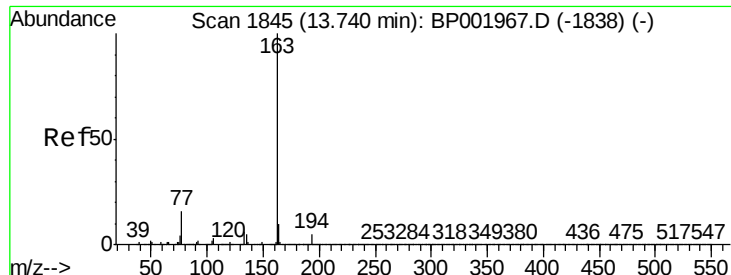

#45

Dimethylphthalate

Concen: 1.434 ng/ul

RT: 13.74 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BP001979.D

Acq: 01 Mar 2020 02:58

Instrument :

BNA_P

ClientSampleId :

C0EH0


Tot Ion:163 Resp: 70215

Ion Ratio Lower Upper

163 100

194 4.7 3.6 5.4

164 11.4 8.2 12.4

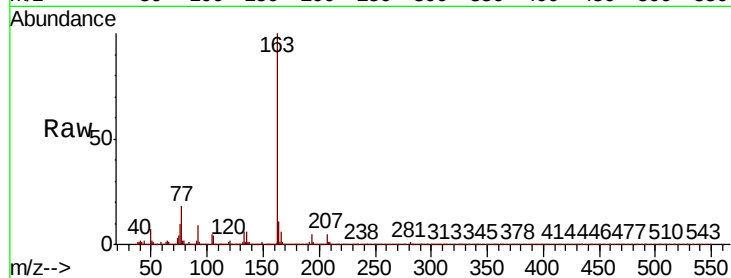

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

