
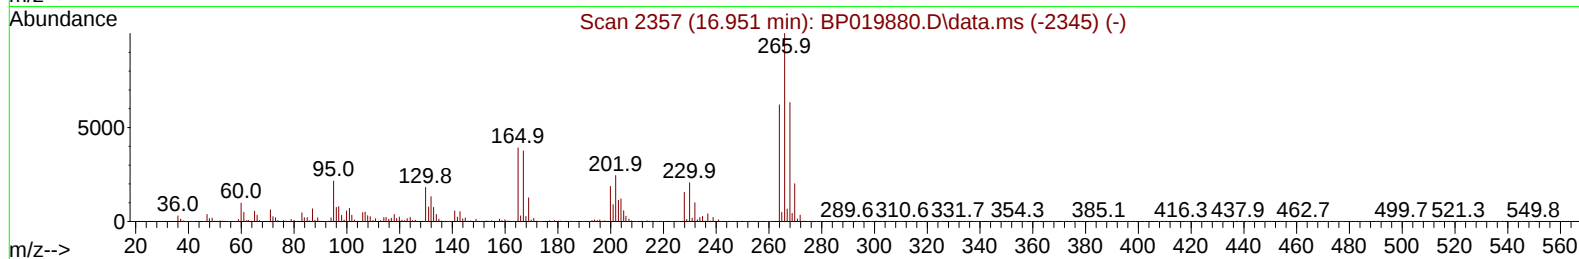
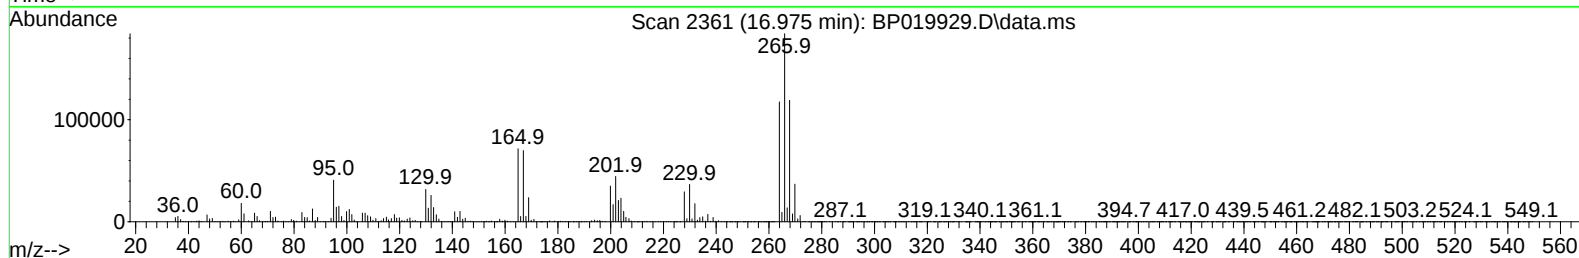


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022924\
Data File : BP019929.D
Acq On : 29 Feb 2024 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 11:20:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

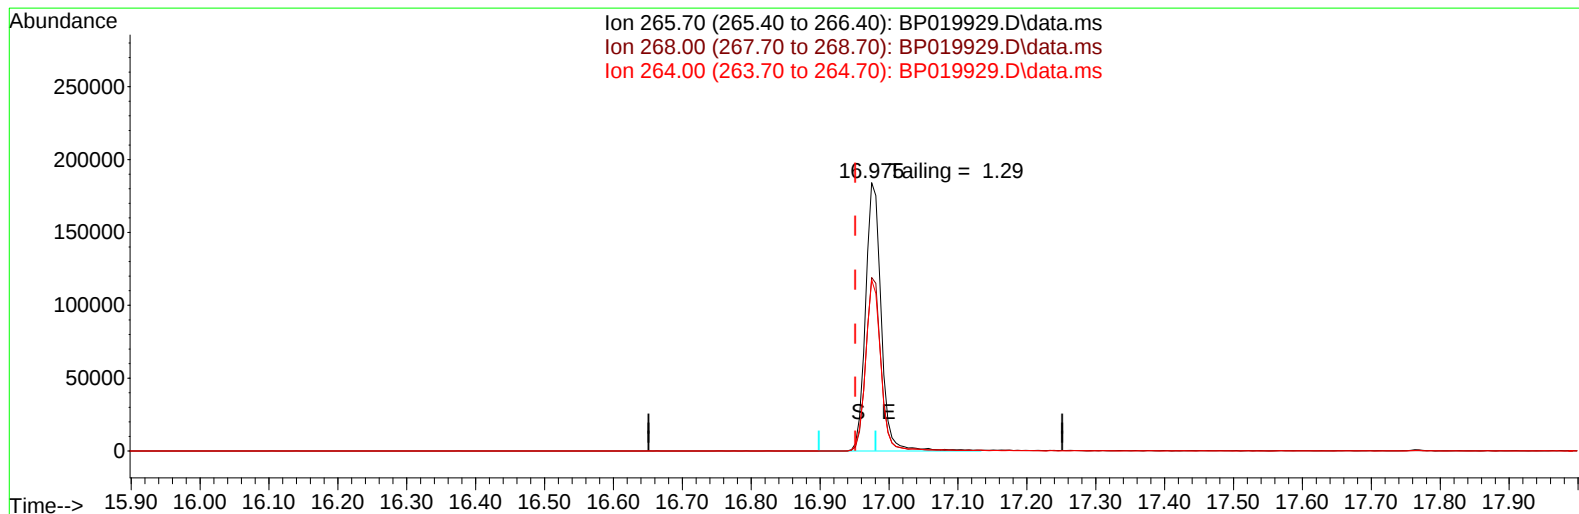

TIC: BP019929.D\data.ms

(70) Pentachlorophenol (C)




16.975min (+ 0.024) 233339.67 ng

response 209292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.62
264.00	62.10	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022924\
Data File : BP019929.D
Acq On : 29 Feb 2024 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 11:20:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

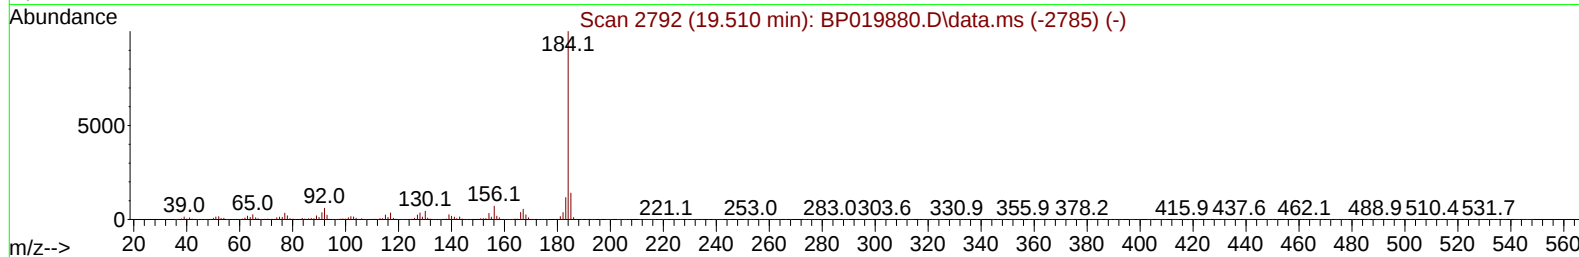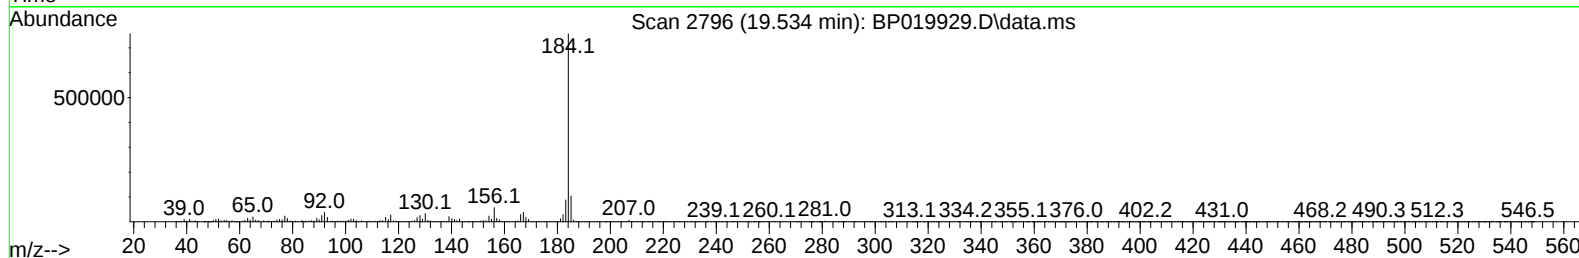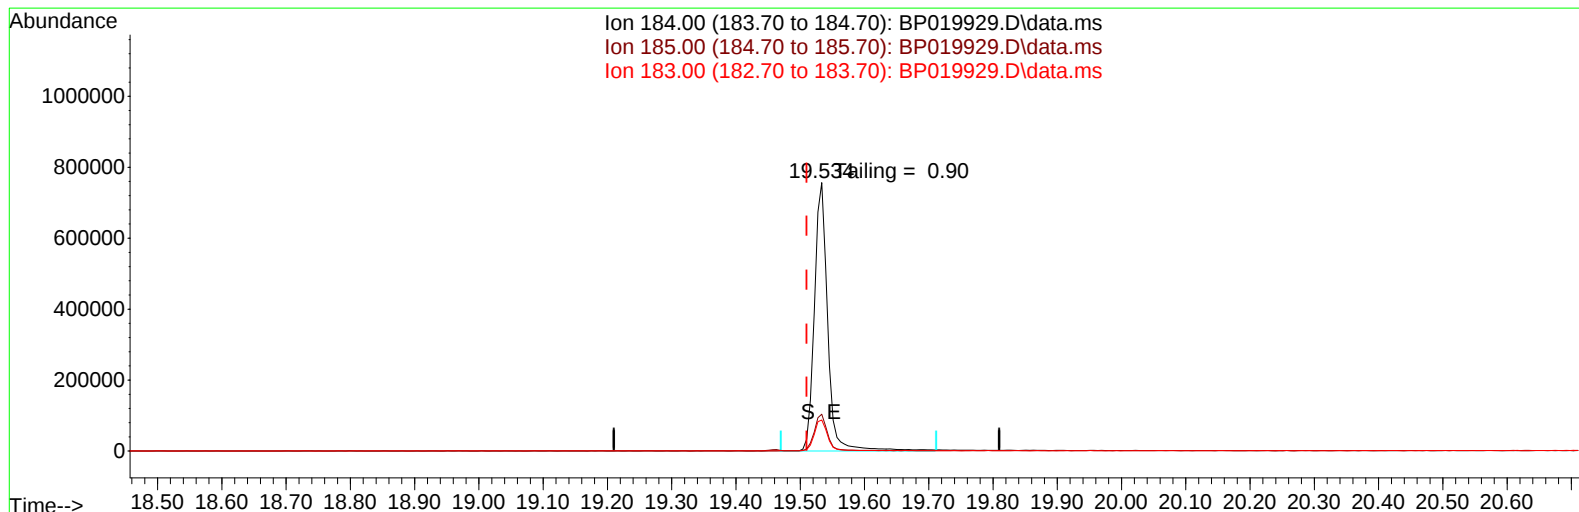

TIC: BP019929.D\data.ms

(77) Benzidine

19.534min (+ 0.024) 94942.97 ng m

response 1088166

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.70
183.00	11.60	11.60
0.00	0.00	0.00