
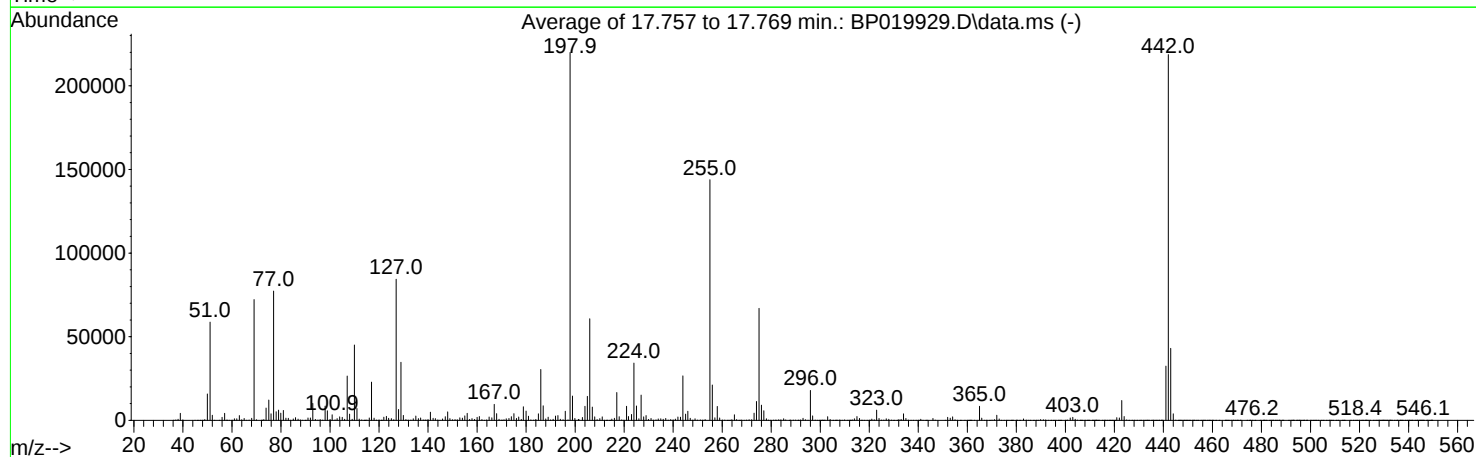


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022924\
Data File : BP019929.D
Acq On : 29 Feb 2024 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 29 12:18:35 2024

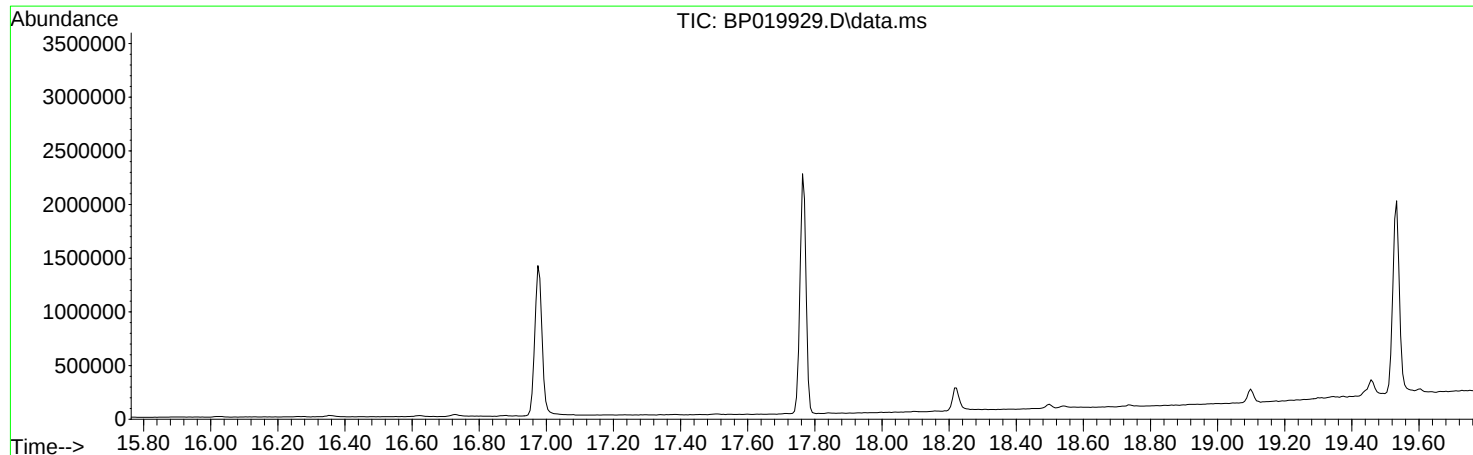




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	26.7	58776	PASS
68	69	0.00	2	1.8	1276	PASS
69	198	0.00	100	32.8	72225	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	38.4	84347	PASS
197	198	0.00	2	0.1	273	PASS
198	198	100	100	100.0	219910	PASS
199	198	5	9	6.6	14569	PASS
275	198	10	60	30.5	66985	PASS
365	198	1	100	3.8	8432	PASS
441	198	0.01	100	14.8	32470	PASS
442	442	100	100	100.0	218651	PASS
443	442	15	24	19.7	43003	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022924\
Data File : BP019929.D
Acq On : 29 Feb 2024 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 29 11:20:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

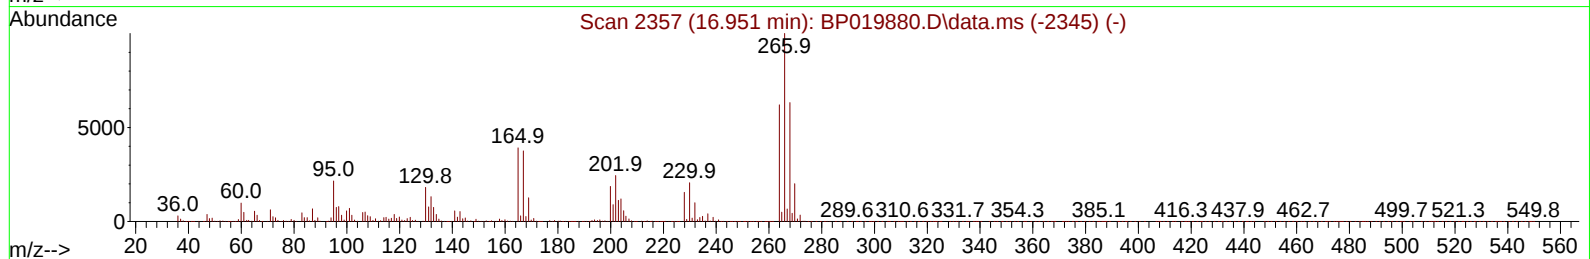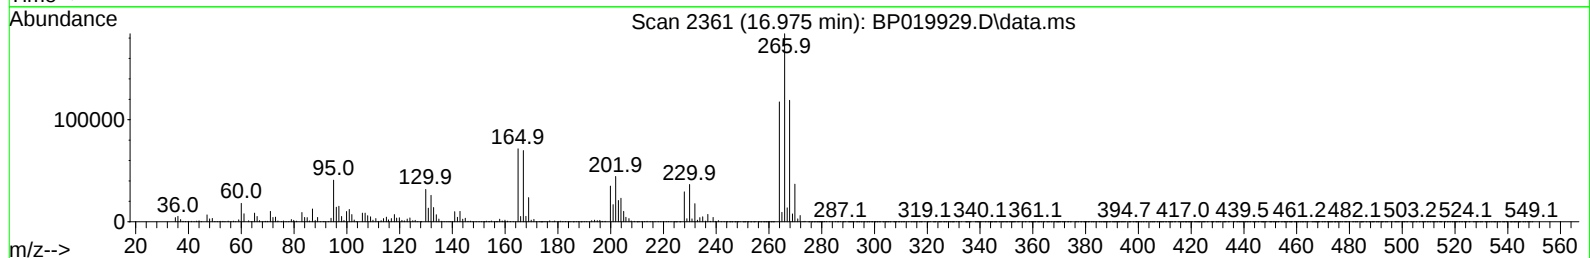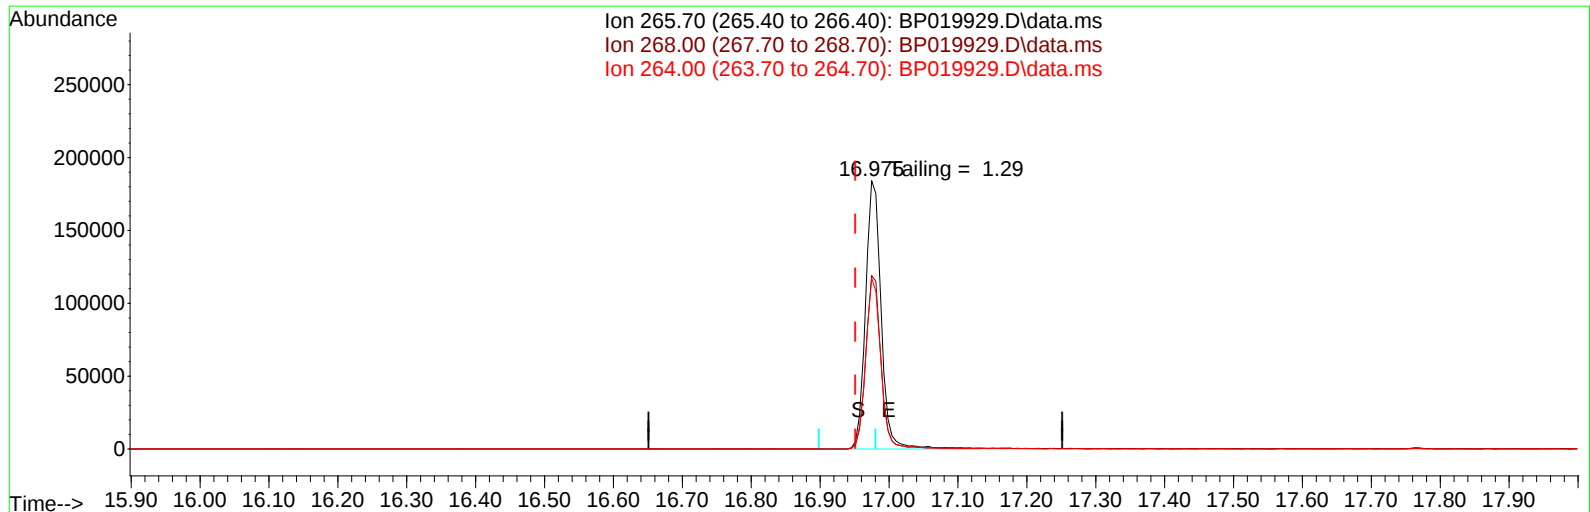

TIC: BP019929.D\data.ms

(70) Pentachlorophenol (C)

16.975min (+ 0.024) 233339.67 ng




response 209292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.62
264.00	62.10	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022924\
Data File : BP019929.D
Acq On : 29 Feb 2024 10:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 29 11:20:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

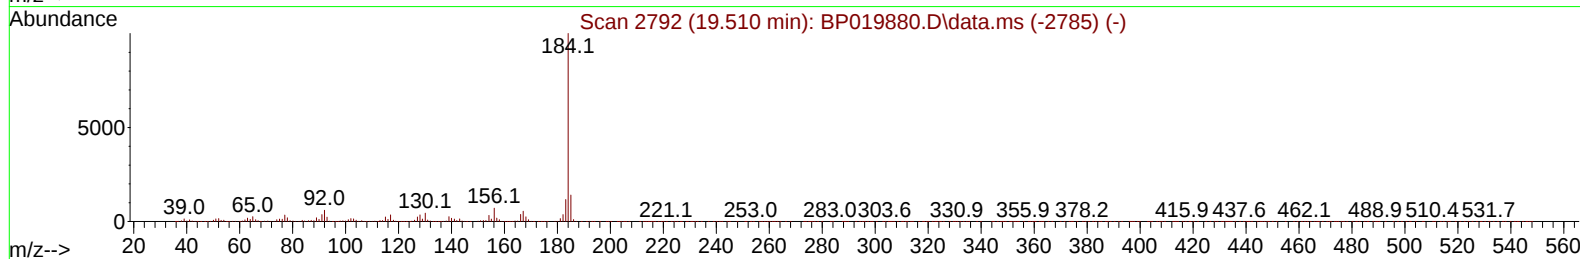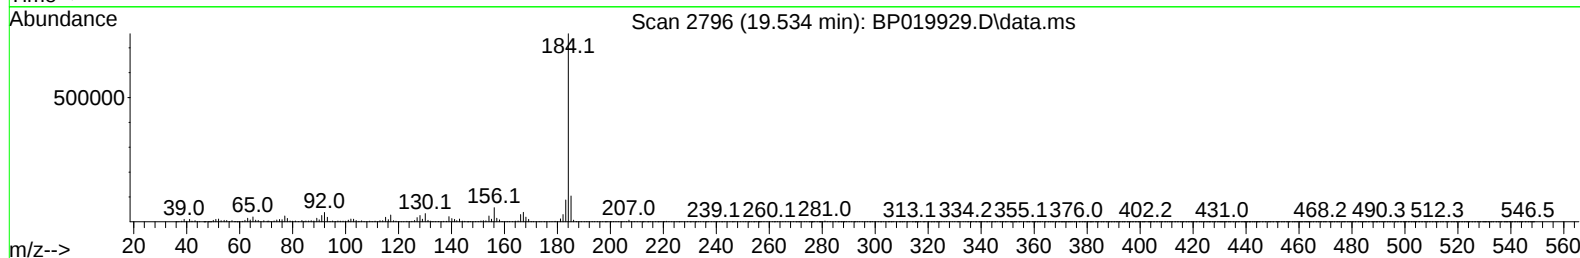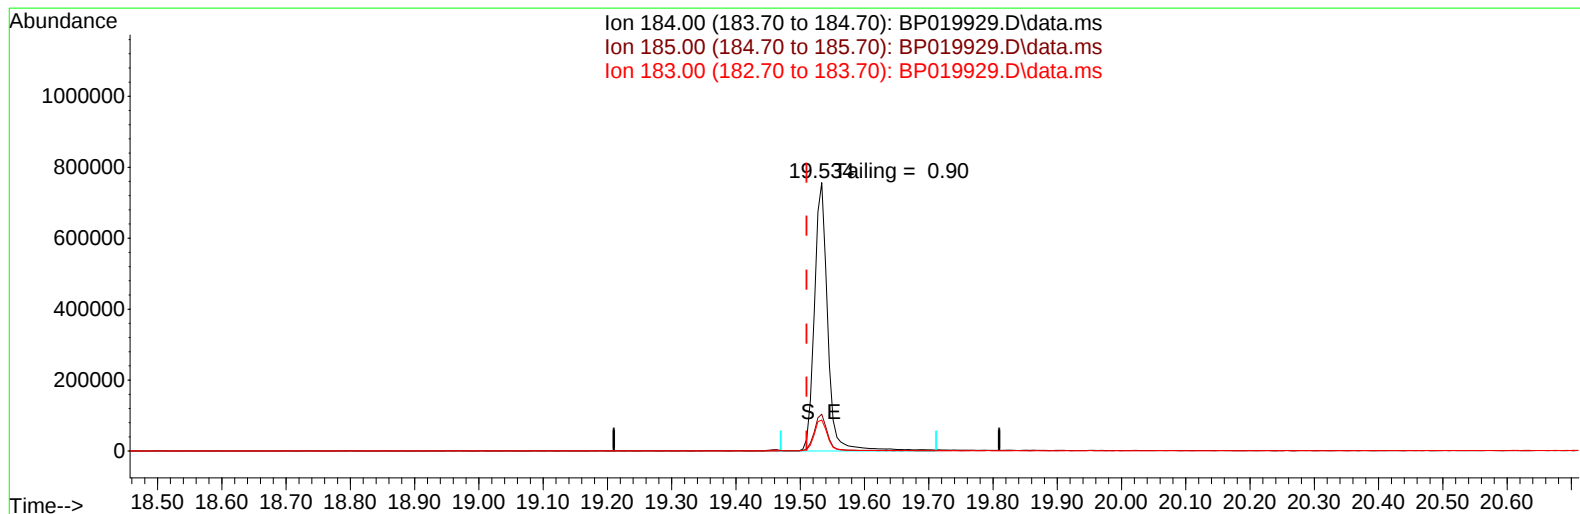

TIC: BP019929.D\data.ms

(77) Benzidine

19.534min (+ 0.024) 94942.97 ng m

response 1088166

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.70
183.00	11.60	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/29/2024	BNA_P	<u>BP019929.D</u>
Compound Name	Response	Retention Time
DDT	788444	20.728
DDD	26132	20.304
DDE	3912	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30044	818488	3.67

Instrument :
BNA_P
ClientSampleId :
DFTPP