

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030321\
 Data File : BP004889.D
 Acq On : 03 Mar 2021 12:19
 Operator : CG/JU
 Sample : M1534-01
 Misc : SOM-MDL-W-01
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Manual Integrations
 APPROVED

mohammad
 3/4/2021 11:33:19 AM

Quant Time: Mar 03 12:52:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 03 10:35:24 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	26132	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	101676	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.40	164	65063	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	148379	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	165879	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	168718	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	2764	4.16	ng/uL	0.00
5) Phenol-d5	6.92	99	66949	31.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	40979	37.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	56429	34.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	54561	32.18	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	26573	35.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	30013	36.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	53168	33.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	70673	39.32	ng/ul	0.00
44) Dimethylphthalate-d6	13.81	166	174484	36.66	ng/ul	0.00
47) Acenaphthylene-d8	14.09	160	208930	35.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.61	143	27741	32.58	ng/ul	0.00
58) Fluorene-d10	15.39	176	149745	37.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	29826	30.83	ng/ul	0.00
71) Anthracene-d10	17.26	188	237508	35.30	ng/ul	0.00
79) Pyrene-d10	19.50	212	275321	35.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	323837	37.45	ng/ul	-0.01

Target Compounds

				Ovalue	
2) 1,4-Dioxane	3.26	88	882	1.220	ng/uL# 79
4) Benzaldehyde	6.89	77	5895	5.420	ng/ul 99
6) Phenol	6.95	94	8823	3.944	ng/ul 98
8) Bis(2-Chloroethyl)ether	7.18	93	6453	3.919	ng/ul 98
10) 2-Chlorophenol	7.31	128	6837m	3.976	ng/ul
11) 2-Methylphenol	8.19	108	5965	3.575	ng/ul 95
12) 2,2'-oxybis(1-Chloropropan	8.27	45	4098	3.850	ng/ul# 91
14) Acetophenone	8.57	105	10779	3.845	ng/ul 95
15) N-Nitroso-di-n-propylamine	8.55	70	5080	3.746	ng/ul 93
16) 4-Methylphenol	8.52	108	6841	3.811	ng/ul 97
17) Hexachloroethane	8.82	117	3099	4.094	ng/ul 89
20) Nitrobenzene	8.95	77	8337	4.152	ng/ul# 93
21) Isophorone	9.47	82	12877	3.748	ng/ul# 95
23) 2-Nitrophenol	9.66	139	3683	3.936	ng/ul 95
24) 2,4-Dimethylphenol	9.72	107	7821	3.765	ng/ul 95
25) Bis(2-Chloroethoxy)methane	9.96	93	8132	3.920	ng/ul# 88
27) 2,4-Dichlorophenol	10.19	162	6470	3.999	ng/ul# 80
28) Naphthalene	10.59	128	20981	3.899	ng/ul 98
30) 4-Chloroaniline	10.70	127	8277	4.467	ng/ul 98
31) Hexachlorobutadiene	10.87	225	4893	4.128	ng/ul 98
32) Caprolactam	11.52	113	1886	3.588	ng/ul 89
33) 4-Chloro-3-methylphenol	11.83	107	6467	3.510	ng/ul# 95
34) 2-Methylnaphthalene	12.21	142	14975	3.912	ng/ul 97

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030321\
 Data File : BP004889.D
 Acq On : 03 Mar 2021 12:19
 Operator : CG/JU
 Sample : M1534-01
 Misc : SOM-MDL-W-01
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 MDL-WATER-01

Manual Integrations
 APPROVED

mohammad
 3/4/2021 11:33:19 AM

Quant Time: Mar 03 12:52:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 03 10:35:24 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.43	142	14705	3.953	ng/ul#	90
37) 1,2,4,5-Tetrachlorobenzene	12.58	216	9105	4.365	ng/ul	96
38) Hexachlorocyclopentadiene	12.56	237	4600	3.461	ng/ul#	96
39) 2,4,6-Trichlorophenol	12.82	196	4675	3.578	ng/ul#	85
40) 2,4,5-Trichlorophenol	12.90	196	5239	3.742	ng/ul	94
41) 1,1'-Biphenyl	13.23	154	20405	4.189	ng/ul	95
42) 2-Chloronaphthalene	13.27	162	15715	4.105	ng/ul	97
43) 2-Nitroaniline	13.48	65	3751	3.424	ng/ul	97
45) Dimethylphthalate	13.86	163	20198	4.128	ng/ul	99
46) 2,6-Dinitrotoluene	13.97	165	3345	3.419	ng/ul	98
48) Acenaphthylene	14.12	152	22596	4.050	ng/ul	97
49) 3-Nitroaniline	14.32	138	3454	3.866	ng/ul#	72
50) Acenaphthene	14.46	153	17343	4.281	ng/ul	96
51) 2,4-Dinitrophenol	14.52	184	1685	2.678	ng/ul	93
53) 4-Nitrophenol	14.63	109	3930	4.251	ng/ul	87
54) Dibenzofuran	14.80	168	24827	4.234	ng/ul	98
55) 2,4-Dinitrotoluene	14.76	165	5424	3.763	ng/ul#	92
56) 2,3,4,6-Tetrachlorophenol	15.03	232	4776	3.863	ng/ul	94
57) Diethylphthalate	15.23	149	20305	4.104	ng/ul	96
59) Fluorene	15.45	166	19844	4.058	ng/ul	94
60) 4-Chlorophenyl-phenylether	15.45	204	10726	4.164	ng/ul	95
61) 4-Nitroaniline	15.47	138	3366	3.298	ng/ul#	84
64) 4,6-Dinitro-2-methylphenol	15.53	198	3745	3.819	ng/ul#	70
65) N-Nitrosodiphenylamine	15.66	169	17017	3.906	ng/ul	99
66) 4-Bromophenyl-phenylether	16.35	248	5985m	3.813	ng/ul	
67) Hexachlorobenzene	16.46	284	7429	4.123	ng/ul#	90
68) Atrazine	16.62	200	5695	3.335	ng/ul	92
69) Pentachlorophenol	16.80	266	3120	2.826	ng/ul	92
70) Phenanthrene	17.20	178	32698	4.055	ng/ul	96
72) Anthracene	17.29	178	32632	3.964	ng/ul	97
73) 1,2,3,4-Tetrachlorobenzene	13.19	216	9091m	4.115	ng/uL	
74) Pentachlorobenzene	14.72	250	8333	3.873	ng/uL#	89
75) Carbazole	17.56	167	26315	3.635	ng/ul	93
76) Di-n-butylphthalate	18.12	149	29567	3.454	ng/ul	99
77) Fluoranthene	19.17	202	37672	3.894	ng/ul#	94
80) Pvrene	19.52	202	41262	4.027	ng/ul	98
81) Butylbenzylphthalate	20.40	149	13083	3.272	ng/ul	94
82) 3,3'-Dichlorobenzidine	21.17	252	12914	3.738	ng/ul#	99
83) Benzo(a)anthracene	21.23	228	40901	3.990	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.16	149	19780	3.311	ng/ul	98
85) Chrysene	21.27	228	41379	4.144	ng/ul	94
87) Di-n-octyl phthalate	22.04	149	34418	3.030	ng/ul	100
88) Benzo(b)fluoranthene	22.84	252	43563	4.061	ng/ul	98
89) Benzo(k)fluoranthene	22.89	252	42746	4.030	ng/ul	98
91) Benzo(a)pyrene	23.44	252	39521	4.196	ng/ul#	98
92) Indeno(1,2,3-cd)pyrene	25.90	276	48087	3.989	ng/ul	98
93) Dibenzo(a,h)anthracene	25.91	278	41450	4.043	ng/ul	98
94) Benzo(a,h,i)perylene	26.62	276	39410	3.927	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030321\
Data File : BP004889.D
Acq On : 03 Mar 2021 12:19
Operator : CG/JU
Sample : M1534-01
Misc : SOM-MDL-W-01
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01


Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

Quant Time: Mar 03 12:52:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 03 10:35:24 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

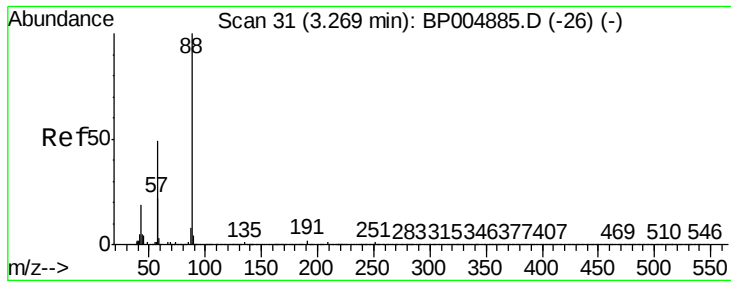

#2

1,4-Dioxane

Concen: 1.220 ng/uL

RT: 3.26 min Scan# 30

Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-01

Tot Ion:	88	Resp:	882
Ion Ratio	Lower	Upper	
88	100		
43	15.9	20.9	31.3#
58	35.9	41.0	61.4#

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

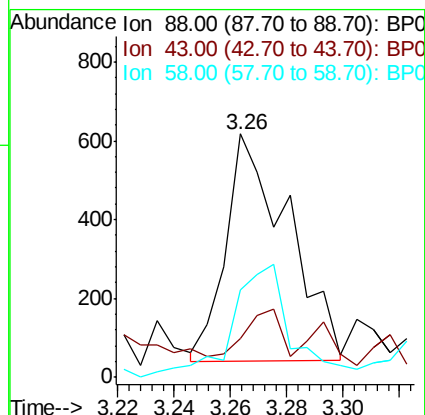

#4

Benzaldehyde

Concen: 5.420 ng/uL




RT: 6.89 min Scan# 647


Delta R.T. 0.00 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:	77	Resp:	5895
Ion Ratio	Lower	Upper	
77	100		
105	95.2	75.4	113.2
106	86.6	69.7	104.5

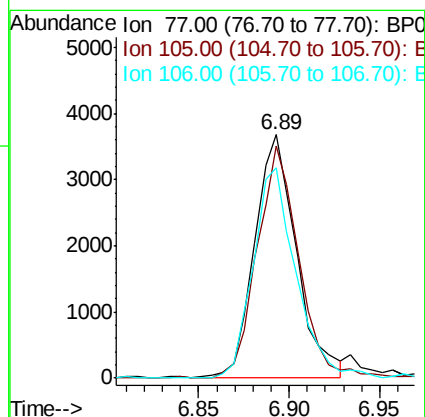



#6

Phenol

Concen: 3.944 ng/ul

RT: 6.95 min Scan# 657

Delta R.T. 0.00 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-01

Tot Ion:	94	Resp:	8823
Ion	Ratio	Lower	Upper
94	100		
65	30.2	22.8	34.2
66	47.7	37.8	56.8

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

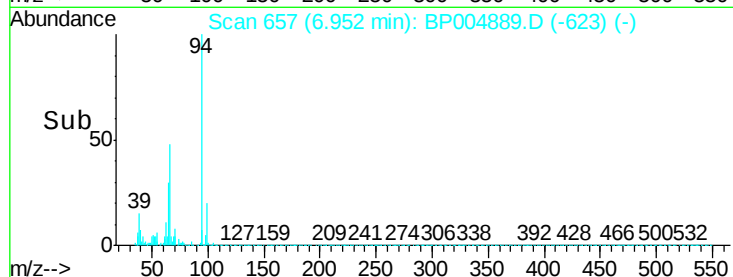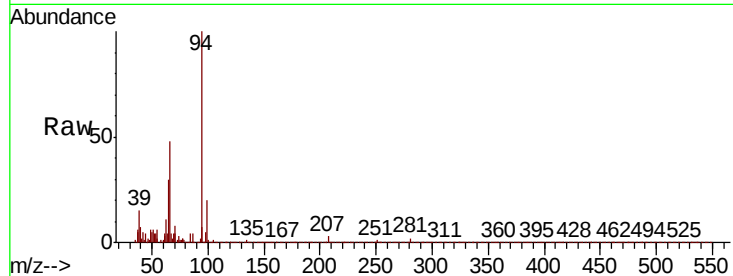

#8

Bis(2-Chloroethyl)ether

Concen: 3.919 ng/ul




RT: 7.18 min Scan# 695


Delta R.T. 0.00 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:	93	Resp:	6453
Ion	Ratio	Lower	Upper
93	100		
63	69.8	56.0	84.0
95	31.9	27.8	41.8

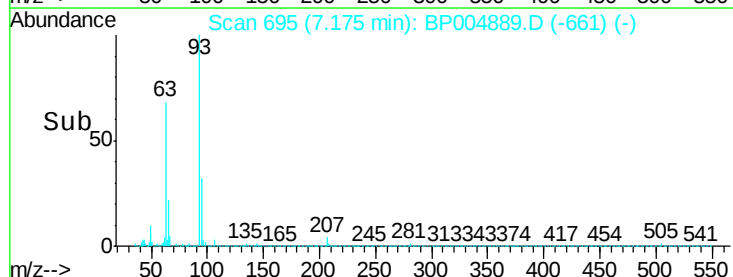







#10
2-Chlorophenol
Concen: 3.976 ng/ul m
RT: 7.31 min Scan# 718
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
128	100		
64	52.9	34.8	52.2#
130	27.4	28.6	43.0#




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

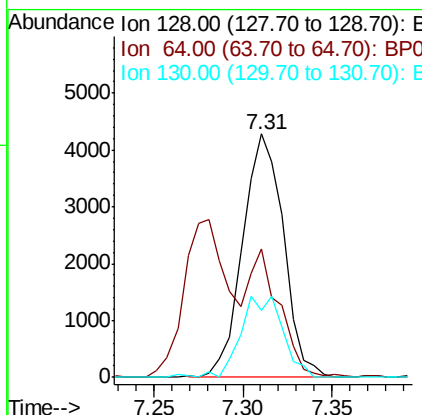

#11
2-Methylphenol
Concen: 3.575 ng/ul
RT: 8.19 min Scan# 868
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
108	100		
107	90.6	68.8	103.2

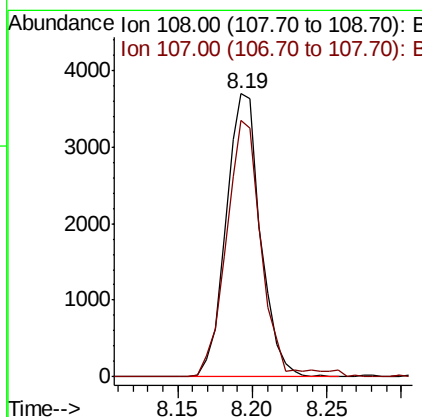







#12
2,2'-oxvbis(1-Chloropropane)
Concen: 3.850 ng/ul
RT: 8.27 min Scan# 881
Delta R.T. -0.02 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
45	100		
77	26.4	21.8	32.8
79	14.9	18.6	27.8




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

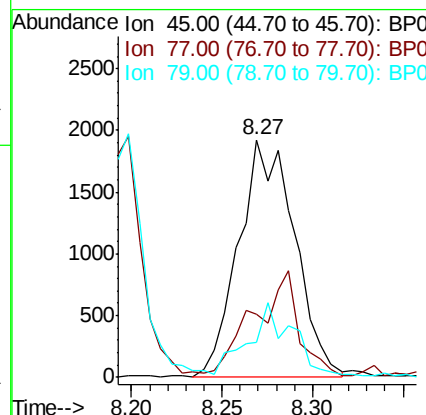

#14
Acetophenone
Concen: 3.845 ng/ul
RT: 8.57 min Scan# 932
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
105	100		
77	76.3	64.4	96.6
51	20.9	19.1	28.7

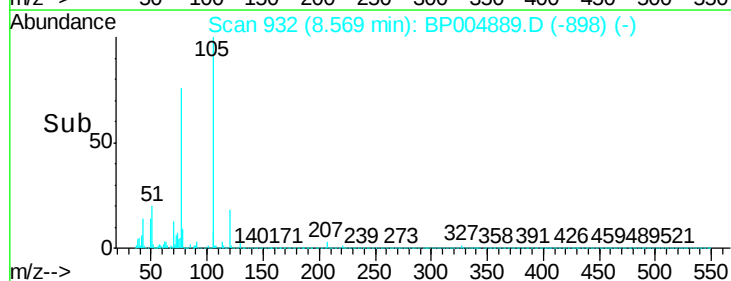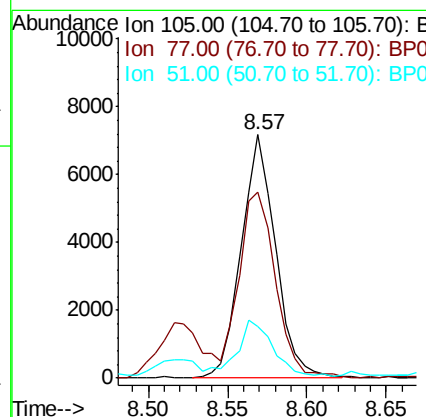







#15
N-Nitroso-di-n-propylamine
Concen: 3.746 ng/ul
RT: 8.55 min Scan# 929
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion:	70	Resp:	5080
Ion Ratio	Lower	Upper	
70	100		
42	47.3	33.1	49.7
101	10.6	8.5	12.7
130	20.8	15.0	22.4




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

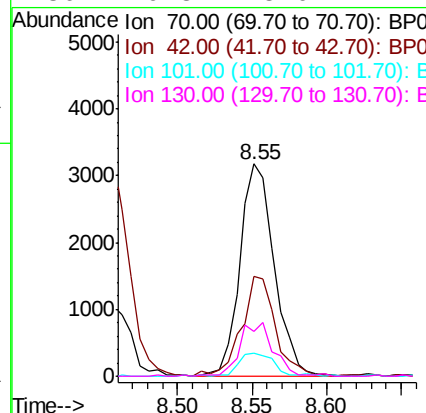

#16
4-Methylphenol
Concen: 3.811 ng/ul
RT: 8.52 min Scan# 924
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion:	108	Resp:	6841
Ion Ratio	Lower	Upper	
108	100		
107	108.4	89.2	133.8

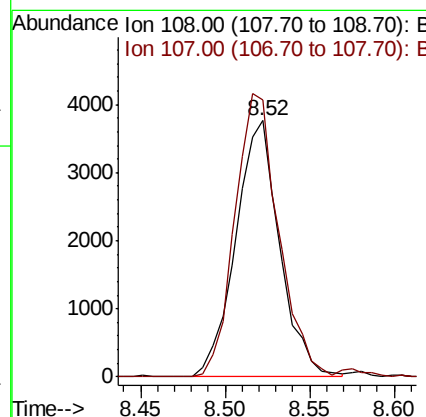







#17
Hexachloroethane
Concen: 4.094 ng/ul
RT: 8.82 min Scan# 974
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
117	100		
201	98.2	86.7	130.1
199	49.2	48.2	72.4




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

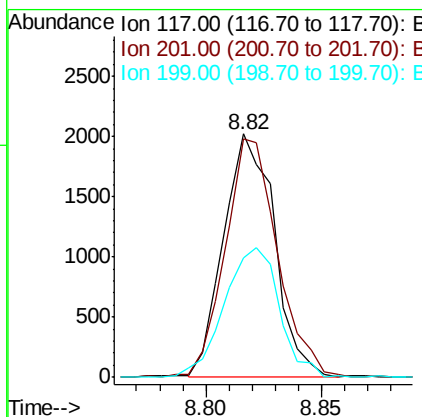

#20
Nitrobenzene
Concen: 4.152 ng/ul
RT: 8.95 min Scan# 996
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
77	100		
123	40.3	29.4	44.2
65	17.0	9.8	14.6

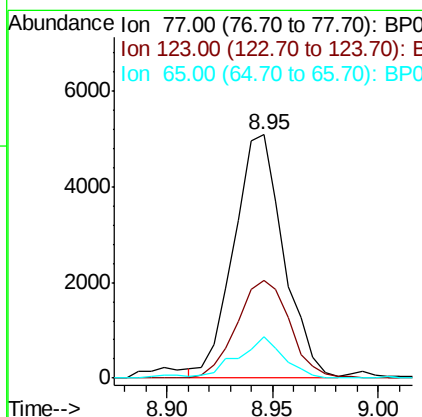







#21
Isophorone
Concen: 3.748 ng/ul
RT: 9.47 min Scan# 1086
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
82	100		
95	10.7	6.6	9.8#
138	16.7	14.6	22.0




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

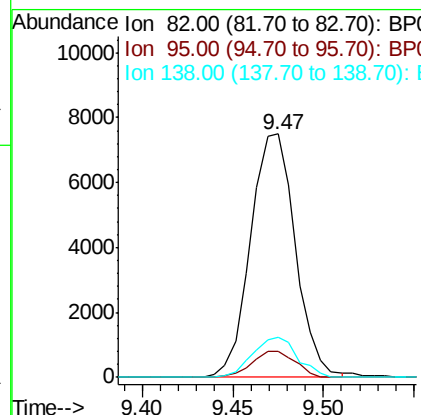

#23
2-Nitrophenol
Concen: 3.936 ng/ul
RT: 9.66 min Scan# 1117
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
139	100		
65	58.2	49.4	74.2
109	42.3	37.1	55.7

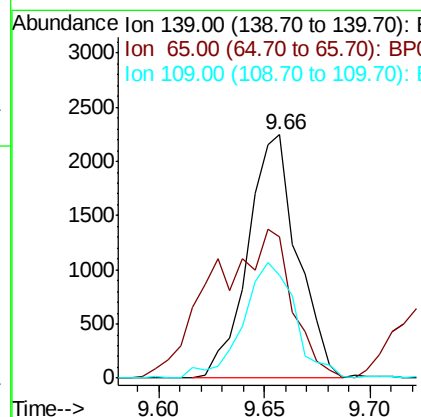



#24

2,4-Dimethylphenol

Concen: 3.765 ng/ul

RT: 9.72 min Scan# 1127

Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-01

Tot Ion:	107	Resp:	7821
Ion Ratio	Lower	Upper	
107	100		
121	45.2	37.1	55.7
122	71.6	61.8	92.8

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

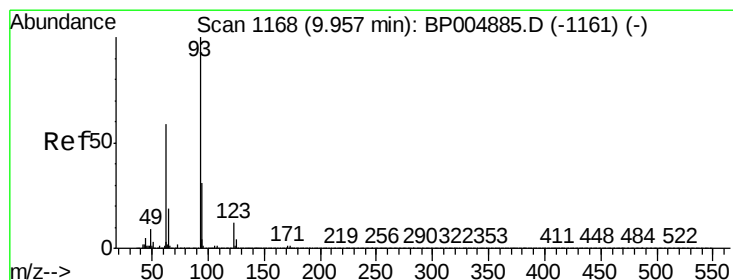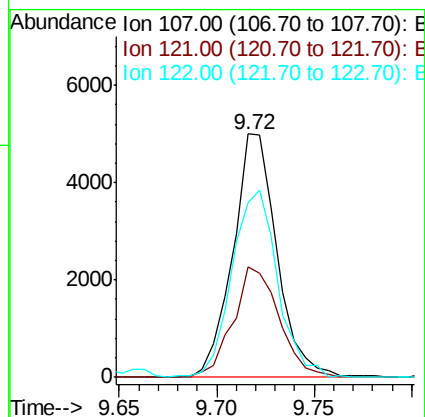

#25

Bis(2-Chloroethoxy)methane

Concen: 3.920 ng/ul




RT: 9.96 min Scan# 1168


Delta R.T. 0.00 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:	93	Resp:	8132
Ion Ratio	Lower	Upper	
93	100		
95	39.1	24.3	36.5#
123	10.4	8.6	13.0

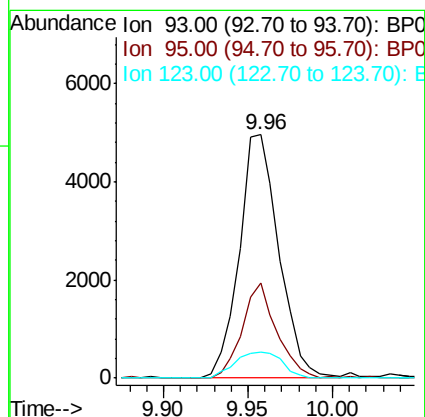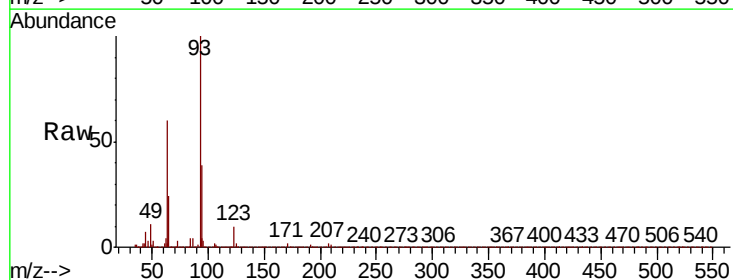







#27
2,4-Dichlorophenol
Concen: 3.999 ng/ul
RT: 10.19 min Scan# 1207
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
162	100		
164	89.0	51.8	77.6#
98	41.9	32.0	48.0




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#28
Naphthalene
Concen: 3.899 ng/ul
RT: 10.59 min Scan# 1275
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
128	100		
129	9.4	9.0	13.6
127	14.2	11.4	17.2









#30
4-Chloroaniline
Concen: 4.467 ng/ul
RT: 10.70 min Scan# 1294
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
127	100		
129	31.0	25.6	38.4




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

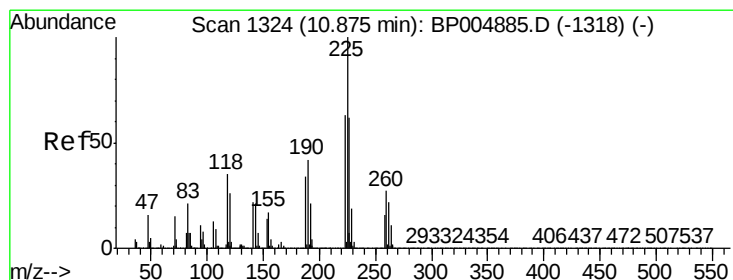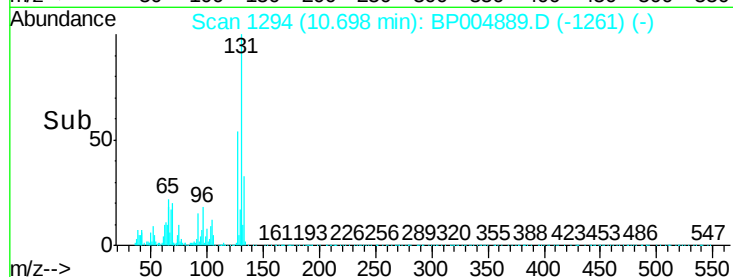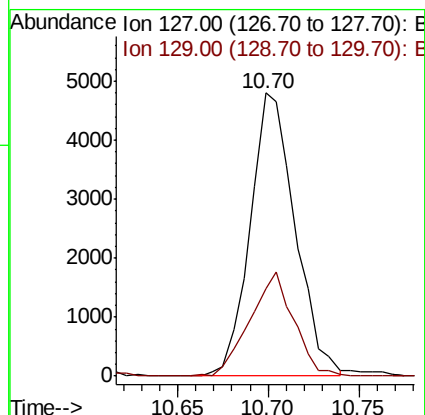

#31
Hexachlorobutadiene
Concen: 4.128 ng/ul
RT: 10.87 min Scan# 1323
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
225	100		
223	64.8	51.2	76.8
227	66.5	51.4	77.2

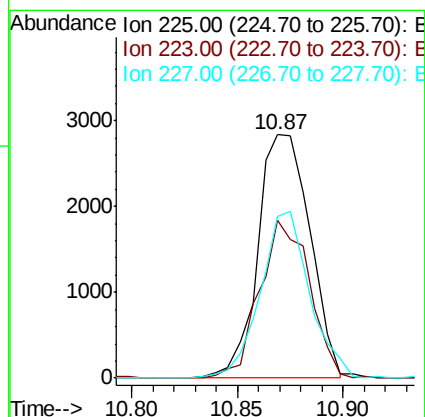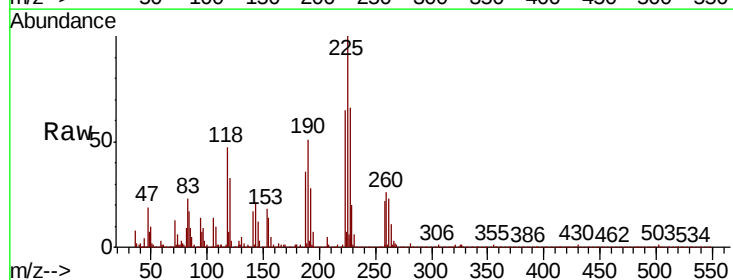







#32
 Caprolactam
 Concen: 3.588 ng/ul
 RT: 11.52 min Scan# 1433
 Delta R.T. 0.03 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Tot Ion:	113	Resp:	1886
Ion Ratio	Lower	Upper	
113	100		
55	76.4	69.5	104.3
56	72.3	65.8	98.6




Manual Integrations
 APPROVED


mohammad
 3/4/2021 11:33:19 AM

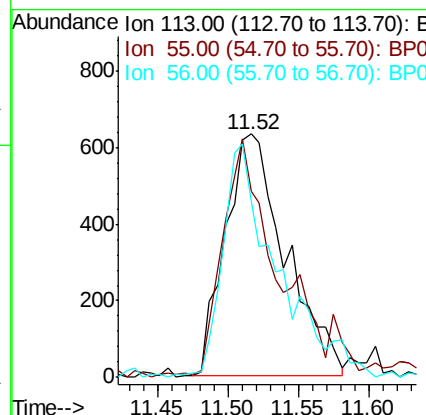

#33
 4-Chloro-3-methylphenol
 Concen: 3.510 ng/ul
 RT: 11.83 min Scan# 1487
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion:	107	Resp:	6467
Ion Ratio	Lower	Upper	
107	100		
144	26.1	17.3	25.9#
142	67.6	56.6	84.8

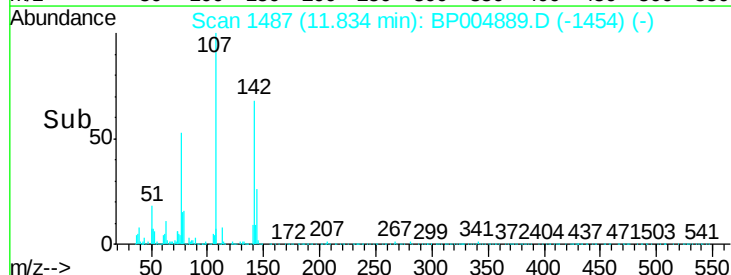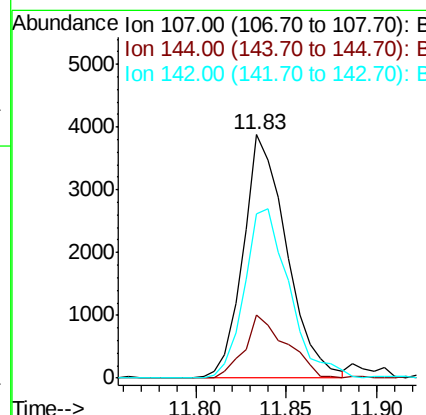







#34
2-Methylnaphthalene
Concen: 3.912 ng/ul
RT: 12.21 min Scan# 1551
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
142	100		
141	89.3	69.4	104.2




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

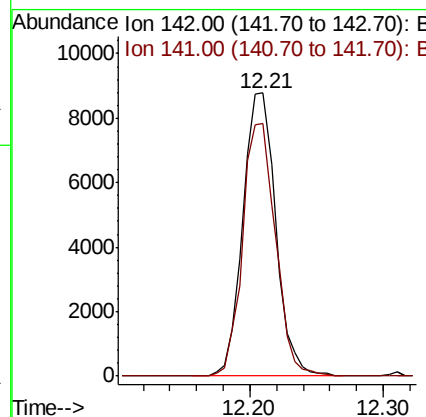

#35
1-Methylnaphthalene
Concen: 3.953 ng/ul
RT: 12.43 min Scan# 1588
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
142	100		
141	99.2	71.5	107.3
116	5.3	3.4	5.0#

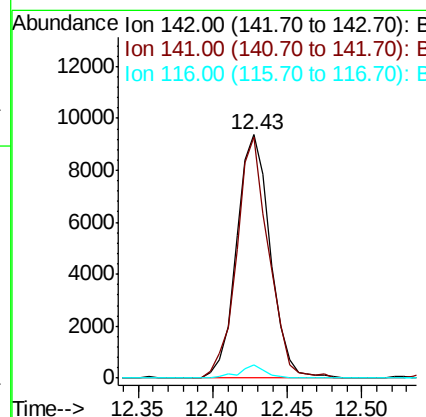




#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 4.365 ng/ul
 RT: 12.58 min Scan# 1614
 Delta R.T. 0.00 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01




Tot Ion	Ion	Ratio	Resp	Lower	Upper
216	100		9105		
214	74.2	62.3	93.5		
179	20.4	17.2	25.8		
108	18.1	15.5	23.3		

Manual Integrations
 APPROVED

mohammad
 3/4/2021 11:33:19 AM




Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E


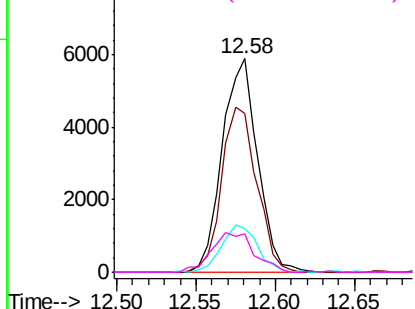



#38
 Hexachlorocyclopentadiene
 Concen: 3.461 ng/ul
 RT: 12.56 min Scan# 1610
 Delta R.T. 0.00 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
237	100		4600		
235	63.5	49.4	74.0		
272	8.8	10.6	15.8#		



Abundance Ion 237.00 (236.70 to 237.70): E
 Ion 235.00 (234.70 to 235.70): E
 Ion 272.00 (271.70 to 272.70): E

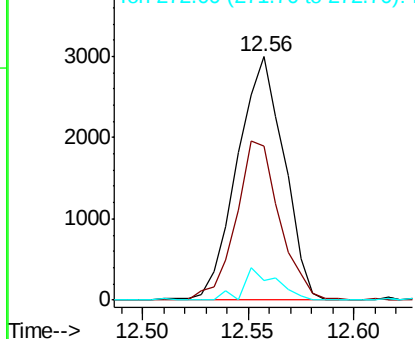







#39
2,4,6-Trichlorophenol
Concen: 3.578 ng/ul
RT: 12.82 min Scan# 1655
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Resp	Lower	Upper
196	100	4675		
198	110.6	78.0	117.0	
200	40.3	23.8	35.8	




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

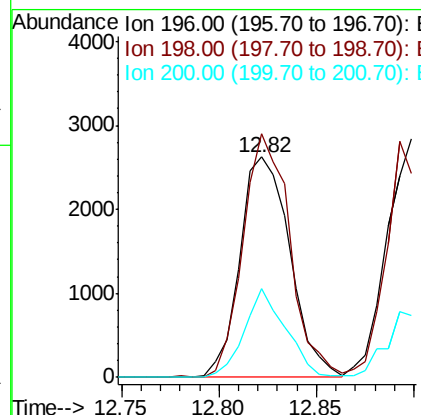

#40
2,4,5-Trichlorophenol
Concen: 3.742 ng/ul
RT: 12.90 min Scan# 1668
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Resp	Lower	Upper
196	100	5239		
198	85.2	72.8	109.2	
200	26.1	23.7	35.5	

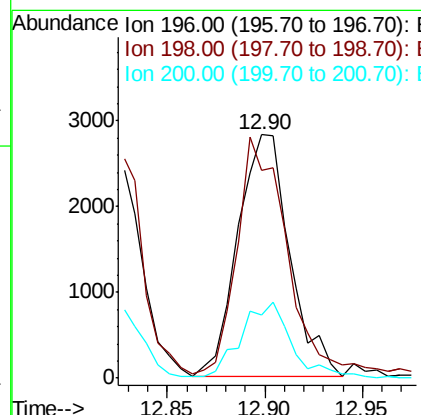







#41
1,1'-Biphenyl
Concen: 4.189 ng/ul
RT: 13.23 min Scan# 1724
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion:	154	Resp:	20405
Ion Ratio	Lower	Upper	
154	100		
153	37.4	33.2	49.8
76	11.7	9.8	14.6




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#42
2-Chloronaphthalene
Concen: 4.105 ng/ul
RT: 13.27 min Scan# 1731
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion:	162	Resp:	15715
Ion Ratio	Lower	Upper	
162	100		
164	34.2	25.7	38.5
127	43.3	33.5	50.3

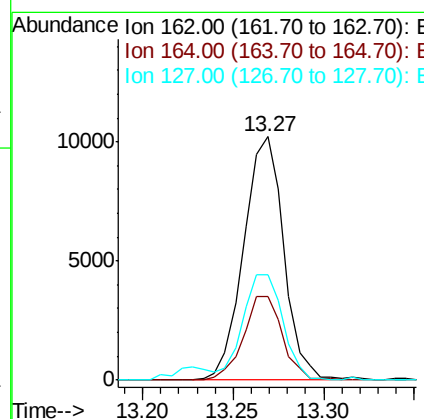







#43
2-Nitroaniline
Concen: 3.424 ng/ul
RT: 13.48 min Scan# 1767
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
65	100		
92	67.4	55.3	82.9
138	102.2	79.0	118.6




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

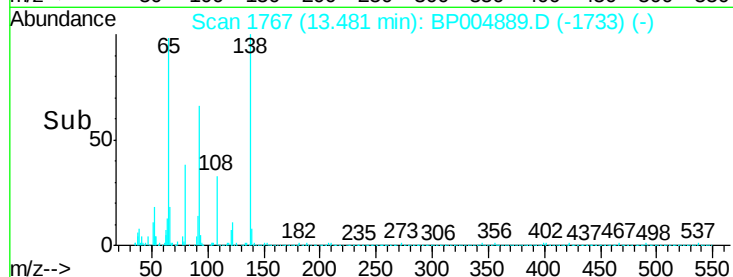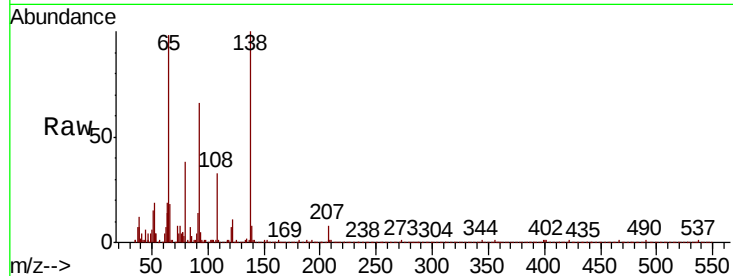

#45
Dimethylphthalate
Concen: 4.128 ng/ul
RT: 13.86 min Scan# 1831
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.8	3.8	5.6
164	10.4	7.8	11.8

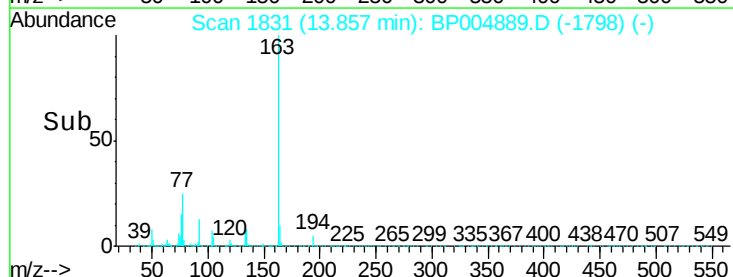







#46
2,6-Dinitrotoluene
Concen: 3.419 ng/ul
RT: 13.97 min Scan# 1851
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
165	100		
89	66.2	54.3	81.5
121	21.1	18.2	27.2




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

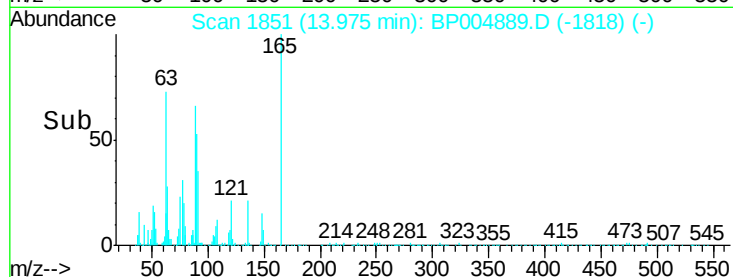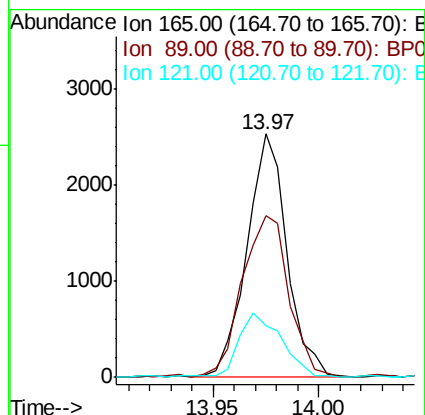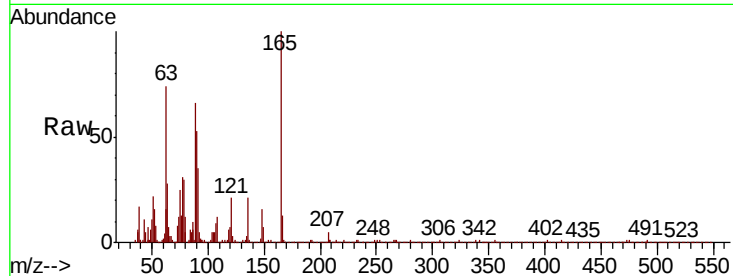

#48
Acenaphthylene
Concen: 4.050 ng/ul
RT: 14.12 min Scan# 1875
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
152	100		
151	22.0	15.7	23.5
153	12.7	10.2	15.4

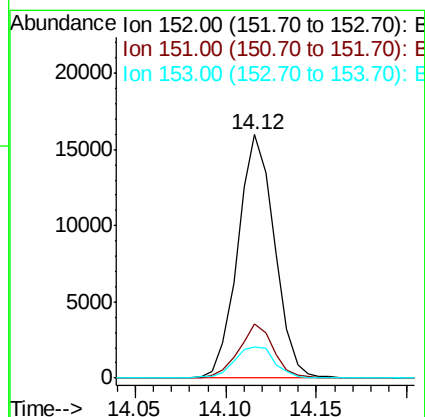







#49
3-Nitroaniline
Concen: 3.866 ng/ul
RT: 14.32 min Scan# 1909
Delta R.T. 0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
138	100		
108	9.4	10.1	15.1#
92	91.0	99.7	149.5#




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#50
Acenaphthene
Concen: 4.281 ng/ul
RT: 14.46 min Scan# 1934
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
153	100		
152	42.5	38.7	58.1
154	88.2	72.2	108.2

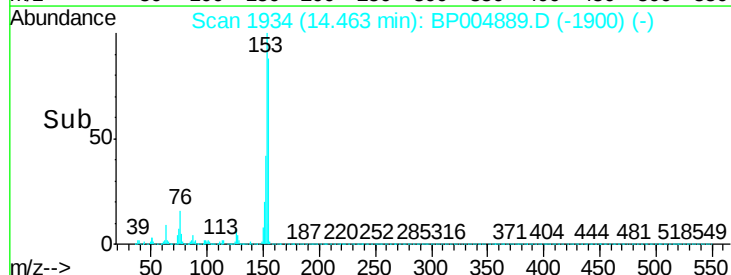







#51
2,4-Dinitrophenol
Concen: 2.678 ng/ul
RT: 14.52 min Scan# 1944
Delta R.T. 0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Resp	Lower	Upper
184	100	1685		
63	65.0	58.3	87.5	
154	68.5	52.0	78.0	




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

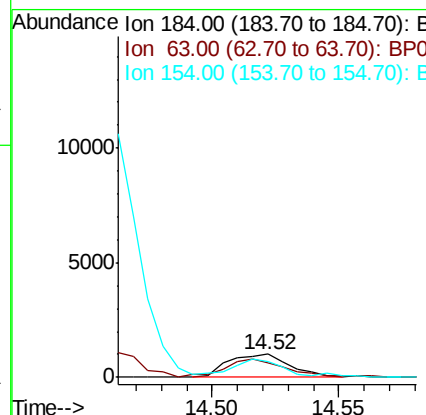

#53
4-Nitrophenol
Concen: 4.251 ng/ul
RT: 14.63 min Scan# 1962
Delta R.T. 0.00 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Resp	Lower	Upper
109	100	3930		
139	80.6	77.6	116.4	
65	96.6	85.5	128.3	

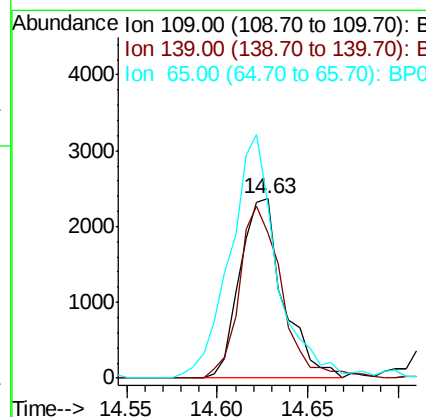







#54
Dibenzofuran
Concen: 4.234 ng/ul
RT: 14.80 min Scan# 1991
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
168	100		
139	39.7	32.6	48.8




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

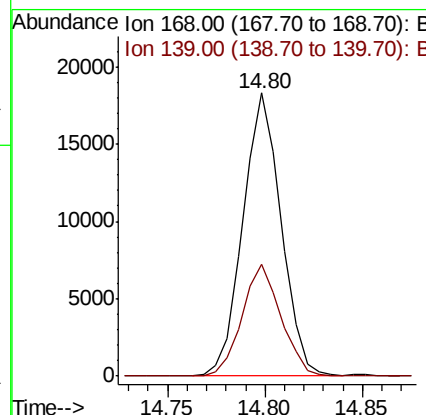

#55
2,4-Dinitrotoluene
Concen: 3.763 ng/ul
RT: 14.76 min Scan# 1985
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
165	100		
63	58.4	42.2	63.2
182	1.3	3.0	4.4#

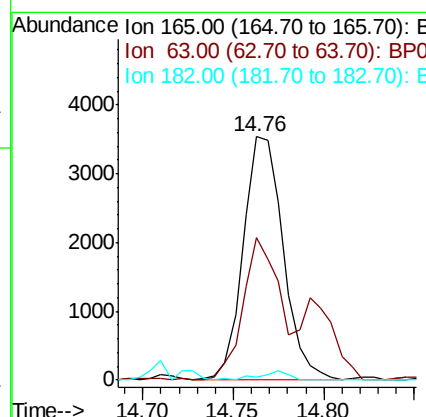







#56
 2,3,4,6-Tetrachlorophenol
 Concen: 3.863 ng/ul
 RT: 15.03 min Scan# 2030
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Tot Ion:	232	Resp:	4776
Ion Ratio	Lower	Upper	
232	100		
131	50.8	38.2	57.4
130	3.1	2.5	3.7
166	27.8	26.6	40.0




Manual Integrations
 APPROVED


mohammad
 3/4/2021 11:33:19 AM

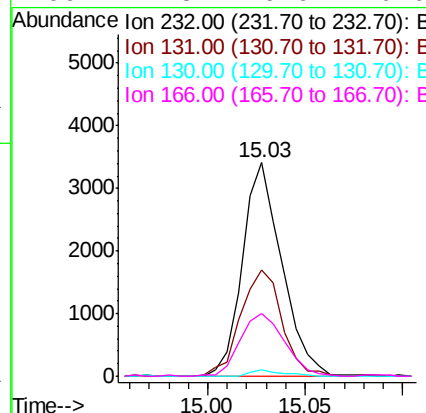

#57
 Diethylphthalate
 Concen: 4.104 ng/ul
 RT: 15.23 min Scan# 2064
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion:	149	Resp:	20305
Ion Ratio	Lower	Upper	
149	100		
177	21.2	18.4	27.6
150	11.2	10.7	16.1

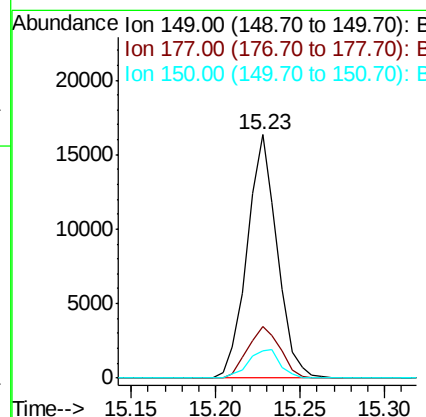



#59

Fluorene

Concen: 4.058 ng/ul

RT: 15.45 min Scan# 2102

Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-01

Tot Ion:	166	Resp:	19844
Ion Ratio	Lower	Upper	
166	100		
165	100.1	75.2	112.8
167	13.0	10.8	16.2

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

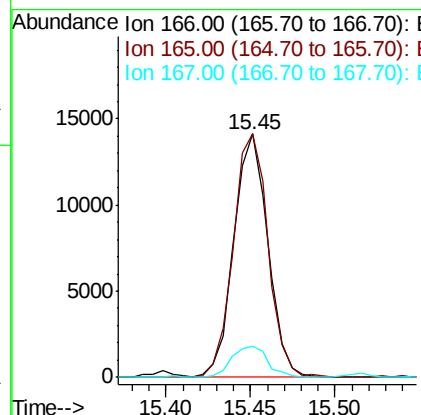

#60

4-Chlorophenyl-phenylether

Concen: 4.164 ng/ul




RT: 15.45 min Scan# 2101


Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:	204	Resp:	10726
Ion Ratio	Lower	Upper	
204	100		
206	33.0	26.3	39.5
141	66.2	48.2	72.2

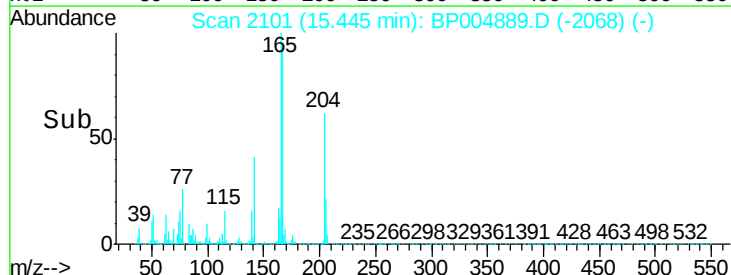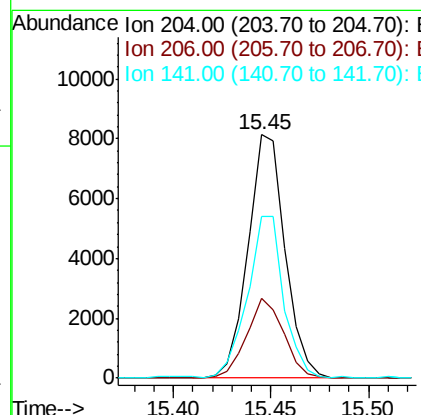







#61
4-Nitroaniline
Concen: 3.298 ng/ul
RT: 15.47 min Scan# 2106
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
138	100		
92	73.2	46.1	69.1#
108	133.0	94.0	141.0




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

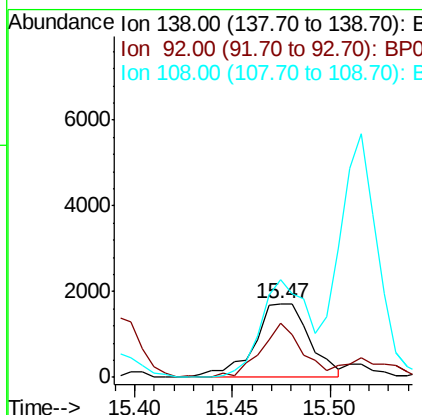

#64
4,6-Dinitro-2-methylphenol
Concen: 3.819 ng/ul
RT: 15.53 min Scan# 2115
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
198	100		
182	8.0	4.0	6.0#
77	47.9	23.9	35.9#

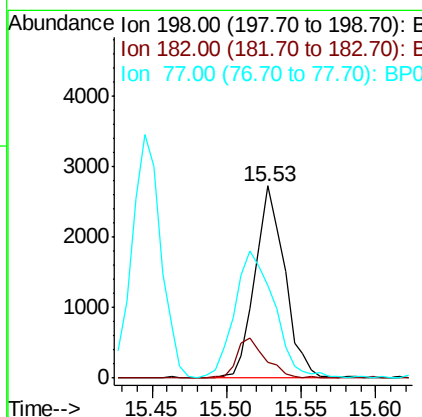







#65
N-Nitrosodiphenylamine
Concen: 3.906 ng/ul
RT: 15.66 min Scan# 2138
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
169	100		
168	68.3	54.1	81.1
167	34.6	29.0	43.4




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

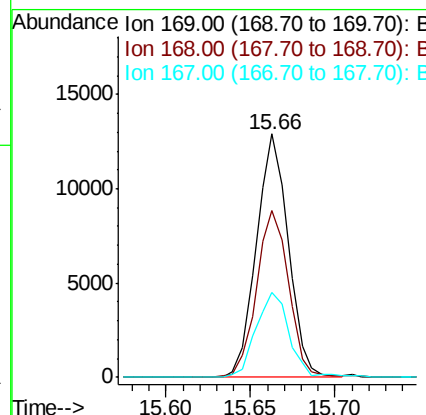

#66
4-Bromophenyl-phenylether
Concen: 3.813 ng/ul m
RT: 16.35 min Scan# 2254
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
248	100		
250	116.3	76.1	114.1#
141	91.4	69.9	104.9

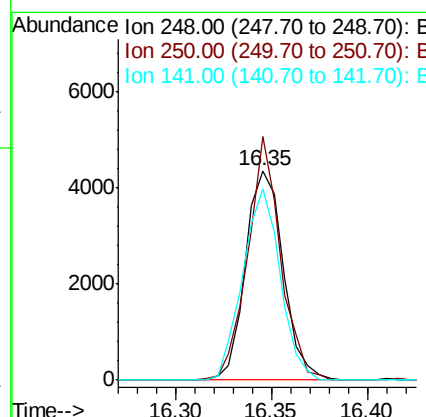







#67
Hexachlorobenzene
Concen: 4.123 ng/ul
RT: 16.46 min Scan# 2273
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
284	100		
142	33.2	33.6	50.4#
249	28.1	25.0	37.4




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#68
Atrazine
Concen: 3.335 ng/ul
RT: 16.62 min Scan# 2301
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
200	100		
173	29.9	21.2	31.8
215	53.6	38.3	57.5









#69
Pentachlorophenol
Concen: 2.826 ng/ul
RT: 16.80 min Scan# 2332
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
266	100		
264	72.9	49.6	74.4
268	67.5	52.6	78.8




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#70
Phenanthrene
Concen: 4.055 ng/ul
RT: 17.20 min Scan# 2399
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.3	12.6	18.8
176	16.0	14.6	21.8

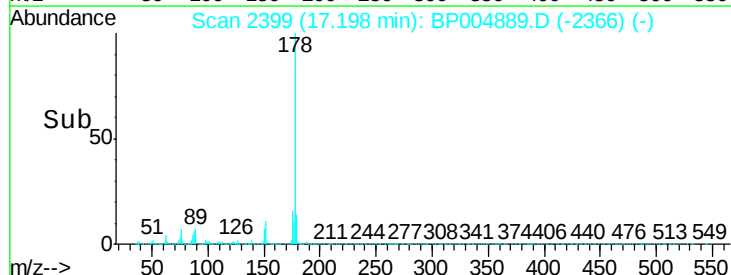



#72

Anthracene

Concen: 3.964 ng/ul

RT: 17.29 min Scan# 2414

Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-01

Tot Ion:	178	Resp:	32632
Ion Ratio	Lower	Upper	
178	100		
179	16.1	11.8	17.8
176	19.4	14.3	21.5

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

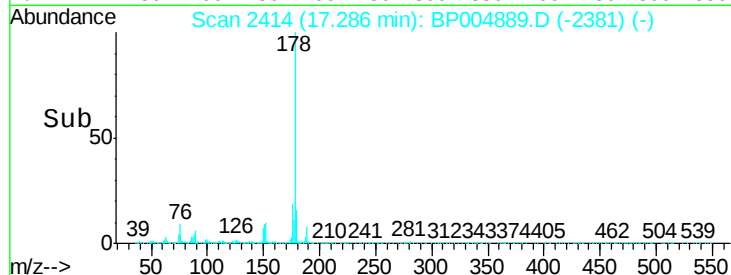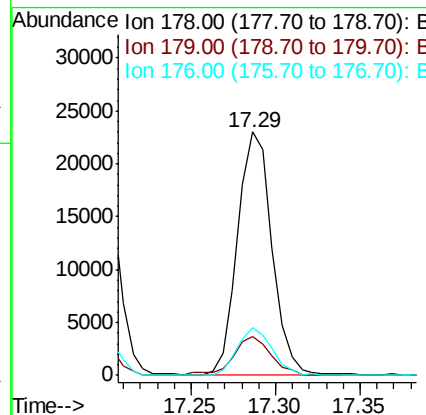

#73

1,2,3,4-Tetrachlorobenzene

Concen: 4.115 ng/uL m




RT: 13.19 min Scan# 1717


Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:	216	Resp:	9091
Ion Ratio	Lower	Upper	
216	100		
214	70.8	60.6	90.8
218	57.9	36.6	55.0#

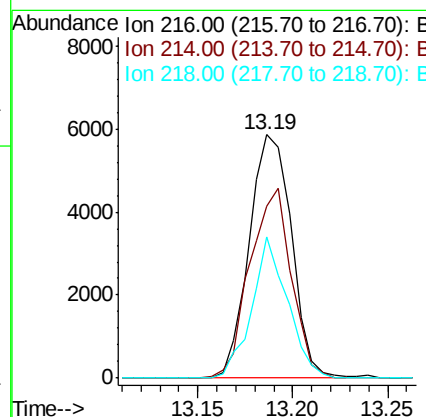







#74
Pentachlorobenzene
Concen: 3.873 ng/uL
RT: 14.72 min Scan# 1977
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
250	100		
248	66.3	50.5	75.7
252	75.9	49.5	74.3




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#75
Carbazole
Concen: 3.635 ng/uL
RT: 17.56 min Scan# 2461
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
167	100		
166	25.3	17.5	26.3
139	16.0	10.9	16.3









#76
Di-n-butylphthalate
Concen: 3.454 ng/ul
RT: 18.12 min Scan# 2556
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
149	100		
150	8.2	7.0	10.4
104	6.0	5.0	7.6




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

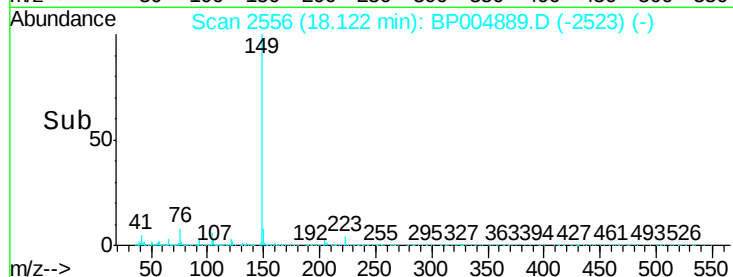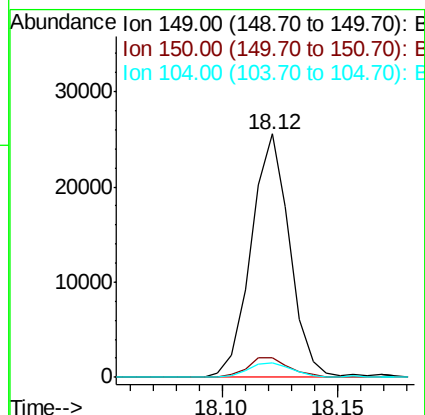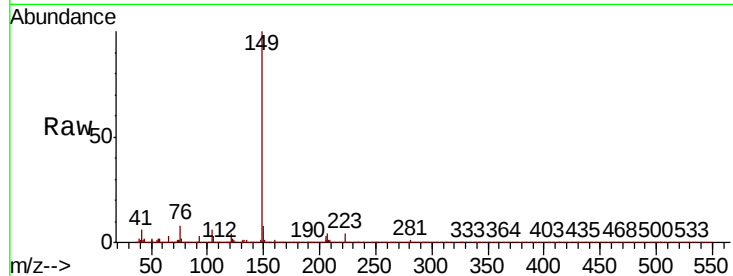

#77
Fluoranthene
Concen: 3.894 ng/ul
RT: 19.17 min Scan# 2734
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
202	100		
101	6.9	7.5	11.3#
100	5.4	5.9	8.9#

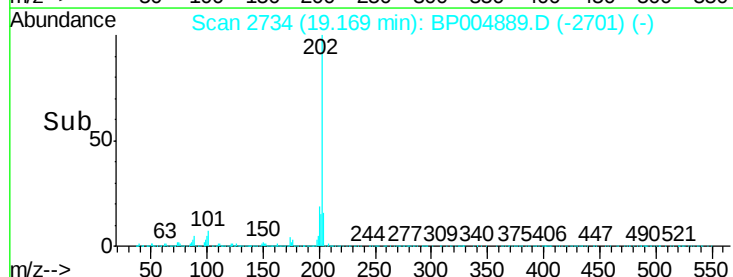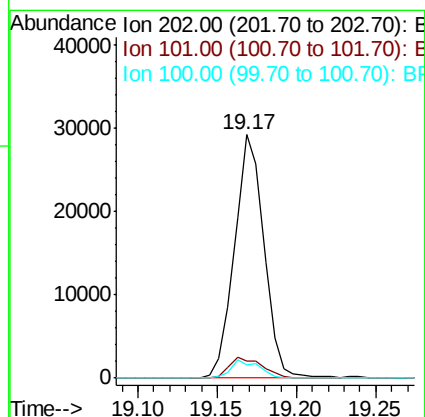







#80
Pvrene
Concen: 4.027 ng/ul
RT: 19.52 min Scan# 2794
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion:	202	Resp:	41262
Ion Ratio	Lower	Upper	
202	100		
101	11.6	8.6	13.0
100	9.0	6.9	10.3




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM

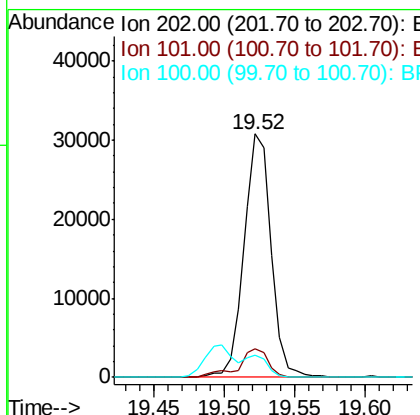

#81
Butylbenzylphthalate
Concen: 3.272 ng/ul
RT: 20.40 min Scan# 2943
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion:	149	Resp:	13083
Ion Ratio	Lower	Upper	
149	100		
91	84.6	62.0	93.0
206	23.9	19.0	28.6

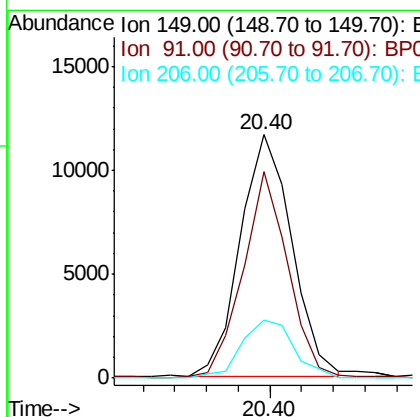







#82
 3,3'-Dichlorobenzidine
 Concen: 3.738 ng/ul
 RT: 21.17 min Scan# 3074
 Delta R.T. 0.00 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
252	100		
254	64.1	50.8	76.2
126	11.8	7.7	11.5




Manual Integrations
 APPROVED


mohammad
 3/4/2021 11:33:19 AM



#83
 Benzo(a)anthracene
 Concen: 3.990 ng/ul
 RT: 21.23 min Scan# 3084
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.4	15.4	23.0
226	25.3	21.1	31.7









#84
 Bis(2-ethylhexyl)phthalate
 Concen: 3.311 ng/ul
 RT: 21.16 min Scan# 3072
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
149	100		
167	27.9	23.0	34.6
279	5.4	4.1	6.1




Manual Integrations
 APPROVED


mohammad
 3/4/2021 11:33:19 AM



#85
 Chrysene
 Concen: 4.144 ng/ul
 RT: 21.27 min Scan# 3092
 Delta R.T. -0.01 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
228	100		
226	24.7	23.3	34.9
229	18.8	15.6	23.4





#87

Di-n-octyl phthalate

Concen: 3.030 ng/ul

RT: 22.04 min Scan# 3223

Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P


ClientSampleId :

MDL-WATER-01




Tgt Ion:149 Resp: 34418

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM



Abundance Ion 149.00 (148.70 to 149.70): E

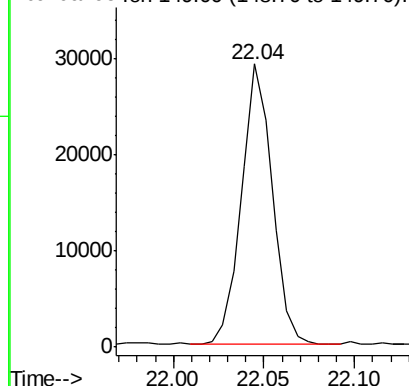

#88

Benzo(b)fluoranthene

Concen: 4.061 ng/ul

RT: 22.84 min Scan# 3358


Delta R.T. -0.01 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Tgt Ion:252 Resp: 43563



Ion	Ratio	Lower	Upper
252	100		
253	20.6	17.6	26.4
125	8.3	6.5	9.7




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

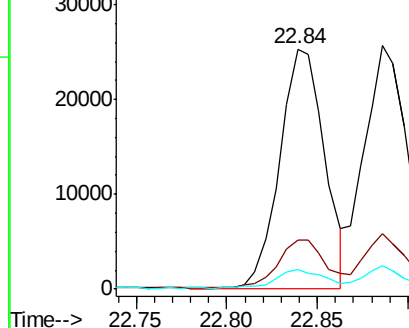







#89
Benzo(k)fluoranthene
Concen: 4.030 ng/ul
RT: 22.89 min Scan# 3366
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-01

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.9	17.6	26.4
125	9.5	6.5	9.7




Manual Integrations
APPROVED


mohammad
3/4/2021 11:33:19 AM



#91
Benzo(a)pyrene
Concen: 4.196 ng/ul
RT: 23.44 min Scan# 3460
Delta R.T. -0.01 min
Lab File: BP004889.D
Acq: 03 Mar 2021 12:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.4	16.9	25.3
125	10.5	6.9	10.3#









#92
 Indeno(1,2,3-cd)pyrene
 Concen: 3.989 ng/ul
 RT: 25.90 min Scan# 3878
 Delta R.T. -0.02 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-01

Tot Ion:	276	Resp:	48087
Ion Ratio	Lower	Upper	
276	100		
138	19.0	16.5	24.7
277	23.8	19.1	28.7




Manual Integrations
 APPROVED


mohammad
 3/4/2021 11:33:19 AM

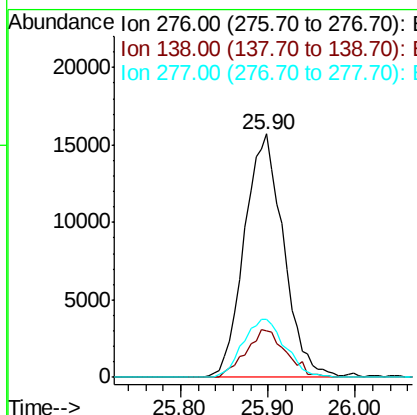

#93
 Dibenzo(a,h)anthracene
 Concen: 4.043 ng/ul
 RT: 25.91 min Scan# 3880
 Delta R.T. -0.02 min
 Lab File: BP004889.D
 Acq: 03 Mar 2021 12:19

Tgt Ion:	278	Resp:	41450
Ion Ratio	Lower	Upper	
278	100		
139	14.3	10.6	16.0
279	24.2	20.0	30.0

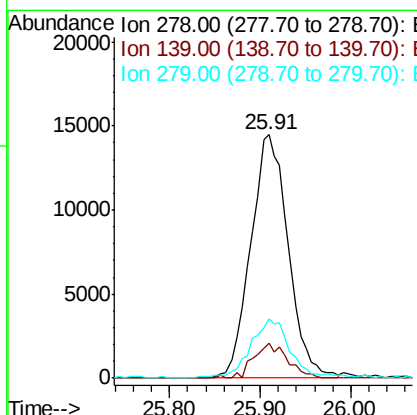



#94

Benzo(a,h,i)perylene

Concen: 3.927 ng/ul

RT: 26.62 min Scan# 4000

Delta R.T. -0.02 min

Lab File: BP004889.D

Acq: 03 Mar 2021 12:19

Instrument :

BNA_P

ClientSampleId :

MDL-WATER-01

Tot Ion:	276	Resp:	39410
Ion Ratio	Lower	Upper	
276	100		
138	17.6	13.8	20.6
277	23.7	18.5	27.7

Manual Integrations
APPROVED

mohammad
3/4/2021 11:33:19 AM

