

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
 Data File : BP009261.D
 Acq On : 04 Mar 2022 09:55
 Operator : CG/JU
 Sample : PB142853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	30	rVB	101169	183519	2.44%	0.246%
2	3.323	53	57	69	rVB	84285	141948	1.89%	0.190%
3	3.723	121	125	146	rBV	935296	1540023	20.48%	2.061%
4	4.052	179	181	189	rVB3	24970	29915	0.40%	0.040%
5	6.987	673	680	693	rBV	1171757	1984252	26.39%	2.656%
6	7.158	702	709	722	rBV	912763	1563097	20.79%	2.092%
7	7.358	735	743	752	rBV	1168808	1999889	26.60%	2.676%
8	7.822	815	822	831	rBV	1025084	1723132	22.92%	2.306%
9	8.269	893	898	901	rVB6	7122	10903	0.15%	0.015%
10	8.528	934	942	957	rBV	1375915	2368373	31.50%	3.170%
11	8.634	957	960	970	rVB	9408	22052	0.29%	0.030%
12	8.905	1002	1006	1010	rBV6	5934	7573	0.10%	0.010%
13	8.975	1010	1018	1031	rBV	965557	1666065	22.16%	2.230%
14	9.699	1133	1141	1152	rBV	684118	1186082	15.78%	1.587%
15	9.793	1154	1157	1164	rVB8	6694	13026	0.17%	0.017%
16	10.034	1193	1198	1204	rVB9	4832	8812	0.12%	0.012%
17	10.234	1223	1232	1246	rBV	1332399	2362240	31.42%	3.161%
18	10.616	1284	1297	1305	rBV	1361386	2439833	32.45%	3.265%
19	10.752	1312	1320	1334	rBV	1364627	2455526	32.66%	3.286%
20	10.969	1353	1357	1361	rBV7	6537	10095	0.13%	0.014%
21	11.899	1510	1515	1520	rBV9	4863	8066	0.11%	0.011%
22	12.210	1561	1568	1573	rBV	24542	45058	0.60%	0.060%
23	12.281	1576	1580	1587	rVB4	9994	16457	0.22%	0.022%
24	12.422	1600	1604	1609	rBV8	4097	7621	0.10%	0.010%
25	12.505	1609	1618	1627	rVB4	10754	22427	0.30%	0.030%
26	12.652	1636	1643	1649	rBV9	11184	23629	0.31%	0.032%
27	12.957	1690	1695	1699	rVB7	5521	8221	0.11%	0.011%
28	13.257	1740	1746	1749	rVV6	11049	20553	0.27%	0.028%
29	13.299	1749	1753	1756	rVV3	12752	21284	0.28%	0.028%
30	13.340	1756	1760	1763	rVB4	9647	15272	0.20%	0.020%
31	13.875	1843	1851	1863	rBV	2498372	3532641	46.99%	4.728%
32	14.151	1889	1898	1910	rBV	2668042	4276508	56.88%	5.723%
33	14.463	1941	1951	1958	rBV	2093545	3248854	43.21%	4.348%
34	14.522	1958	1961	1967	rVB2	12566	20510	0.27%	0.027%
35	14.646	1974	1982	1998	rBV	969274	1459014	19.41%	1.953%
36	14.781	2002	2005	2010	rVV7	7881	12167	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
 Data File : BP009261.D
 Acq On : 04 Mar 2022 09:55
 Operator : CG/JU
 Sample : PB142853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

37	14.863	2015	2019	2024	rVB3	12194	21370	0.28%	0.029%
38	15.093	2053	2058	2062	rBV8	5007	9393	0.12%	0.013%
39	15.298	2088	2093	2098	rBV5	8790	15424	0.21%	0.021%
40	15.457	2113	2120	2127	rBV	3434842	5362969	71.33%	7.177%
41	15.510	2127	2129	2133	rVV3	25808	33973	0.45%	0.045%
42	15.569	2133	2139	2150	rVB	672006	964594	12.83%	1.291%
43	15.698	2157	2161	2171	rVB6	17658	41394	0.55%	0.055%
44	16.128	2231	2234	2236	rBV4	7090	8910	0.12%	0.012%
45	16.251	2251	2255	2258	rBV5	6506	9346	0.12%	0.013%
46	16.410	2279	2282	2286	rBV5	7913	10097	0.13%	0.014%
47	16.528	2297	2302	2309	rVB10	11718	19347	0.26%	0.026%
48	16.687	2326	2329	2333	rVB5	8458	12339	0.16%	0.017%
49	16.869	2357	2360	2363	rBV5	6259	9641	0.13%	0.013%
50	17.004	2379	2383	2388	rBV4	11056	14470	0.19%	0.019%
51	17.222	2413	2420	2430	rBV	2573250	3884330	51.66%	5.198%
52	17.322	2430	2437	2452	rVV	3912843	5929505	78.87%	7.935%
53	17.628	2485	2489	2494	rVB3	10593	15655	0.21%	0.021%
54	18.198	2582	2586	2588	rBV2	11971	15586	0.21%	0.021%
55	19.145	2742	2747	2752	rBV2	54001	87686	1.17%	0.117%
56	19.210	2754	2758	2761	rBV	55401	77566	1.03%	0.104%
57	19.563	2812	2818	2828	rBV	5053460	7226088	96.11%	9.671%
58	21.328	3113	3118	3127	rBV	3272658	4387655	58.36%	5.872%
59	23.575	3493	3500	3513	rVB2	3638863	7518384	100.00%	10.062%
60	23.733	3520	3527	3537	rVB2	2128374	4591448	61.07%	6.145%




Sum of corrected areas: 74721807

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009261.D
Acq On : 04 Mar 2022 09:55
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

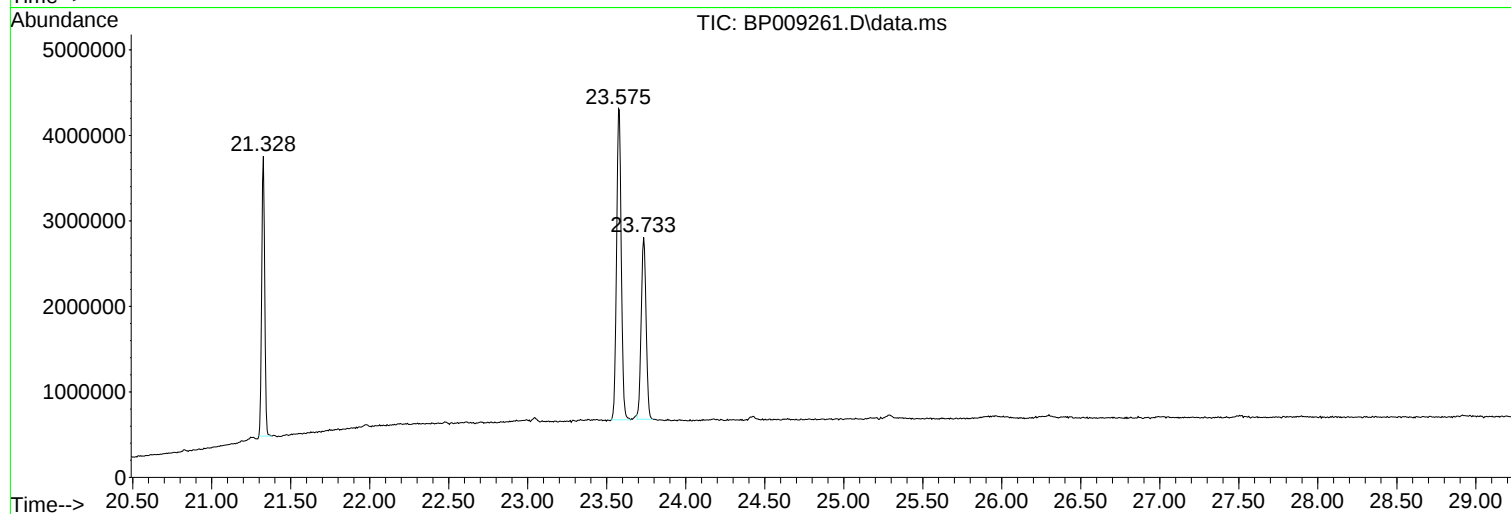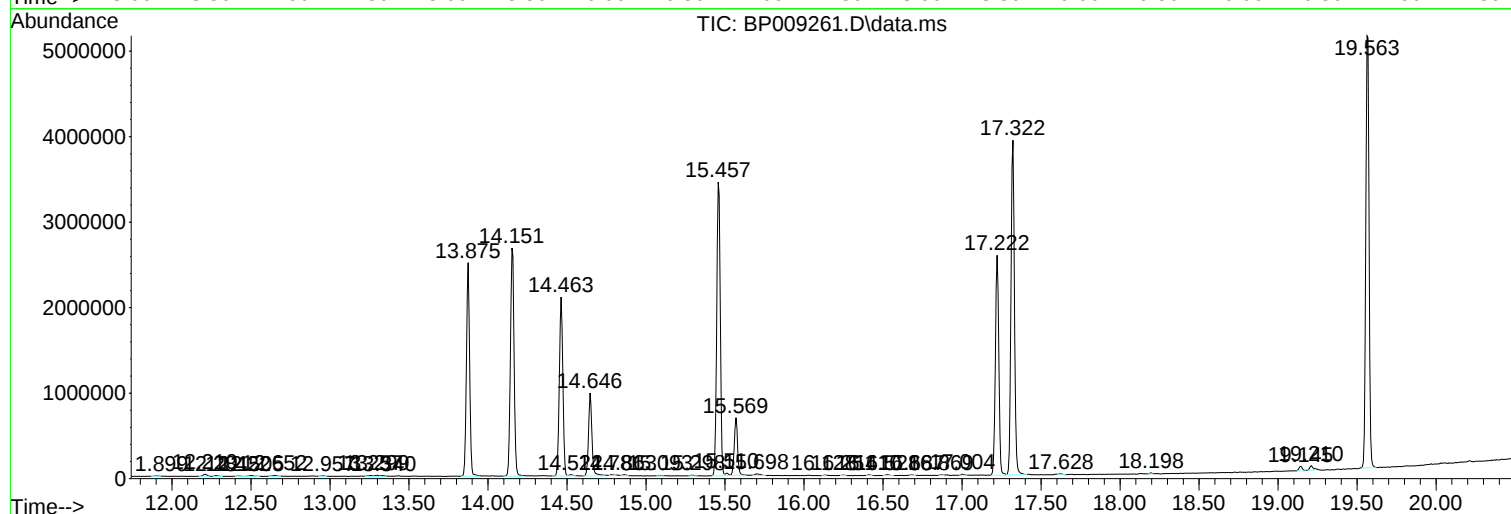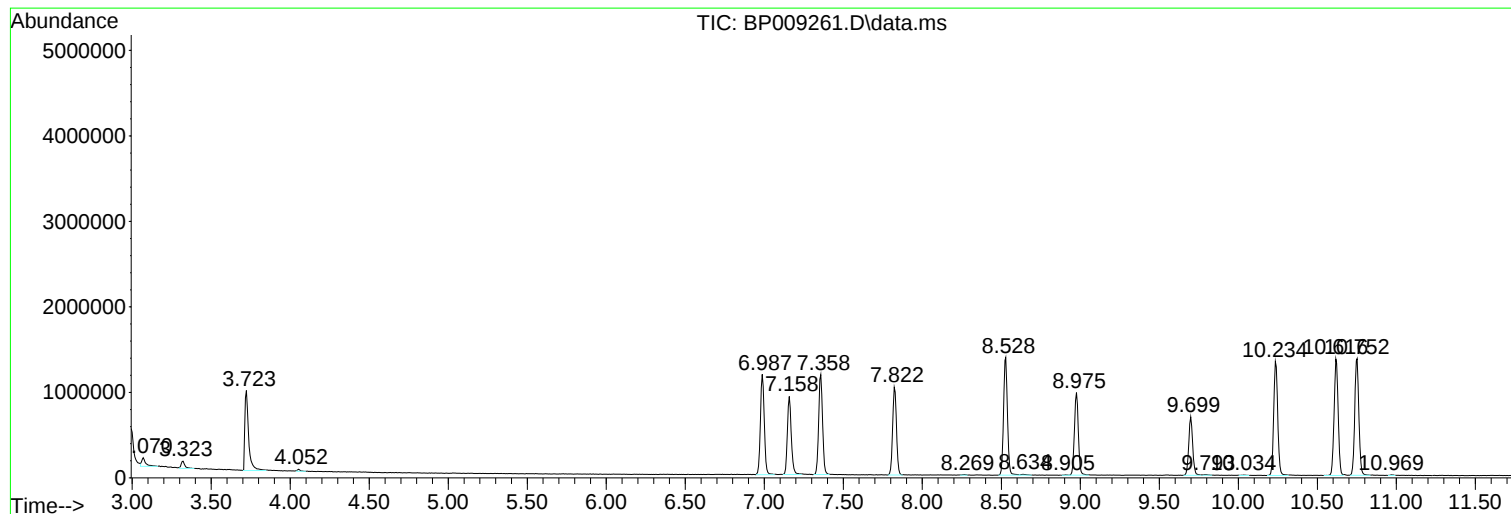

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009261.D
Acq On : 04 Mar 2022 09:55
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.070	2.13 ng/ul	183519	1,4-Dichlorobenzene-d4	7.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	80		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	40		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

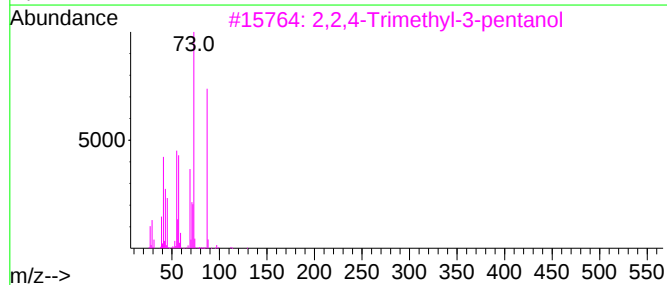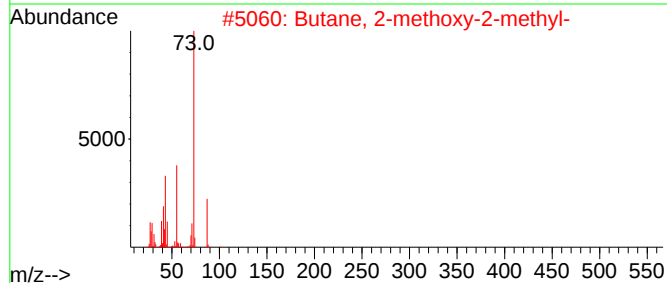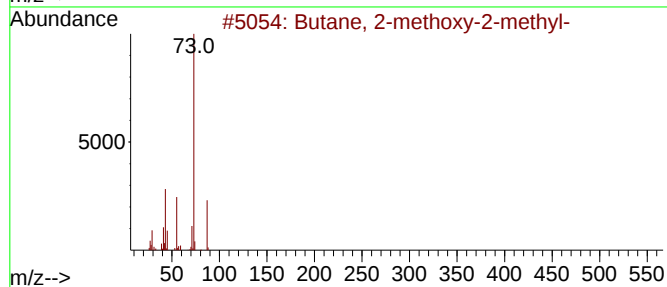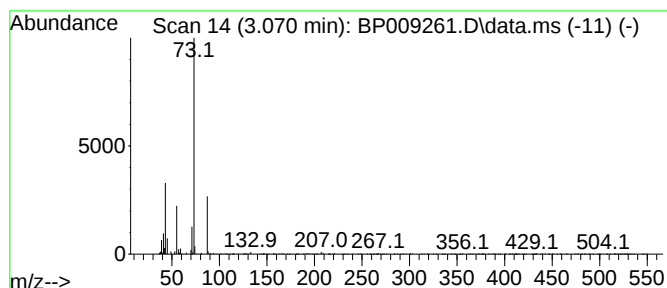

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009261.D
Acq On : 04 Mar 2022 09:55
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.070	2.1	ng/ul	183519	1	7.822	1723130	20.0