

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
 Data File : BP009263.D
 Acq On : 04 Mar 2022 11:28
 Operator : CG/JU
 Sample : PB142784BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK784

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	23	rVB	98520	148696	2.01%	0.197%
2	3.322	53	57	64	rVB	88951	129752	1.75%	0.172%
3	3.722	122	125	144	rBV	1036775	1651902	22.30%	2.188%
4	4.052	178	181	187	rVB2	20062	31671	0.43%	0.042%
5	6.993	673	681	691	rBV	1212417	2037181	27.51%	2.699%
6	7.163	703	710	724	rBV	919254	1640016	22.14%	2.172%
7	7.358	734	743	758	rVB	1247444	2115351	28.56%	2.802%
8	7.828	815	823	833	rBV	1085692	1823364	24.62%	2.415%
9	8.528	934	942	952	rBV	1407256	2458058	33.19%	3.256%
10	8.981	1011	1019	1031	rBV	984983	1725151	23.29%	2.285%
11	9.705	1134	1142	1154	rBV	703118	1220685	16.48%	1.617%
12	10.240	1224	1233	1248	rBV	1419616	2457386	33.18%	3.255%
13	10.622	1290	1298	1311	rBV	1400195	2525133	34.10%	3.345%
14	10.757	1313	1321	1331	rBV	1385850	2538830	34.28%	3.363%
15	12.216	1563	1569	1577	rVV3	28489	47343	0.64%	0.063%
16	12.434	1600	1606	1612	rBV3	5218	12518	0.17%	0.017%
17	13.204	1729	1737	1740	rBV8	5990	12321	0.17%	0.016%
18	13.263	1740	1747	1750	rVB8	4116	9189	0.12%	0.012%
19	13.440	1770	1777	1783	rBV6	5465	12438	0.17%	0.016%
20	13.881	1844	1852	1866	rBV	2506319	3627507	48.98%	4.805%
21	14.157	1892	1899	1911	rBV	2760845	4346681	58.69%	5.758%
22	14.469	1945	1952	1960	rBV	2161548	3336176	45.05%	4.419%
23	14.528	1960	1962	1967	rVB6	7296	9215	0.12%	0.012%
24	14.651	1976	1983	2000	rBV	939527	1459185	19.70%	1.933%
25	14.863	2017	2019	2026	rVB6	5976	9539	0.13%	0.013%
26	15.310	2089	2095	2098	rBV8	5801	10642	0.14%	0.014%
27	15.469	2114	2122	2129	rBV	3626487	5471888	73.88%	7.248%
28	15.575	2134	2140	2150	rBV	668248	992672	13.40%	1.315%
29	15.704	2158	2162	2172	rVB7	18534	39875	0.54%	0.053%
30	16.134	2233	2235	2241	rVB7	6576	10069	0.14%	0.013%
31	16.904	2363	2366	2371	rVB7	6097	10068	0.14%	0.013%
32	17.016	2379	2385	2390	rBV4	10831	19140	0.26%	0.025%
33	17.228	2414	2421	2431	rBV	2544554	3884020	52.44%	5.145%
34	17.328	2431	2438	2453	rBV2	3917070	5959956	80.47%	7.895%
35	17.610	2481	2486	2487	rBV5	5532	8939	0.12%	0.012%
36	18.133	2573	2575	2578	rBV4	6903	8510	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009263.D
Acq On : 04 Mar 2022 11:28
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Title : SVOA CALIBRATION

37	19.151	2744	2748	2752	rBV2	48290	66305	0.90%	0.088%
38	19.216	2755	2759	2766	rVV	50211	77838	1.05%	0.103%
39	19.575	2814	2820	2832	rVB	5168818	7143504	96.46%	9.463%
40	21.333	3114	3119	3126	rBV	3262561	4347308	58.70%	5.759%
41	23.592	3496	3503	3514	rVB	3637191	7406038	100.00%	9.810%
42	23.751	3523	3530	3543	rVB	2133169	4649411	62.78%	6.159%




Sum of corrected areas: 75491471

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009263.D
Acq On : 04 Mar 2022 11:28
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

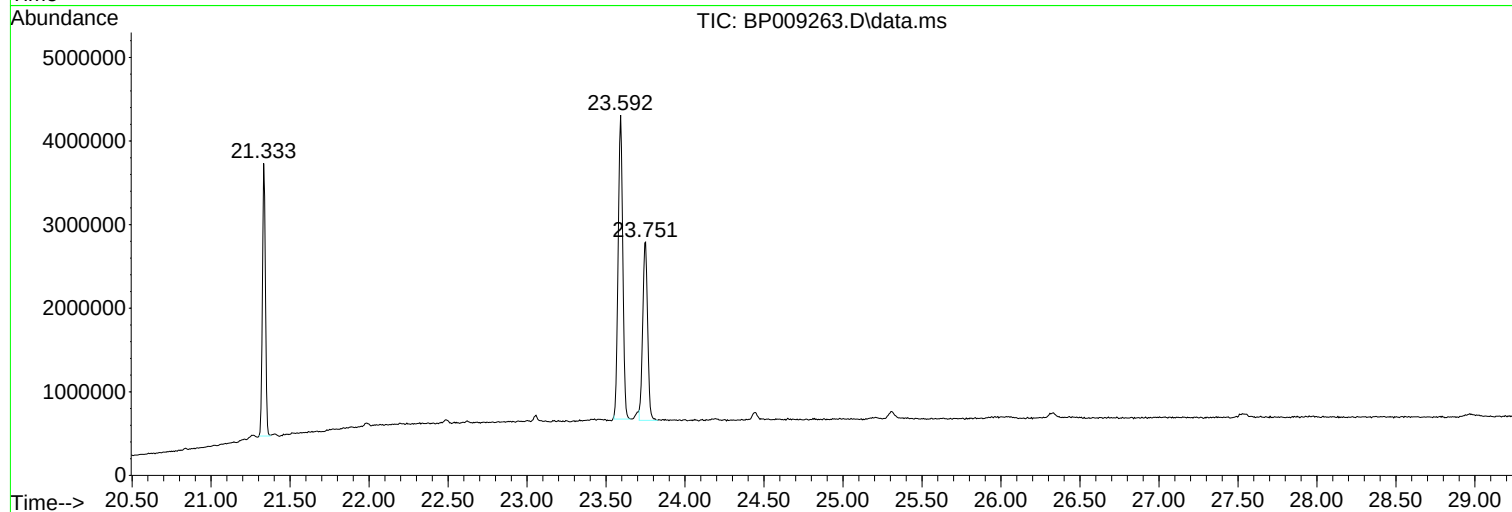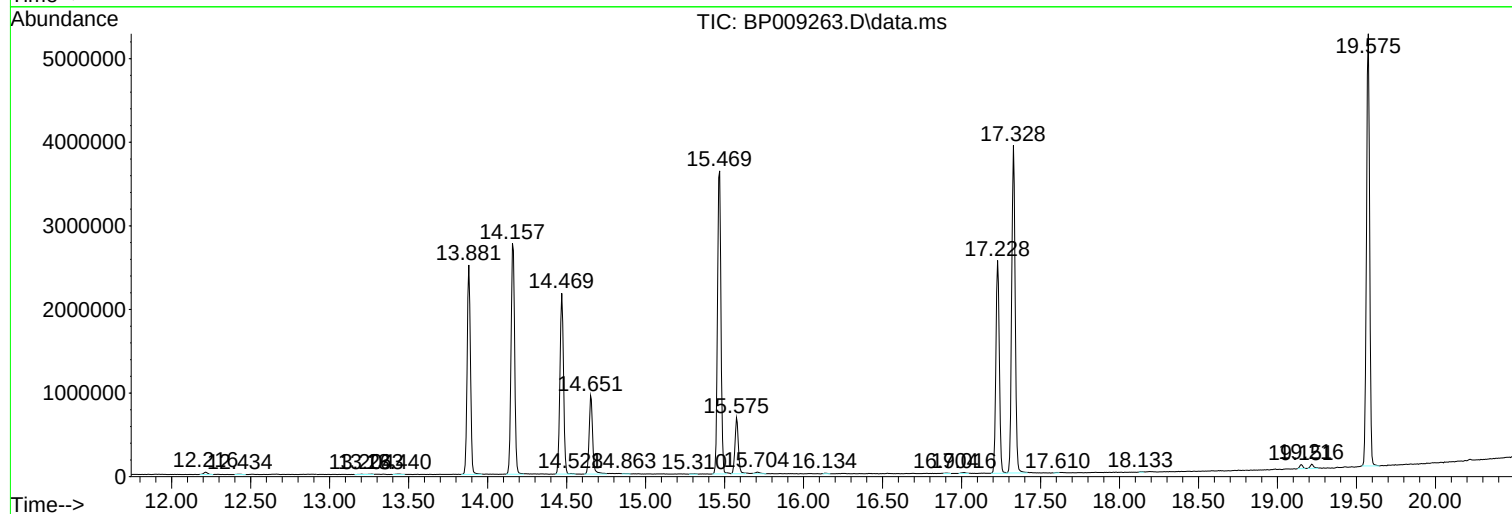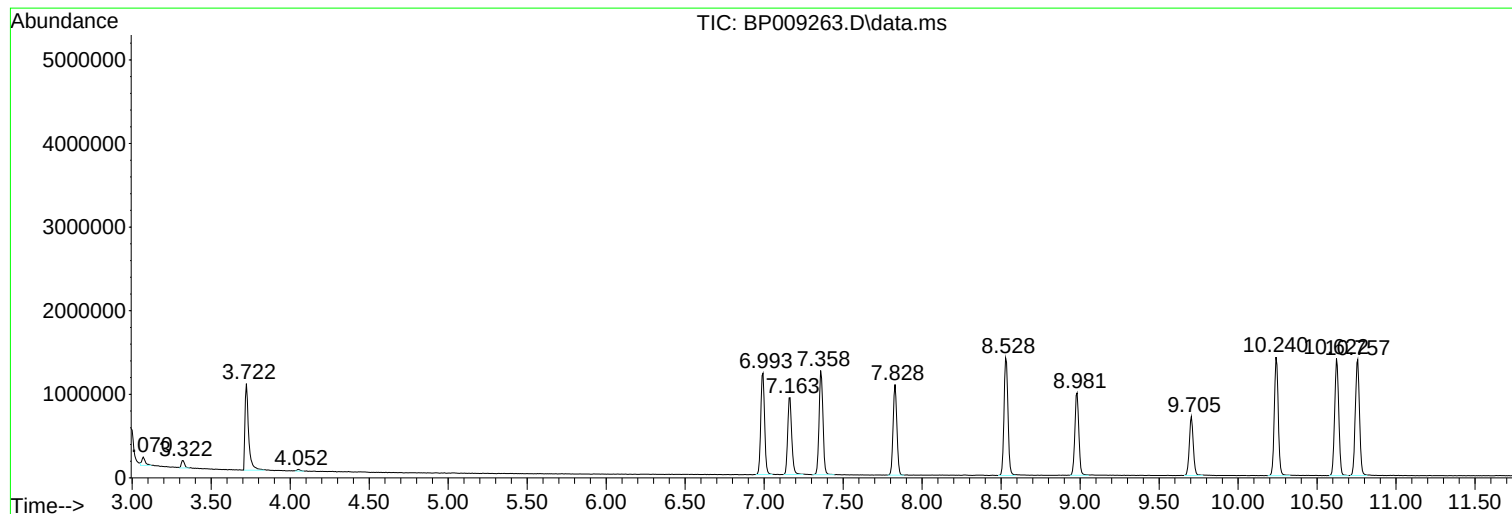

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009263.D
Acq On : 04 Mar 2022 11:28
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009263.D
Acq On : 04 Mar 2022 11:28
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc