

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
 Data File : BP009265.D
 Acq On : 04 Mar 2022 12:41
 Operator : CG/JU
 Sample : PB142852BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK852

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	21	rVB	115331	156616	1.94%	0.179%
2	3.323	53	57	67	rVB	110240	169899	2.11%	0.194%
3	3.723	121	125	145	rBV	1229782	1939779	24.06%	2.211%
4	4.046	178	180	187	rVB	24365	38279	0.47%	0.044%
5	6.987	673	680	692	rBV	1455882	2497333	30.98%	2.847%
6	7.158	702	709	722	rBV	1138571	2007952	24.91%	2.289%
7	7.358	736	743	754	rVB	1510504	2562733	31.79%	2.921%
8	7.828	815	823	833	rVB	1283921	2197465	27.26%	2.505%
9	8.528	933	942	952	rBV	1790383	2989213	37.08%	3.407%
10	8.975	1010	1018	1032	rBV	1216090	2151558	26.69%	2.453%
11	9.699	1133	1141	1151	rBV	873457	1551028	19.24%	1.768%
12	10.240	1223	1233	1248	rBV	1703637	3000860	37.22%	3.421%
13	10.622	1288	1298	1311	rVB	1673815	3069059	38.07%	3.498%
14	10.752	1311	1320	1332	rBV	1761277	3074725	38.14%	3.505%
15	12.210	1562	1568	1574	rBV	32136	57084	0.71%	0.065%
16	12.281	1576	1580	1585	rBV8	6260	11380	0.14%	0.013%
17	12.651	1638	1643	1650	rBV10	5569	12460	0.15%	0.014%
18	13.198	1731	1736	1742	rBV10	5333	11526	0.14%	0.013%
19	13.251	1742	1745	1748	rBV5	6069	8784	0.11%	0.010%
20	13.434	1769	1776	1781	rVB5	5765	11011	0.14%	0.013%
21	13.875	1844	1851	1858	rBV	2859495	4229034	52.46%	4.821%
22	14.157	1890	1899	1912	rBV	3320906	5274329	65.43%	6.012%
23	14.463	1944	1951	1959	rBV	2494400	3972078	49.27%	4.528%
24	14.651	1975	1983	2001	rBV	1118263	1743532	21.63%	1.987%
25	15.463	2113	2121	2128	rBV	4143491	6463957	80.18%	7.368%
26	15.510	2128	2129	2133	rVV4	11483	13331	0.17%	0.015%
27	15.575	2133	2140	2150	rVV	808372	1178830	14.62%	1.344%
28	15.704	2157	2162	2172	rVB5	21577	48471	0.60%	0.055%
29	16.134	2231	2235	2239	rBV7	6956	12100	0.15%	0.014%
30	16.416	2277	2283	2289	rBV7	5533	13263	0.16%	0.015%
31	17.010	2380	2384	2388	rVB	13590	18182	0.23%	0.021%
32	17.222	2413	2420	2430	rBV	2960837	4439880	55.07%	5.061%
33	17.322	2430	2437	2457	rVB	4564740	6856221	85.05%	7.815%
34	17.598	2480	2484	2487	rBV6	5656	10596	0.13%	0.012%
35	19.145	2743	2747	2752	rVB2	49664	69516	0.86%	0.079%
36	19.210	2755	2758	2762	rVV2	48012	63038	0.78%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009265.D
Acq On : 04 Mar 2022 12:41
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK852

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Title : SVOA CALIBRATION

37	19.569	2813	2819	2831	rVB	5647963	7926644	98.33%	9.036%
38	21.327	3113	3118	3126	rBV	3592744	4758563	59.03%	5.424%
39	23.580	3494	3501	3512	rVB2	3863222	8061537	100.00%	9.189%
40	23.739	3522	3528	3542	rVB	2430297	5055213	62.71%	5.762%




Sum of corrected areas: 87727059

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009265.D
Acq On : 04 Mar 2022 12:41
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

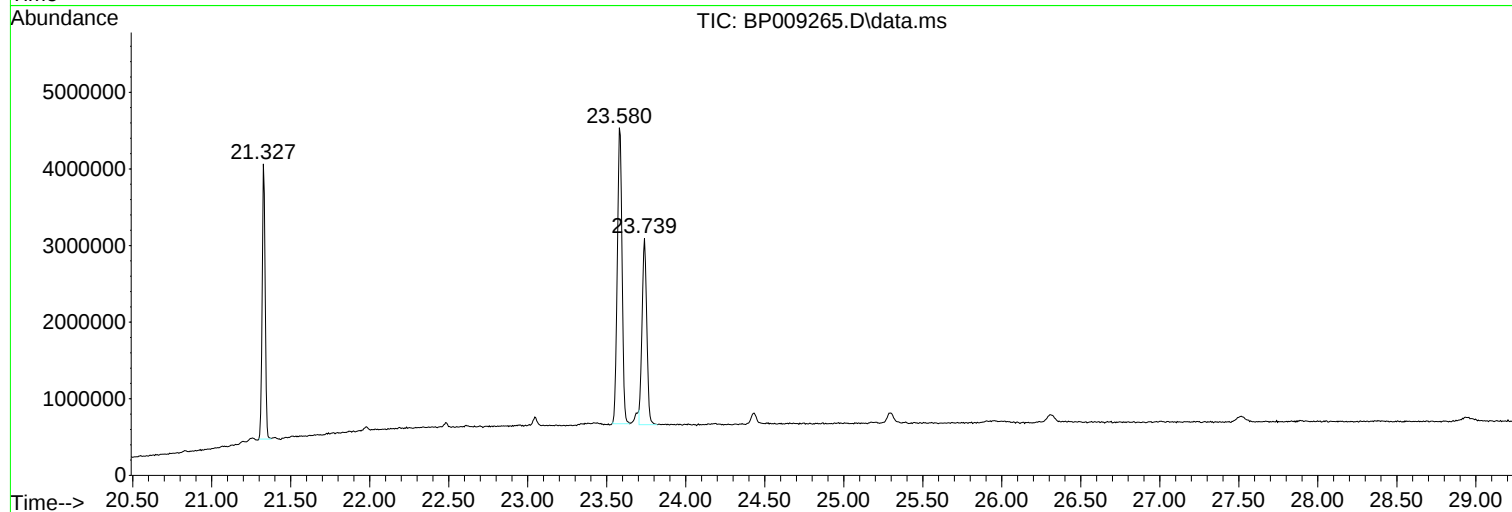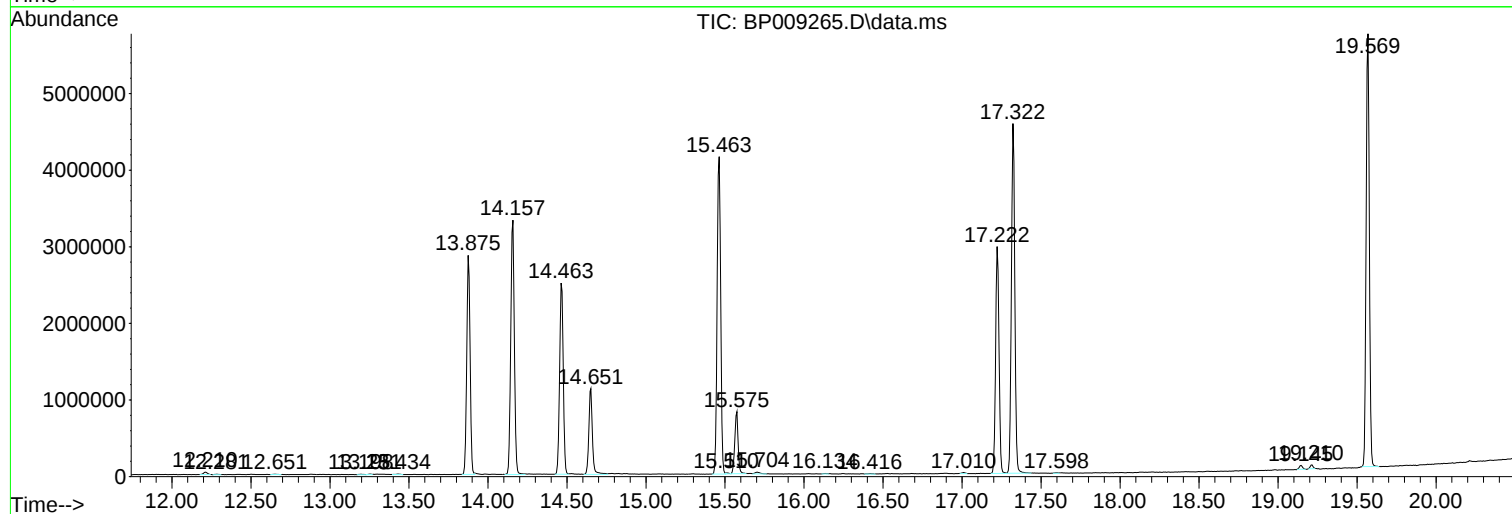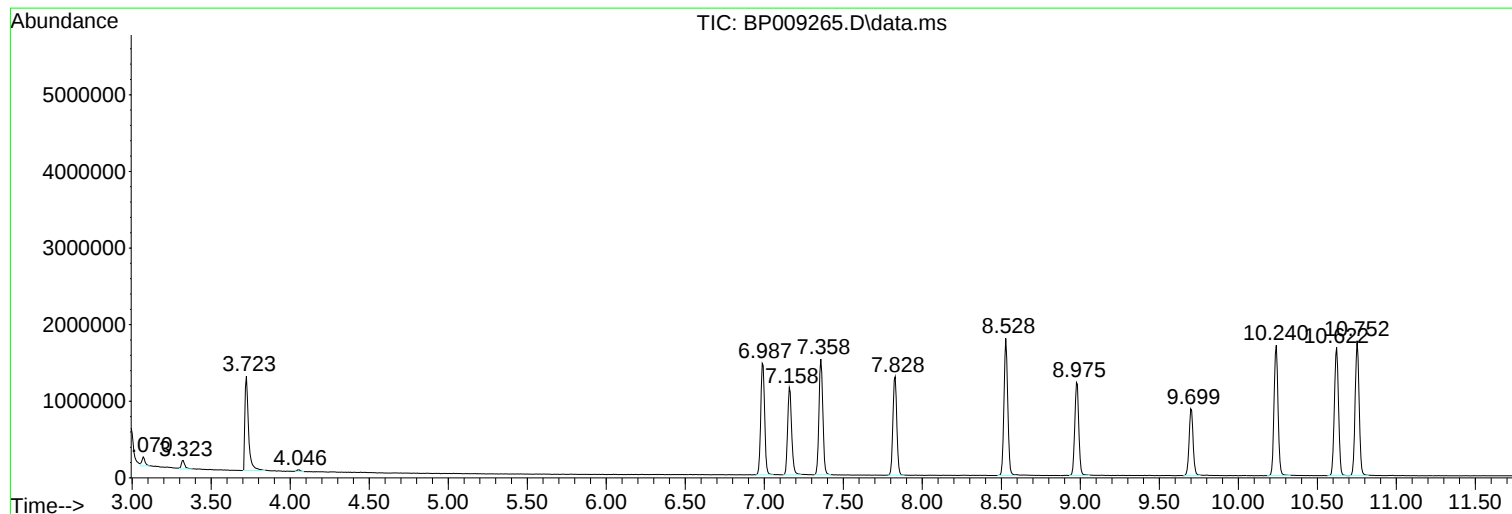

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009265.D
Acq On : 04 Mar 2022 12:41
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030422\
Data File : BP009265.D
Acq On : 04 Mar 2022 12:41
Operator : CG/JU
Sample : PB142852BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK852

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
