




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:59:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

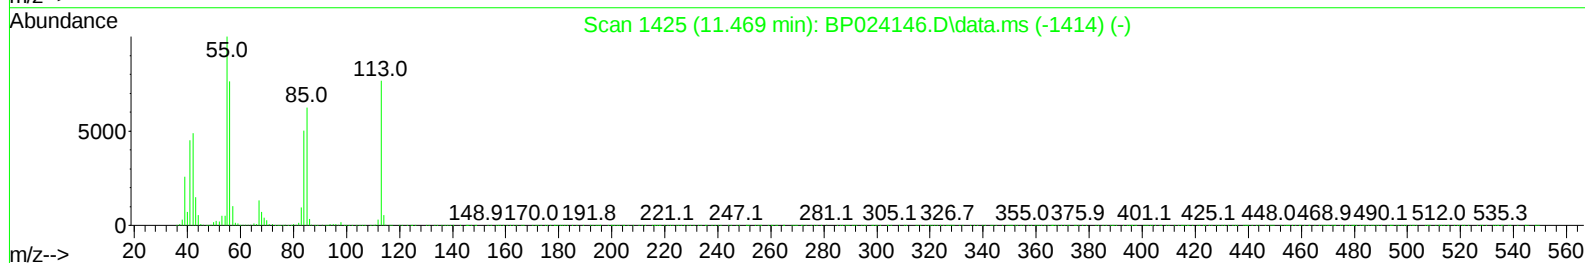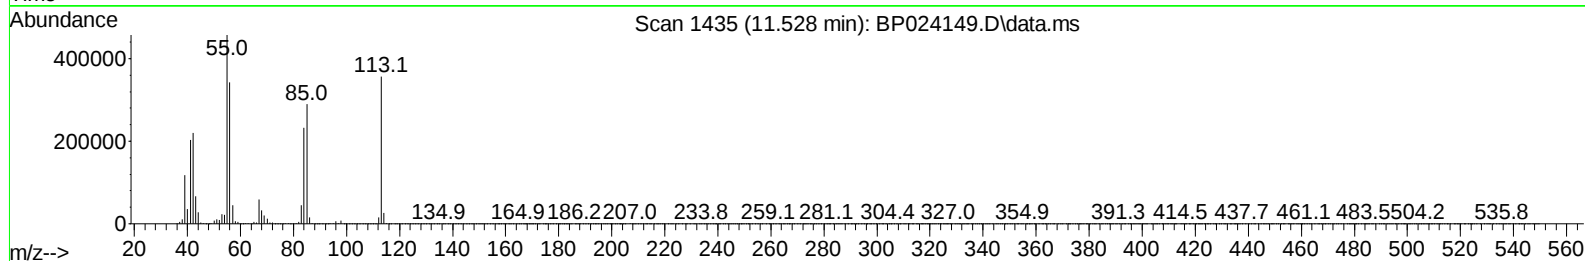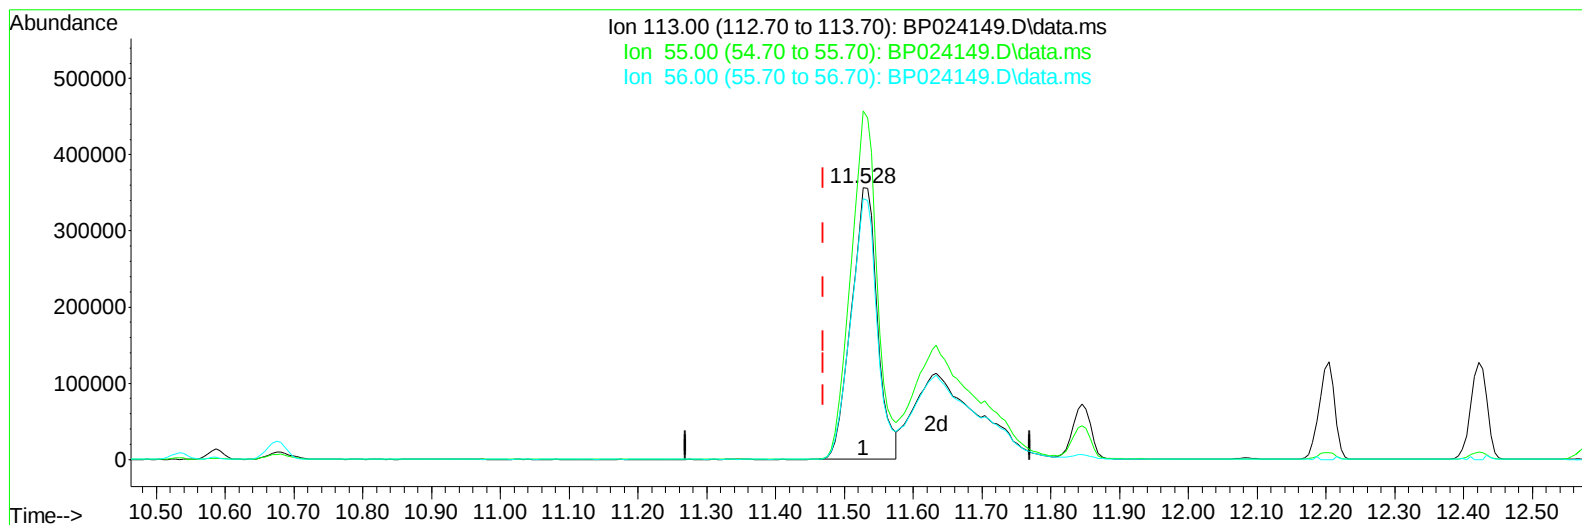

TIC: BP024149.D\data.ms

(34) Caprolactam

11.528min (+ 0.059) 97.48 ng/ul

response 943454

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	130.90	128.29
56.00	99.70	96.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:59:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

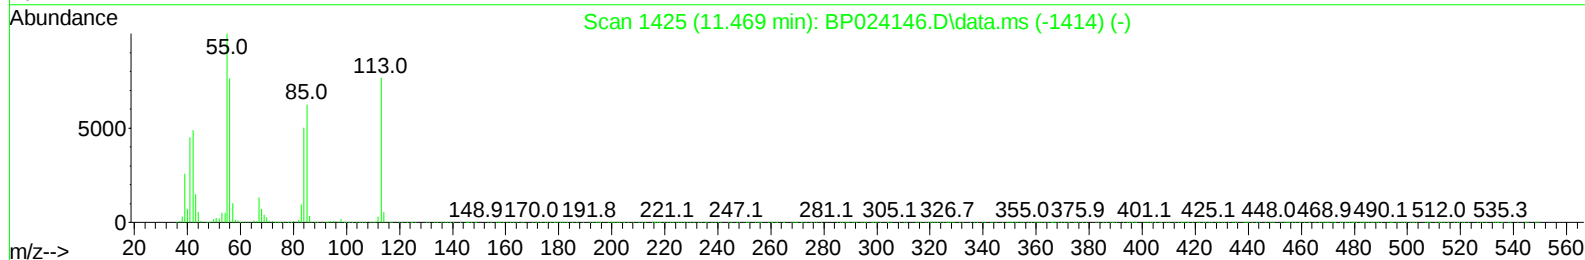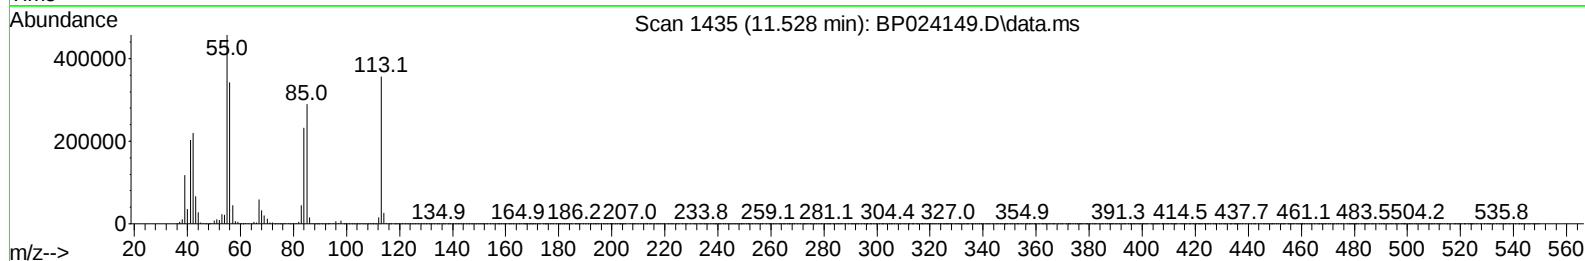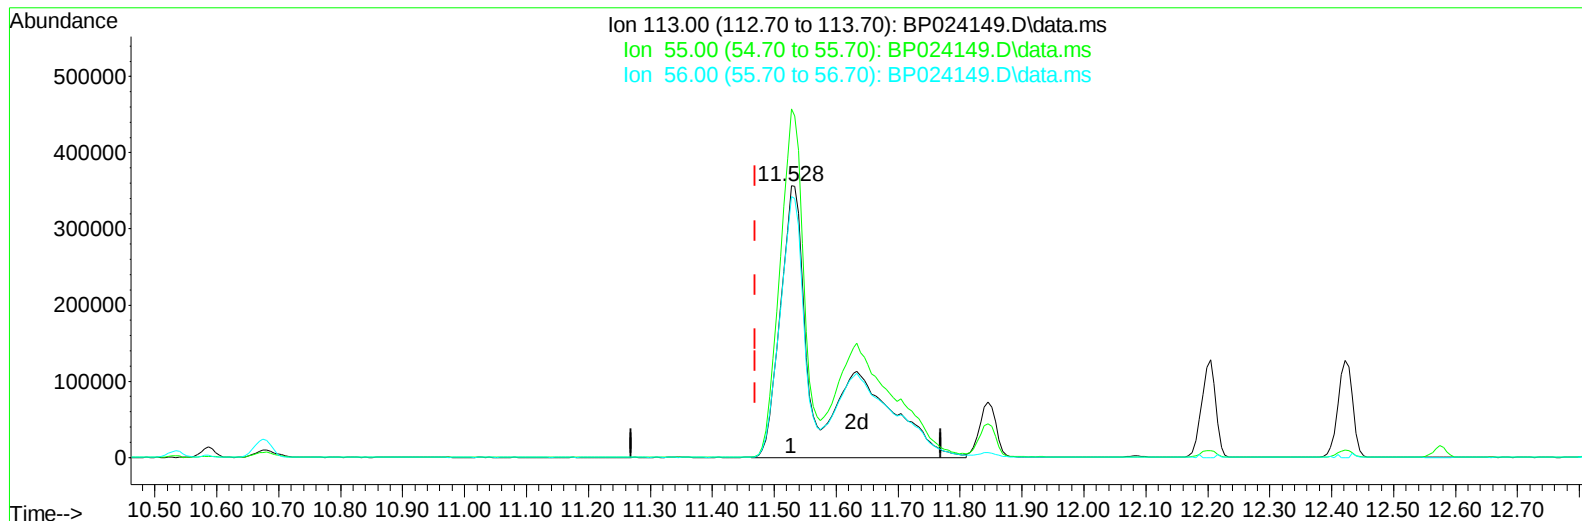

TIC: BP024149.D\data.ms

(34) Caprolactam

11.528min (+ 0.059) 173.72 ng/u1 m

response 1681351

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	130.90	128.29
56.00	99.70	96.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:59:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

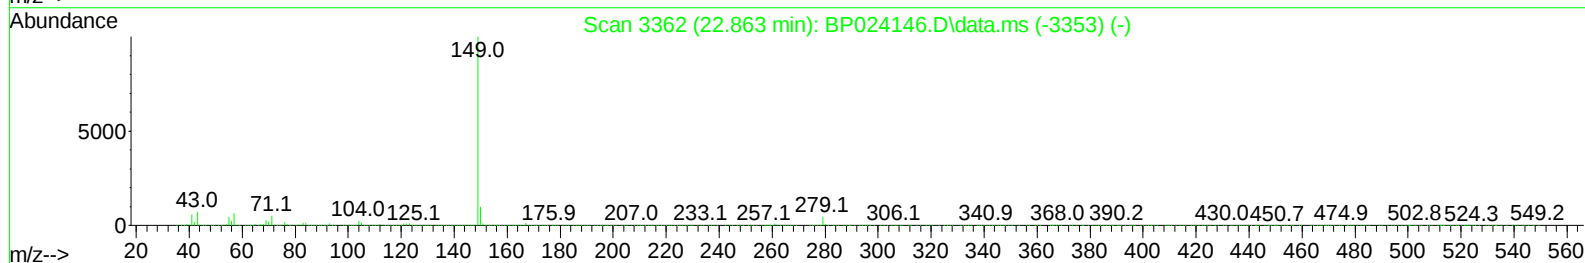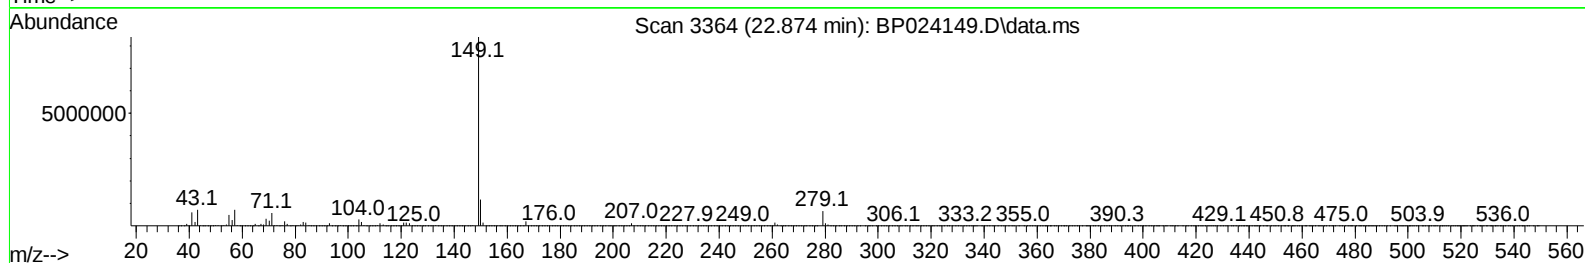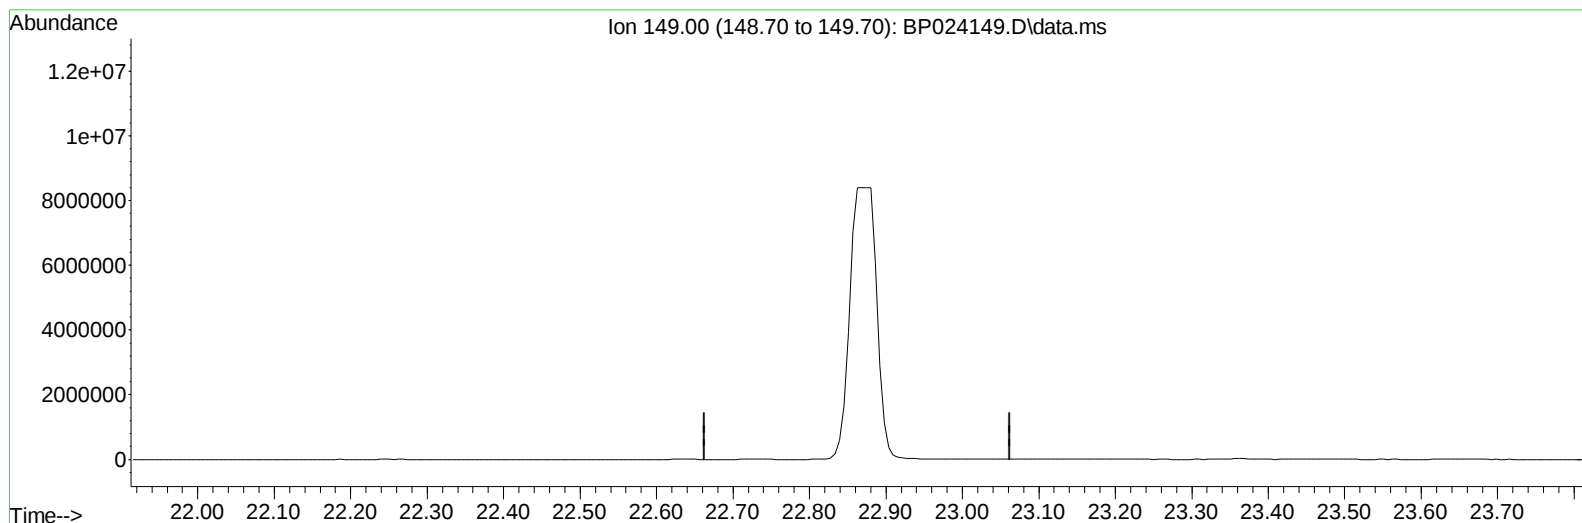

TIC: BP024149.D\data.ms

(89) Di-n-octyl phthalate

22.863min (-22.863) 0.00 ng/u1

response 0

Ion	Exp%	Act%
149.00	100.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:59:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

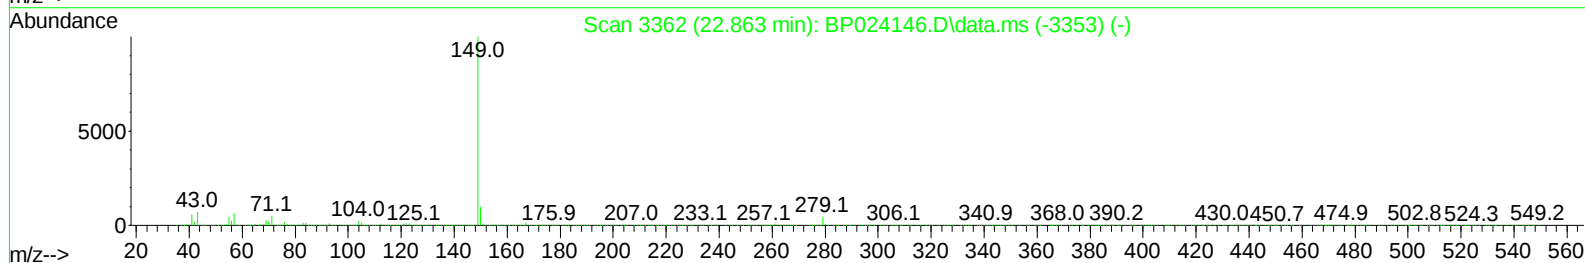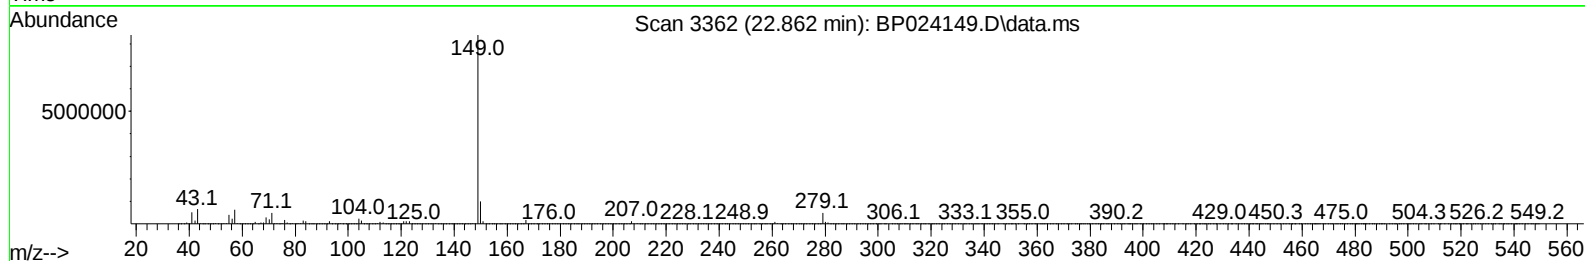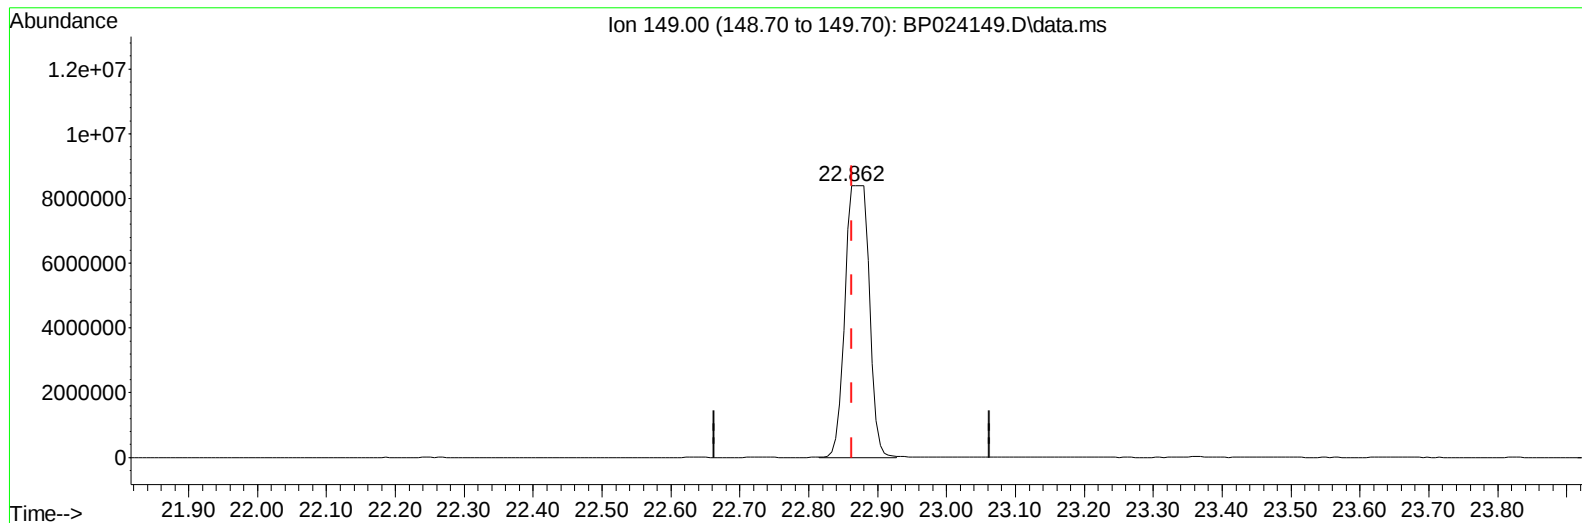

TIC: BP024149.D\data.ms

(89) Di-n-octyl phthalate

22.862min (-0.000) 146.58 ng/ul m

response 20376312

Ion	Exp%	Act%
149.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
 Data File : BP024149.D
 Acq On : 04 Mar 2025 13:01
 Operator : RC/JU
 Sample : SSTD16090
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 14:01:22 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 04 13:32:01 2025
 Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
 Supervised By :Jagrut Upadhyay 03/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	348021	20.00	ng/ul	0.00
20) Naphthalene-d8	10.534	136	1601035	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	1068668	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	2208240	20.00	ng/ul	0.00
79) Chrysene-d12	21.657	240	2169168	20.00	ng/ul	0.00
88) Perylene-d12	25.050	264	2324669	20.00	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.00	ng/uL	
4) Pyridine-d5	3.675	84	3960447	162.68	ng/ul	0.00
7) Phenol-d5	6.946	99	5198597	168.71	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.098	67	2630480	159.57	ng/ul	0.00
11) 2-Chlorophenol-d4	0.000	132	0d	0.00	ng/ul	
15) 4-Methylphenol-d8	8.475	113	4167053	167.47	ng/ul	0.02
21) Nitrobenzene-d5	0.000	128	0d	0.00	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.00	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.00	ng/ul	
31) 4-Chloroaniline-d4	10.675	131	5841361	155.28	ng/ul	0.00
46) Dimethylphthalate-d6	0.000	166	0d	0.00	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.00	ng/ul	
54) 4-Nitrophenol-d4	14.639	143	2652085	167.82	ng/ul	0.03
60) Fluorene-d10	0.000	176	0d	0.00	ng/ul	
65) 4,6-Dinitro-2-methylph...	15.545	200	2455471	177.76	ng/ul	0.02
73) Anthracene-d10	0.000	188	0d	0.00	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.00	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.00	ng/ul	
Target Compounds						
						Qvalue
5) Pyridine	3.693	79	3967641	161.79	ng/ul	98
6) Benzaldehyde	6.904	77	1433027	94.50	ng/ul	99
8) Phenol	6.975	94	5287033	166.67	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.187	93	3832053	158.30	ng/ul	99
13) 2-Methylphenol	8.204	108	3936382	166.40	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.275	45	3916733	156.46	ng/ul	97
16) Acetophenone	8.581	105	5961624	156.99	ng/ul	98
18) 4-Methylphenol	8.545	108	4341795	165.70	ng/ul	99
32) 4-Chloroaniline	10.704	127	5508328	154.72	ng/ul	98
34) Caprolactam	11.528	113	1681351m	173.72	ng/ul	
40) Hexachlorocyclopentadiene	12.557	237	2505806	140.03	ng/ul	99
51) 3-Nitroaniline	14.316	138	2709596	159.73	ng/ul	99
53) 2,4-Dinitrophenol	14.522	184	1929564	207.09	ng/ul	92
55) 4-Nitrophenol	14.663	109	1724352	155.17	ng/ul	94
63) 4-Nitroaniline	15.504	138	2264778	136.12	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.563	198	2600014	172.17	ng/ul#	97
70) Atrazine	16.663	200	3370245	129.27	ng/ul	100
71) Pentachlorophenol	16.845	266	3082412	165.10	ng/ul	100
77) Carbazole	17.621	167	15451705	139.56	ng/ul#	90
84) 3,3'-Dichlorobenzidine	21.557	252	5637208	119.52	ng/ul	98
89) Di-n-octyl phthalate	22.862	149	20376312m	146.58	ng/ul	

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

Quant Time: Mar 04 14:01:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed							

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024149.D
Acq On : 04 Mar 2025 13:01
Operator : RC/JU
Sample : SSTD16090
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD160628

Manual IntegrationsAPPROVED

Quant Time: Mar 04 14:01:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 04 13:32:01 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 03/05/2025
Supervised By :Jagrut Upadhyay 03/05/2025

