

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
 Data File : BP024153.D
 Acq On : 04 Mar 2025 18:16
 Operator : RC/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664

Quant Time: Mar 05 08:50:27 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 04 14:51:41 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.752	152	265637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.534	136	1248037	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	848708	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	1760454	20.000	ng/ul	0.00
79) Chrysene-d12	21.669	240	1939367	20.000	ng/ul	0.02
88) Perylene-d12	25.063	264	2078390	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	55028	8.252	ng/uL	0.00
4) Pyridine-d5	3.681	84	419623	21.875	ng/ul	0.00
7) Phenol-d5	6.928	99	525841	22.311	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.087	67	304774	23.481	ng/ul	0.00
11) 2-Chlorophenol-d4	7.293	132	412344	22.791	ng/ul	0.00
15) 4-Methylphenol-d8	8.458	113	435381	23.396	ng/ul	0.00
21) Nitrobenzene-d5	8.899	128	217660	21.599	ng/ul	0.00
24) 2-Nitrophenol-d4	9.616	143	228657	21.733	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.157	165	421917	22.303	ng/ul	0.00
31) 4-Chloroaniline-d4	10.663	131	654799	22.647	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1382098	22.473	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	1579195	22.138	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	273686	21.737	ng/ul	0.00
60) Fluorene-d10	15.404	176	1166625	22.327	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	221355	19.915	ng/ul	0.00
73) Anthracene-d10	17.304	188	1883827	21.927	ng/ul	0.00
81) Pyrene-d10	19.680	212	2198918	22.631	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.839	264	2392024	22.199	ng/ul	0.04
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.305	88	58667	8.342	ng/uL	99
5) Pyridine	3.699	79	423181	21.786	ng/ul	99
6) Benzaldehyde	6.899	77	332671	27.375	ng/ul	99
8) Phenol	6.958	94	557056	22.744	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.181	93	433130	23.244	ng/ul	100
12) 2-Chlorophenol	7.322	128	434198	23.011	ng/ul	99
13) 2-Methylphenol	8.193	108	410865	22.954	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.269	45	471672	24.137	ng/ul	99
16) Acetophenone	8.569	105	715915	24.855	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.552	70	347564	25.729	ng/ul	98
18) 4-Methylphenol	8.522	108	473617	23.878	ng/ul	98
19) Hexachloroethane	8.828	117	168899	22.449	ng/ul	100
22) Nitrobenzene	8.940	77	500402	22.082	ng/ul	99
23) Isophorone	9.469	82	975596	22.984	ng/ul	99
25) 2-Nitrophenol	9.652	139	259196	22.246	ng/ul	99
26) 2,4-Dimethylphenol	9.710	107	473405	22.670	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.946	93	608307	22.527	ng/ul	99
29) 2,4-Dichlorophenol	10.187	162	429584	22.234	ng/ul	99
30) Naphthalene	10.581	128	1488268	22.023	ng/ul	100
32) 4-Chloroaniline	10.687	127	627644	22.755	ng/ul	99
33) Hexachlorobutadiene	10.869	225	249572	21.095	ng/ul	99
34) Caprolactam	11.463	113	169479	23.098	ng/ul	96
35) 4-Chloro-3-methylphenol	11.828	107	473377	23.548	ng/ul	99
36) 2-Methylnaphthalene	12.198	142	1031587	22.626	ng/ul	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
 Data File : BP024153.D
 Acq On : 04 Mar 2025 18:16
 Operator : RC/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664

Quant Time: Mar 05 08:50:27 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 04 14:51:41 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.416	142	1037793	23.029	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.569	216	522509	20.372	ng/ul	99
40) Hexachlorocyclopentadiene	12.551	237	258176	19.369	ng/ul	98
41) 2,4,6-Trichlorophenol	12.810	196	342017	21.197	ng/ul	99
42) 2,4,5-Trichlorophenol	12.887	196	375606	21.386	ng/ul	99
43) 1,1'-Biphenyl	13.210	154	1361322	21.093	ng/ul	99
44) 2-Chloronaphthalene	13.251	162	1059002	21.154	ng/ul	100
45) 2-Nitroaniline	13.463	65	293358	22.525	ng/ul	95
47) Dimethylphthalate	13.845	163	1389868	22.591	ng/ul	99
48) 2,6-Dinitrotoluene	13.957	165	275787	22.857	ng/ul	99
50) Acenaphthylene	14.110	152	1705804	22.071	ng/ul	100
51) 3-Nitroaniline	14.293	138	310104	22.107	ng/ul	99
52) Acenaphthene	14.457	153	1180478	21.698	ng/ul	99
53) 2,4-Dinitrophenol	14.510	184	143033	19.016	ng/ul	92
55) 4-Nitrophenol	14.616	109	193134	22.128	ng/ul	97
56) Dibenzofuran	14.798	168	1631574	21.749	ng/ul	100
57) 2,4-Dinitrotoluene	14.763	165	417949	23.272	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.034	232	322615	22.336	ng/ul	98
59) Diethylphthalate	15.228	149	1408205	23.120	ng/ul	99
61) Fluorene	15.457	166	1377766	22.464	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.451	204	655669	22.130	ng/ul	97
63) 4-Nitroaniline	15.475	138	340408	24.662	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.540	198	248677	20.502	ng/ul	97
67) N-Nitrosodiphenylamine	15.669	169	1157274	21.561	ng/ul	100
68) 4-Bromophenyl-phenylether	16.369	248	417482	21.522	ng/ul	97
69) Hexachlorobenzene	16.486	284	501954	21.303	ng/ul	95
70) Atrazine	16.651	200	441060	22.697	ng/ul	98
71) Pentachlorophenol	16.839	266	299087	20.223	ng/ul	100
72) Phenanthrene	17.245	178	2161655	21.478	ng/ul	100
74) Anthracene	17.339	178	2225577	21.947	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.181	216	528237	19.926	ng/uL	99
76) Pentachlorobenzene	14.716	250	575409	20.757	ng/uL	99
77) Carbazole	17.622	167	2045814	22.220	ng/ul	99
78) Di-n-butylphthalate	18.210	149	2378135	22.176	ng/ul	100
80) Fluoranthene	19.333	202	2549495	22.507	ng/ul	98
82) Pyrene	19.710	202	2731161	22.374	ng/ul	99
83) Butylbenzylphthalate	20.663	149	1111040	22.573	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.563	252	844994	21.783	ng/ul	98
85) Benzo(a)anthracene	21.651	228	2802375	22.085	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.586	149	1625985	22.013	ng/ul	99
87) Chrysene	21.716	228	2616292	21.952	ng/ul	100
89) Di-n-octyl phthalate	22.892	149	2664199	21.958	ng/ul	100
90) Benzo(b)fluoranthene	23.992	252	2776460	22.460	ng/ul	100
91) Benzo(k)fluoranthene	24.063	252	2805024	22.356	ng/ul	100
93) Benzo(a)pyrene	24.904	252	2611339	22.340	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	28.927	276	3254499	21.056	ng/ul	99
95) Dibenzo(a,h)anthracene	28.992	278	2659721	21.194	ng/ul	98
96) Benzo(g,h,i)perylene	30.109	276	2521054	21.019	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed

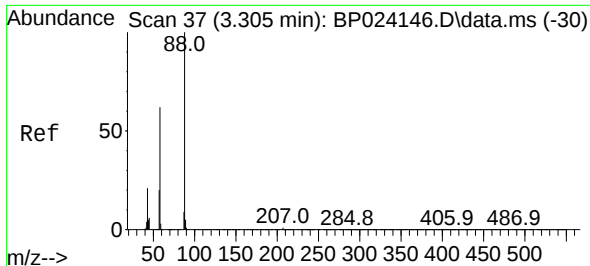

#2
1,4-Dioxane
Concen: 8.342 ng/uL
RT: 3.305 min Scan# 31
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion: 88 Resp: 58667
Ion Ratio Lower Upper
88 100
43 22.5 17.6 26.4
58 60.1 48.8 73.2

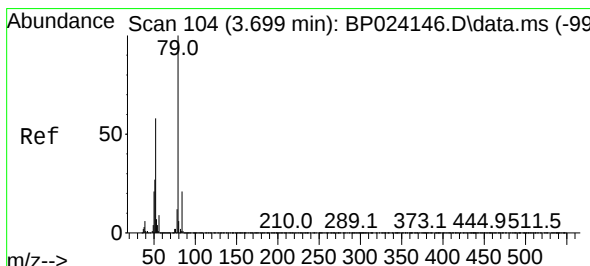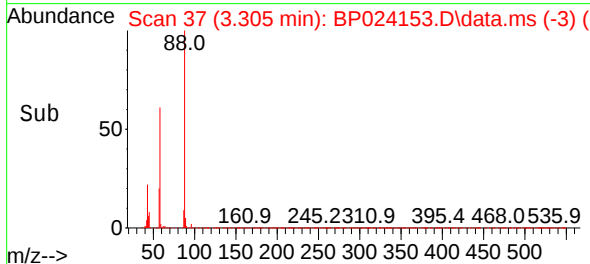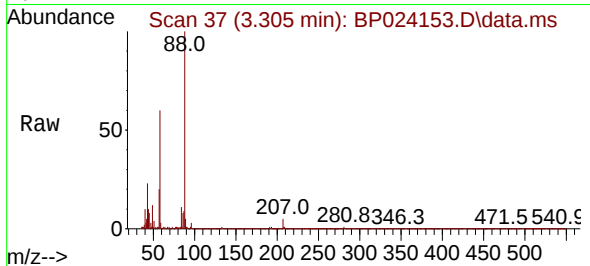

#5
Pyridine
Concen: 21.786 ng/uL
RT: 3.699 min Scan# 104
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion: 79 Resp: 423181
Ion Ratio Lower Upper
79 100
52 60.1 48.8 73.2
51 27.6 21.9 32.9


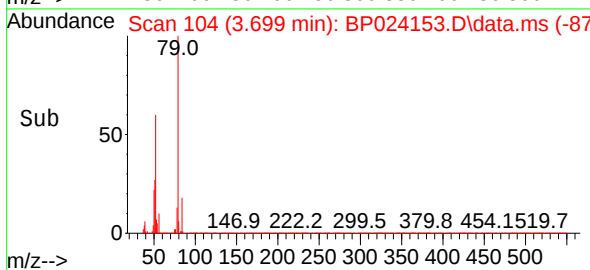

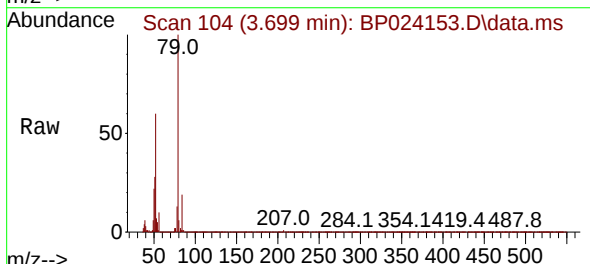




#6
Benzaldehyde
Concen: 27.375 ng/ul
RT: 6.899 min Scan# 649
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion: 77 Resp: 332671
Ion Ratio Lower Upper
77 100
105 98.9 80.5 120.7
106 96.7 77.7 116.5



#8
Phenol
Concen: 22.744 ng/ul
RT: 6.958 min Scan# 658
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion: 94 Resp: 557056
Ion Ratio Lower Upper
94 100
65 23.9 19.6 29.4
66 31.1 24.9 37.3









#10
 Bis(2-Chloroethyl)ether
 Concen: 23.244 ng/ul
 RT: 7.181 min Scan# 696
 Delta R.T. 0.000 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664


Tgt Ion: 93	Resp: 433130
Ion Ratio	Lower Upper
93 100	
63 68.3	54.2 81.2
95 32.2	25.8 38.6



#12
 2-Chlorophenol
 Concen: 23.011 ng/ul
 RT: 7.322 min Scan# 720
 Delta R.T. -0.006 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16

Tgt Ion:128	Resp: 434198
Ion Ratio	Lower Upper
128 100	
64 41.9	33.4 50.0
130 32.1	26.5 39.7

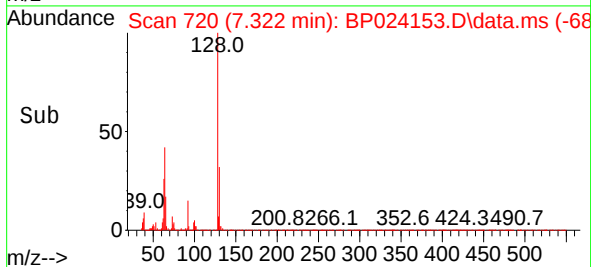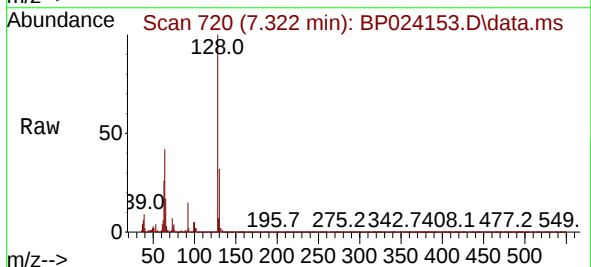



#13

2-Methylphenol

Concen: 22.954 ng/ul

RT: 8.193 min Scan# 8

Delta R.T. -0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :





SSTD020664

Tgt Ion:108 Resp: 410865

Ion Ratio Lower Upper

108 100

107 88.2 71.2 106.8

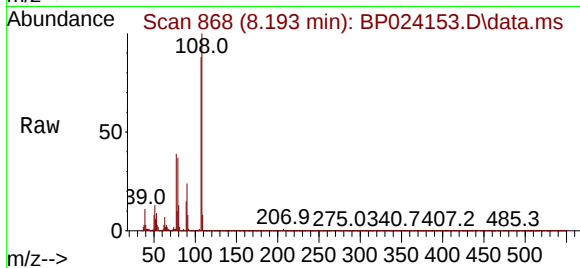

#14

2,2'-oxybis(1-Chloropropane)

Concen: 24.137 ng/ul

RT: 8.269 min Scan# 881

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion: 45 Resp: 471672


Ion Ratio Lower Upper

45 100

77 18.5 14.5 21.7

79 13.5 10.9 16.3



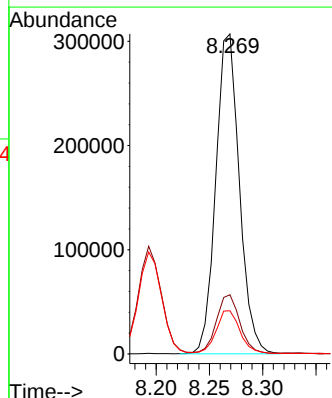
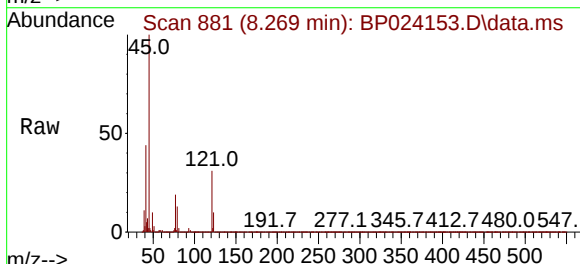




#16
Acetophenone
Concen: 24.855 ng/ul
RT: 8.569 min Scan# 932
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:105 Resp: 715915
Ion Ratio Lower Upper
105 100
77 73.9 58.3 87.5
51 20.1 16.1 24.1



#17
N-Nitroso-di-n-propylamine
Concen: 25.729 ng/ul
RT: 8.552 min Scan# 929
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion: 70 Resp: 347564
Ion Ratio Lower Upper
70 100
42 46.5 36.2 54.2
101 10.4 8.6 12.8
130 23.6 18.2 27.2









#18
4-Methylphenol
Concen: 23.878 ng/ul
RT: 8.522 min Scan# 918
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:108 Resp: 473617
Ion Ratio Lower Upper
108 100
107 109.1 88.8 133.2



#19
Hexachloroethane
Concen: 22.449 ng/ul
RT: 8.828 min Scan# 976
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:117 Resp: 168899
Ion Ratio Lower Upper
117 100
201 98.7 79.2 118.8
199 60.7 48.6 73.0

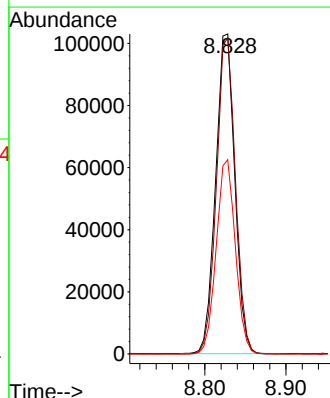



#22

Nitrobenzene

Concen: 22.082 ng/ul

RT: 8.940 min Scan# 996

Delta R.T. -0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion: 77 Resp: 500402

Ion Ratio Lower Upper

77 100

123 48.8 39.7 59.5

65 12.2 9.8 14.8



#23

Isophorone

Concen: 22.984 ng/ul

RT: 9.469 min Scan# 1085

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion: 82 Resp: 975596


Ion Ratio Lower Upper

82 100

95 6.7 5.3 7.9

138 18.4 15.4 23.0









#25
2-Nitrophenol
Concen: 22.246 ng/ul
RT: 9.652 min Scan# 1116
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:139 Resp: 259196
Ion Ratio Lower Upper
139 100
65 43.1 34.1 51.1
109 26.4 20.1 30.1



#26
2,4-Dimethylphenol
Concen: 22.670 ng/ul
RT: 9.710 min Scan# 1126
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:107 Resp: 473405
Ion Ratio Lower Upper
107 100
121 52.4 40.6 60.8
122 87.0 71.4 107.0









#27
 Bis(2-Chloroethoxy)methane
 Concen: 22.527 ng/ul
 RT: 9.946 min Scan# 1165
 Delta R.T. 0.006 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664


Tgt Ion: 93 Resp: 608307
 Ion Ratio Lower Upper
 93 100
 95 32.5 25.3 37.9
 123 11.9 9.5 14.3



#29
 2,4-Dichlorophenol
 Concen: 22.234 ng/ul
 RT: 10.187 min Scan# 1207
 Delta R.T. 0.000 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16

Tgt Ion: 162 Resp: 429584
 Ion Ratio Lower Upper
 162 100
 164 65.2 52.6 79.0
 98 35.4 28.5 42.7


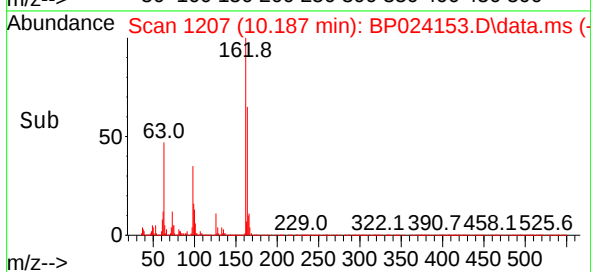






#30
Naphthalene
Concen: 22.023 ng/ul
RT: 10.581 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:128 Resp: 1488268
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 12.9 10.3 15.5



#32
4-Chloroaniline
Concen: 22.755 ng/ul
RT: 10.687 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:127 Resp: 627644
Ion Ratio Lower Upper
127 100
129 32.5 25.5 38.3





#33

Hexachlorobutadiene

Concen: 21.095 ng/ul

RT: 10.869 min Scan# 1424

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:225 Resp: 249572

Ion Ratio Lower Upper

225 100

223 62.7 50.2 75.4

227 63.6 52.2 78.2



#34

Caprolactam

Concen: 23.098 ng/ul

RT: 11.463 min Scan# 1424

Delta R.T. -0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:113 Resp: 169479


Ion Ratio Lower Upper

113 100

55 136.3 104.7 157.1

56 102.1 79.8 119.6


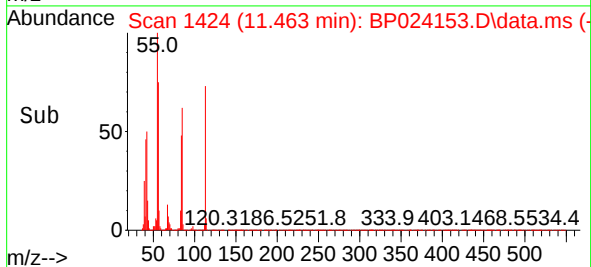

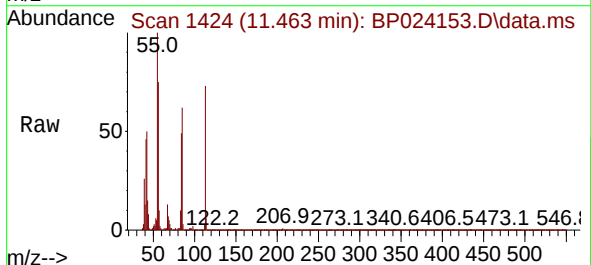


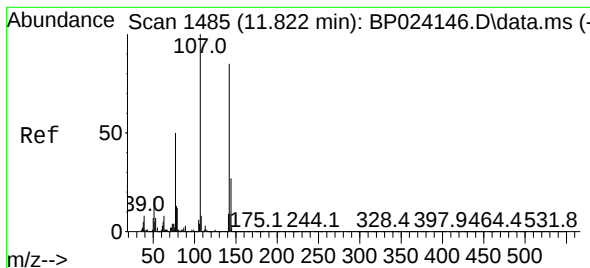

#35
4-Chloro-3-methylphenol
Concen: 23.548 ng/ul
RT: 11.828 min Scan# 1485
Delta R.T. 0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:107 Resp: 473377
Ion Ratio Lower Upper
107 100
144 26.7 21.8 32.6
142 84.1 67.8 101.6

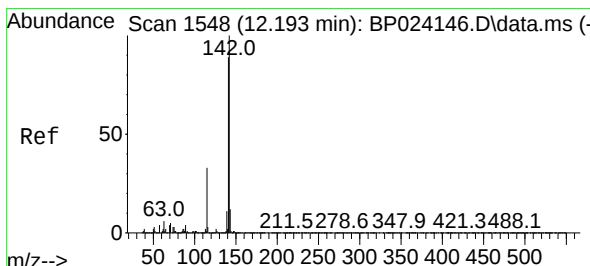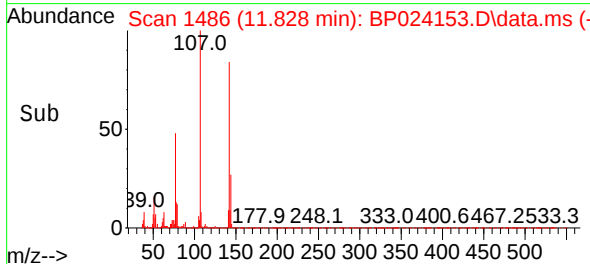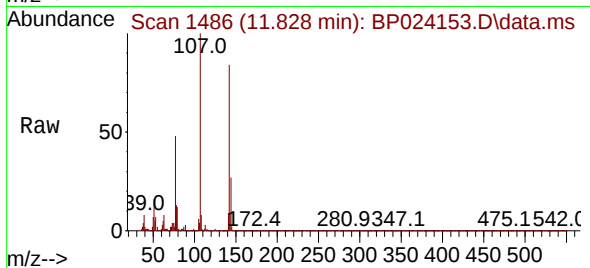

#36
2-Methylnaphthalene
Concen: 22.626 ng/ul
RT: 12.198 min Scan# 1549
Delta R.T. 0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:142 Resp: 1031587
Ion Ratio Lower Upper
142 100
141 88.4 71.3 106.9


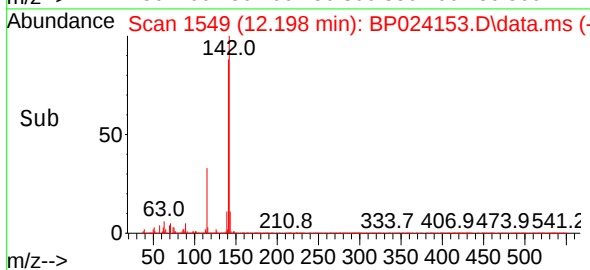

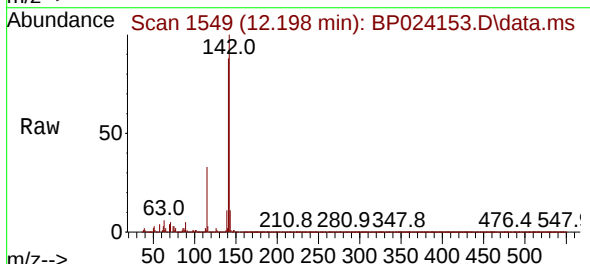




#37
1-Methylnaphthalene
Concen: 23.029 ng/ul
RT: 12.416 min Scan# 1586
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:142 Resp: 1037793
Ion Ratio Lower Upper
142 100
141 91.7 72.4 108.6
116 3.6 2.8 4.2



#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.372 ng/ul
RT: 12.569 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:216 Resp: 522509
Ion Ratio Lower Upper
216 100
214 77.0 62.6 93.8
179 20.5 16.2 24.2
108 17.4 13.5 20.3

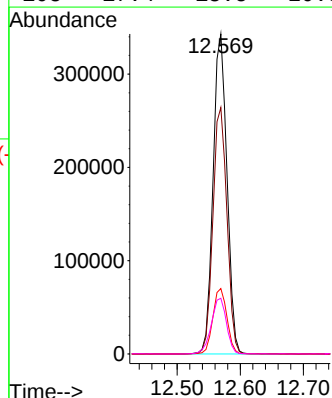



#40

Hexachlorocyclopentadiene

Concen: 19.369 ng/ul

RT: 12.551 min Scan# 1609

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:237 Resp: 258176

Ion Ratio Lower Upper

237 100

235 63.8 49.3 73.9

272 14.3 11.4 17.2



#41

2,4,6-Trichlorophenol

Concen: 21.197 ng/ul

RT: 12.810 min Scan# 1653

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:196 Resp: 342017


Ion Ratio Lower Upper

196 100

198 95.7 77.0 115.6

200 30.7 24.8 37.2





#42

2,4,5-Trichlorophenol

Concen: 21.386 ng/ul

RT: 12.887 min Scan# 1666

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:196 Resp: 375606

Ion Ratio Lower Upper

196 100

198 94.2 74.7 112.1

200 30.7 24.2 36.2

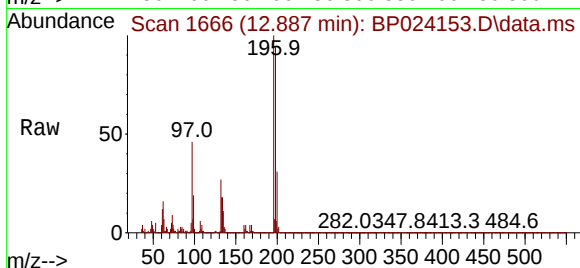

#43

1,1'-Biphenyl

Concen: 21.093 ng/ul

RT: 13.210 min Scan# 1721

Delta R.T. -0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:154 Resp: 1361322


Ion Ratio Lower Upper

154 100

153 40.0 31.9 47.9

76 13.1 10.0 15.0




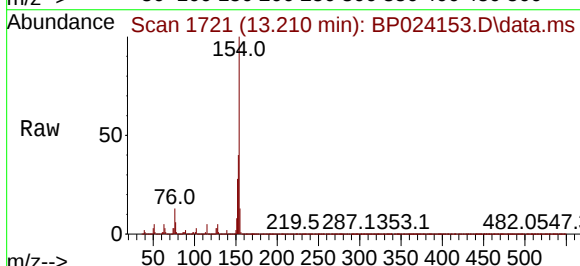




#44
2-Chloronaphthalene
Concen: 21.154 ng/ul
RT: 13.251 min Scan# 1728
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:162 Resp: 1059002
Ion Ratio Lower Upper
162 100
164 33.0 26.3 39.5
127 38.5 30.5 45.7



#45
2-Nitroaniline
Concen: 22.525 ng/ul
RT: 13.463 min Scan# 1764
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion: 65 Resp: 293358
Ion Ratio Lower Upper
65 100
92 79.6 62.1 93.1
138 132.7 100.5 150.7


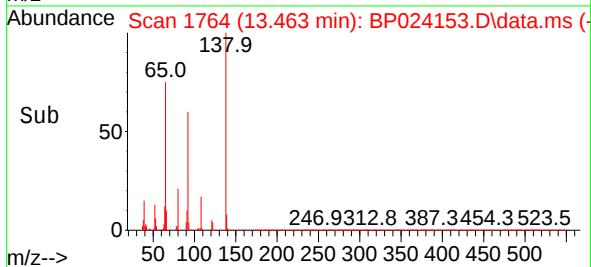

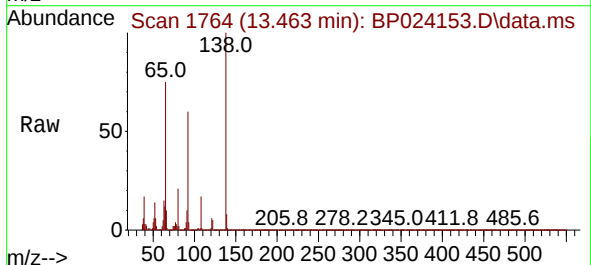




#47
Dimethylphthalate
Concen: 22.591 ng/ul
RT: 13.845 min Scan# 1829
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:163 Resp: 1389868
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.2
164 10.0 8.2 12.2



#48
2,6-Dinitrotoluene
Concen: 22.857 ng/ul
RT: 13.957 min Scan# 1848
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:165 Resp: 275787
Ion Ratio Lower Upper
165 100
89 53.7 42.6 63.8
121 21.1 17.7 26.5





#50

Acenaphthylene

Concen: 22.071 ng/ul

RT: 14.110 min Scan# 1875

Delta R.T. -0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:152 Resp: 1705804

Ion Ratio Lower Upper

152 100

151 19.5 15.7 23.5

153 13.3 10.5 15.7



#51

3-Nitroaniline

Concen: 22.107 ng/ul

RT: 14.293 min Scan# 1905

Delta R.T. 0.000 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:138 Resp: 310104


Ion Ratio Lower Upper

138 100

108 11.3 8.5 12.7

92 111.8 88.3 132.5









#52
Acenaphthene
Concen: 21.698 ng/ul
RT: 14.457 min Scan# 1933
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:153 Resp: 1180478
Ion Ratio Lower Upper
153 100
152 47.7 38.2 57.4
154 90.1 71.0 106.6



#53
2,4-Dinitrophenol
Concen: 19.016 ng/ul
RT: 14.510 min Scan# 1942
Delta R.T. 0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:184 Resp: 143033
Ion Ratio Lower Upper
184 100
63 50.8 47.8 71.8
154 56.4 47.0 70.6









#55
4-Nitrophenol
Concen: 22.128 ng/ul
RT: 14.616 min Scan# 1960
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:109 Resp: 193134
Ion Ratio Lower Upper
109 100
139 153.5 127.4 191.2
65 134.8 106.3 159.5



#56
Dibenzofuran
Concen: 21.749 ng/ul
RT: 14.798 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:168 Resp: 1631574
Ion Ratio Lower Upper
168 100
139 36.3 28.9 43.3


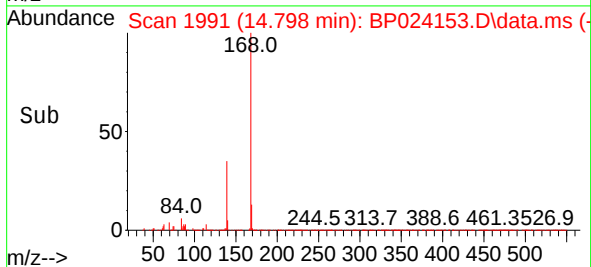

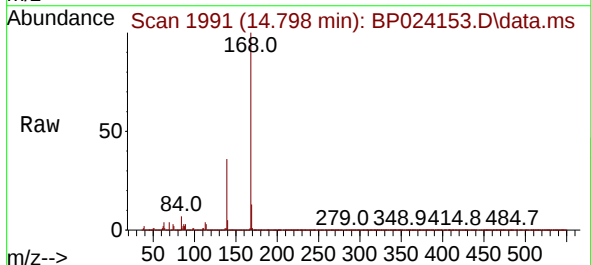




#57
2,4-Dinitrotoluene
Concen: 23.272 ng/ul
RT: 14.763 min Scan# 1985
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:165 Resp: 417949
Ion Ratio Lower Upper
165 100
63 36.3 28.7 43.1
182 3.1 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 22.336 ng/ul
RT: 15.034 min Scan# 2031
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:232 Resp: 322615
Ion Ratio Lower Upper
232 100
131 43.3 36.1 54.1
130 2.3 1.8 2.8
166 30.1 24.7 37.1


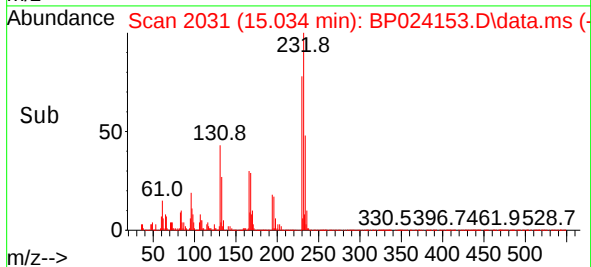

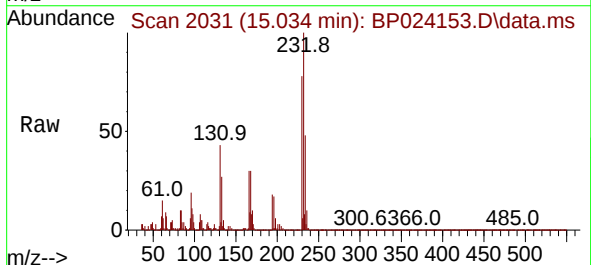




#59
Diethylphthalate
Concen: 23.120 ng/ul
RT: 15.228 min Scan# 2064
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:149 Resp: 1408205
Ion Ratio Lower Upper
149 100
177 21.8 17.7 26.5
150 12.2 10.1 15.1



#61
Fluorene
Concen: 22.464 ng/ul
RT: 15.457 min Scan# 2103
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:166 Resp: 1377766
Ion Ratio Lower Upper
166 100
165 97.5 77.1 115.7
167 13.7 10.6 16.0









#62
4-Chlorophenyl-phenylether
Concen: 22.130 ng/ul
RT: 15.451 min Scan# 2102
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:204 Resp: 655669
Ion Ratio Lower Upper
204 100
206 33.0 25.8 38.8
141 59.5 45.1 67.7

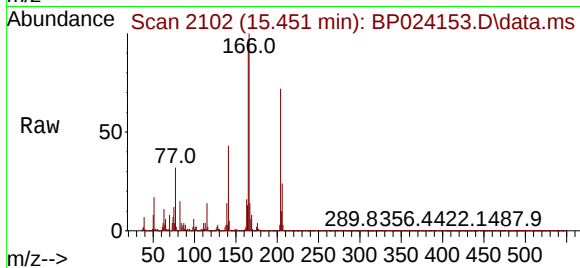

#63
4-Nitroaniline
Concen: 24.662 ng/ul
RT: 15.475 min Scan# 2106
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:138 Resp: 340408
Ion Ratio Lower Upper
138 100
92 49.3 38.9 58.3
108 70.1 55.3 82.9


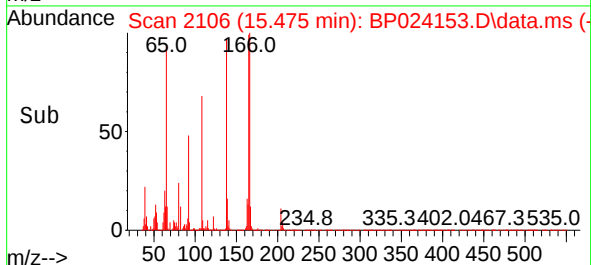
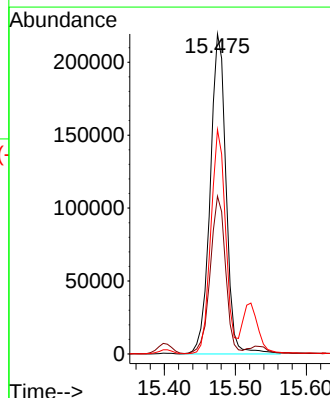
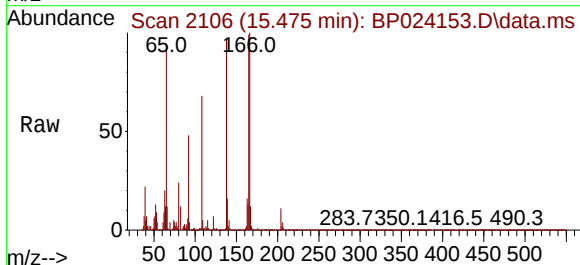


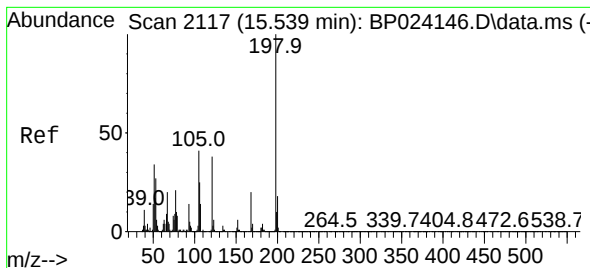

#66
4,6-Dinitro-2-methylphenol
Concen: 20.502 ng/ul
RT: 15.540 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:198 Resp: 248677
Ion Ratio Lower Upper
198 100
182 4.2 3.5 5.3
77 20.4 17.6 26.4

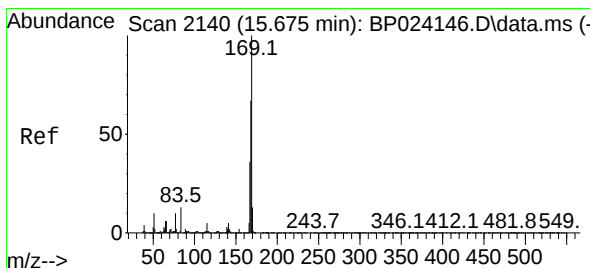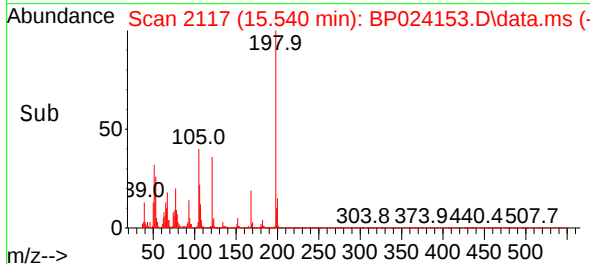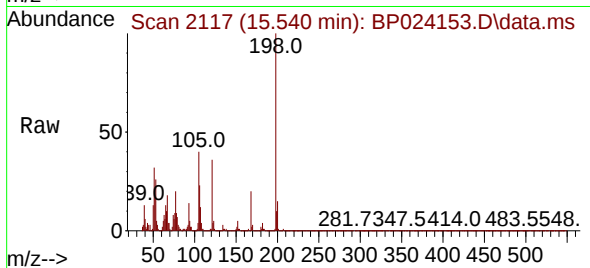

#67
N-Nitrosodiphenylamine
Concen: 21.561 ng/ul
RT: 15.669 min Scan# 2139
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:169 Resp: 1157274
Ion Ratio Lower Upper
169 100
168 66.8 53.4 80.0
167 36.4 29.0 43.4


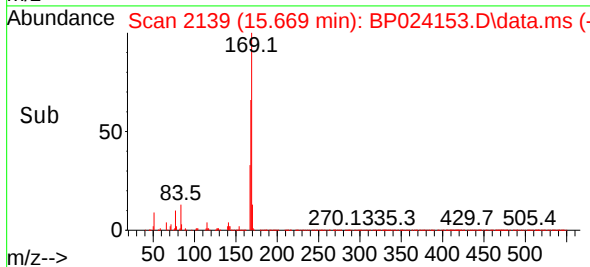

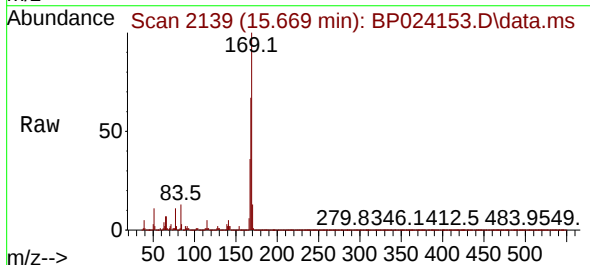




#68
4-Bromophenyl-phenylether
Concen: 21.522 ng/ul
RT: 16.369 min Scan# 2258
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:248 Resp: 417482
Ion Ratio Lower Upper
248 100
250 97.0 77.9 116.9
141 71.3 52.9 79.3

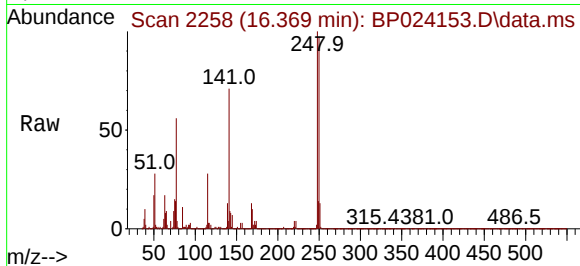

#69
Hexachlorobenzene
Concen: 21.303 ng/ul
RT: 16.486 min Scan# 2278
Delta R.T. 0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:284 Resp: 501954
Ion Ratio Lower Upper
284 100
142 30.9 27.7 41.5
249 29.1 24.9 37.3




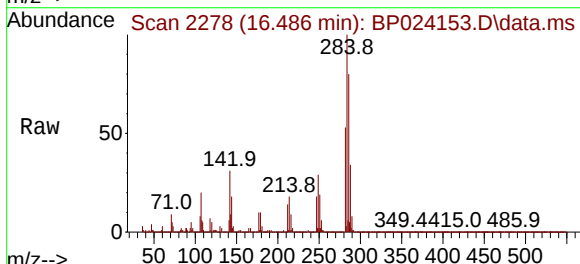




#70
Atrazine
Concen: 22.697 ng/ul
RT: 16.651 min Scan# 2306
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:200 Resp: 441060
Ion Ratio Lower Upper
200 100
173 27.0 21.9 32.9
215 48.8 40.4 60.6

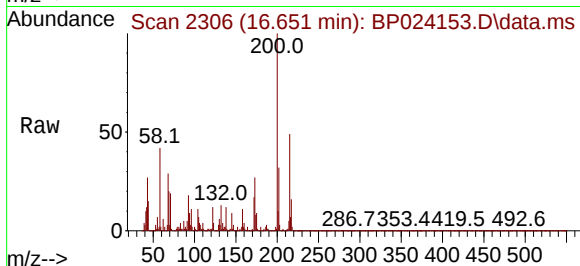

#71
Pentachlorophenol
Concen: 20.223 ng/ul
RT: 16.839 min Scan# 2338
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:266 Resp: 299087
Ion Ratio Lower Upper
266 100
264 63.4 50.6 76.0
268 62.9 50.6 76.0

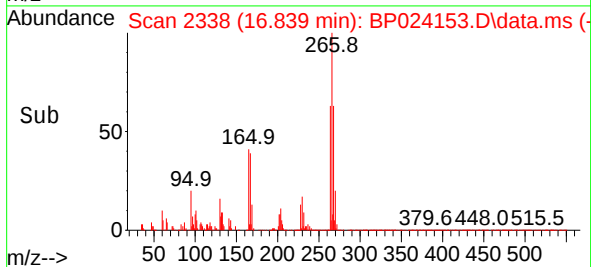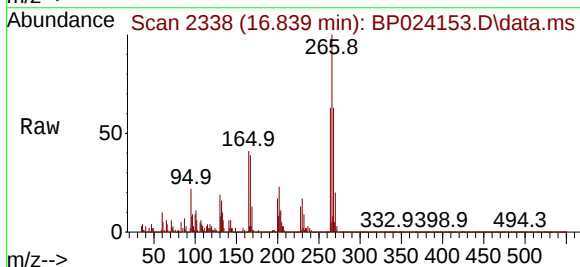



#72

Phenanthrene

Concen: 21.478 ng/ul

RT: 17.245 min Scan# 2406

Delta R.T. 0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:178 Resp: 2161655

Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.4

176 19.2 15.4 23.2

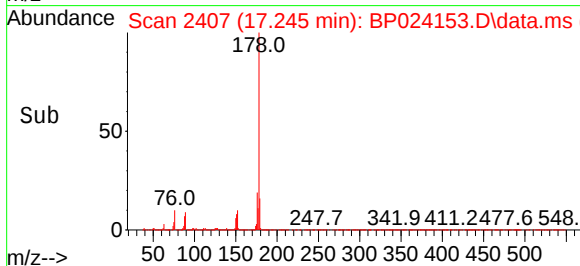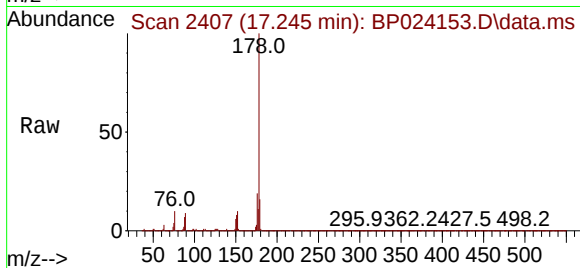

#74

Anthracene

Concen: 21.947 ng/ul

RT: 17.339 min Scan# 2423

Delta R.T. 0.006 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:178 Resp: 2225577


Ion Ratio Lower Upper

178 100

179 15.5 12.4 18.6

176 18.7 15.1 22.7


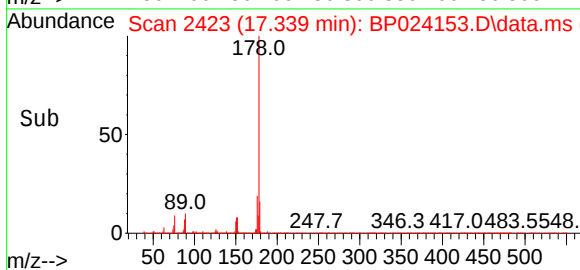

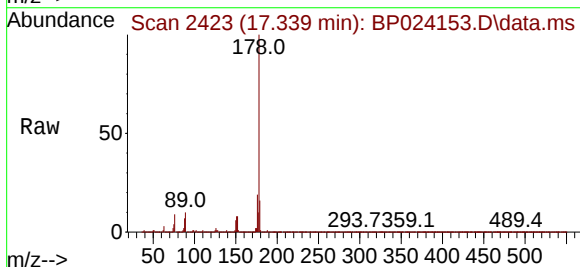


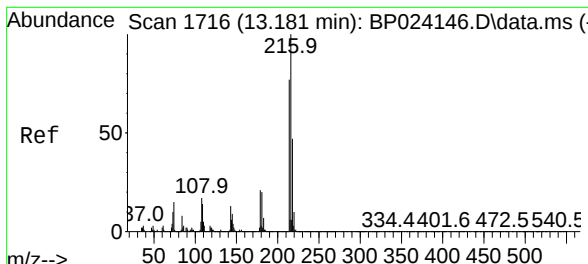

#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.926 ng/uL
RT: 13.181 min Scan# 1716
Delta R.T. 0.000 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:216 Resp: 528237
Ion Ratio Lower Upper
216 100
214 77.7 61.4 92.0
218 47.9 37.8 56.6

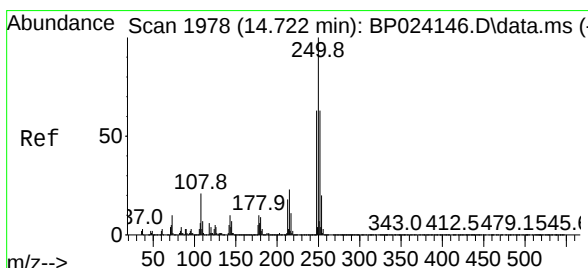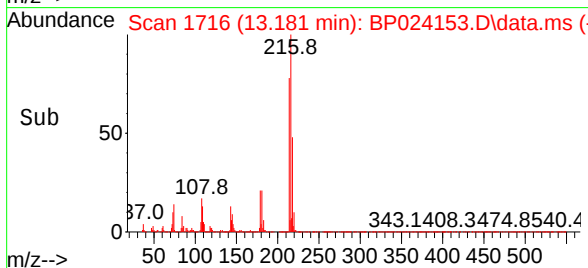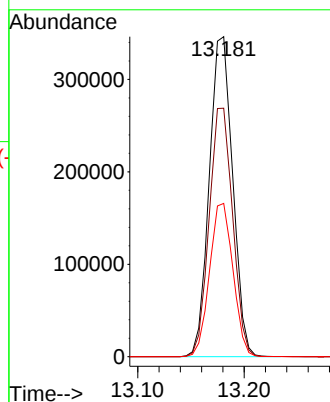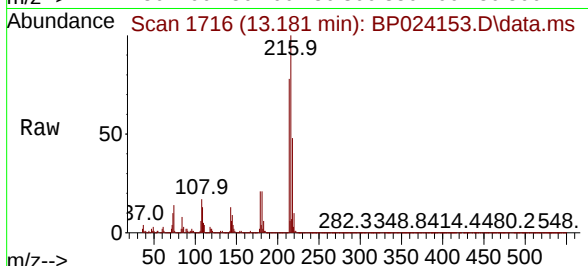

#76
Pentachlorobenzene
Concen: 20.757 ng/uL
RT: 14.716 min Scan# 1977
Delta R.T. -0.006 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:250 Resp: 575409
Ion Ratio Lower Upper
250 100
248 62.3 50.2 75.4
252 63.8 50.7 76.1


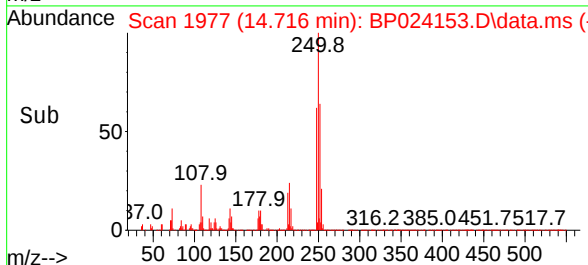

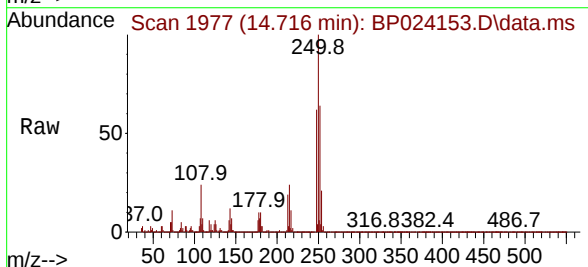




#77
 Carbazole
 Concen: 22.220 ng/ul
 RT: 17.622 min Scan# 2471
 Delta R.T. 0.006 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664


Tgt Ion:167 Resp: 2045814
 Ion Ratio Lower Upper
 167 100
 166 21.3 16.8 25.2
 139 12.9 10.2 15.4



#78
 Di-n-butylphthalate
 Concen: 22.176 ng/ul
 RT: 18.210 min Scan# 2571
 Delta R.T. 0.006 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16

Tgt Ion:149 Resp: 2378135
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.0
 104 5.1 3.8 5.8









#80
Fluoranthene
Concen: 22.507 ng/ul
RT: 19.333 min Scan# 21
Delta R.T. 0.012 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:202 Resp: 2549495
Ion Ratio Lower Upper
202 100
101 12.6 9.4 14.2
100 9.6 7.1 10.7

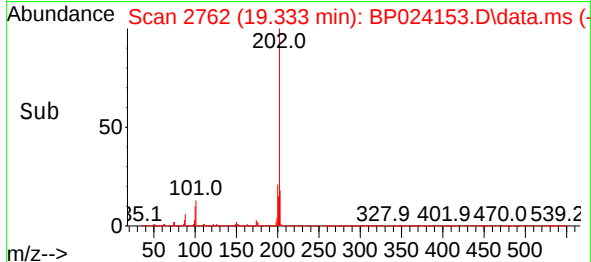

#82
Pyrene
Concen: 22.374 ng/ul
RT: 19.710 min Scan# 2826
Delta R.T. 0.012 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:202 Resp: 2731161
Ion Ratio Lower Upper
202 100
101 13.8 11.5 17.3
100 11.3 9.5 14.3

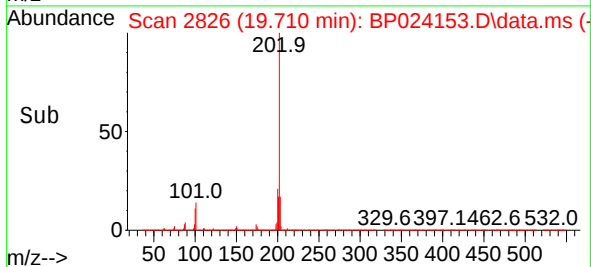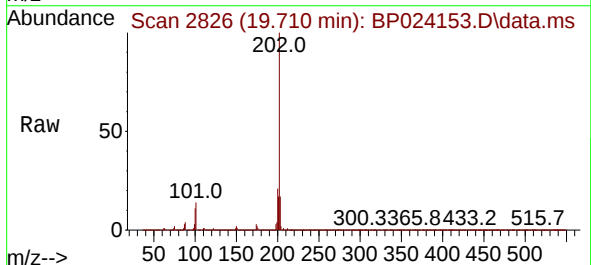



#83

Butylbenzylphthalate

Concen: 22.573 ng/ul

RT: 20.663 min Scan# 20

Delta R.T. 0.012 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:149 Resp: 1111040

Ion Ratio Lower Upper

149 100

91 69.2 53.0 79.4

206 20.8 17.6 26.4

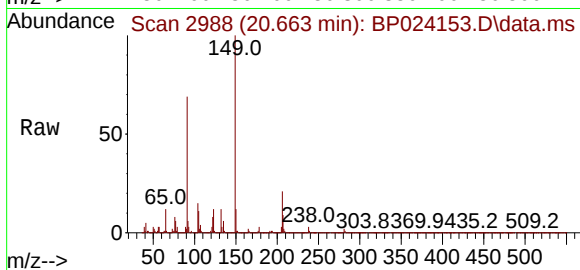

#84

3,3'-Dichlorobenzidine

Concen: 21.783 ng/ul

RT: 21.563 min Scan# 3141

Delta R.T. 0.018 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:252 Resp: 844994


Ion Ratio Lower Upper

252 100

254 65.4 51.2 76.8

126 11.0 9.3 13.9




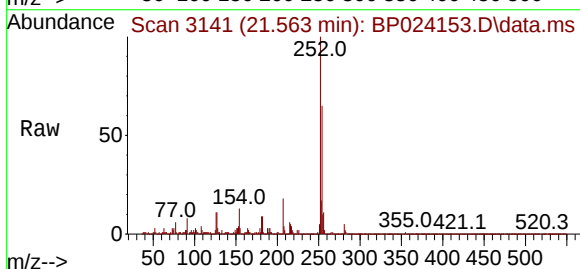




#85
Benzo(a)anthracene
Concen: 22.085 ng/ul
RT: 21.651 min Scan# 3156
Delta R.T. 0.024 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16




Instrument :
BNA_P
ClientSampleId :
SSTD020664


Tgt Ion:228 Resp: 2802375
Ion Ratio Lower Upper
228 100
229 19.8 15.7 23.5
226 27.3 21.4 32.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 22.013 ng/ul
RT: 21.586 min Scan# 3145
Delta R.T. 0.018 min
Lab File: BP024153.D
Acq: 04 Mar 2025 18:16

Tgt Ion:149 Resp: 1625985
Ion Ratio Lower Upper
149 100
167 27.3 22.2 33.4
279 4.5 3.7 5.5





#87

Chrysene

Concen: 21.952 ng/ul

RT: 21.716 min Scan# 3167

Delta R.T. 0.018 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:228 Resp: 2616292

Ion Ratio Lower Upper

228 100

226 29.9 24.2 36.4

229 19.6 15.8 23.6



#89

Di-n-octyl phthalate

Concen: 21.958 ng/ul




RT: 22.892 min Scan# 3367


Delta R.T. 0.029 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Tgt Ion:149 Resp: 2664199

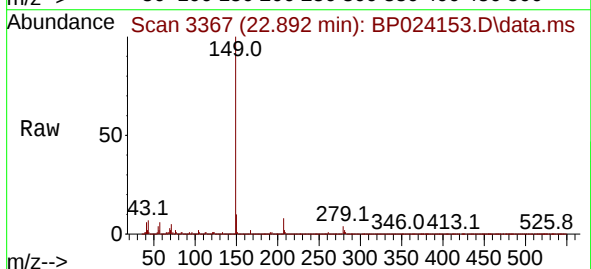



#90

Benzo(b)fluoranthene

Concen: 22.460 ng/ul

RT: 23.992 min Scan# 3554

Delta R.T. 0.029 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:252 Resp: 2776460

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 10.5 8.4 12.6



#91

Benzo(k)fluoranthene

Concen: 22.356 ng/ul

RT: 24.063 min Scan# 3566

Delta R.T. 0.024 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:252 Resp: 2805024


Ion Ratio Lower Upper

252 100

253 21.9 17.8 26.6

125 10.7 8.6 12.8





#93

Benzo(a)pyrene

Concen: 22.340 ng/ul

RT: 24.904 min Scan# 31

Delta R.T. 0.024 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16

Instrument :

BNA_P

ClientSampleId :

SSTD020664





Tgt Ion:252 Resp: 2611339

Ion Ratio Lower Upper

252 100

253 21.8 17.4 26.2

125 12.1 9.8 14.6

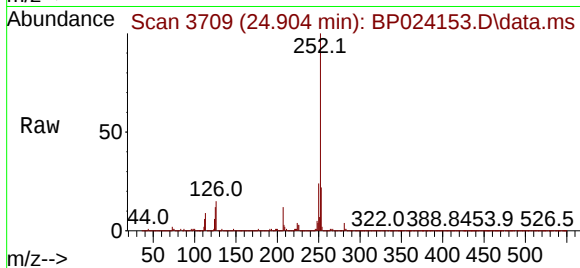

#94

Indeno(1,2,3-cd)pyrene

Concen: 21.056 ng/ul

RT: 28.927 min Scan# 4393

Delta R.T. 0.047 min

Lab File: BP024153.D

Acq: 04 Mar 2025 18:16




Tgt Ion:276 Resp: 3254499


Ion Ratio Lower Upper

276 100

138 21.0 16.2 24.4

277 23.8 18.9 28.3




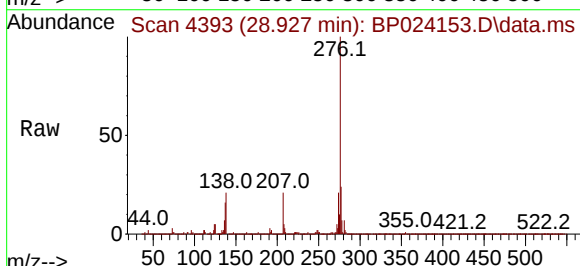


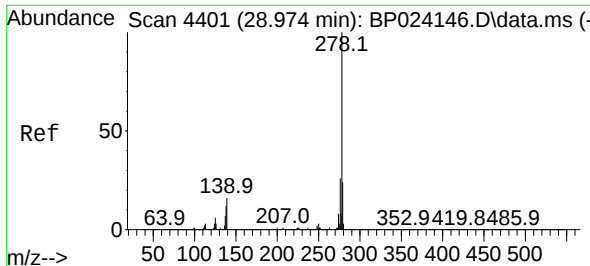

#95
 Dibenzo(a,h)anthracene
 Concen: 21.194 ng/ul
 RT: 28.992 min Scan# 4404
 Delta R.T. 0.018 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020664

Tgt Ion:278 Resp: 2659721
 Ion Ratio Lower Upper
 278 100
 139 17.0 12.4 18.6
 279 24.0 19.4 29.0

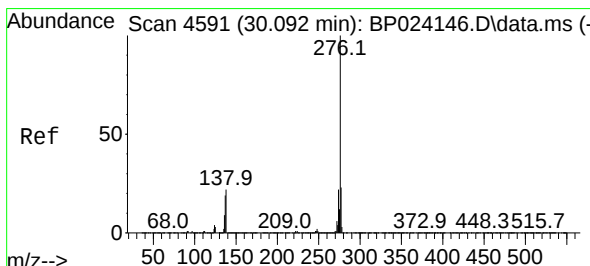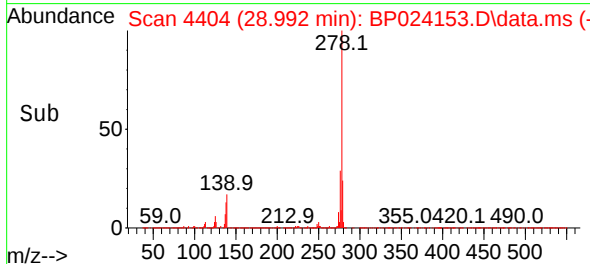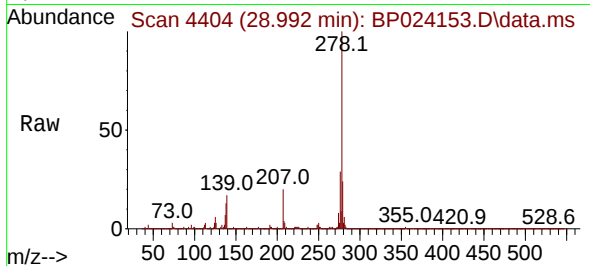

#96
 Benzo(g,h,i)perylene
 Concen: 21.019 ng/ul
 RT: 30.109 min Scan# 4594
 Delta R.T. 0.018 min
 Lab File: BP024153.D
 Acq: 04 Mar 2025 18:16

Tgt Ion:276 Resp: 2521054
 Ion Ratio Lower Upper
 276 100
 138 22.7 17.3 25.9
 277 23.8 18.7 28.1

