
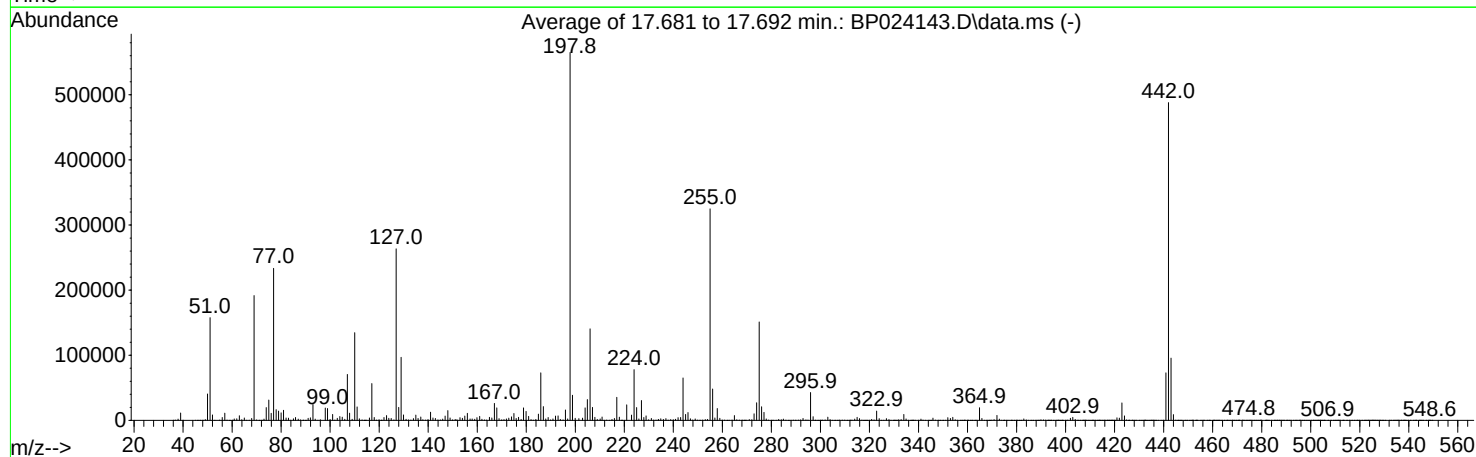


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030425\
Data File : BP024143.D
Acq On : 04 Mar 2025 08:57
Operator : RC/JU
Sample : DFTPP617
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP617

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Mar 04 14:51:41 2025

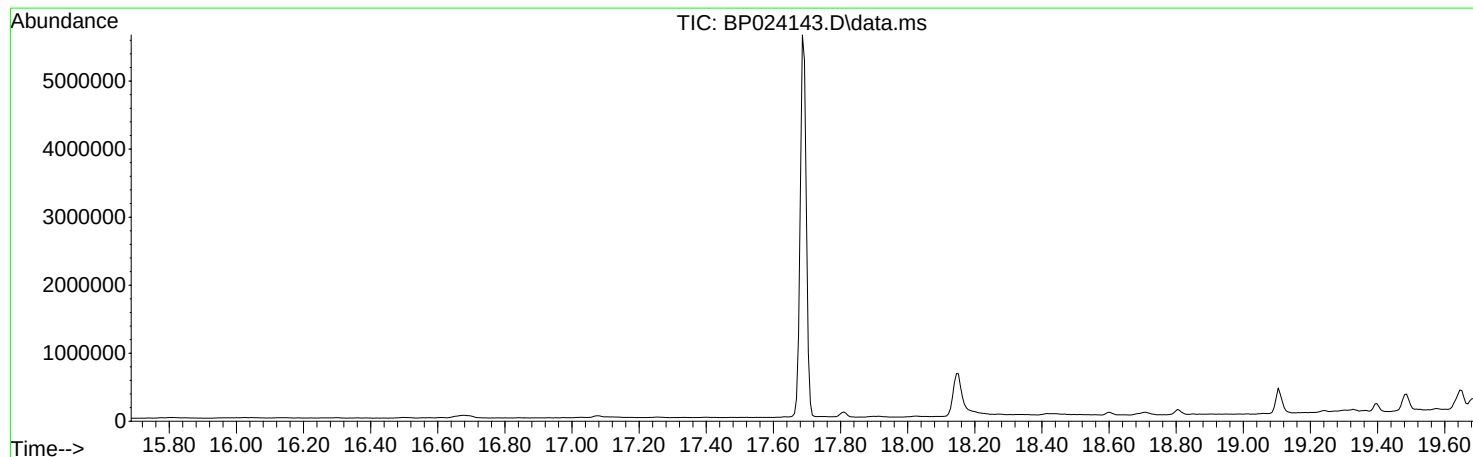

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.9	157900	PASS
68	69	0.00	2	1.5	2858	PASS
69	198	0.00	100	33.9	191679	PASS
70	69	0.00	2	0.4	816	PASS
127	198	10	80	46.6	263547	PASS
197	198	0.00	2	0.4	2354	PASS
198	198	100	100	100.0	564986	PASS
199	198	5	9	6.8	38577	PASS
275	198	10	60	26.8	151221	PASS
365	198	1	100	3.4	19427	PASS
441	198	0.01	100	12.9	72923	PASS
442	198	50	100	86.4	488021	PASS
443	442	15	24	19.6	95506	PASS