




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004908.D
Acq On : 05 Mar 2021 10:05
Operator : CG/JU
Sample : SSTD01081
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD01081

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:21:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 11:17:24 2021
Response via : Initial Calibration

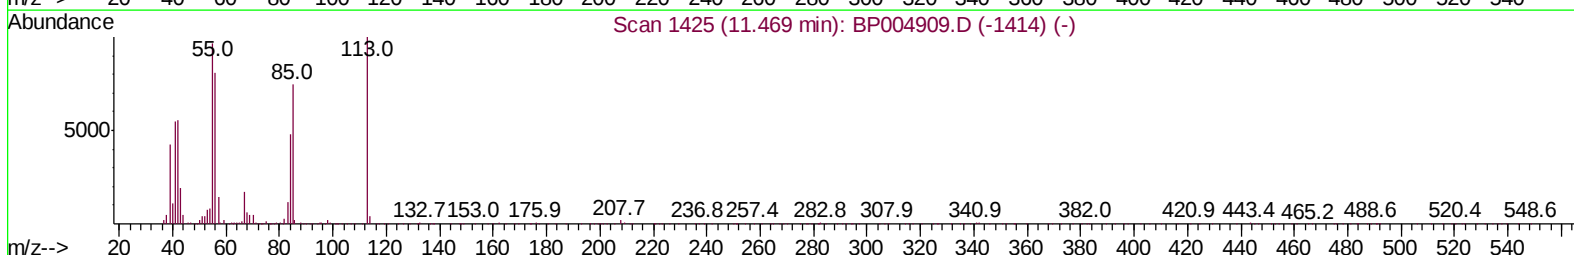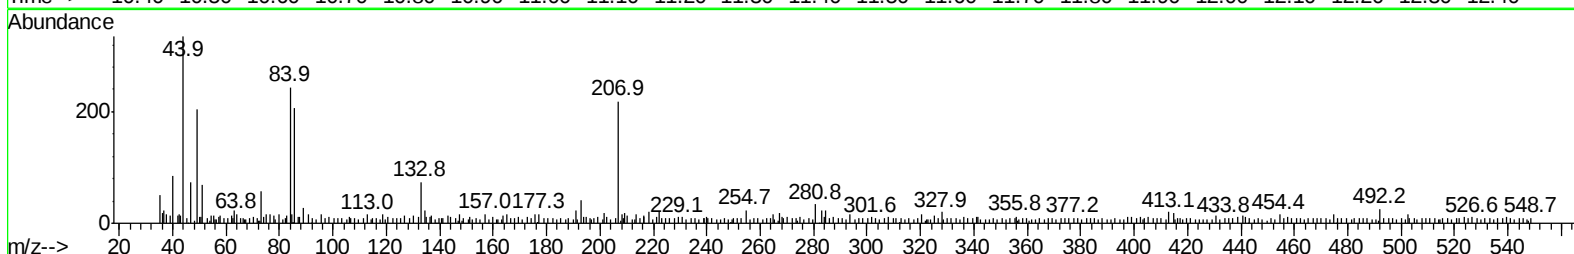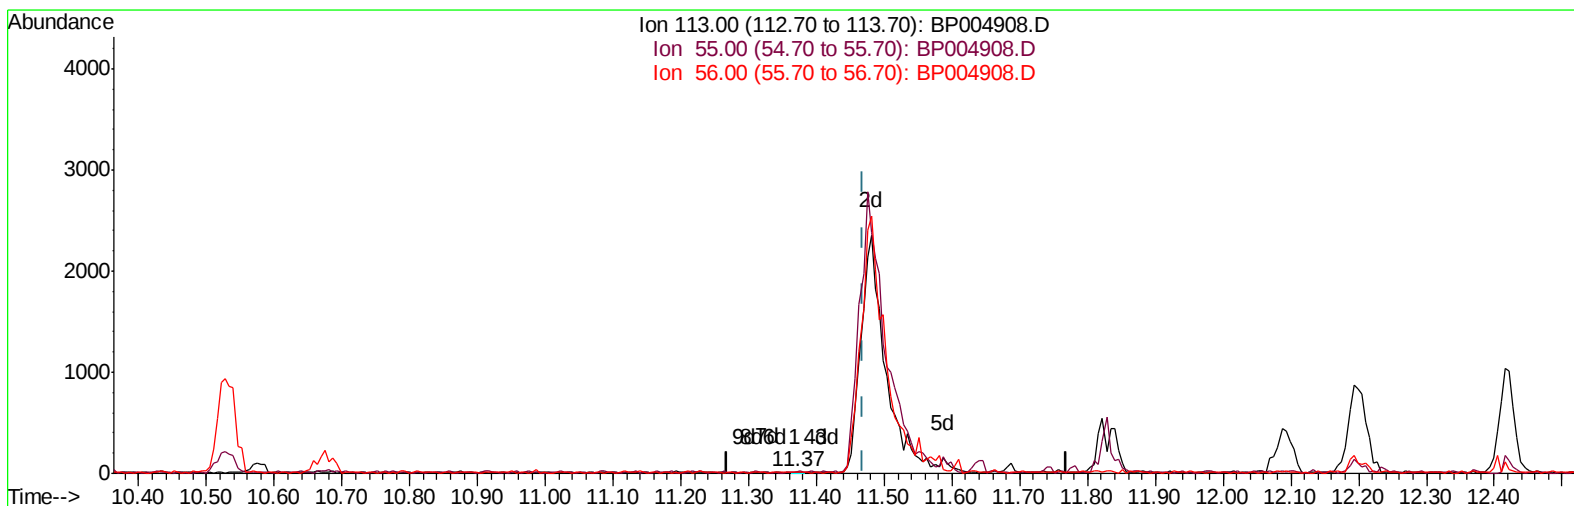

TIC: BP004908.D

(32) Caprolactam

11.369min (-0.100) 0.01ng/ul

response 10

Ion	Exp%	Act%
113.00	100	100
55.00	96.70	81.25
56.00	80.80	87.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
 Data File : BP004908.D
 Acq On : 05 Mar 2021 10:05
 Operator : CG/JU
 Sample : SST01081
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST01081

Manual Integrations
 APPROVED

mohammad
 3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:21:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 05 11:17:24 2021
 Response via : Initial Calibration

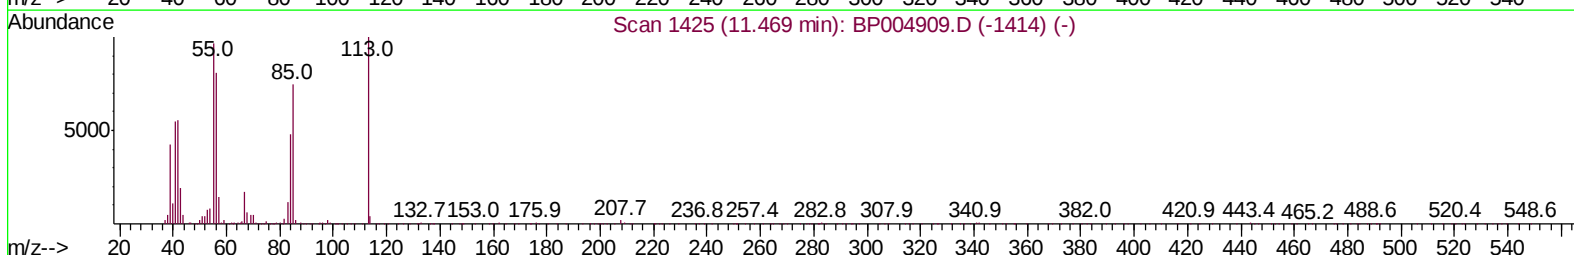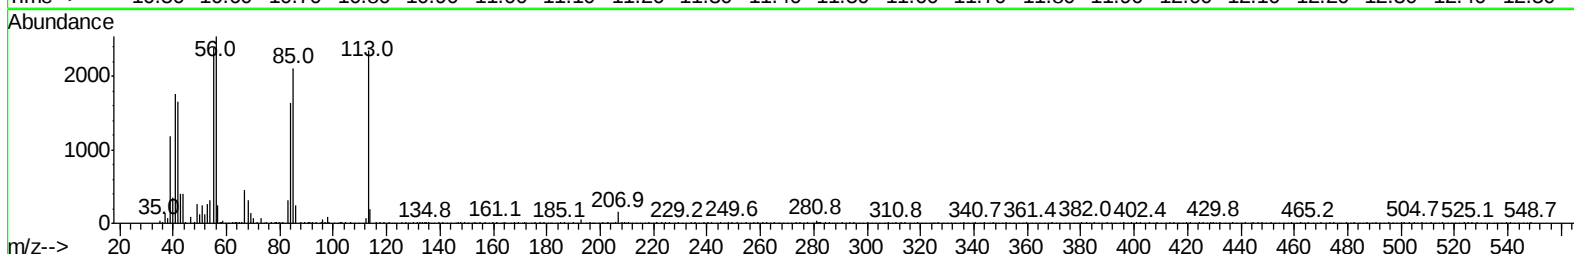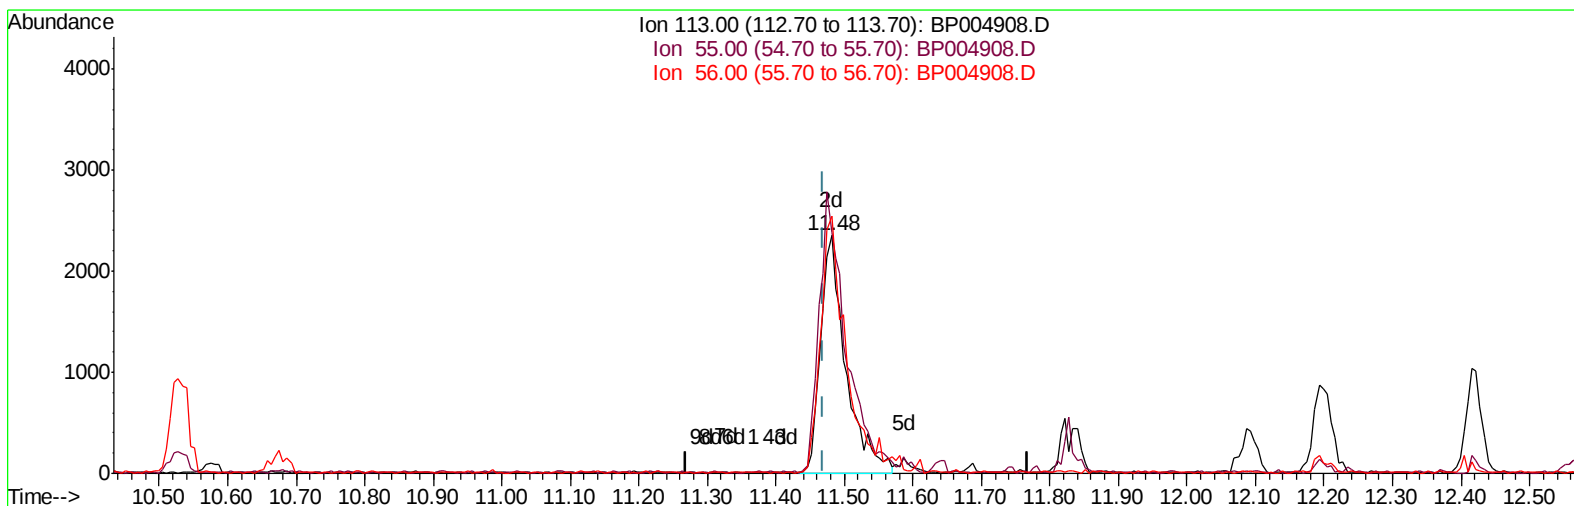

TIC: BP004908.D

(32) Caprolactam

11.481min (+0.012) 8.26ng/ul m

response 5959

Ion	Exp%	Act%
113.00	100	100
55.00	96.70	101.06
56.00	80.80	107.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
 Data File : BP004908.D
 Acq On : 05 Mar 2021 10:05
 Operator : CG/JU
 Sample : SSTD01081
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD01081

Manual Integrations
 APPROVED

mohammad
 3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:22:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 05 11:17:24 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	35037	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	139496	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	93650	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.15	188	219642	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	258802	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	271910	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	3526	3.96	ng/uL	0.00
5) Phenol-d5	6.91	99	24865	8.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	13781	9.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	20380	9.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	20374	8.96	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	10005	9.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	10556	9.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	21524	9.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	25499	10.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	66897	9.76	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	80912	9.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	9888	8.07	ng/ul	0.00
58) Fluorene-d10	15.39	176	60232	10.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.51	200	12277	8.57	ng/ul	0.00
71) Anthracene-d10	17.25	188	95582	9.60	ng/ul	0.00
79) Pyrene-d10	19.49	212	114107	9.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	134265	9.63	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.26	88	3277	3.382	ng/uL 92
4) Benzaldehyde	6.89	77	16611	11.391	ng/ul 92
6) Phenol	6.94	94	26478	8.828	ng/ul 96
8) Bis(2-Chloroethyl)ether	7.17	93	19987	9.054	ng/ul 92
10) 2-Chlorophenol	7.30	128	21326	9.251	ng/ul 99
11) 2-Methylphenol	8.19	108	20335	9.090	ng/ul 99
12) 2,2'-oxybis(1-Chloropropan	8.26	45	21990	15.408	ng/ul 98
14) Acetophenone	8.56	105	34734	9.241	ng/ul 95
15) N-Nitroso-di-n-propylamine	8.55	70	16388	9.013	ng/ul 91
16) 4-Methylphenol	8.51	108	21908	9.102	ng/ul 96
17) Hexachloroethane	8.82	117	9544	9.403	ng/ul 95
20) Nitrobenzene	8.94	77	26368	9.571	ng/ul 95
21) Isophorone	9.46	82	42808	9.082	ng/ul 97
23) 2-Nitrophenol	9.65	139	11900	9.270	ng/ul 95
24) 2,4-Dimethylphenol	9.71	107	27329	9.589	ng/ul 97
25) Bis(2-Chloroethoxy)methane	9.95	93	26962	9.473	ng/ul 99
27) 2,4-Dichlorophenol	10.18	162	21280	9.586	ng/ul 97
28) Naphthalene	10.58	128	72415	9.809	ng/ul 99
30) 4-Chloroaniline	10.70	127	25900	10.189	ng/ul 96
31) Hexachlorobutadiene	10.86	225	17878	10.994	ng/ul 96
32) Caprolactam	11.48	113	5959m	8.263	ng/ul
33) 4-Chloro-3-methylphenol	11.83	107	23842	9.432	ng/ul 95
34) 2-Methylnaphthalene	12.20	142	51783	9.859	ng/ul 98

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
 Data File : BP004908.D
 Acq On : 05 Mar 2021 10:05
 Operator : CG/JU
 Sample : SSTD01081
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 SSTD01081

Manual Integrations
 APPROVED

mohammad
 3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:22:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 05 11:17:24 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.42	142	48978	9.596	ng/ul	97
37) 1,2,4,5-Tetrachlorobenzene	12.57	216	32217	10.731	ng/ul	96
38) Hexachlorocyclopentadiene	12.55	237	18303	9.567	ng/ul	93
39) 2,4,6-Trichlorophenol	12.82	196	18710	9.950	ng/ul	93
40) 2,4,5-Trichlorophenol	12.89	196	20575	10.210	ng/ul	95
41) 1,1'-Biphenyl	13.22	154	69280	9.881	ng/ul	99
42) 2-Chloronaphthalene	13.26	162	54776	9.940	ng/ul	98
43) 2-Nitroaniline	13.47	65	13763	8.727	ng/ul	99
45) Dimethylphthalate	13.85	163	70074	9.950	ng/ul	97
46) 2,6-Dinitrotoluene	13.97	165	13033	9.254	ng/ul	96
48) Acenaphthylene	14.11	152	78920	9.827	ng/ul	98
49) 3-Nitroaniline	14.30	138	11189	8.701	ng/ul	98
50) Acenaphthene	14.46	153	57657	9.887	ng/ul	99
51) 2,4-Dinitrophenol	14.51	184	7069	7.805	ng/ul#	84
53) 4-Nitrophenol	14.62	109	11134	8.367	ng/ul	88
54) Dibenzofuran	14.79	168	85180	10.093	ng/ul	98
55) 2,4-Dinitrotoluene	14.76	165	19362	9.331	ng/ul#	90
56) 2,3,4,6-Tetrachlorophenol	15.02	232	19405	10.904	ng/ul#	94
57) Diethylphthalate	15.22	149	67888	9.532	ng/ul	98
59) Fluorene	15.45	166	70527	10.020	ng/ul	98
60) 4-Chlorophenyl-phenylether	15.44	204	40134	10.826	ng/ul	93
61) 4-Nitroaniline	15.47	138	12755	8.682	ng/ul#	83
64) 4,6-Dinitro-2-methylphenol	15.52	198	12716	8.760	ng/ul#	93
65) N-Nitrosodiphenylamine	15.66	169	60534	9.386	ng/ul	98
66) 4-Bromophenyl-phenylether	16.34	248	24166	10.401	ng/ul	95
67) Hexachlorobenzene	16.45	284	28396	10.647	ng/ul	98
68) Atrazine	16.62	200	23145	9.156	ng/ul	96
69) Pentachlorophenol	16.80	266	14822	9.068	ng/ul	91
70) Phenanthrene	17.19	178	115044	9.637	ng/ul	98
72) Anthracene	17.28	178	117799	9.666	ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.18	216	32234	9.857	ng/uL	96
74) Pentachlorobenzene	14.71	250	33472	10.509	ng/uL	95
75) Carbazole	17.56	167	98755	9.214	ng/ul	97
76) Di-n-butylphthalate	18.12	149	111279	8.783	ng/ul	99
77) Fluoranthene	19.17	202	139030	9.709	ng/ul	100
80) Pvrene	19.52	202	149463	9.350	ng/ul	99
81) Butylbenzylphthalate	20.40	149	49522	7.939	ng/ul	96
82) 3,3'-Dichlorobenzidine	21.16	252	47320	8.779	ng/ul	99
83) Benzo(a)anthracene	21.23	228	156301	9.774	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.16	149	73759	7.914	ng/ul	97
85) Chrysene	21.27	228	152002	9.756	ng/ul	99
87) Di-n-octyl phthalate	22.04	149	129883	7.096	ng/ul	100
88) Benzo(b)fluoranthene	22.84	252	166097	9.607	ng/ul	98
89) Benzo(k)fluoranthene	22.89	252	162439	9.501	ng/ul	99
91) Benzo(a)pyrene	23.43	252	146684	9.663	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.89	276	187757	9.664	ng/ul	98
93) Dibenzo(a,h)anthracene	25.90	278	159153	9.631	ng/ul	98
94) Benzo(a,h,i)perylene	26.62	276	156977	9.706	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004908.D
Acq On : 05 Mar 2021 10:05
Operator : CG/JU
Sample : SSTD01081
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD01081

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:22:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 11:17:24 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004908.D
Acq On : 05 Mar 2021 10:05
Operator : CG/JU
Sample : SST01081
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
Client Sampled :
SST01081

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:11 AM

Quant Time: Mar 05 11:22:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 11:17:24 2021
Response via : Initial Calibration

