




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004923.D
Acq On : 05 Mar 2021 18:59
Operator : CG/JU
Sample : PB134931BL
Misc : SOM-MDL-ME-S-BL-04
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK31

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:50 AM

Quant Time: Mar 05 23:07:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 22:20:13 2021
Response via : Initial Calibration

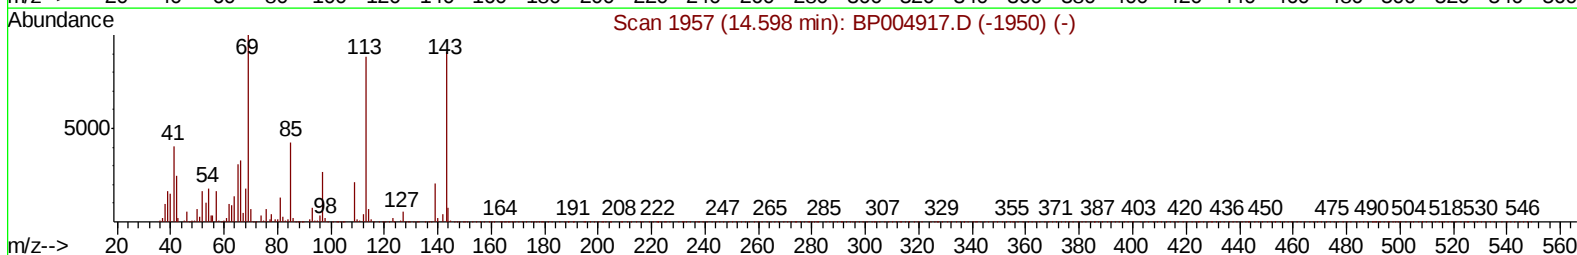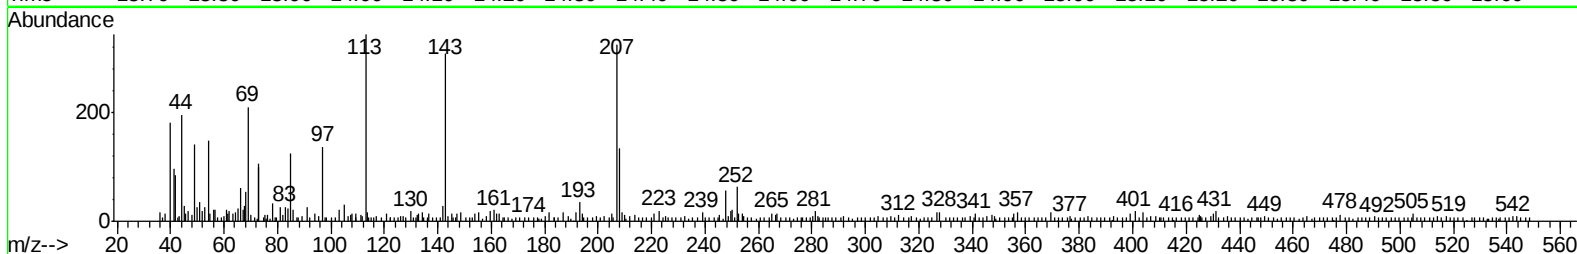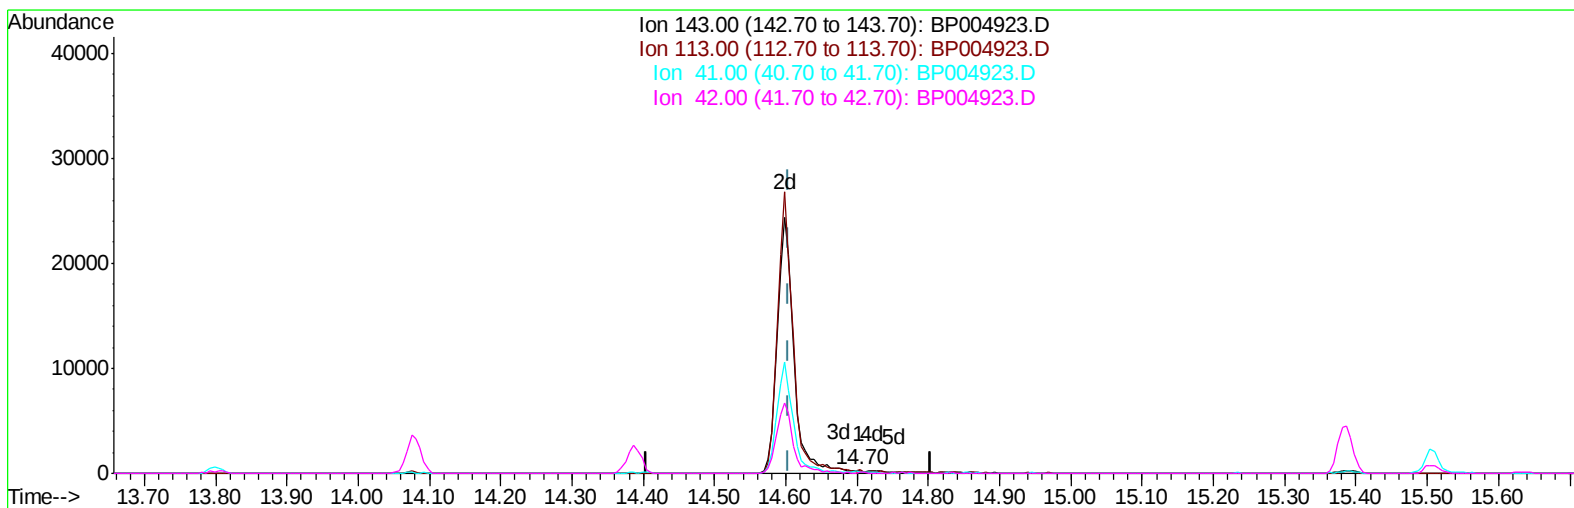

TIC: BP004923.D

(52) 4-Nitrophenol-d4 (S)

14.704min (+0.100) 0.08ng/ul

response 90

Ion	Exp%	Act%
143.00	100	100
113.00	100.70	111.00
41.00	34.00	31.39
42.00	24.20	27.51




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004923.D
Acq On : 05 Mar 2021 18:59
Operator : CG/JU
Sample : PB134931BL
Misc : SOM-MDL-ME-S-BL-04
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK31

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:50 AM

Quant Time: Mar 05 23:07:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 22:20:13 2021
Response via : Initial Calibration

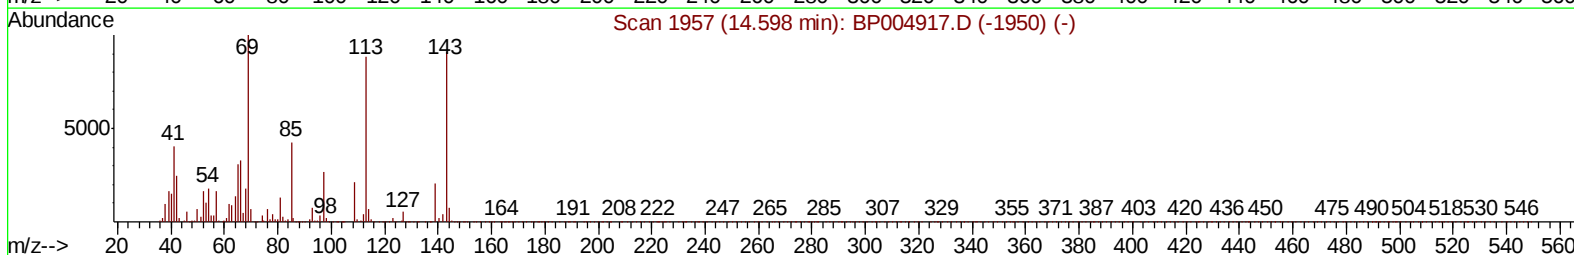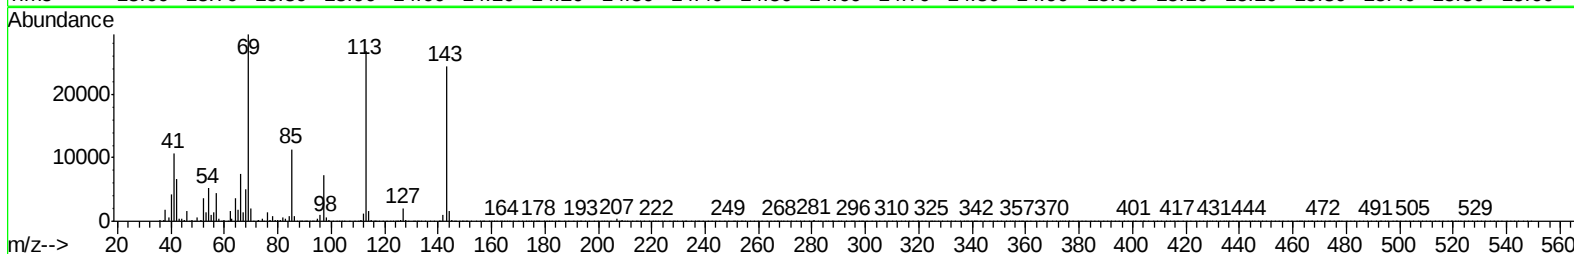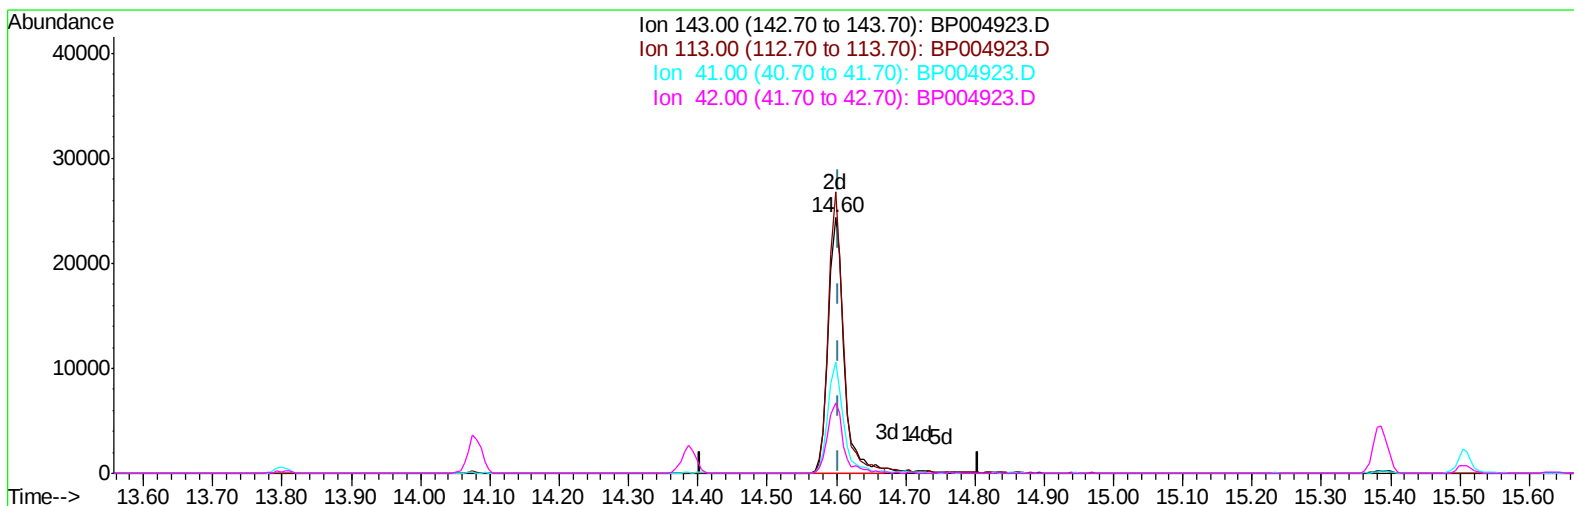

TIC: BP004923.D

(52) 4-Nitrophenol-d4 (S)

14.598min (-0.006) 33.94ng/ul m

response 38407

Ion	Exp%	Act%
143.00	100	100
113.00	100.70	110.12
41.00	34.00	43.57#
42.00	24.20	27.75

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
 Data File : BP004923.D
 Acq On : 05 Mar 2021 18:59
 Operator : CG/JU
 Sample : PB134931BL
 Misc : SOM-MDL-ME-S-BL-04
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK31

Manual Integrations
 APPROVED

mohammad
 3/8/2021 9:36:50 AM

Quant Time: Mar 05 23:12:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 05 22:20:13 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	33356	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	135936	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	89599	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.15	188	206618	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	225029	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	236569	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	5319	6.47	ng/uL	0.00
5) Phenol-d5	6.91	99	87369	34.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	48197	36.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	70574	34.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	71807	34.85	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	35507	36.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	39241	35.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	71487	32.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	95944	40.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	252398	39.16	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	289533	36.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	38407m	33.94	ng/ul	0.00
58) Fluorene-d10	15.39	176	212492	36.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.51	200	44234	32.70	ng/ul	0.00
71) Anthracene-d10	17.25	188	354958	38.26	ng/ul	0.00
79) Pyrene-d10	19.49	212	422374	41.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	475688	39.56	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP030521\
Data File : BP004923.D
Acq On : 05 Mar 2021 18:59
Operator : CG/JU
Sample : PB134931BL
Misc : SOM-MDL-ME-S-BL-04
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK31

Manual Integrations
APPROVED

mohammad
3/8/2021 9:36:50 AM

Quant Time: Mar 05 23:12:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030521MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 05 22:20:13 2021
Response via : Initial Calibration

