
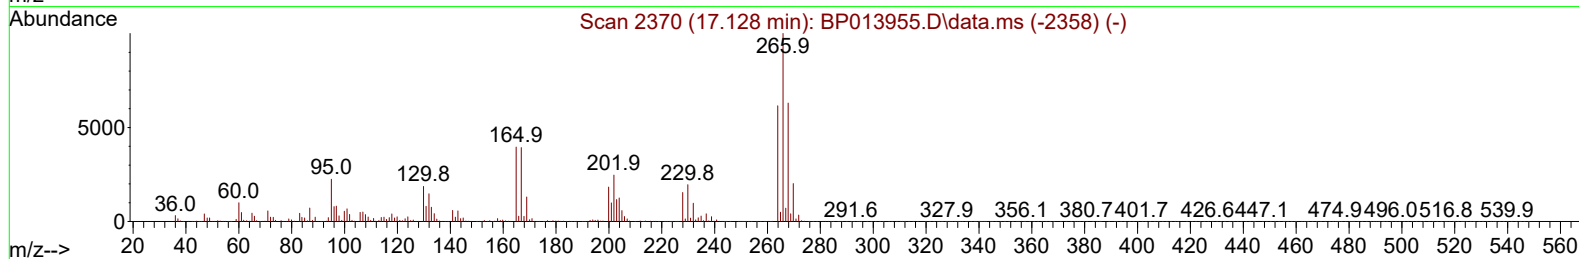
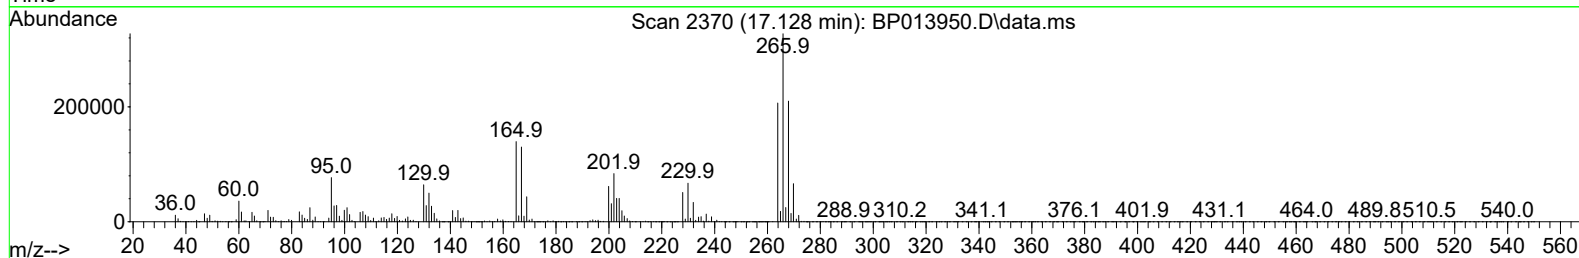


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030623\
Data File : BP013950.D
Acq On : 06 Mar 2023 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:18:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:35:43 2023
Response via : Initial Calibration

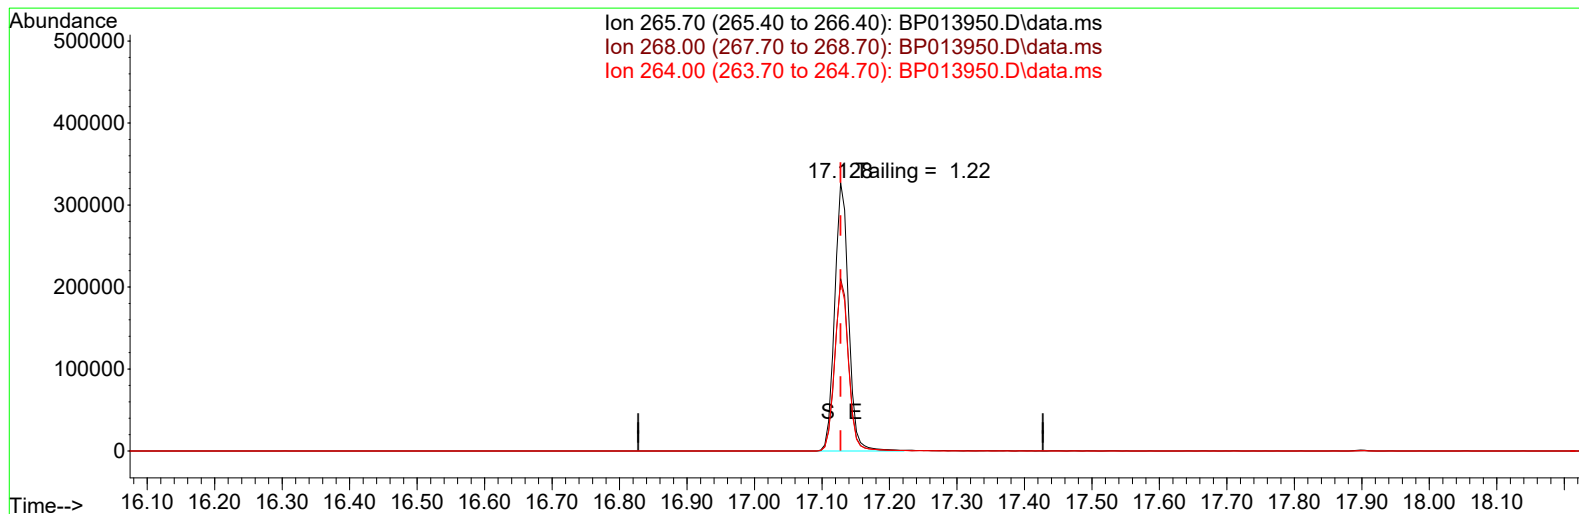

TIC: BP013950.D\data.ms

(70) Pentachlorophenol (C)




17.128min (0.000) 233515.23 ng

response 468007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.16
264.00	61.50	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030623\
Data File : BP013950.D
Acq On : 06 Mar 2023 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:18:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:35:43 2023
Response via : Initial Calibration

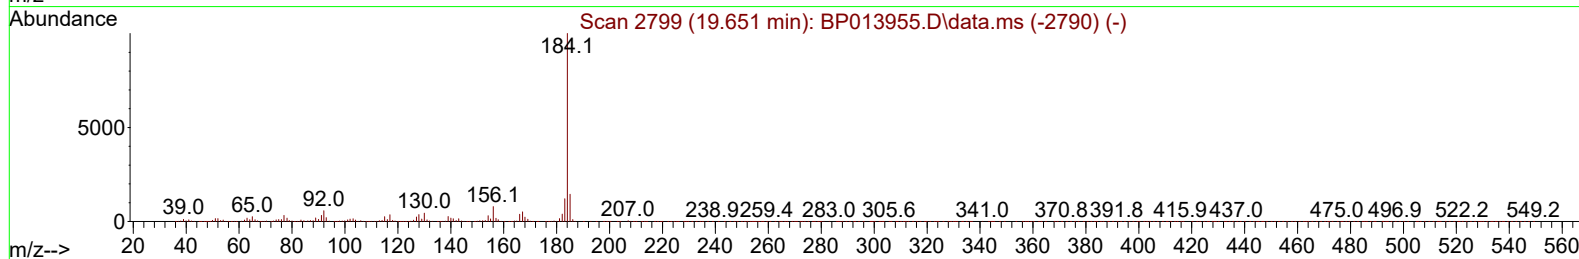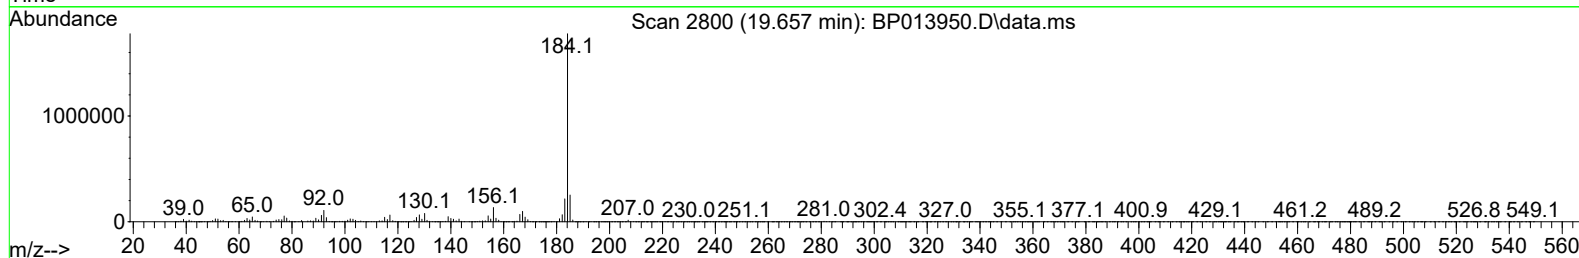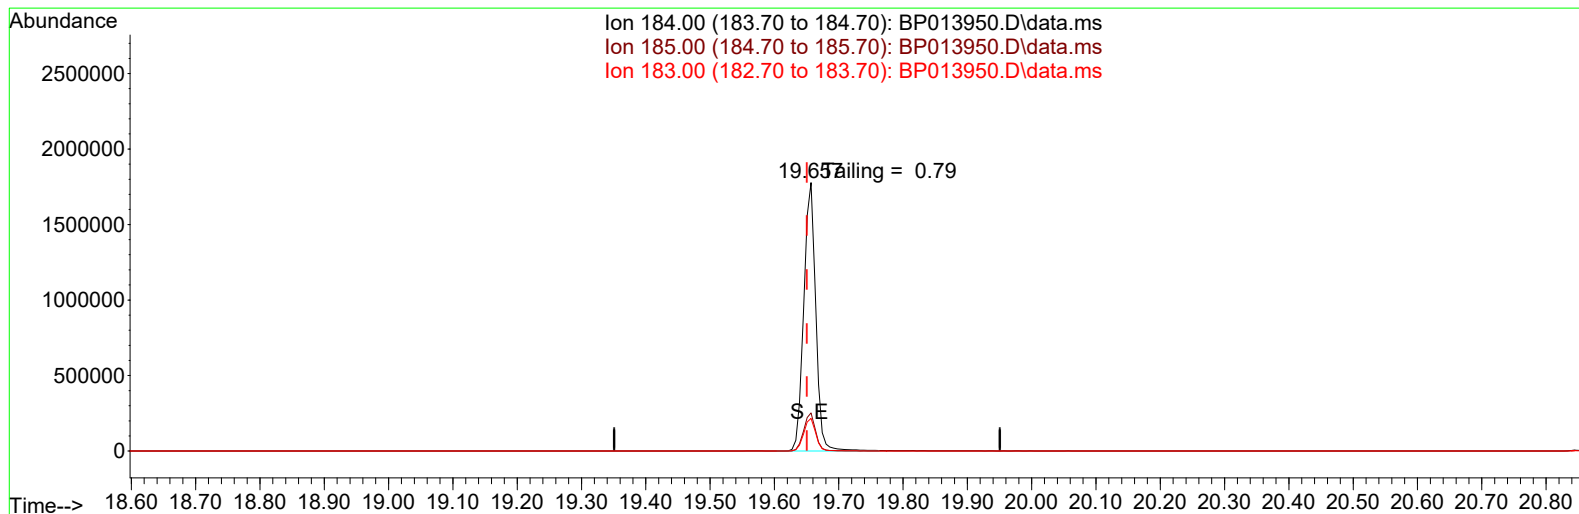

TIC: BP013950.D\data.ms

(77) Benzidine

19.657min (+ 0.006) -20.00 ng

response 2320243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.24
183.00	12.10	12.17
0.00	0.00	0.00