
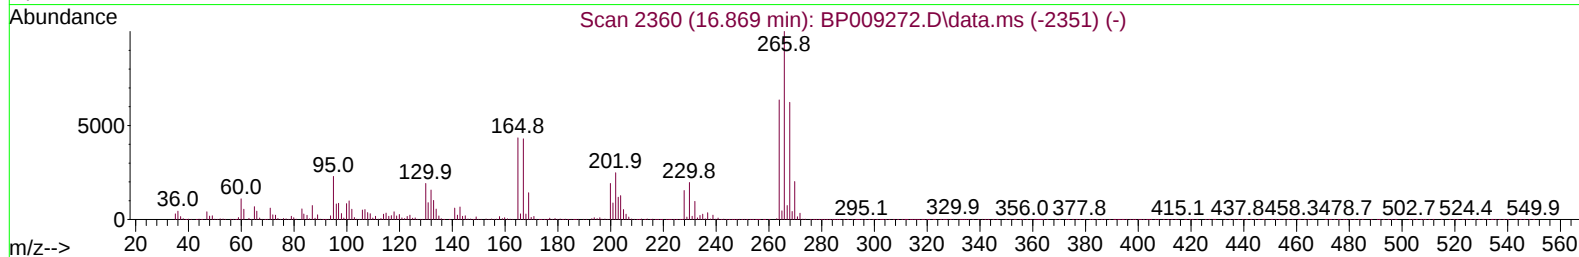
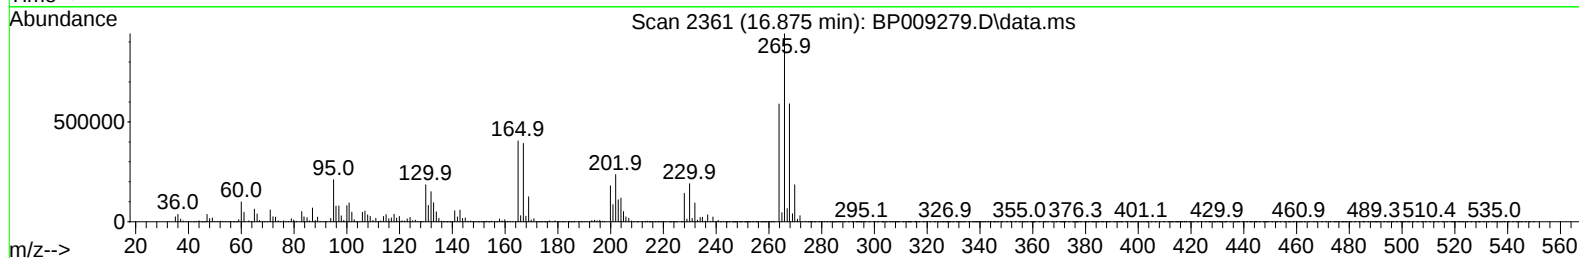


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009279.D
Acq On : 07 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 16:29:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

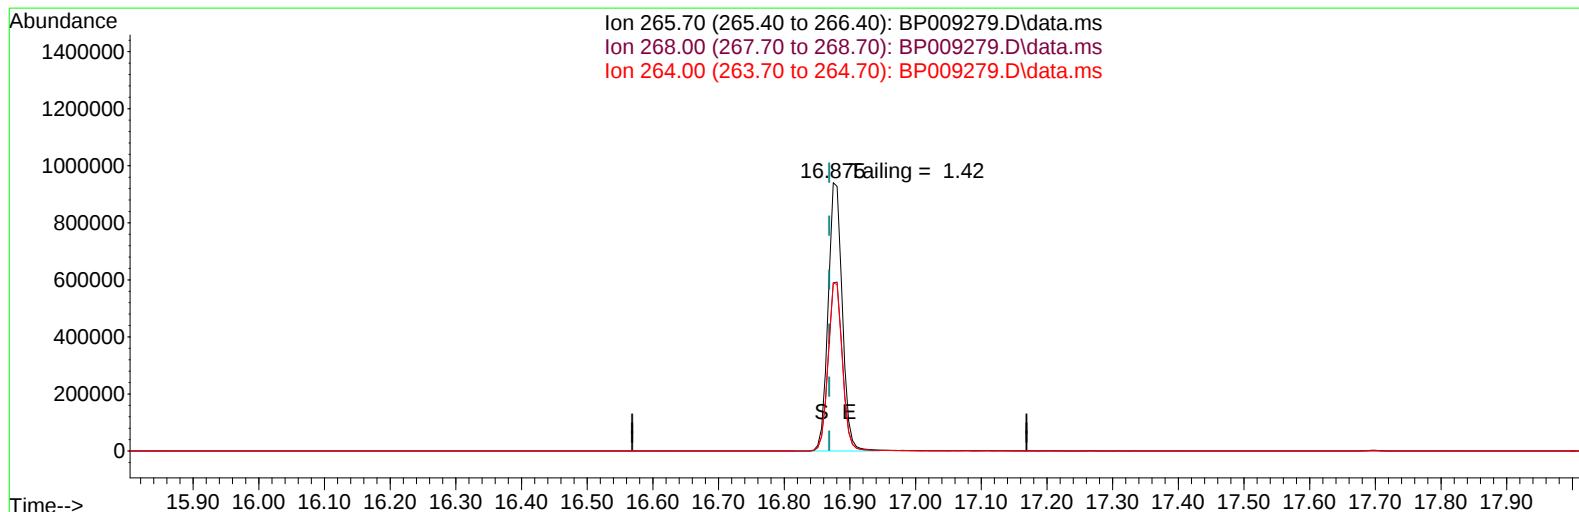

TIC: BP009279.D\data.ms

(70) Pentachlorophenol (C)




16.875min (+ 0.006) 936837.16 ng

response 1412800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.69
264.00	63.60	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009279.D
Acq On : 07 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 16:29:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

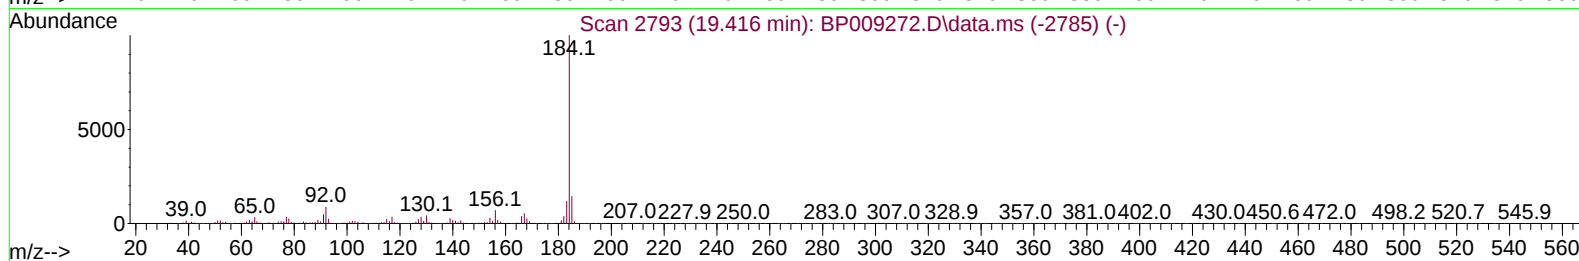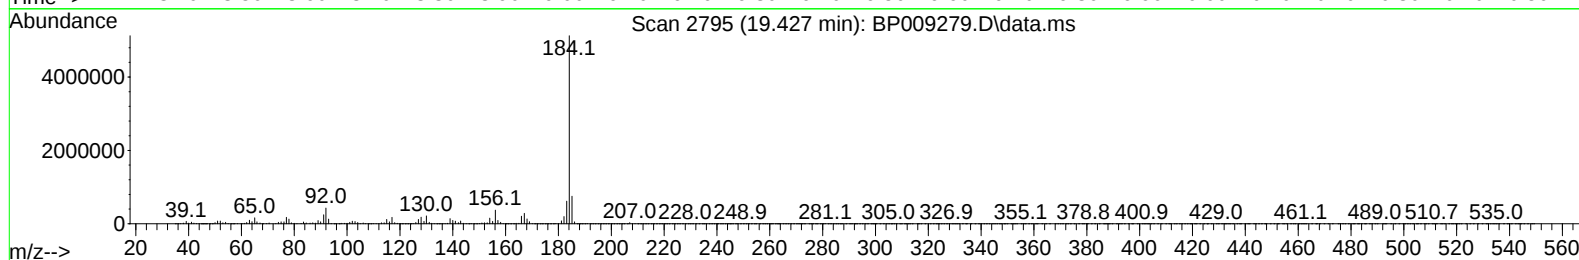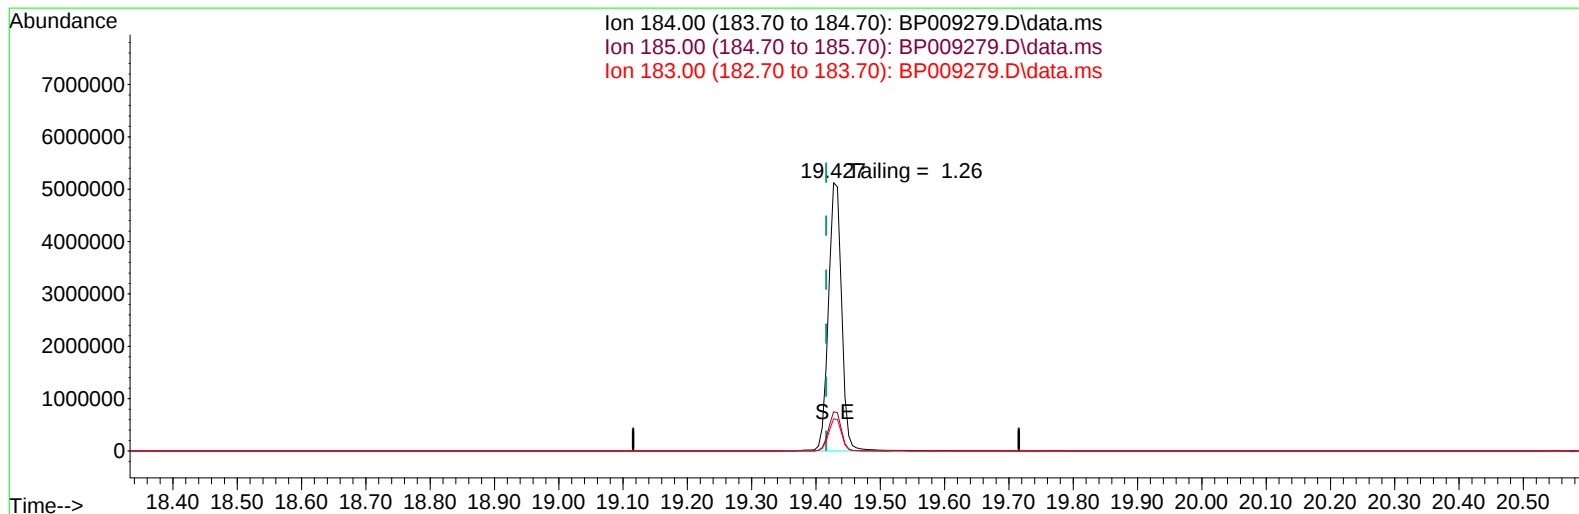

TIC: BP009279.D\data.ms

(77) Benzidine

19.427min (+ 0.012) 2091.51 ng

response 7317501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.62
183.00	11.70	11.99
0.00	0.00	0.00