

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
 Data File : BP009281.D
 Acq On : 07 Mar 2022 11:27
 Operator : CG/JU
 Sample : PB143105BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143105BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	405	413	426	rBV	6869458	11079575	48.31%	10.699%
2	6.993	672	681	695	rBV	6432004	11093342	48.37%	10.712%
3	7.822	814	822	830	rBV	1369477	2322815	10.13%	2.243%
4	8.975	1008	1018	1027	rBV	4004773	6981224	30.44%	6.741%
5	10.616	1284	1297	1306	rBV	1734439	3154012	13.75%	3.046%
6	13.087	1708	1717	1730	rBV	10130971	16481258	71.87%	15.915%
7	14.457	1942	1950	1959	rBV	2437459	3914734	17.07%	3.780%
8	15.951	2196	2204	2220	rBV	7458838	10867259	47.39%	10.494%
9	17.216	2412	2419	2429	rBV	2960829	4504576	19.64%	4.350%
10	19.798	2851	2858	2868	rBV	16784023	22932457	100.00%	22.144%
11	21.322	3112	3117	3124	rBV	3848534	4962967	21.64%	4.792%
12	23.727	3520	3526	3538	rVB2	2462156	5264582	22.96%	5.084%




Sum of corrected areas: 103558801

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009281.D
Acq On : 07 Mar 2022 11:27
Operator : CG/JU
Sample : PB143105BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143105BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

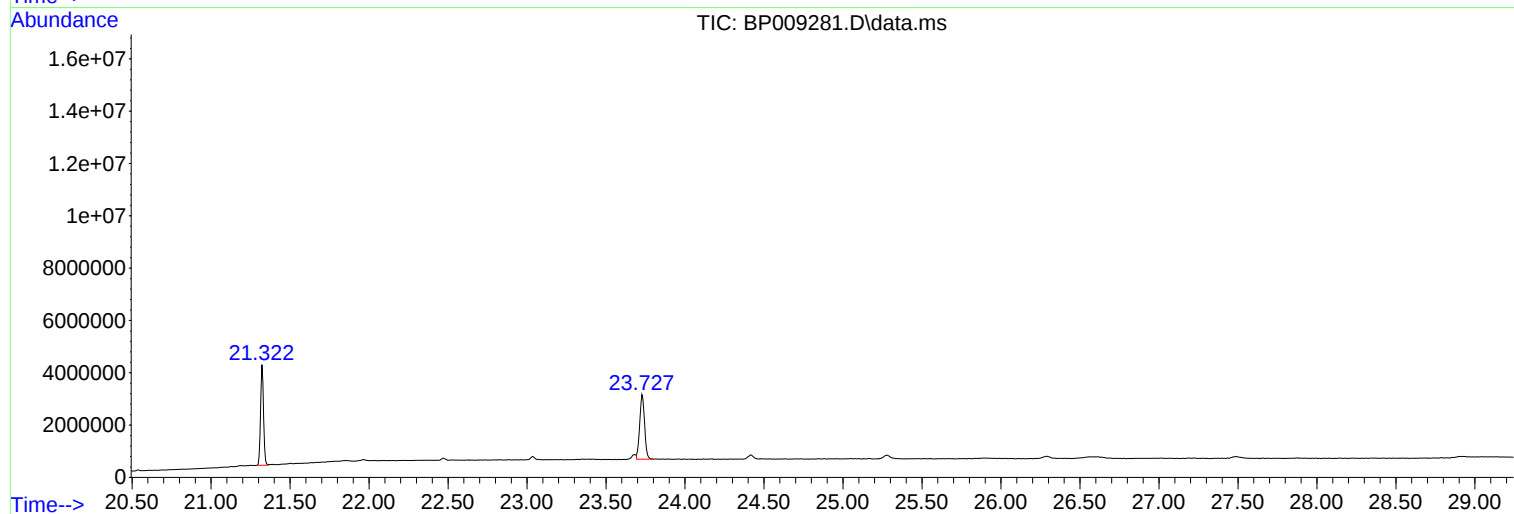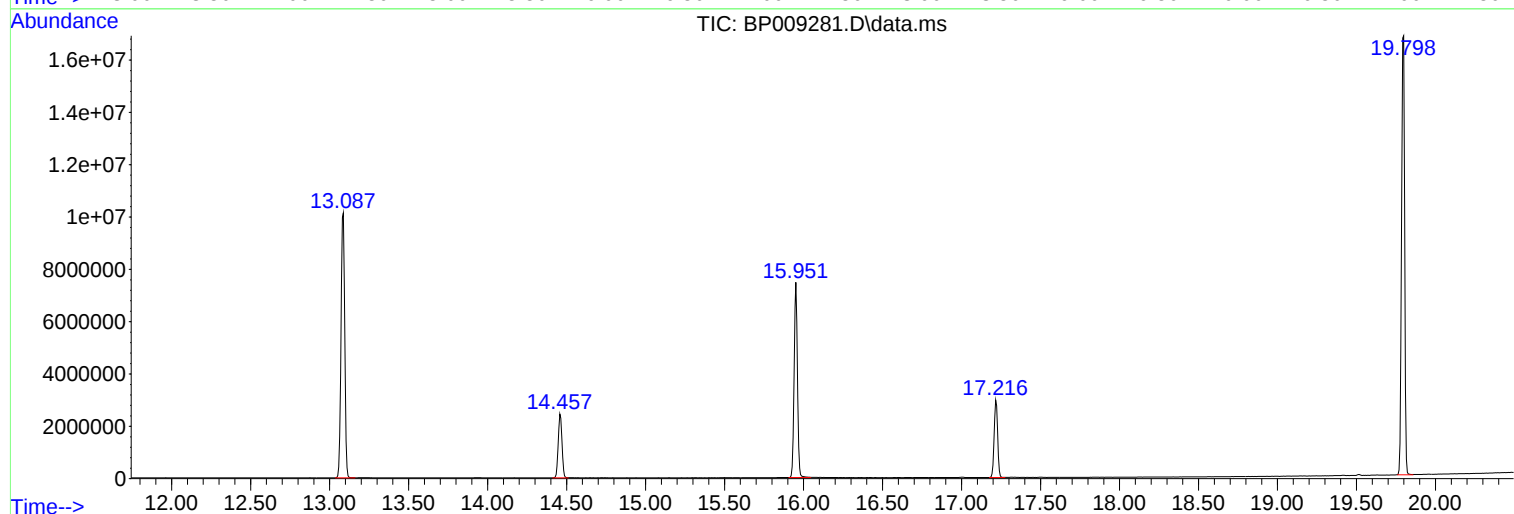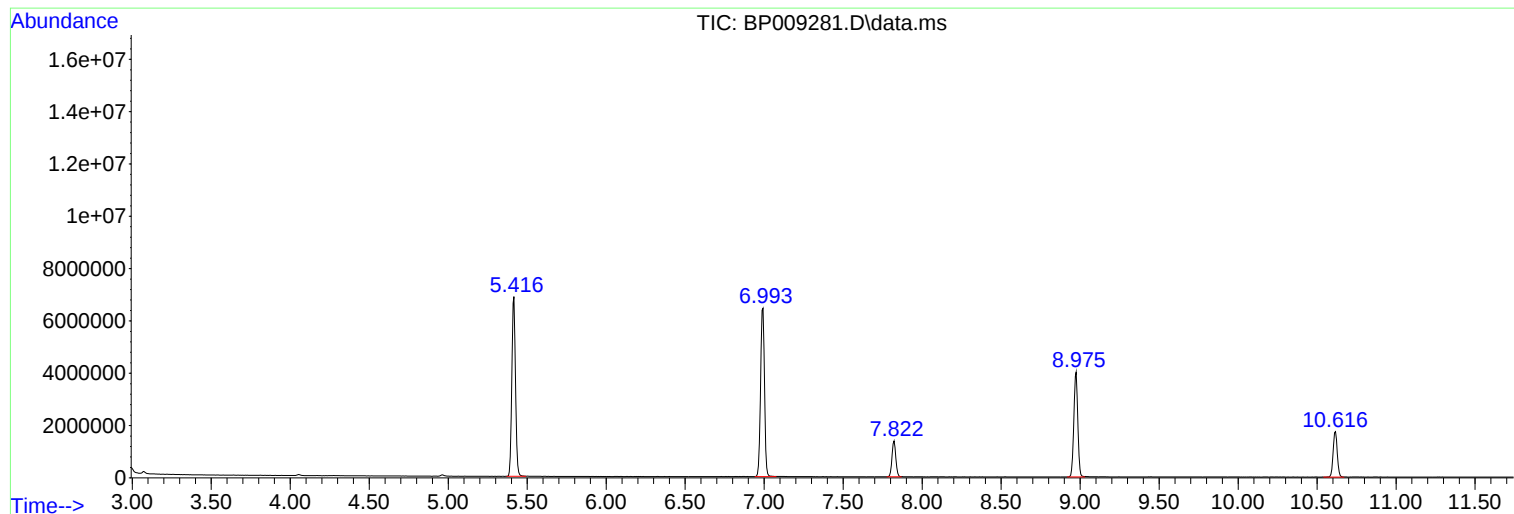

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009281.D
Acq On : 07 Mar 2022 11:27
Operator : CG/JU
Sample : PB143105BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143105BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009281.D
Acq On : 07 Mar 2022 11:27
Operator : CG/JU
Sample : PB143105BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143105BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------