
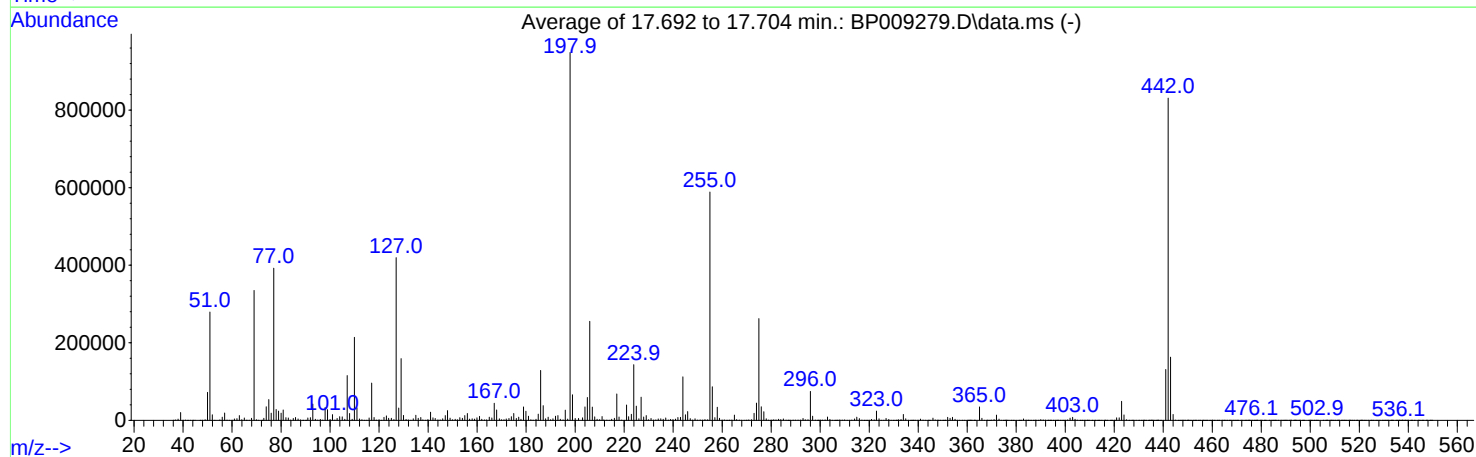


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
 Data File : BP009279.D
 Acq On : 07 Mar 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

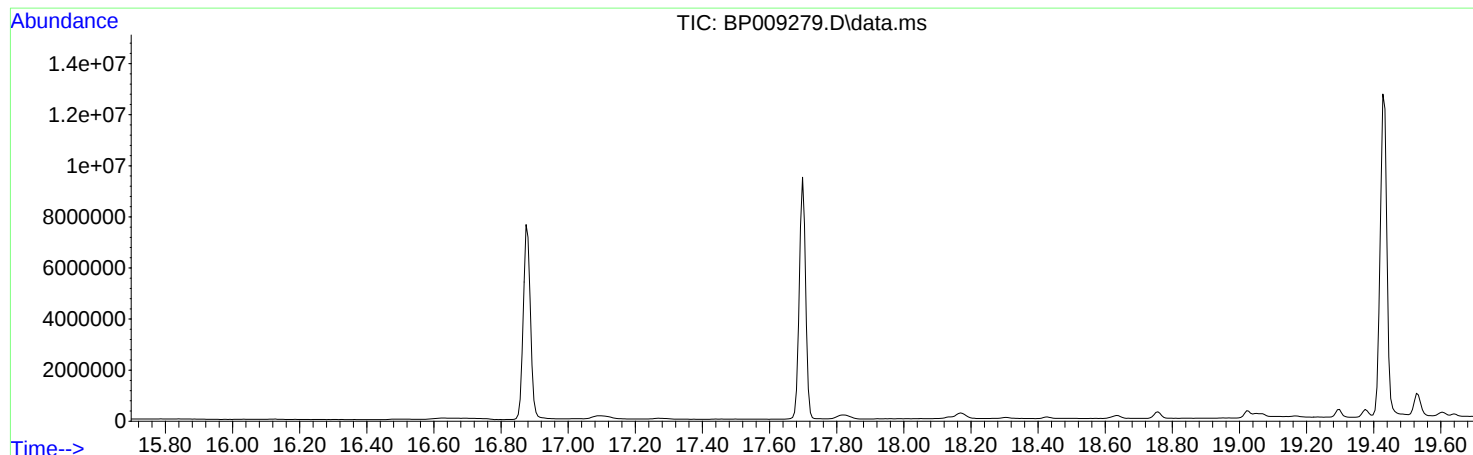




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	279215	PASS
68	69	0.00	2	1.7	5553	PASS
69	198	0.00	100	35.3	334833	PASS
70	69	0.00	2	0.5	1794	PASS
127	198	10	80	44.3	419720	PASS
197	198	0.00	2	0.3	3296	PASS
198	198	100	100	100.0	948501	PASS
199	198	5	9	6.9	65886	PASS
275	198	10	60	27.7	262464	PASS
365	198	1	100	3.7	34771	PASS
441	198	0.01	100	13.8	131096	PASS
442	442	100	100	100.0	830848	PASS
443	442	15	24	19.6	163149	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009279.D
Acq On : 07 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 07 16:29:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

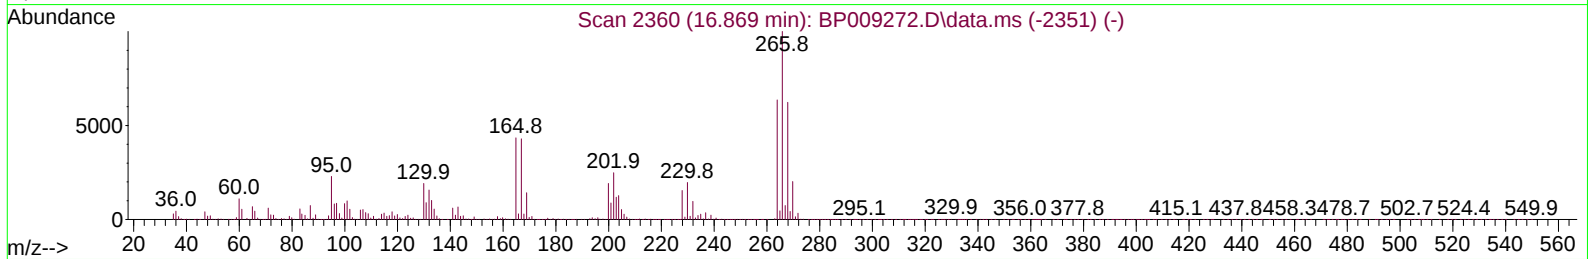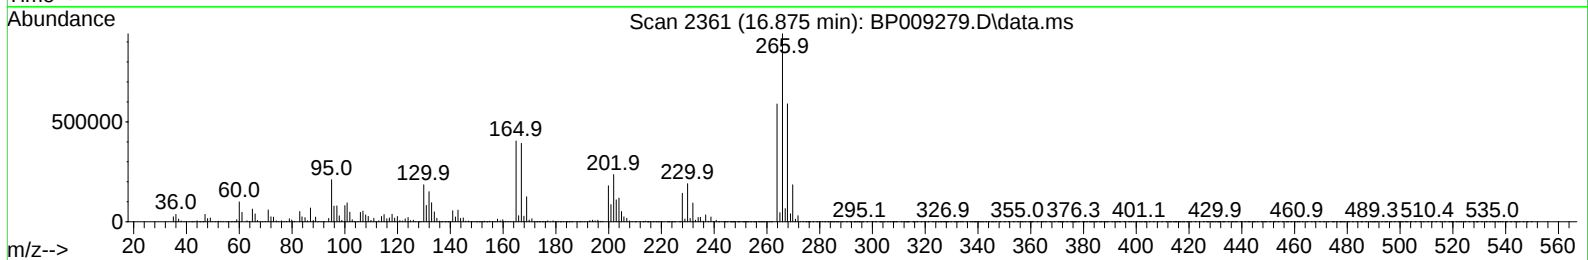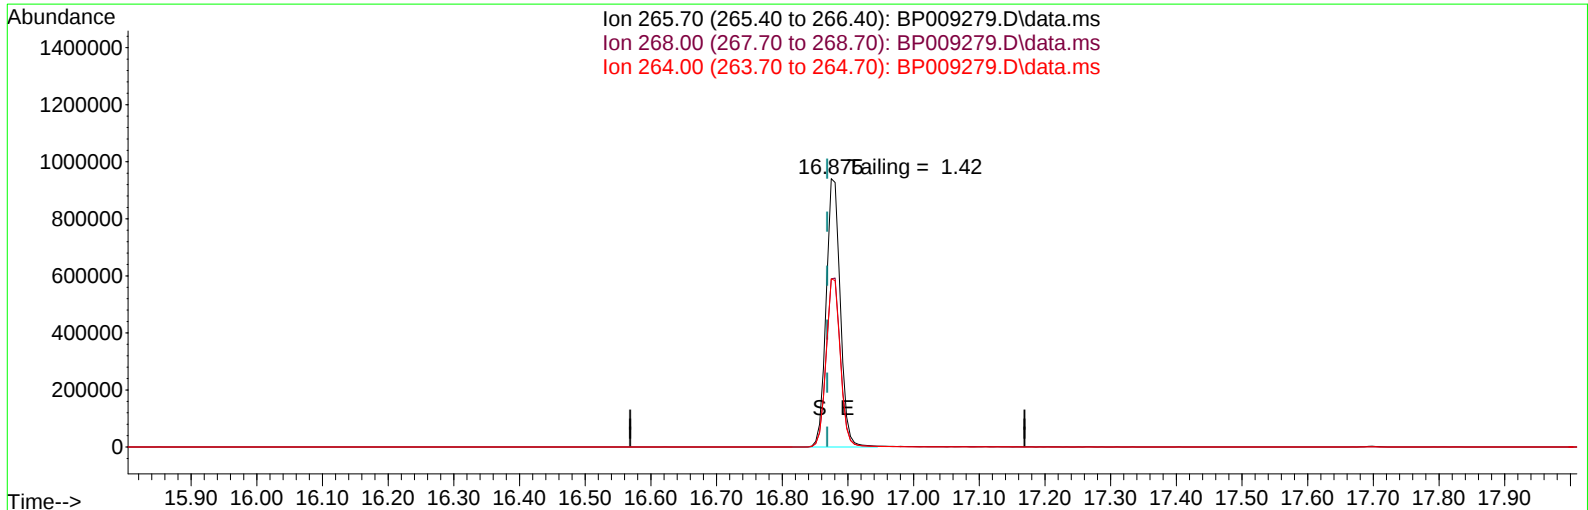

TIC: BP009279.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.006) 936837.16 ng




response 1412800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.69
264.00	63.60	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030722\
Data File : BP009279.D
Acq On : 07 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 07 16:29:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

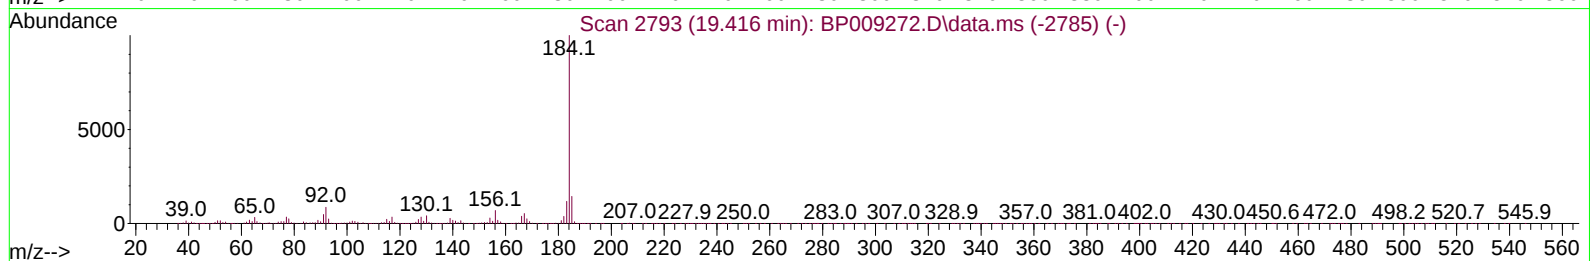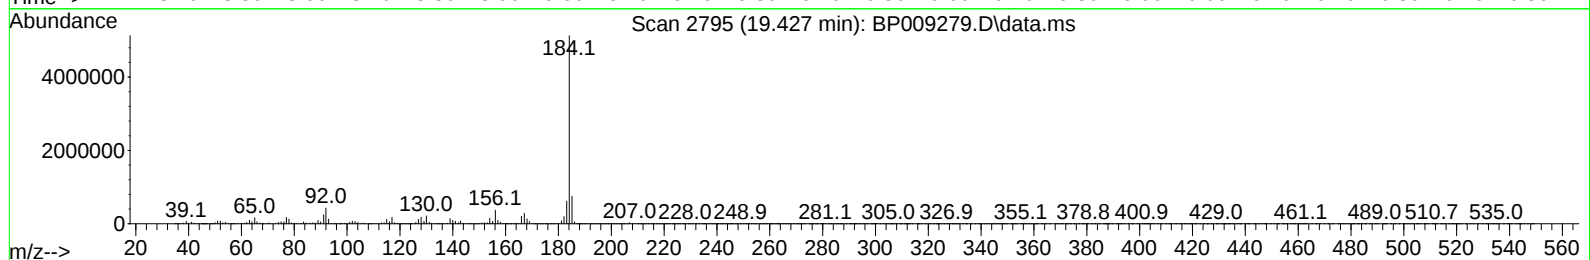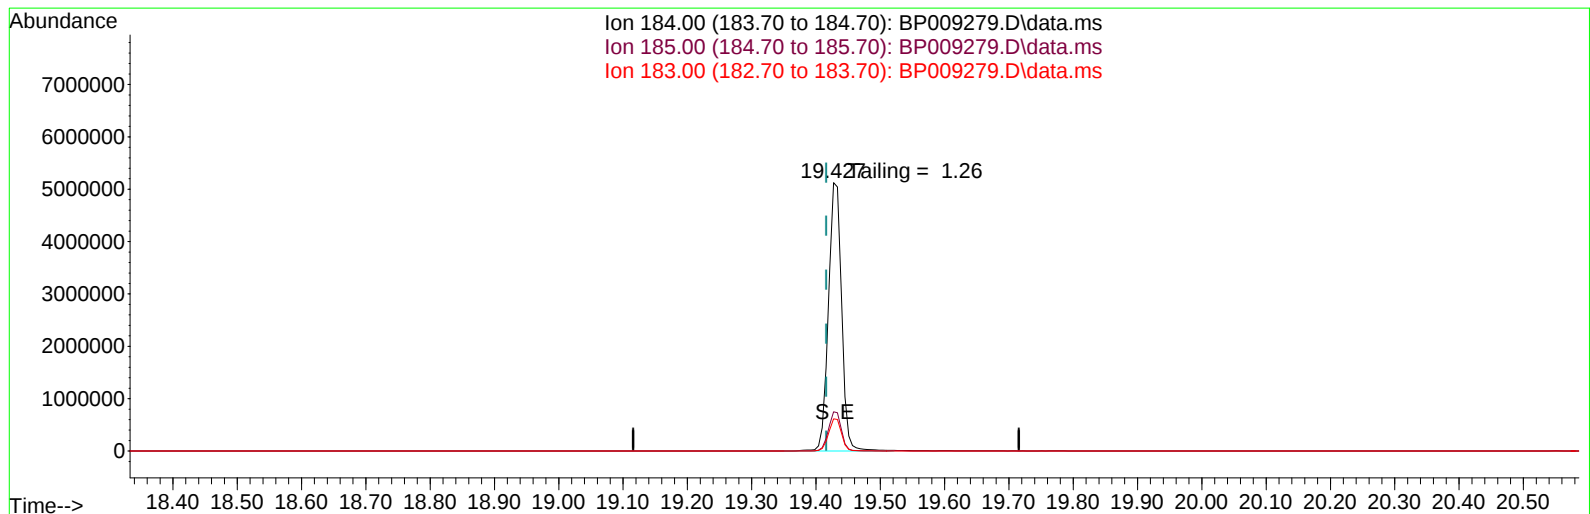

TIC: BP009279.D\data.ms

(77) Benzidine

19.427min (+ 0.012) 2091.51 ng

response 7317501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.62
183.00	11.70	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2022	BNA_P	BP009279.D
Compound Name	Response	Retention Time
DDT	3957219	20.65
DDD	26066	20.21
DDE	2565	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28631	3985850	0.72

Instrument :
BNA_P
ClientSampleId :
DFTPP