

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030921\
 Data File : BP004964.D
 Acq On : 10 Mar 2021 12:12
 Operator : CG/JU
 Sample : M1534-06
 Misc : SOM-MDL-W-06
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 3/11/2021 9:25:32 AM

Quant Time: Mar 10 12:44:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 10 10:08:47 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	26611	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	107709	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.38	164	71740	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	162749	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	187314	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	183949	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	3840	5.39	ng/uL	0.00
5) Phenol-d5	6.90	99	72928	34.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	43819	39.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	58742	35.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.44	113	57891	32.88	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	29530	37.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	32987	37.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	56828	33.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	74043	39.49	ng/ul	0.00
44) Dimethylphthalate-d6	13.79	166	189324	35.86	ng/ul	0.00
47) Acenaphthylene-d8	14.07	160	224197	34.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	28827	31.78	ng/ul	0.00
58) Fluorene-d10	15.38	176	162866	35.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	33867	32.45	ng/ul	0.00
71) Anthracene-d10	17.24	188	259810	35.62	ng/ul	0.00
79) Pyrene-d10	19.48	212	304049	35.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	349041	37.11	ng/ul	0.00

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.27	88	819	1.185	ng/uL#	83
4) Benzaldehyde	6.88	77	5082	4.694	ng/ul	97
6) Phenol	6.93	94	7858	3.526	ng/ul#	90
8) Bis(2-Chloroethyl)ether	7.16	93	5842	3.552	ng/ul#	94
10) 2-Chlorophenol	7.30	128	6344	3.718	ng/ul	99
11) 2-Methylphenol	8.18	108	5361	3.164	ng/ul	93
12) 2,2'-oxybis(1-Chloropropan	8.26	45	5958m	3.396	ng/ul	
14) Acetophenone	8.55	105	10110	3.452	ng/ul	94
15) N-Nitroso-di-n-propylamine	8.54	70	4839	3.474	ng/ul#	96
16) 4-Methylphenol	8.50	108	5915	3.162	ng/ul	99
17) Hexachloroethane	8.80	117	2894	3.647	ng/ul#	82
20) Nitrobenzene	8.93	77	7655	3.592	ng/ul#	94
21) Isophorone	9.46	82	11633	3.197	ng/ul#	92
23) 2-Nitrophenol	9.64	139	3467	3.652	ng/ul	90
24) 2,4-Dimethylphenol	9.70	107	7303	3.331	ng/ul	94
25) Bis(2-Chloroethoxy)methane	9.94	93	6945	3.154	ng/ul#	87
27) 2,4-Dichlorophenol	10.17	162	5691	3.367	ng/ul#	87
28) Naphthalene	10.57	128	19693	3.531	ng/ul#	94
30) 4-Chloroaniline	10.69	127	7908	4.050	ng/ul	98
31) Hexachlorobutadiene	10.86	225	4656	3.562	ng/ul	88
32) Caprolactam	11.50	113	1611m	2.921	ng/ul	
33) 4-Chloro-3-methylphenol	11.82	107	5543	2.819	ng/ul	92
34) 2-Methylnaphthalene	12.19	142	13569	3.363	ng/ul	95

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030921\
 Data File : BP004964.D
 Acq On : 10 Mar 2021 12:12
 Operator : CG/JU
 Sample : M1534-06
 Misc : SOM-MDL-W-06
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 3/11/2021 9:25:32 AM

Quant Time: Mar 10 12:44:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 10 10:08:47 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

35) 1-Methylnaphthalene	12.41	142	13156	3.314	ng/ul	93
37) 1,2,4,5-Tetrachlorobenzene	12.56	216	7925	3.316	ng/ul	92
38) Hexachlorocyclopentadiene	12.54	237	4374	2.821	ng/ul#	87
39) 2,4,6-Trichlorophenol	12.81	196	4155	2.917	ng/ul#	90
40) 2,4,5-Trichlorophenol	12.88	196	4132	2.671	ng/ul	85
41) 1,1'-Biphenyl	13.21	154	17709	3.355	ng/ul	97
42) 2-Chloronaphthalene	13.25	162	14328	3.463	ng/ul	95
43) 2-Nitroaniline	13.47	65	3414	2.841	ng/ul	91
45) Dimethylphthalate	13.84	163	19241	3.559	ng/ul	98
46) 2,6-Dinitrotoluene	13.96	165	3155	2.911	ng/ul	95
48) Acenaphthylene	14.10	152	20384	3.348	ng/ul	99
49) 3-Nitroaniline	14.30	138	3166	3.306	ng/ul#	96
50) Acenaphthene	14.45	153	15447	3.451	ng/ul	93
51) 2,4-Dinitrophenol	14.50	184	1406	1.962	ng/ul#	72
53) 4-Nitrophenol	14.60	109	3455	3.408	ng/ul#	82
54) Dibenzofuran	14.79	168	22335	3.424	ng/ul	92
55) 2,4-Dinitrotoluene	14.75	165	4722	3.004	ng/ul#	90
56) 2,3,4,6-Tetrachlorophenol	15.01	232	4267	2.905	ng/ul#	92
57) Diethylphthalate	15.22	149	17498	3.165	ng/ul	97
59) Fluorene	15.43	166	17849	3.275	ng/ul	93
60) 4-Chlorophenyl-phenylether	15.43	204	9914	3.310	ng/ul	99
61) 4-Nitroaniline	15.46	138	2915	2.608	ng/ul#	77
64) 4,6-Dinitro-2-methylphenol	15.52	198	3404	3.210	ng/ul#	83
65) N-Nitrosodiphenylamine	15.65	169	14967	3.270	ng/ul	98
66) 4-Bromophenyl-phenylether	16.33	248	6083	3.386	ng/ul	90
67) Hexachlorobenzene	16.44	284	7216	3.558	ng/ul	94
68) Atrazine	16.61	200	4967	2.702	ng/ul	94
69) Pentachlorophenol	16.79	266	3302m	2.573	ng/ul	
70) Phenanthrene	17.18	178	29674	3.424	ng/ul#	95
72) Anthracene	17.27	178	29953	3.369	ng/ul	95
73) 1,2,3,4-Tetrachlorobenzene	13.17	216	7987	3.381	ng/uL	93
74) Pentachlorobenzene	14.70	250	7816	3.256	ng/uL	94
75) Carbazole	17.55	167	23619	3.086	ng/ul	97
76) Di-n-butylphthalate	18.10	149	26212	2.934	ng/ul	96
77) Fluoranthene	19.16	202	34456	3.255	ng/ul#	95
80) Pvrene	19.50	202	38153	3.404	ng/ul#	95
81) Butylbenzylphthalate	20.39	149	11499	2.829	ng/ul	95
82) 3,3'-Dichlorobenzidine	21.15	252	10923	2.839	ng/ul	99
83) Benzo(a)anthracene	21.21	228	38725	3.415	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.14	149	16592	2.720	ng/ul	93
85) Chrysene	21.26	228	38013	3.421	ng/ul	98
87) Di-n-octyl phthalate	22.03	149	29127	2.676	ng/ul	100
88) Benzo(b)fluoranthene	22.82	252	38615m	3.342	ng/ul	
89) Benzo(k)fluoranthene	22.86	252	38740	3.399	ng/ul	99
91) Benzo(a)pyrene	23.41	252	33972	3.350	ng/ul#	90
92) Indeno(1,2,3-cd)pyrene	25.86	276	43908	3.389	ng/ul	94
93) Dibenzo(a,h)anthracene	25.86	278	36871	3.363	ng/ul	97
94) Benzo(a,h,i)perylene	26.56	276	36478	3.399	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030921\
Data File : BP004964.D
Acq On : 10 Mar 2021 12:12
Operator : CG/JU
Sample : M1534-06
Misc : SOM-MDL-W-06
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06


Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

Quant Time: Mar 10 12:44:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP030921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 10 10:08:47 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 1.185 ng/uL

RT: 3.27 min Scan# 31

Delta R.T. 0.01 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P





ClientSampled :

MDL-WATER-06

Tot Ion:	88	Resp:	819
Ion Ratio	Lower	Upper	
88	100		
43	31.7	26.0	39.0
58	45.3	52.0	78.0#

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

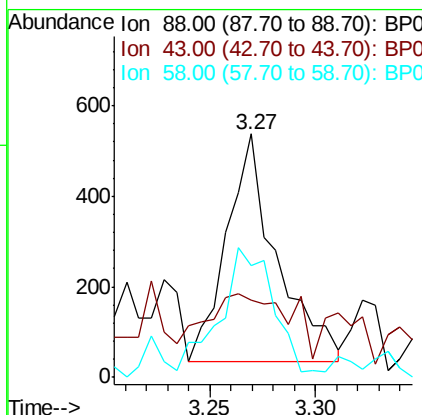

#4

Benzaldehyde

Concen: 4.694 ng/uL




RT: 6.88 min Scan# 645


Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Tgt Ion:	77	Resp:	5082
Ion Ratio	Lower	Upper	
77	100		
105	86.7	73.6	110.4
106	88.8	71.3	106.9

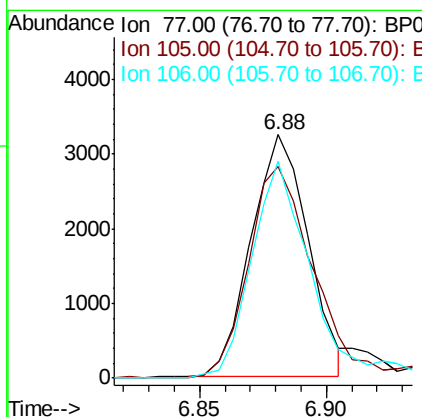

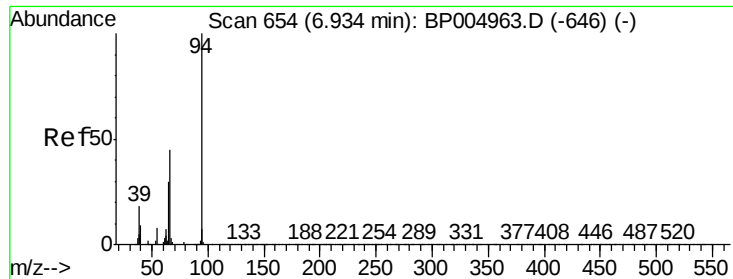

#6

Phenol

Concen: 3.526 ng/ul

RT: 6.93 min Scan# 653

Delta R.T. -0.01 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-06

Tot Ion:	94	Resp:	7858
Ion	Ratio	Lower	Upper
94	100		
65	25.4	27.6	41.4#
66	45.2	39.0	58.6

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

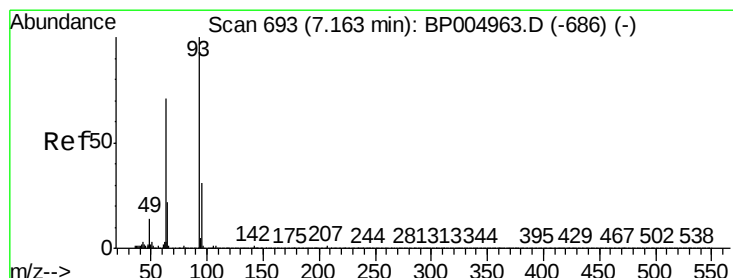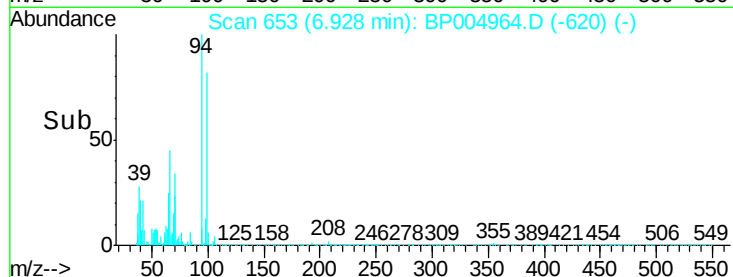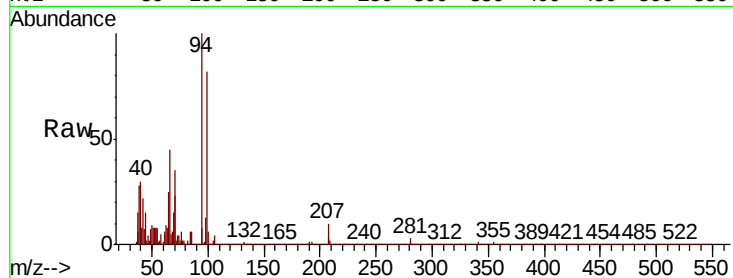

#8

Bis(2-Chloroethyl)ether

Concen: 3.552 ng/ul




RT: 7.16 min Scan# 693


Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Tgt Ion:	93	Resp:	5842
Ion	Ratio	Lower	Upper
93	100		
63	67.8	54.2	81.2
95	41.7	24.5	36.7#

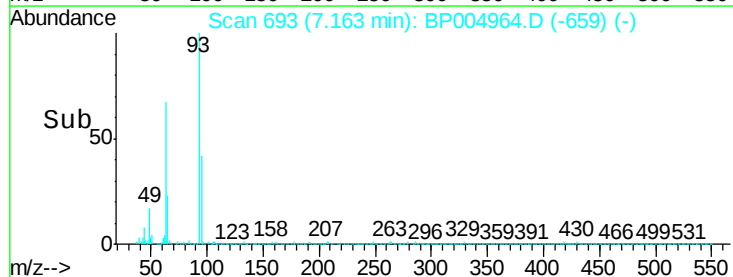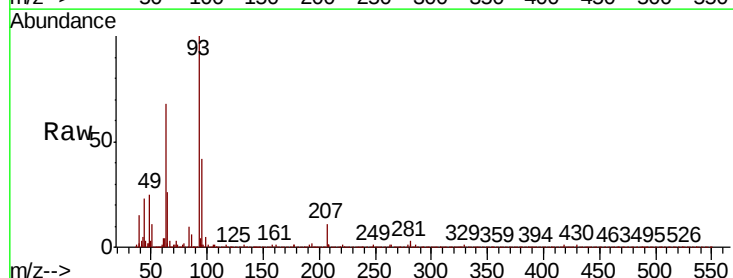







#10
2-Chlorophenol
Concen: 3.718 ng/ul
RT: 7.30 min Scan# 716
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
128	100		
64	48.7	38.7	58.1
130	33.8	26.5	39.7




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

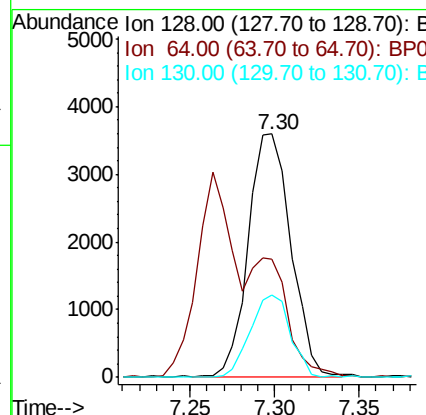

#11
2-Methylphenol
Concen: 3.164 ng/ul
RT: 8.18 min Scan# 866
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
108	100		
107	89.7	77.5	116.3

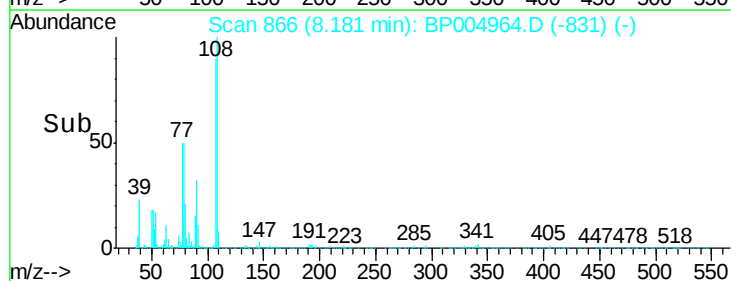







#12
2,2'-oxvbis(1-Chloropropane)
Concen: 3.396 ng/ul m
RT: 8.26 min Scan# 879
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion:	45	Resp:	5958
Ion Ratio	Lower	Upper	
45	100		
77	24.2	16.5	24.7
79	15.8	11.8	17.6




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

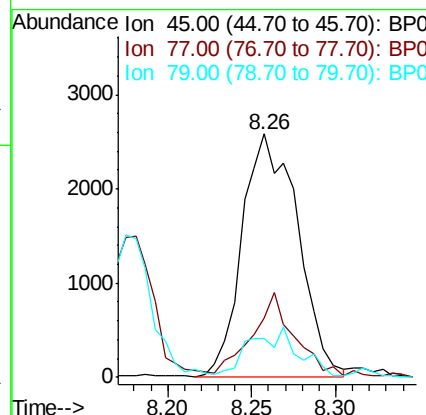

#14
Acetophenone
Concen: 3.452 ng/ul
RT: 8.55 min Scan# 929
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion:	105	Resp:	10110
Ion Ratio	Lower	Upper	
105	100		
77	75.8	65.8	98.6
51	29.8	23.1	34.7









#15
N-Nitroso-di-n-propylamine
Concen: 3.474 ng/ul
RT: 8.54 min Scan# 927
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
70	100		
42	57.5	46.6	70.0
101	13.5	8.8	13.2#
130	17.4	17.9	26.9#




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

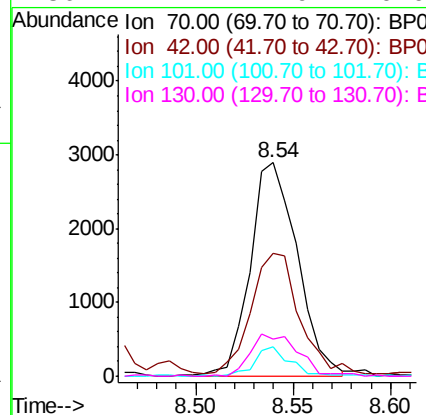

#16
4-Methylphenol
Concen: 3.162 ng/ul
RT: 8.50 min Scan# 921
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
108	100		
107	117.6	92.8	139.2









#17
Hexachloroethane
Concen: 3.647 ng/ul
RT: 8.80 min Scan# 972
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
117	100		
201	114.7	82.4	123.6
199	76.5	44.6	66.8




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

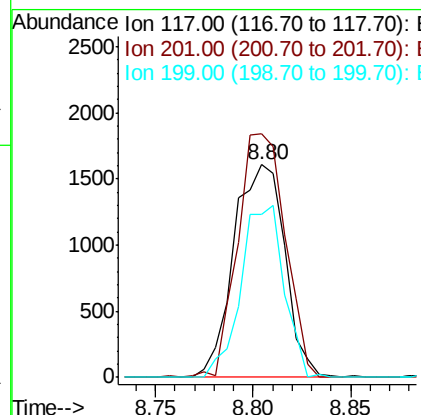

#20
Nitrobenzene
Concen: 3.592 ng/ul
RT: 8.93 min Scan# 994
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
77	100		
123	38.4	32.7	49.1
65	9.2	10.9	16.3

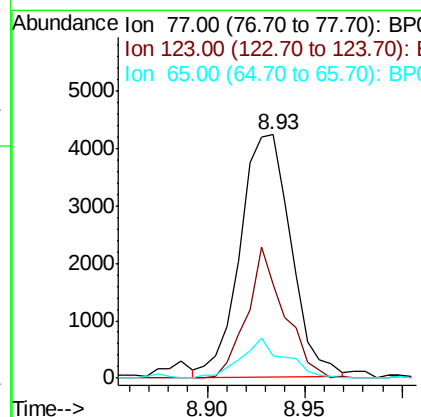







#21
Isophorone
Concen: 3.197 ng/ul
RT: 9.46 min Scan# 1083
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
82	100		
95	12.2	8.0	12.0#
138	21.3	13.8	20.6#




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

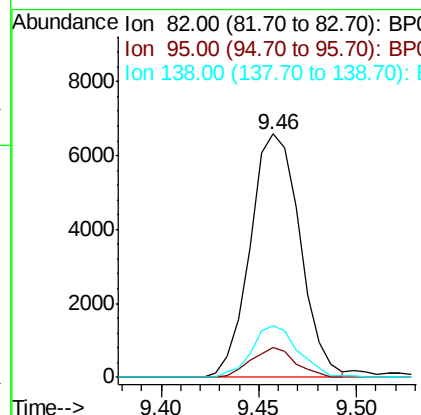

#23
2-Nitrophenol
Concen: 3.652 ng/ul
RT: 9.64 min Scan# 1114
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
139	100		
65	51.5	48.7	73.1
109	39.5	35.4	53.0

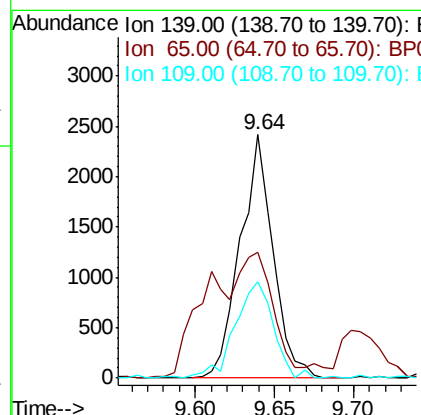

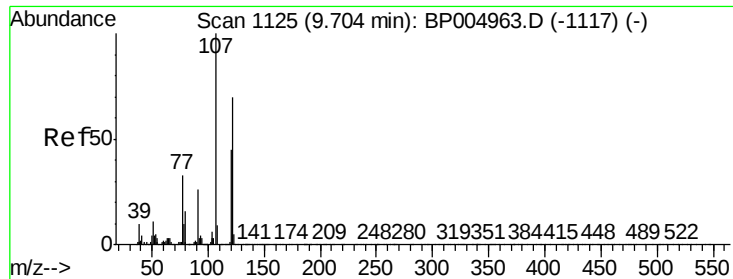





#24
2,4-Dimethylphenol
Concen: 3.331 ng/ul
RT: 9.70 min Scan# 1125
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
107	100		
121	46.8	35.9	53.9
122	76.5	55.7	83.5




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

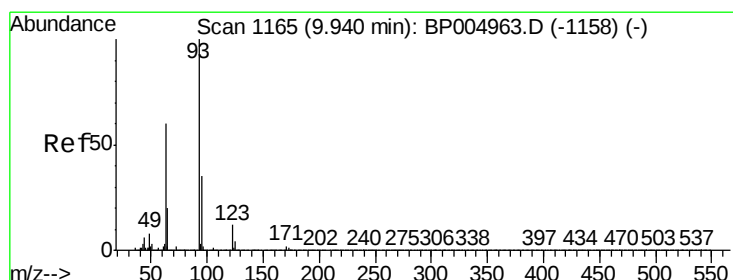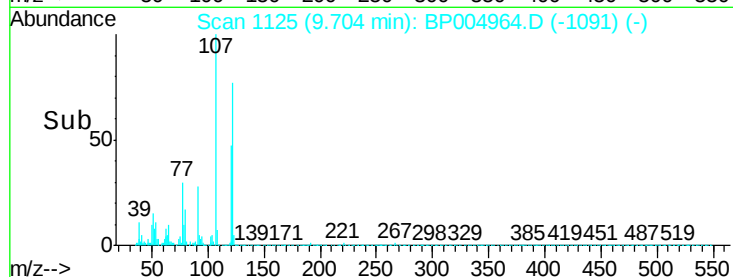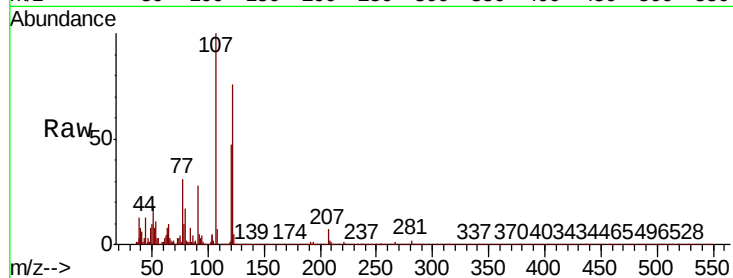

#25
Bis(2-Chloroethoxy)methane
Concen: 3.154 ng/ul
RT: 9.94 min Scan# 1165
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
93	100		
95	40.4	25.4	38.0#
123	9.8	9.8	14.8#

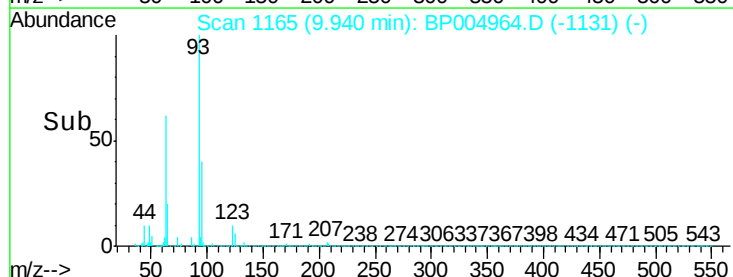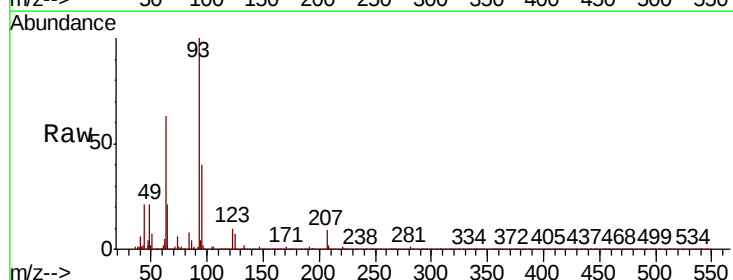







#27
2,4-Dichlorophenol
Concen: 3.367 ng/ul
RT: 10.17 min Scan# 1204
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
162	100		
164	72.1	46.3	69.5#
98	40.1	30.3	45.5




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#28
Naphthalene
Concen: 3.531 ng/ul
RT: 10.57 min Scan# 1272
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
128	100		
129	9.5	8.4	12.6
127	10.4	11.0	16.4#









#30
4-Chloroaniline
Concen: 4.050 ng/ul
RT: 10.69 min Scan# 1292
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampled :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
127	100		
129	34.8	27.0	40.4




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

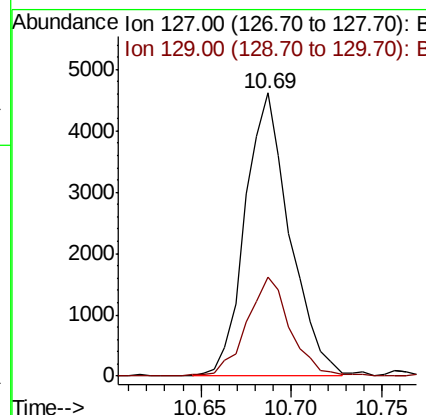

#31
Hexachlorobutadiene
Concen: 3.562 ng/ul
RT: 10.86 min Scan# 1321
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
225	100		
223	57.2	51.0	76.6
227	72.1	48.1	72.1









#32
 Caprolactam
 Concen: 2.921 ng/ul m
 RT: 11.50 min Scan# 1430
 Delta R.T. 0.03 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
113	100		
55	114.6	96.7	145.1
56	82.6	85.7	128.5




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM



#33
 4-Chloro-3-methylphenol
 Concen: 2.819 ng/ul
 RT: 11.82 min Scan# 1484
 Delta R.T. -0.01 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
107	100		
144	17.8	17.4	26.0
142	60.8	53.6	80.4









#34
2-Methylnaphthalene
Concen: 3.363 ng/ul
RT: 12.19 min Scan# 1548
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
142	100		
141	87.2	73.5	110.3




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

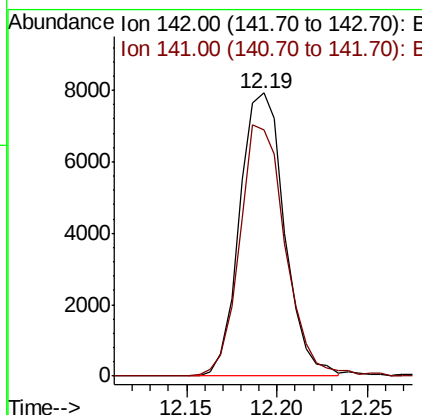

#35
1-Methylnaphthalene
Concen: 3.314 ng/ul
RT: 12.41 min Scan# 1585
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
142	100		
141	86.3	74.6	111.8
116	5.4	3.6	5.4

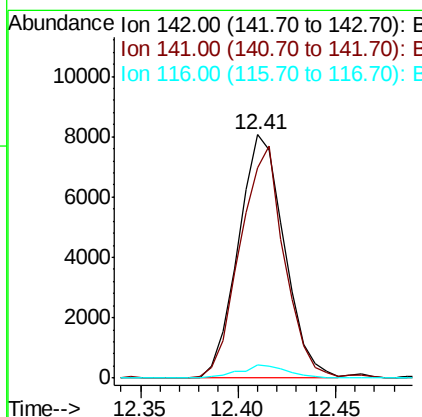







#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 3.316 ng/ul
 RT: 12.56 min Scan# 1611
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
216	100		
214	88.7	62.9	94.3
179	21.4	16.6	24.8
108	15.6	13.3	19.9




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM

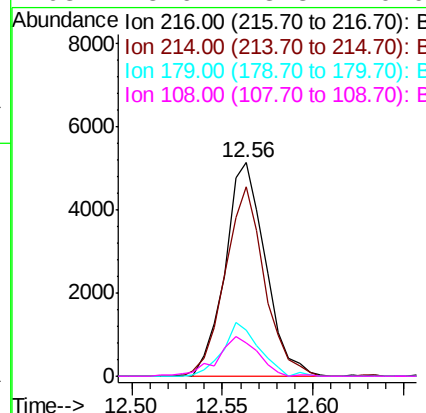

#38
 Hexachlorocyclopentadiene
 Concen: 2.821 ng/ul
 RT: 12.54 min Scan# 1607
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
237	100		
235	68.2	49.0	73.6
272	0.7	10.6	15.8#









#39
 2,4,6-Trichlorophenol
 Concen: 2.917 ng/ul
 RT: 12.81 min Scan# 1653
 Delta R.T. 0.01 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
196	100		
198	89.9	78.2	117.2
200	21.8	24.5	36.7




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM

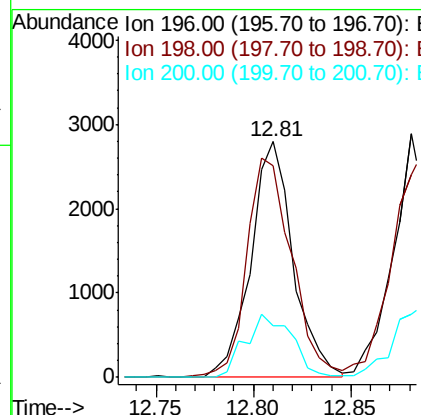

#40
 2,4,5-Trichlorophenol
 Concen: 2.671 ng/ul
 RT: 12.88 min Scan# 1665
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
196	100		
198	83.3	80.0	120.0
200	25.7	24.8	37.2

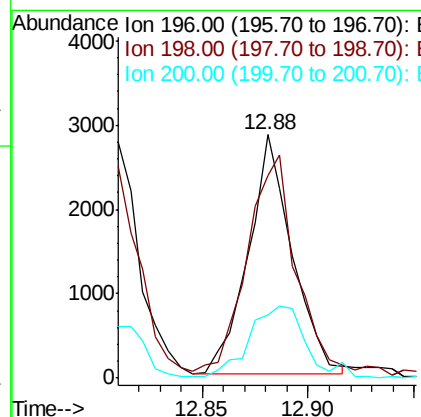



#41

1,1'-Biphenyl

Concen: 3.355 ng/ul

RT: 13.21 min Scan# 1721

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-06

Tot Ion:	154	Resp:	17709
Ion Ratio	Lower	Upper	
154	100		
153	42.4	32.4	48.6
76	11.6	9.8	14.8

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

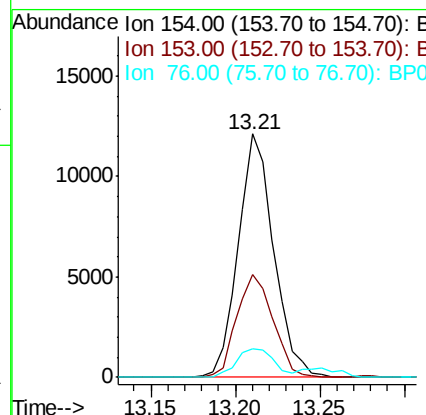

#42

2-Chloronaphthalene

Concen: 3.463 ng/ul




RT: 13.25 min Scan# 1728


Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Tgt Ion:	162	Resp:	14328
Ion Ratio	Lower	Upper	
162	100		
164	30.7	28.1	42.1
127	42.3	32.6	49.0

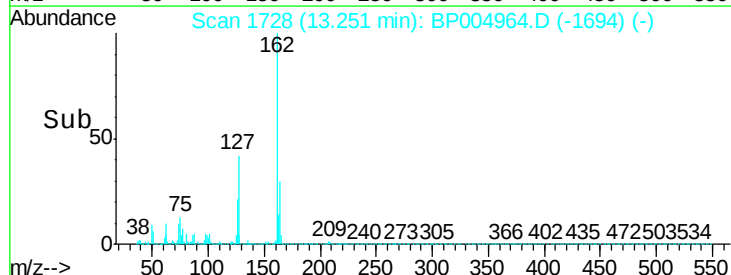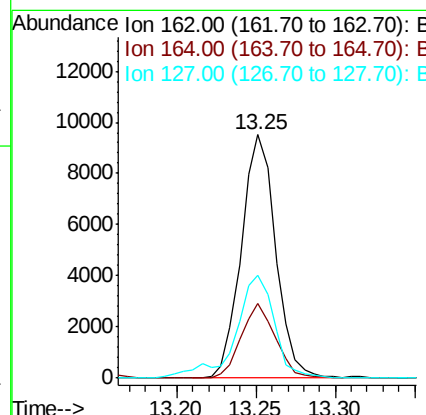







#43
2-Nitroaniline
Concen: 2.841 ng/ul
RT: 13.47 min Scan# 1765
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
65	100		
92	61.9	56.1	84.1
138	92.9	80.3	120.5




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

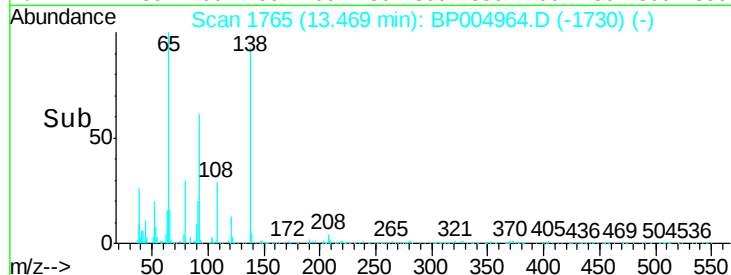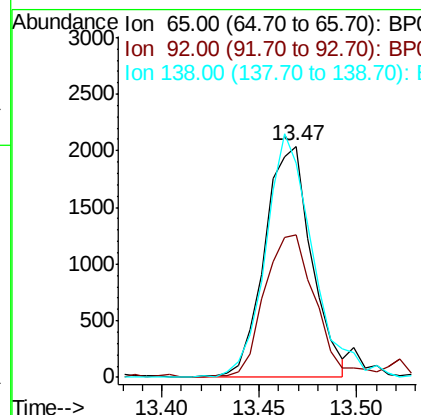

#45
Dimethylphthalate
Concen: 3.559 ng/ul
RT: 13.84 min Scan# 1828
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.8	5.6
164	10.9	7.8	11.6

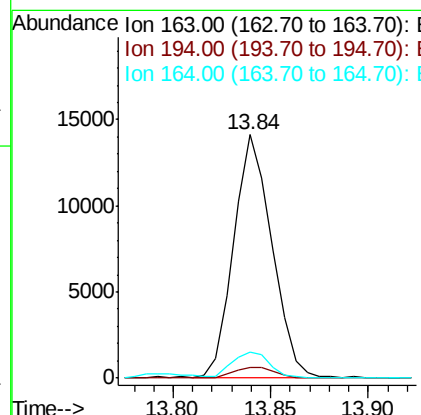







#46
2,6-Dinitrotoluene
Concen: 2.911 ng/ul
RT: 13.96 min Scan# 1849
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
165	100		
89	74.5	56.0	84.0
121	24.8	18.7	28.1




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#48
Acenaphthylene
Concen: 3.348 ng/ul
RT: 14.10 min Scan# 1872
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.0	16.4	24.6
153	13.0	10.0	15.0



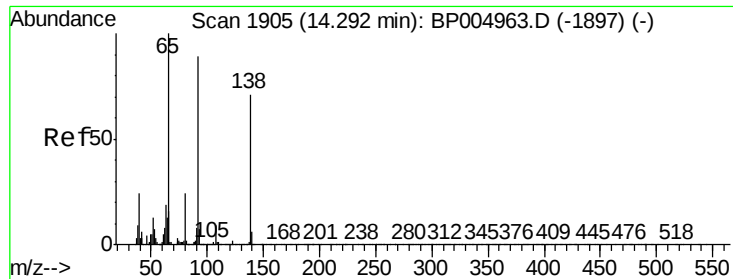





#49
3-Nitroaniline
Concen: 3.306 ng/ul
RT: 14.30 min Scan# 1906
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
138	100		
108	23.8	9.4	14.2#
92	123.1	99.8	149.8




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

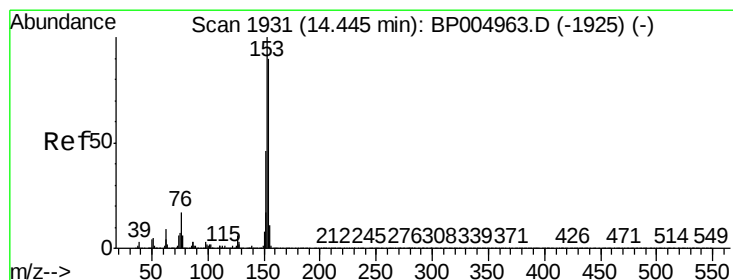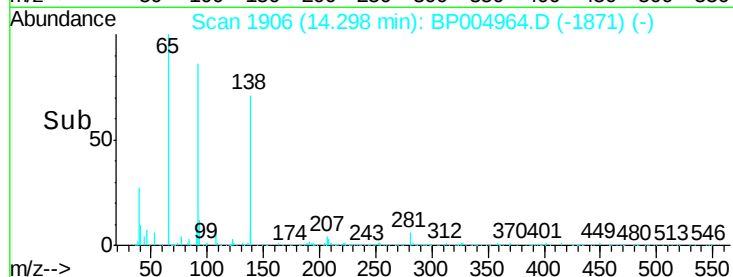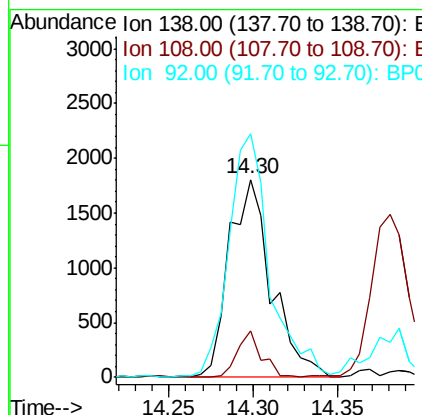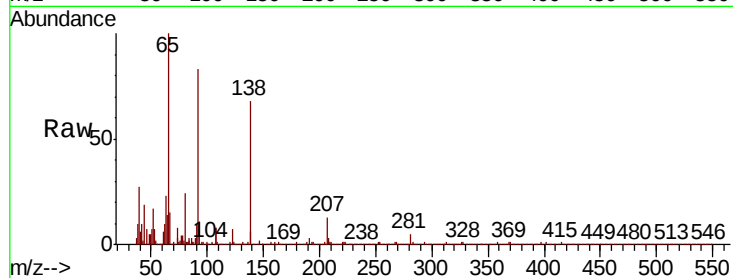

#50
Acenaphthene
Concen: 3.451 ng/ul
RT: 14.45 min Scan# 1931
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
153	100		
152	53.8	38.8	58.2
154	83.4	71.8	107.6

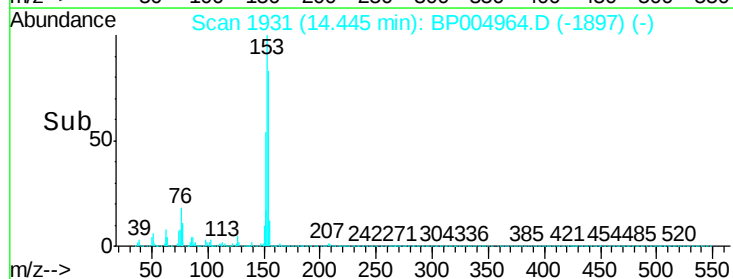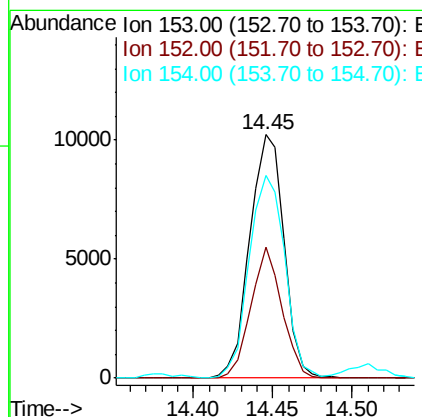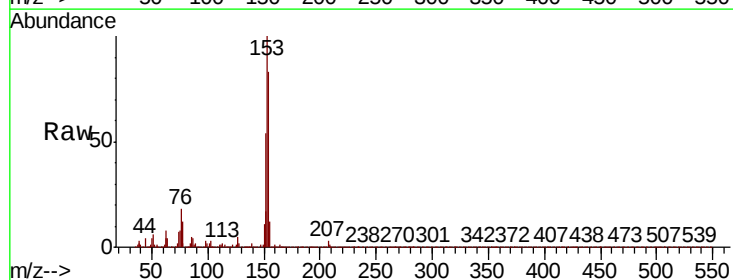







#51
2,4-Dinitrophenol
Concen: 1.962 ng/ul
RT: 14.50 min Scan# 1941
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
184	100		
63	101.1	51.4	77.0#
154	51.1	43.4	65.2




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#53
4-Nitrophenol
Concen: 3.408 ng/ul
RT: 14.60 min Scan# 1958
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
109	100		
139	90.4	69.7	104.5
65	130.2	79.2	118.8#

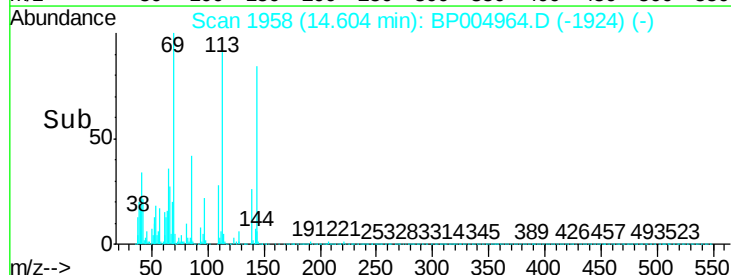



#54

Dibenzofuran

Concen: 3.424 ng/ul

RT: 14.79 min Scan# 1989

Delta R.T. 0.01 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P

ClientSampleId :

MDL-WATER-06

Tot Ion:168 Resp: 22335


Ion Ratio Lower Upper

168 100

139 44.6 31.6 47.4




Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

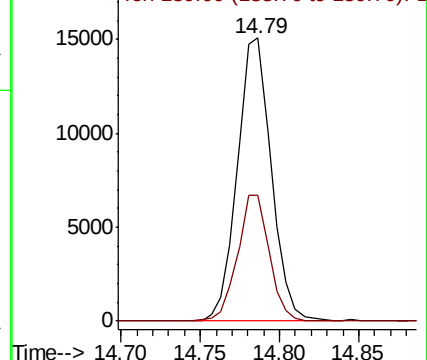

#55

2,4-Dinitrotoluene

Concen: 3.004 ng/ul

RT: 14.75 min Scan# 1983

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12


Tgt Ion:165 Resp: 4722

Ion Ratio Lower Upper

165 100

63 55.3 38.4 57.6



182 3.8 2.2 3.2#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BP0

Ion 182.00 (181.70 to 182.70): E

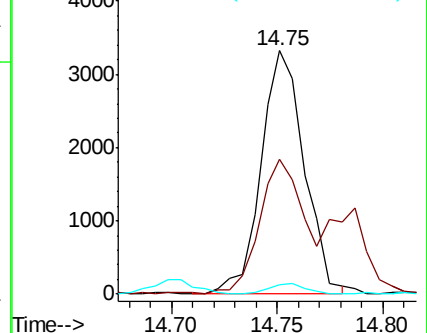







#56
2,3,4,6-Tetrachlorophenol
Concen: 2.905 ng/ul
RT: 15.01 min Scan# 2027
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
232	100		
131	36.4	32.6	48.8
130	3.6	3.1	4.7
166	23.1	23.5	35.3




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

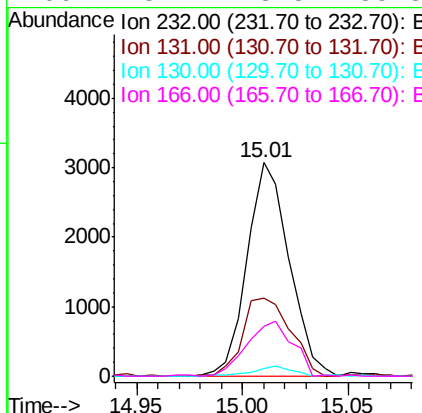

#57
Diethylphthalate
Concen: 3.165 ng/ul
RT: 15.22 min Scan# 2062
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
149	100		
177	23.9	17.3	25.9
150	12.1	9.8	14.8

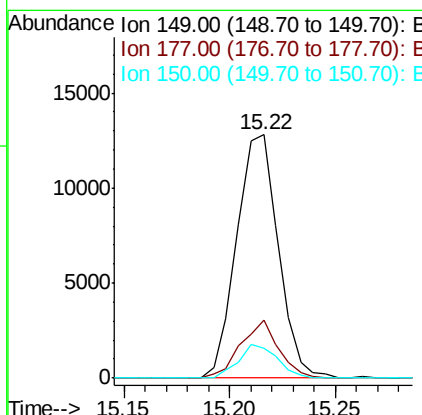

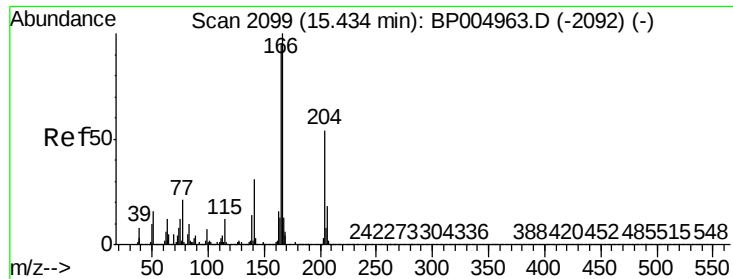

#59

Fluorene

Concen: 3.275 ng/ul

RT: 15.43 min Scan# 2099

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P

ClientSampleId :

MDL-WATER-06

Tot Ion:166 Resp: 17849

Ion Ratio Lower Upper





166 100

165 103.3 76.4 114.6

167 15.0 11.4 17.0

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

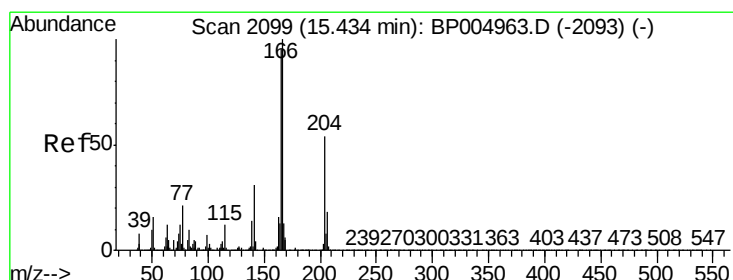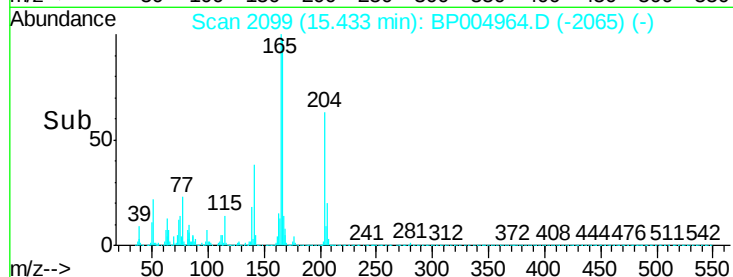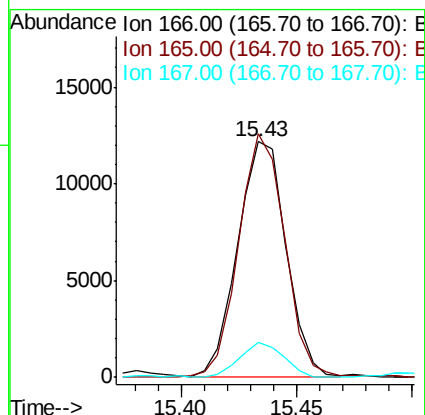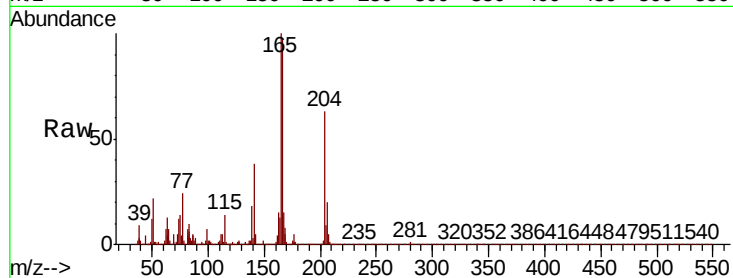

#60

4-Chlorophenyl-phenylether

Concen: 3.310 ng/ul

RT: 15.43 min Scan# 2099

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12




Tgt Ion:204 Resp: 9914


Ion Ratio Lower Upper

204 100

206 31.6 24.6 37.0

141 59.5 46.8 70.2

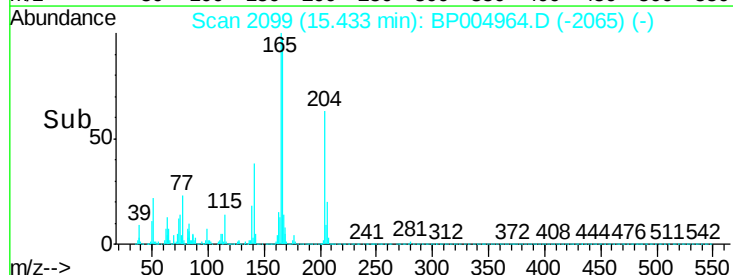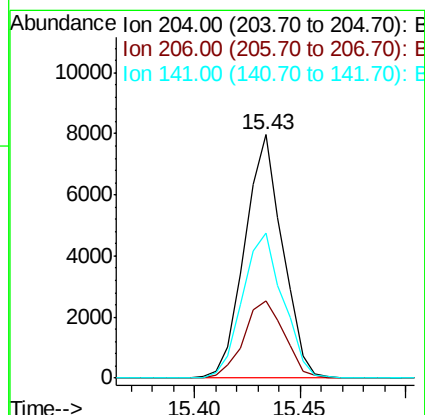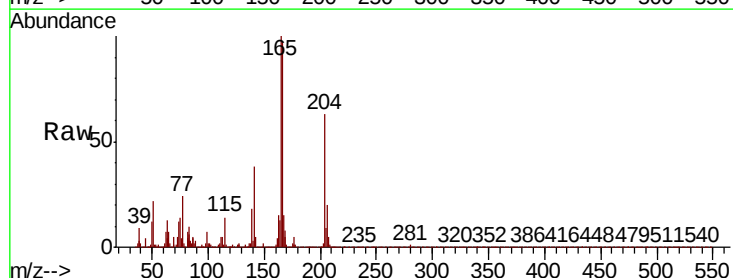







#61
4-Nitroaniline
Concen: 2.608 ng/ul
RT: 15.46 min Scan# 2103
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
138	100		
92	53.1	53.8	80.6#
108	95.0	99.4	149.0#




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#64
4,6-Dinitro-2-methylphenol
Concen: 3.210 ng/ul
RT: 15.52 min Scan# 2113
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
198	100		
182	7.9	3.5	5.3#
77	38.9	23.3	34.9#

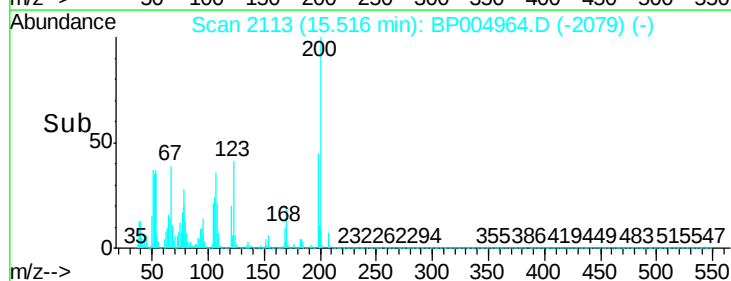



#65





N-Nitrosodiphenylamine
Concen: 3.270 ng/ul
RT: 15.65 min Scan# 2135
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
169	100		
168	63.6	51.9	77.9
167	33.2	28.0	42.0

Manual Integrations
APPROVED




mohammad
3/11/2021 9:25:32 AM

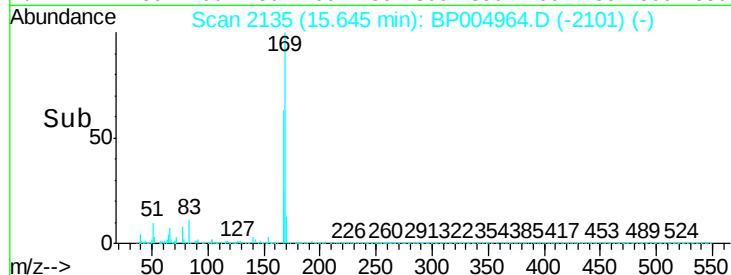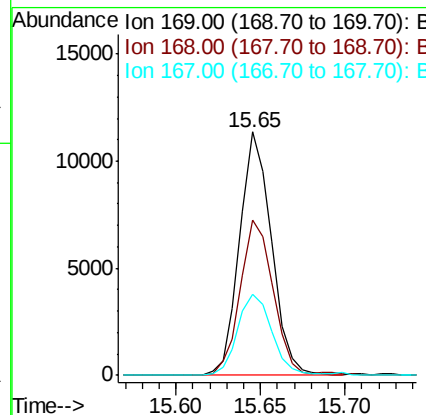


#66

4-Bromophenyl-phenylether
Concen: 3.386 ng/ul
RT: 16.33 min Scan# 2251
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
248	100		
250	87.9	77.6	116.4
141	69.1	63.6	95.4

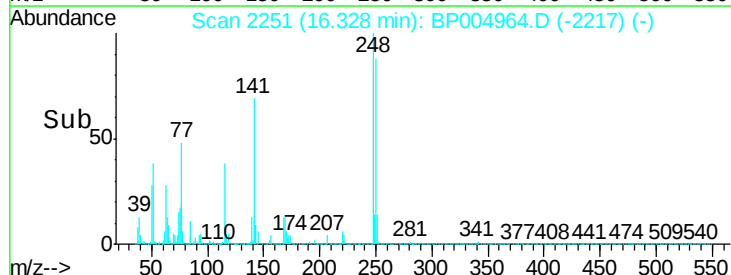







#67
Hexachlorobenzene
Concen: 3.558 ng/ul
RT: 16.44 min Scan# 2270
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampled :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
284	100		
142	32.1	27.1	40.7
249	30.5	28.3	42.5




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#68
Atrazine
Concen: 2.702 ng/ul
RT: 16.61 min Scan# 2299
Delta R.T. 0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
200	100		
173	26.5	20.7	31.1
215	43.1	38.8	58.2

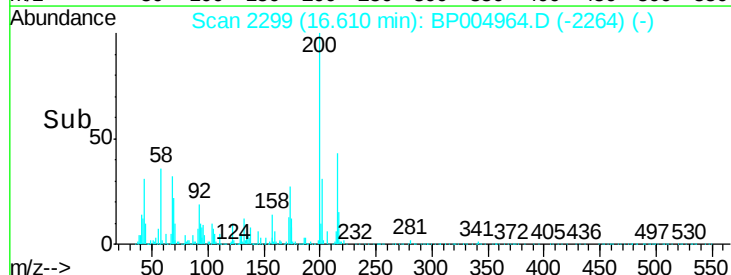







#69
 Pentachlorophenol
 Concen: 2.573 ng/ul m
 RT: 16.79 min Scan# 2330
 Delta R.T. 0.01 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
266	100		
264	55.6	55.8	83.6#
268	70.1	52.1	78.1




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM



#70
 Phenanthrene
 Concen: 3.424 ng/ul
 RT: 17.18 min Scan# 2396
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
178	100		
179	17.6	11.4	17.0#
176	19.7	15.0	22.6





#72

Anthracene

Concen: 3.369 ng/ul

RT: 17.27 min Scan# 2412

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-06

Tot Ion:	178	Resp:	29953
Ion Ratio	Lower	Upper	
178	100		
179	17.6	12.4	18.6
176	20.4	14.7	22.1

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM

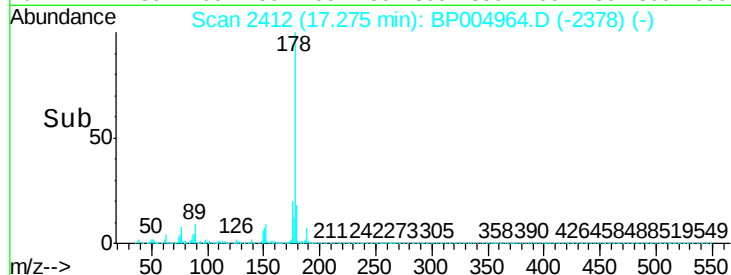

#73

1,2,3,4-Tetrachlorobenzene

Concen: 3.381 ng/uL




RT: 13.17 min Scan# 1714


Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Tgt Ion:	216	Resp:	7987
Ion Ratio	Lower	Upper	
216	100		
214	83.4	62.4	93.6
218	44.3	39.6	59.4



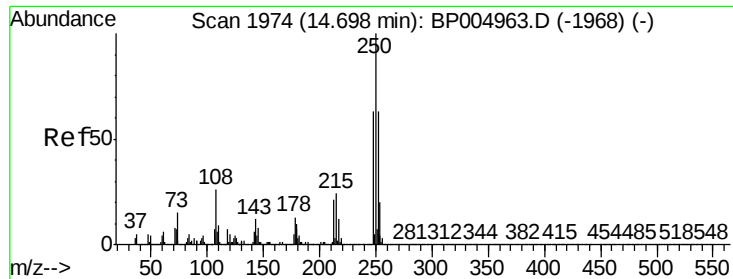





#74
 Pentachlorobenzene
 Concen: 3.256 ng/uL
 RT: 14.70 min Scan# 1974
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion:	250	Resp:	7816
Ion Ratio	Lower	Upper	
250	100		
248	58.6	52.4	78.6
252	66.1	50.9	76.3




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM

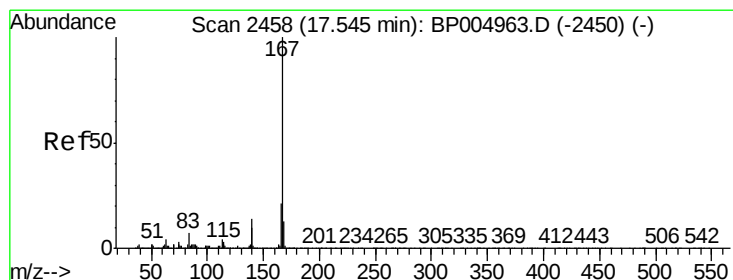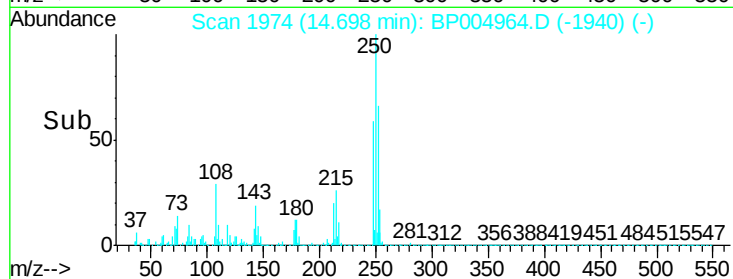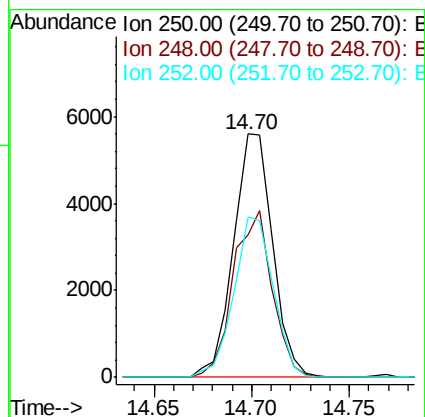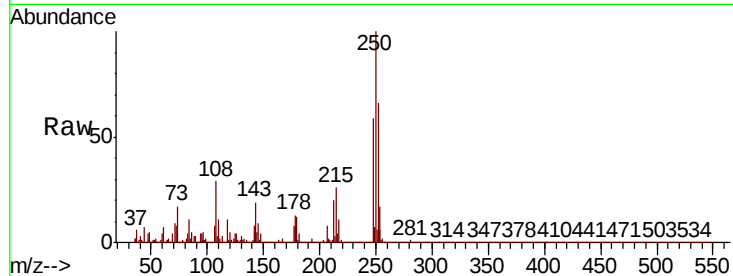

#75
 Carbazole
 Concen: 3.086 ng/uL
 RT: 17.55 min Scan# 2459
 Delta R.T. 0.01 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion:	167	Resp:	23619
Ion Ratio	Lower	Upper	
167	100		
166	22.8	17.3	25.9
139	11.6	10.5	15.7

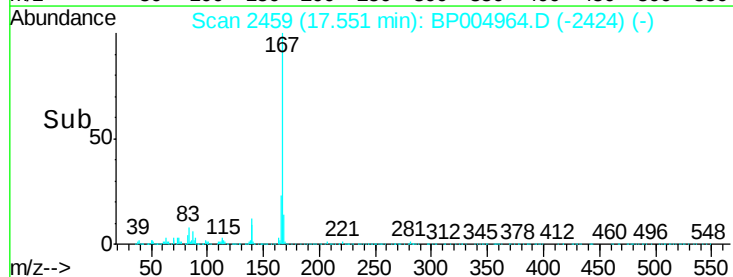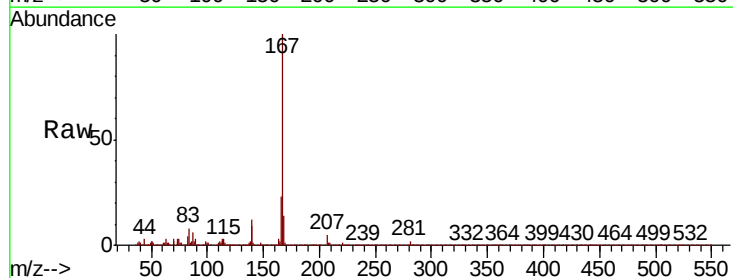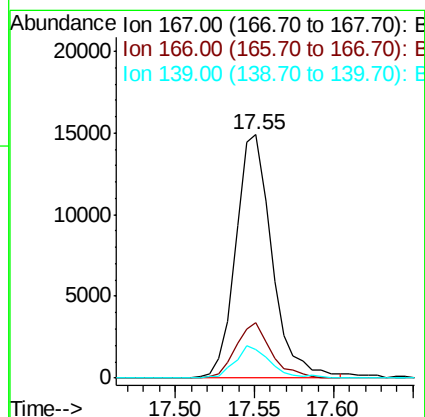







#76
Di-n-butylphthalate
Concen: 2.934 ng/ul
RT: 18.10 min Scan# 2553
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion:	149	Resp:	26212
Ion Ratio	Lower	Upper	
149	100		
150	11.2	7.8	11.8
104	7.8	5.3	7.9




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#77
Fluoranthene
Concen: 3.255 ng/ul
RT: 19.16 min Scan# 2732
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion:	202	Resp:	34456
Ion Ratio	Lower	Upper	
202	100		
101	6.1	7.0	10.6#
100	6.5	5.7	8.5









#80
Pvrene
Concen: 3.404 ng/ul
RT: 19.50 min Scan# 2791
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	12.0	7.9	11.9#
100	9.7	6.8	10.2




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

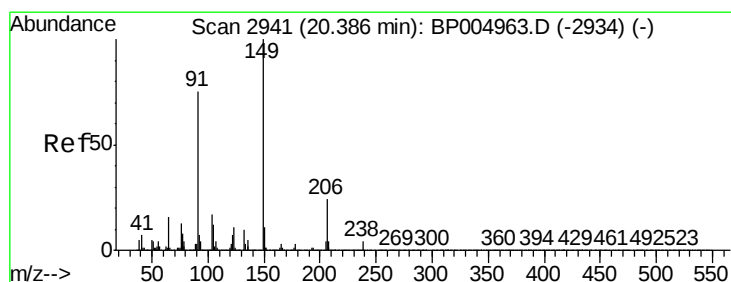

#81
Butylbenzylphthalate
Concen: 2.829 ng/ul
RT: 20.39 min Scan# 2941
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Resp Lower	Upper
149	100		
91	78.9	59.4	89.2
206	21.8	19.0	28.6









#82
 3,3'-Dichlorobenzidine
 Concen: 2.839 ng/ul
 RT: 21.15 min Scan# 3071
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampled :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
252	100		
254	62.4	50.6	75.8
126	9.0	7.5	11.3




Manual Integrations
 APPROVED


mohammad
 3/11/2021 9:25:32 AM



#83
 Benzo(a)anthracene
 Concen: 3.415 ng/ul
 RT: 21.21 min Scan# 3081
 Delta R.T. -0.00 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.0	15.0	22.4
226	26.1	21.2	31.8





#84

Bis(2-ethylhexyl)phthalate

Concen: 2.720 ng/ul

RT: 21.14 min Scan# 3069

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P





ClientSampleId :

MDL-WATER-06

Tot Ion:	149	Resp:	16592
Ion Ratio	Lower	Upper	
149	100		
167	24.5	22.6	34.0
279	5.7	3.8	5.8

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM



#85

Chrysene

Concen: 3.421 ng/ul




RT: 21.26 min Scan# 3090


Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Tgt Ion:	228	Resp:	38013
Ion Ratio	Lower	Upper	
228	100		
226	29.4	22.9	34.3
229	20.5	15.4	23.2





#87

Di-n-octyl phthalate

Concen: 2.676 ng/ul

RT: 22.03 min Scan# 3220

Delta R.T. -0.00 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12

Instrument :

BNA_P


ClientSampleId :

MDL-WATER-06




Tgt Ion:149 Resp: 29127

Manual Integrations
APPROVED

mohammad
3/11/2021 9:25:32 AM



Abundance Ion 149.00 (148.70 to 149.70): E

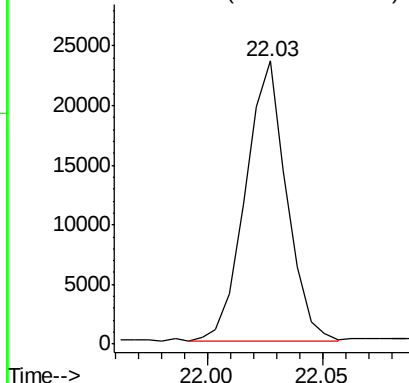

#88

Benzo(b)fluoranthene

Concen: 3.342 ng/ul m

RT: 22.82 min Scan# 3354

Delta R.T. -0.01 min

Lab File: BP004964.D

Acq: 10 Mar 2021 12:12


Tgt Ion:252 Resp: 38615

Ion Ratio Lower Upper



252 100


253 20.2 17.4 26.2

125 10.4 6.4 9.6#



Abundance Ion 252.00 (251.70 to 252.70): E

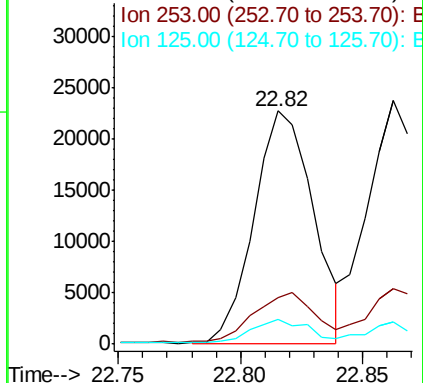







#89
Benzo(k)fluoranthene
Concen: 3.399 ng/ul
RT: 22.86 min Scan# 3362
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.5	17.8	26.8
125	9.1	6.3	9.5




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM



#91
Benzo(a)pyrene
Concen: 3.350 ng/ul
RT: 23.41 min Scan# 3456
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
252	100		
253	28.2	17.6	26.4#
125	9.5	7.0	10.4









#92
Indeno(1,2,3-cd)pyrene
Concen: 3.389 ng/ul
RT: 25.86 min Scan# 3871
Delta R.T. -0.00 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.3	14.7	22.1
277	28.3	19.4	29.0




Manual Integrations
APPROVED


mohammad
3/11/2021 9:25:32 AM

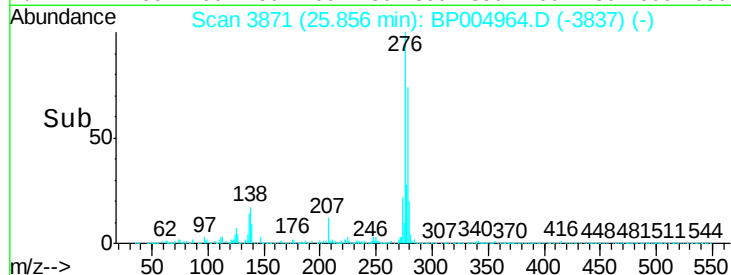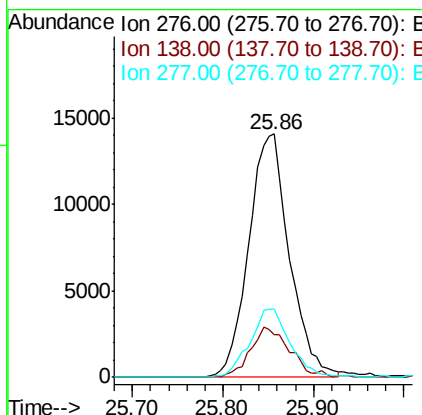

#93
Dibenzo(a,h)anthracene
Concen: 3.363 ng/ul
RT: 25.86 min Scan# 3872
Delta R.T. -0.01 min
Lab File: BP004964.D
Acq: 10 Mar 2021 12:12

Tgt Ion	Ratio	Lower	Upper
278	100		
139	13.6	10.2	15.2
279	25.3	18.9	28.3

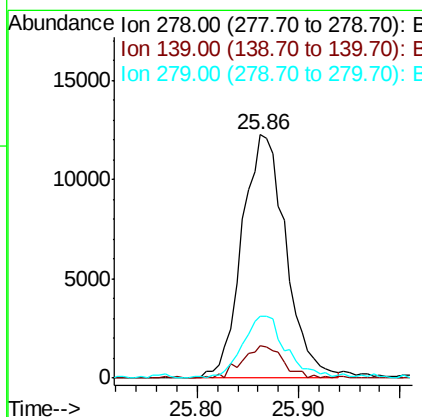



#94
 Benzo(a,h,i)perylene
 Concen: 3.399 ng/ul
 RT: 26.56 min Scan# 3991
 Delta R.T. -0.01 min
 Lab File: BP004964.D
 Acq: 10 Mar 2021 12:12

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-06

Tot Ion:	276	Resp:	36478
Ion Ratio	Lower	Upper	
276	100		
138	16.2	13.4	20.0
277	22.8	17.8	26.6

Manual Integrations
 APPROVED

mohammad
 3/11/2021 9:25:32 AM

