

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
 Data File : BP009319.D
 Acq On : 09 Mar 2022 12:04
 Operator : CG/JU
 Sample : PB143171BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143171BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	406	413	428	rBV	8010863	12670554	50.84%	10.564%
2	6.993	673	681	700	rBV	7345994	12671247	50.84%	10.564%
3	7.822	813	822	830	rBV	1568519	2677192	10.74%	2.232%
4	8.975	1009	1018	1031	rBV	4698915	8299236	33.30%	6.919%
5	10.616	1287	1297	1307	rBV	2029698	3699828	14.85%	3.085%
6	13.086	1706	1717	1733	rBV	12133801	19818264	79.52%	16.523%
7	14.457	1943	1950	1966	rBV	2961644	4792639	19.23%	3.996%
8	15.951	2197	2204	2232	rBV	8513493	13928704	55.89%	11.612%
9	17.215	2411	2419	2432	rBV	3558257	5387892	21.62%	4.492%
10	19.515	2805	2810	2815	rBV	261088	333378	1.34%	0.278%
11	19.792	2851	2857	2869	rBV	17859930	24921662	100.00%	20.777%
12	21.321	3112	3117	3127	rBV	3745467	5286348	21.21%	4.407%
13	23.727	3520	3526	3539	rVB2	2481099	5459255	21.91%	4.551%




Sum of corrected areas: 119946199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009319.D
Acq On : 09 Mar 2022 12:04
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

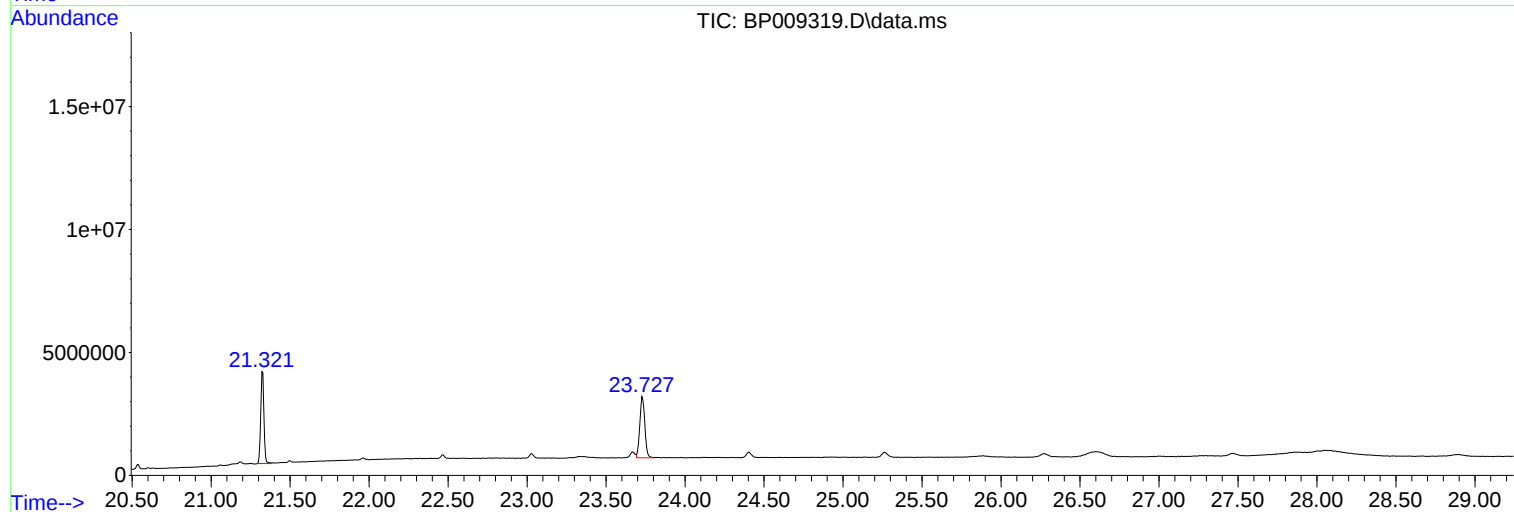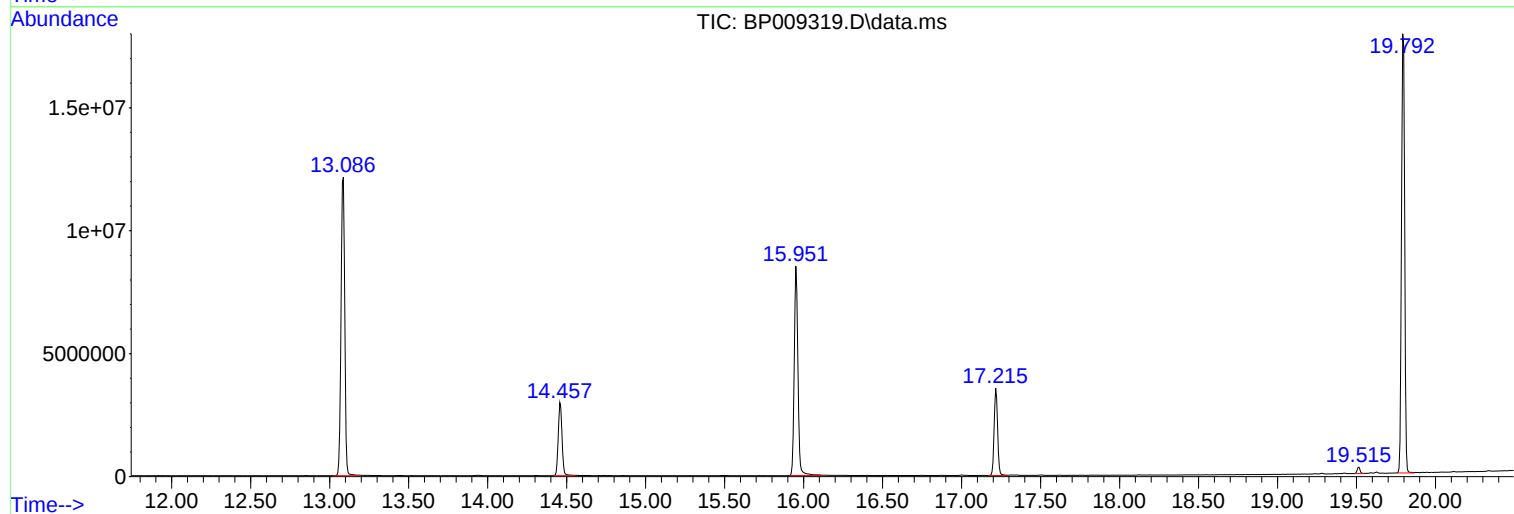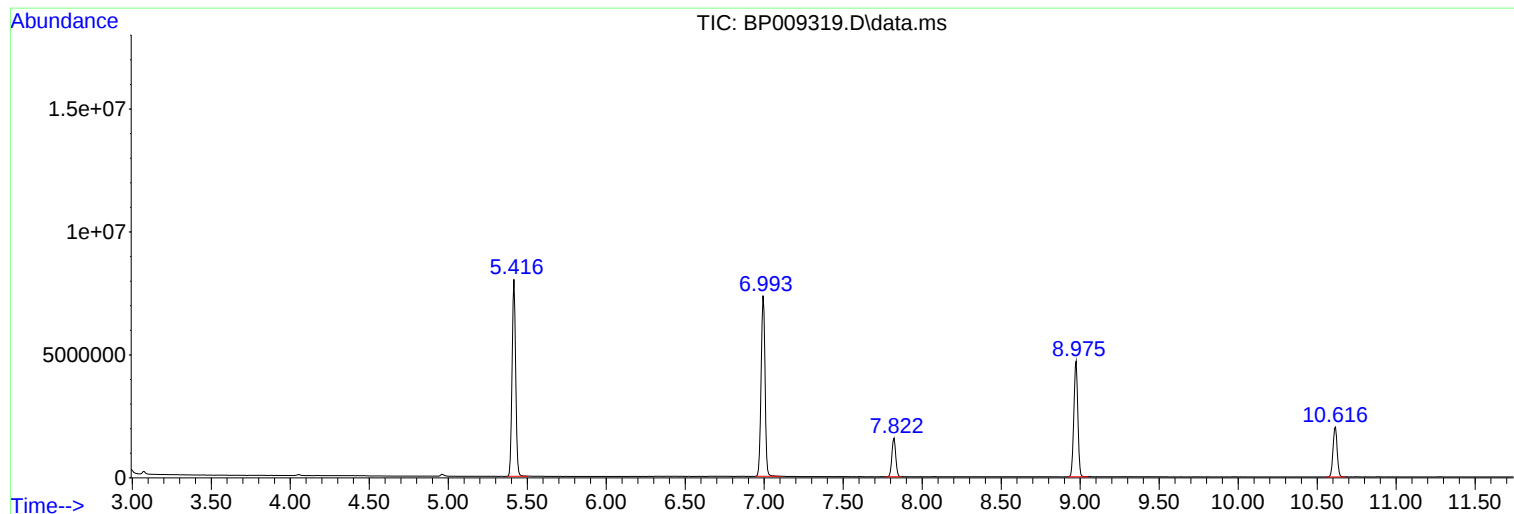

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009319.D
Acq On : 09 Mar 2022 12:04
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009319.D
Acq On : 09 Mar 2022 12:04
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------