

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
 Data File : BP009335.D
 Acq On : 09 Mar 2022 21:31
 Operator : CG/JU
 Sample : N1845-14 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SAMPLE-14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	20	rVB	86861	137066	1.08%	0.192%
2	4.364	229	234	245	rBV	82453	139773	1.11%	0.196%
3	4.952	328	334	346	rBV	515321	887354	7.02%	1.242%
4	5.411	405	412	421	rBV	528706	916884	7.25%	1.284%
5	6.987	672	680	690	rBV	1115638	2022870	16.01%	2.832%
6	7.816	814	821	829	rBV	815989	1405993	11.12%	1.968%
7	8.969	1002	1017	1027	rBV	702801	1316825	10.42%	1.844%
8	10.610	1286	1296	1303	rBV	1290962	2381763	18.85%	3.335%
9	13.075	1708	1715	1727	rBV	2393985	3821288	30.24%	5.350%
10	14.457	1942	1950	1956	rVV	2443272	3992279	31.59%	5.589%
11	14.516	1956	1960	1968	rVB	94063	167241	1.32%	0.234%
12	14.851	2013	2017	2025	rVB	72025	140228	1.11%	0.196%
13	15.945	2198	2203	2213	rVB2	214573	373624	2.96%	0.523%
14	16.198	2241	2246	2248	rBV2	110915	163588	1.29%	0.229%
15	16.863	2355	2359	2366	rVB	102042	160833	1.27%	0.225%
16	16.998	2378	2382	2385	rBV	96910	138176	1.09%	0.193%
17	17.210	2412	2418	2423	rBV	3831298	6314839	49.96%	8.841%
18	17.257	2423	2426	2432	rVB	1321297	1803172	14.27%	2.525%
19	17.345	2437	2441	2447	rVB	307561	462558	3.66%	0.648%
20	17.616	2480	2487	2493	rBV	125552	277765	2.20%	0.389%
21	17.739	2504	2508	2512	rBV	135199	162722	1.29%	0.228%
22	18.086	2563	2567	2570	rBV	163450	226585	1.79%	0.317%
23	18.134	2571	2575	2580	rVB	265880	409144	3.24%	0.573%
24	18.275	2594	2599	2603	rBV2	212928	394538	3.12%	0.552%
25	18.416	2619	2623	2629	rBV2	143745	211152	1.67%	0.296%
26	18.575	2646	2650	2653	rBV	132160	205364	1.62%	0.288%
27	18.863	2696	2699	2703	rBV2	109456	154283	1.22%	0.216%
28	18.981	2715	2719	2723	rBV2	154712	217702	1.72%	0.305%
29	19.028	2723	2727	2731	rBV5	205340	301357	2.38%	0.422%
30	19.110	2738	2741	2747	rVB3	169238	232499	1.84%	0.326%
31	19.233	2757	2762	2769	rBV	2481031	3417065	27.04%	4.784%
32	19.586	2813	2822	2830	rBV	2211470	4005024	31.69%	5.607%
33	19.786	2848	2856	2867	rBV	8260859	11625816	91.99%	16.277%
34	21.051	3068	3071	3076	rBV3	735206	1104784	8.74%	1.547%
35	21.322	3110	3117	3121	rBV2	7808687	12638568	100.00%	17.695%
36	23.727	3520	3526	3533	rBV2	4418502	9094639	71.96%	12.733%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009335.D
Acq On : 09 Mar 2022 21:31
Operator : CG/JU
Sample : N1845-14 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-14

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 71425361

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009335.D
Acq On : 09 Mar 2022 21:31
Operator : CG/JU
Sample : N1845-14 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

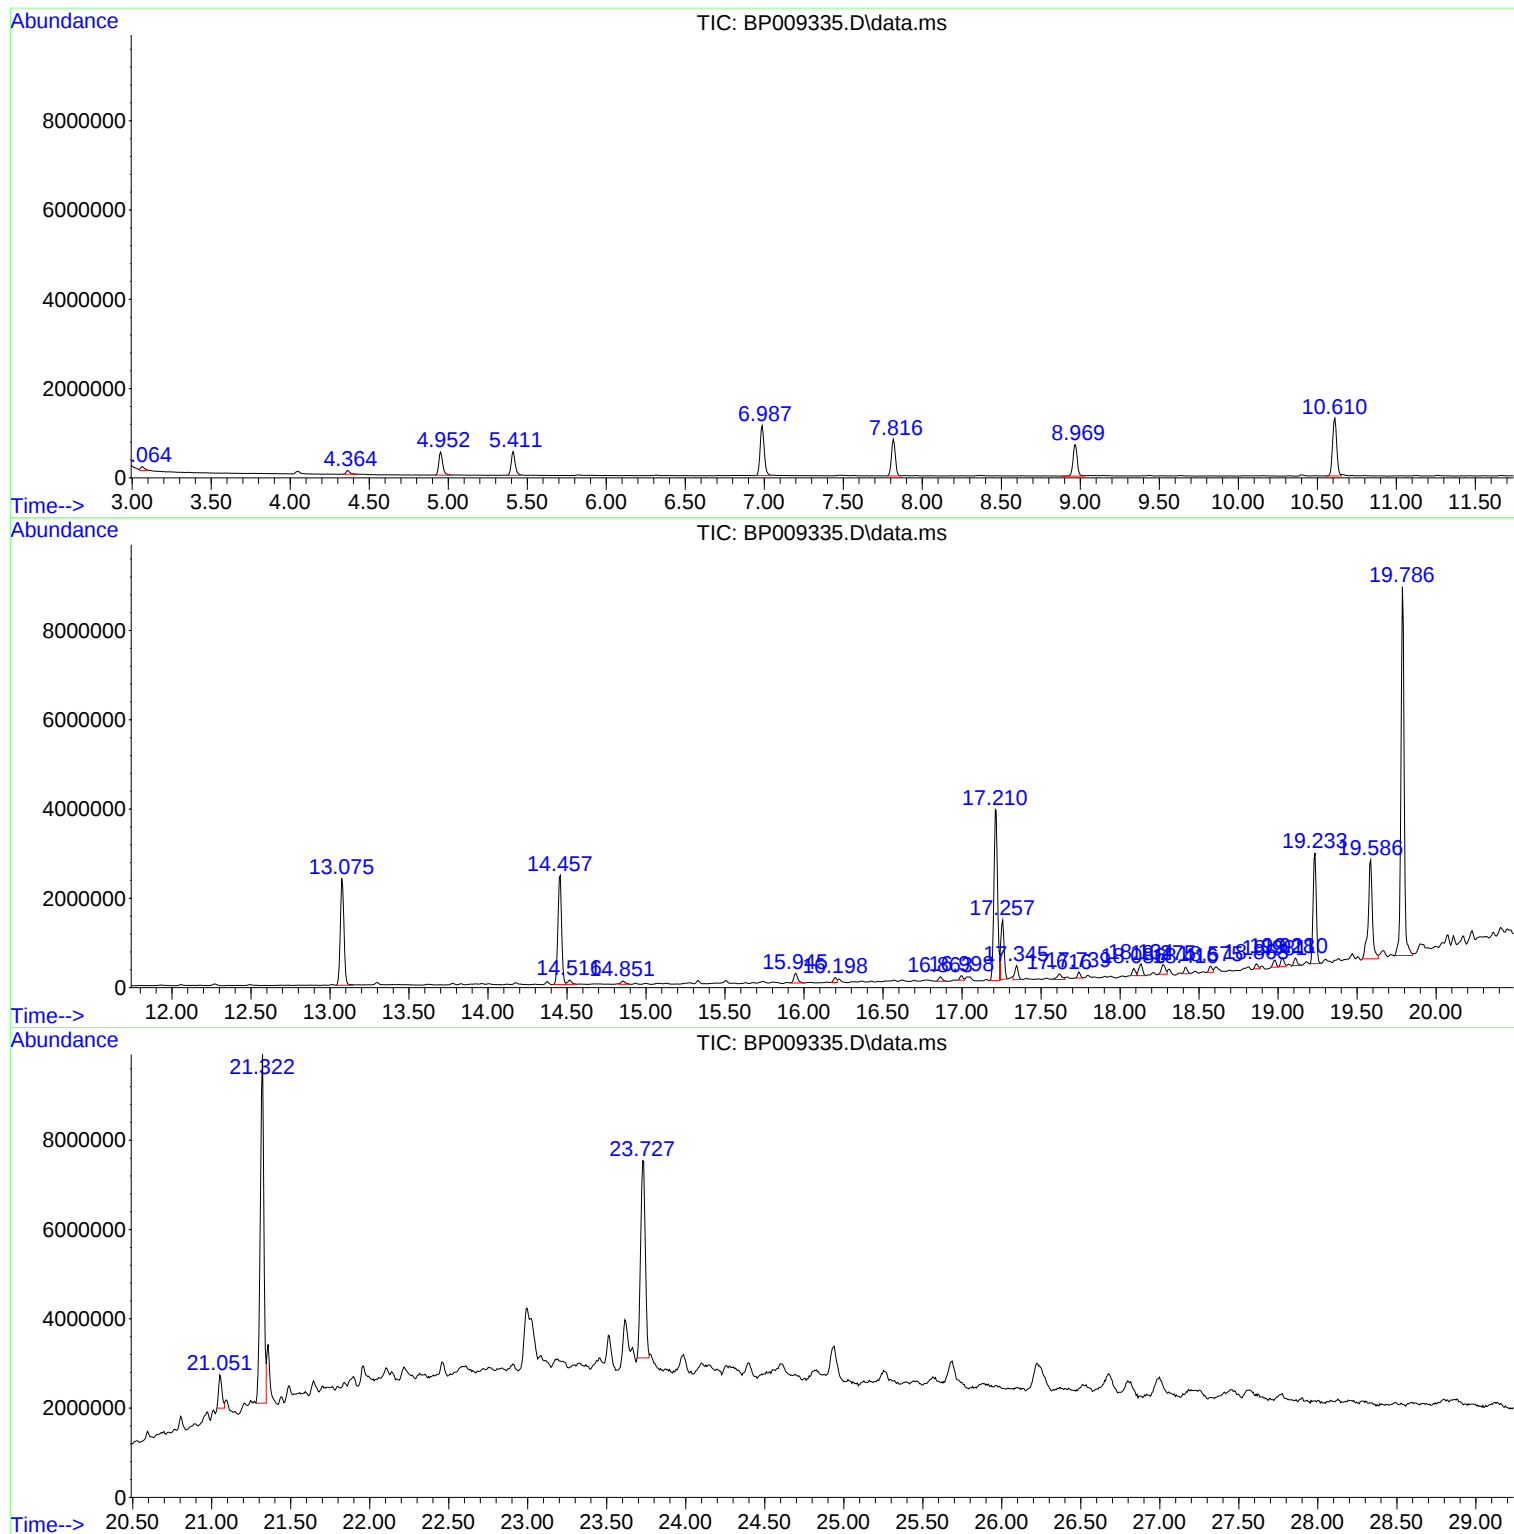

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009335.D
Acq On : 09 Mar 2022 21:31
Operator : CG/JU
Sample : N1845-14 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-14










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.952	12.62 ng	887354	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

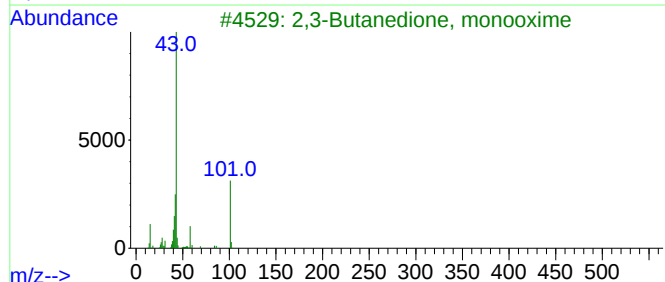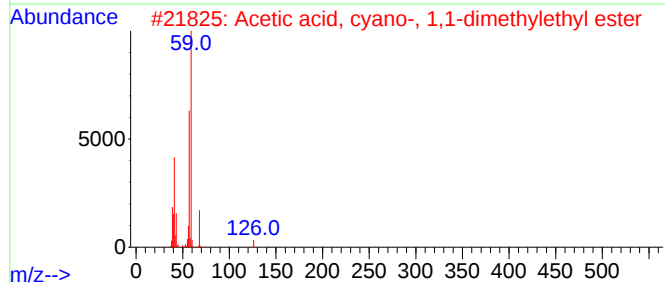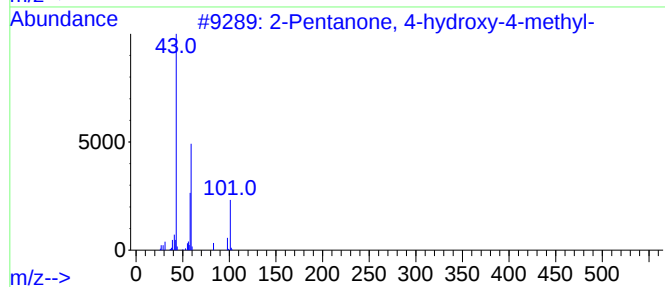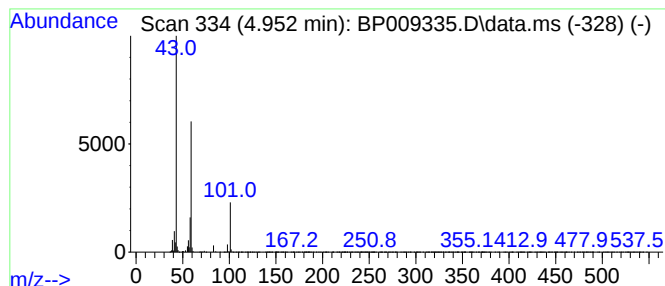

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
Data File : BP009335.D
Acq On : 09 Mar 2022 21:31
Operator : CG/JU
Sample : N1845-14 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.952	12.6	ng	887354	1	7.816	1405990	20.0