
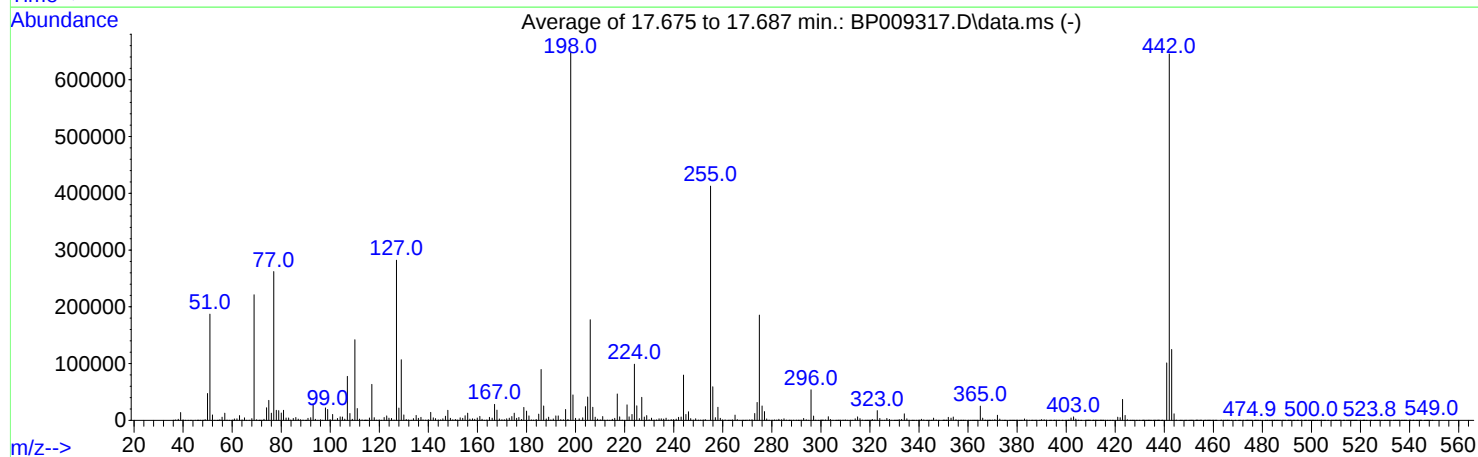


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030922\
 Data File : BP009317.D
 Acq On : 09 Mar 2022 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

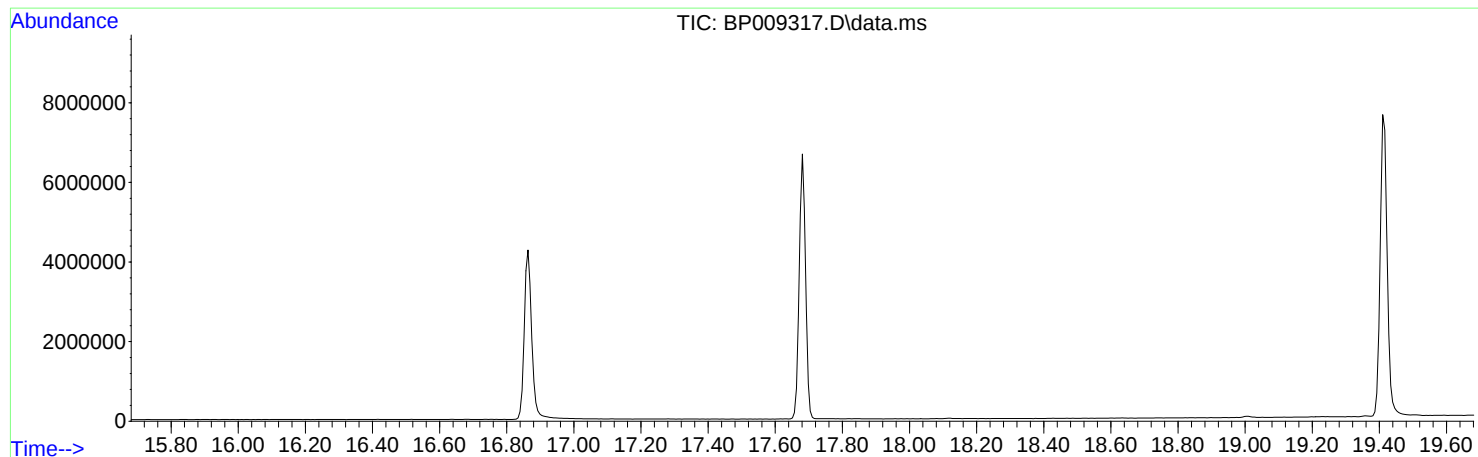

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	187041	PASS
68	69	0.00	2	1.4	3186	PASS
69	198	0.00	100	34.2	221394	PASS
70	69	0.00	2	0.5	1139	PASS
127	198	10	80	43.5	282080	PASS
197	198	0.00	2	0.2	1213	PASS
198	198	100	100	100.0	648014	PASS
199	198	5	9	6.9	44728	PASS
275	198	10	60	28.6	185422	PASS
365	198	1	100	3.9	25019	PASS
441	198	0.01	100	15.6	101107	PASS
442	442	100	100	100.0	645504	PASS
443	442	15	24	19.3	124878	PASS