

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
 Data File : BP009348.D
 Acq On : 10 Mar 2022 17:16
 Operator : CG/JU
 Sample : N1847-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CG-B1-030722-0-2-BD

Quant Time: Mar 11 05:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	523539	20.000	ng	0.00
21) Naphthalene-d8	10.610	136	2131922	20.000	ng	0.00
39) Acenaphthene-d10	14.457	164	1303225	20.000	ng	0.00
64) Phenanthrene-d10	17.215	188	2544448	20.000	ng	0.00
76) Chrysene-d12	21.321	240	1899172	20.000	ng	0.00
86) Perylene-d12	23.727	264	2067206	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	3360366	93.690	ng	0.00
7) Phenol-d6	6.992	99	4309058	94.540	ng	0.00
23) Nitrobenzene-d5	8.969	82	2763719	71.401	ng	0.00
42) 2,4,6-Tribromophenol	15.951	330	1864952	118.511	ng	0.00
45) 2-Fluorobiphenyl	13.080	172	6390527	67.435	ng	0.00
79) Terphenyl-d14	19.792	244	7971994	79.214	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.245	149	3931810	53.116	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009348.D
Acq On : 10 Mar 2022 17:16
Operator : CG/JU
Sample : N1847-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD

Quant Time: Mar 11 05:02:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration




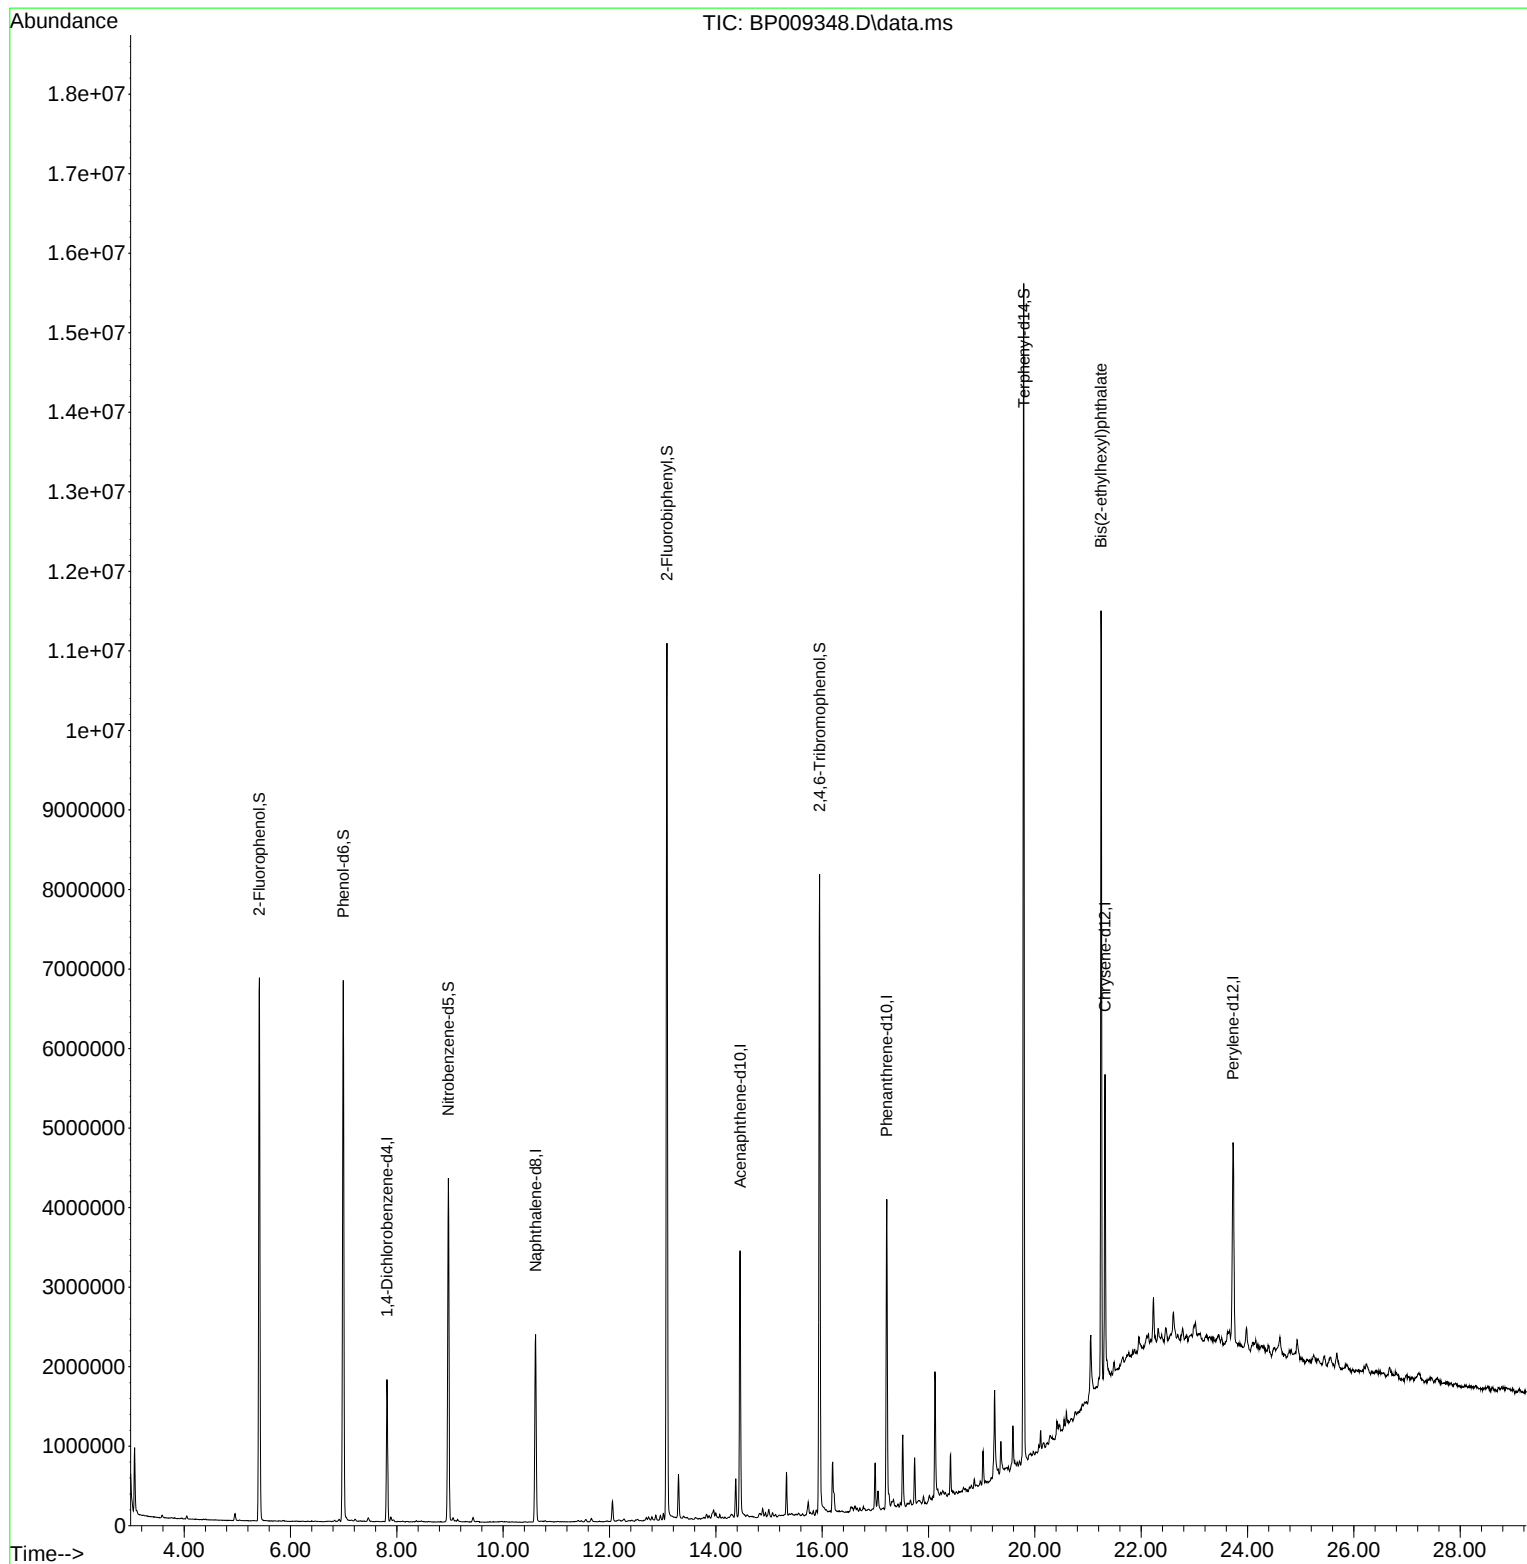




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.816 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16




Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD

Tgt Ion:152 Resp: 523539
Ion Ratio Lower Upper
152 100
150 153.6 124.5 186.7
115 58.1 48.2 72.4

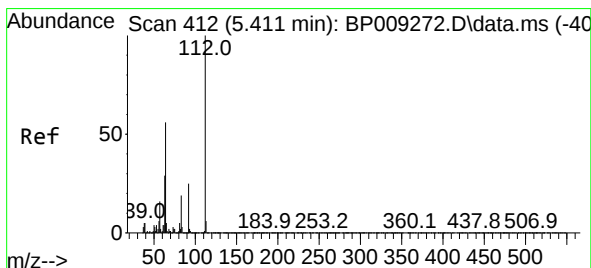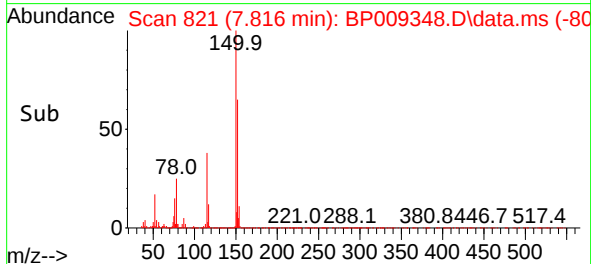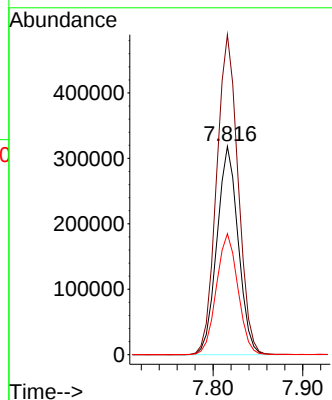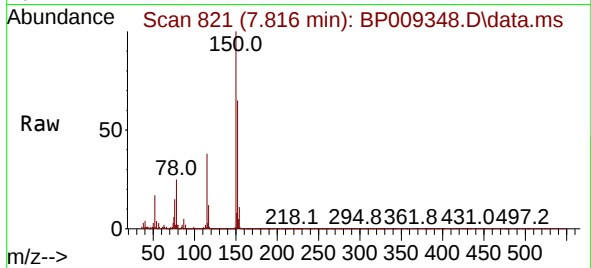

#5
2-Fluorophenol
Concen: 93.690 ng
RT: 5.416 min Scan# 413
Delta R.T. 0.005 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16

Tgt Ion:112 Resp: 3360366
Ion Ratio Lower Upper
112 100
64 54.5 45.0 67.4
63 27.8 23.0 34.6


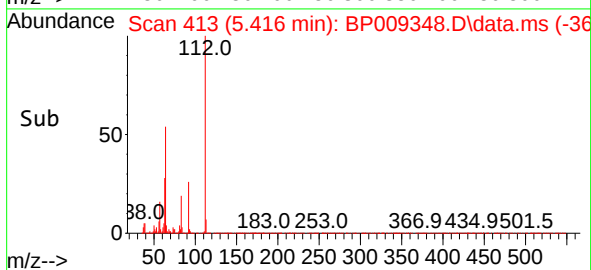
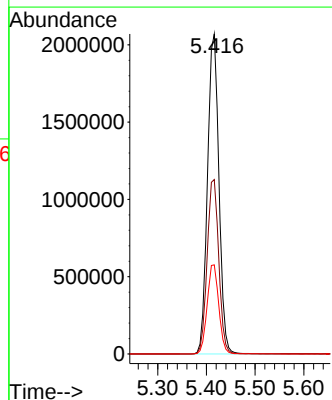
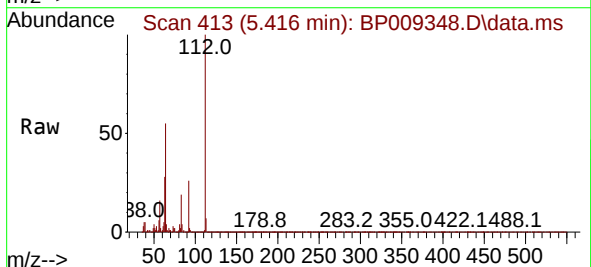




#7
Phenol-d6
Concen: 94.540 ng
RT: 6.992 min Scan# 61
Delta R.T. 0.005 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16




Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD


Tgt Ion: 99 Resp: 4309058
Ion Ratio Lower Upper
99 100
42 15.5 12.8 19.2
71 33.5 26.3 39.5

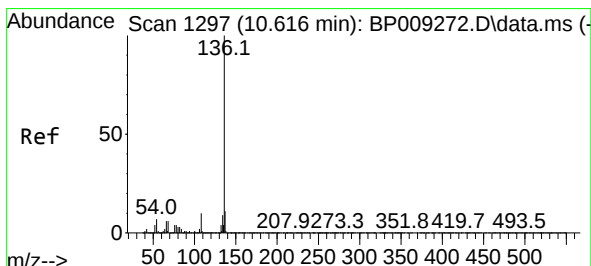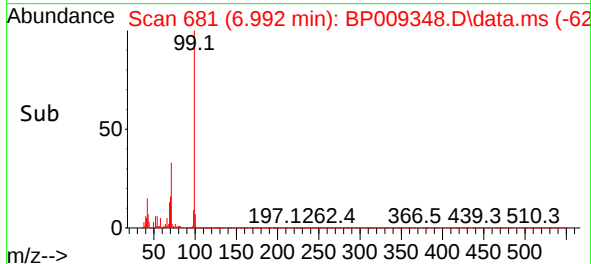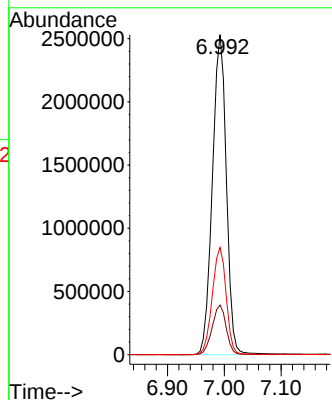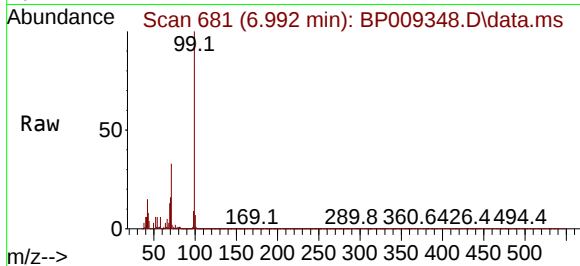

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.610 min Scan# 1296
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16

Tgt Ion:136 Resp: 2131922
Ion Ratio Lower Upper
136 100
137 11.2 8.6 12.8
54 6.8 5.8 8.8
68 6.0 5.2 7.8


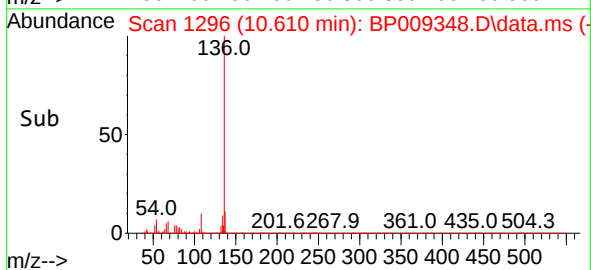
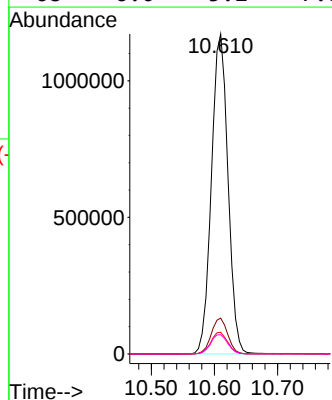
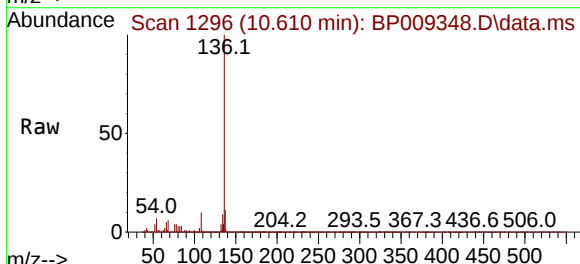


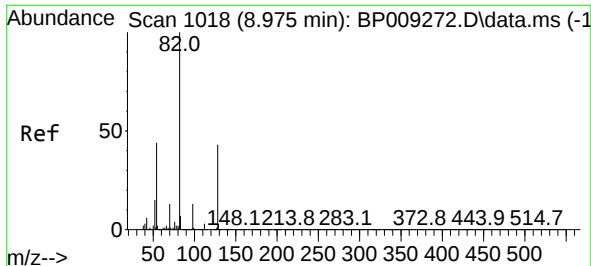

#23
Nitrobenzene-d5
Concen: 71.401 ng
RT: 8.969 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16




Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD


Tgt Ion: 82 Resp: 2763719
Ion Ratio Lower Upper
82 100
128 44.0 34.2 51.4
54 42.4 34.7 52.1

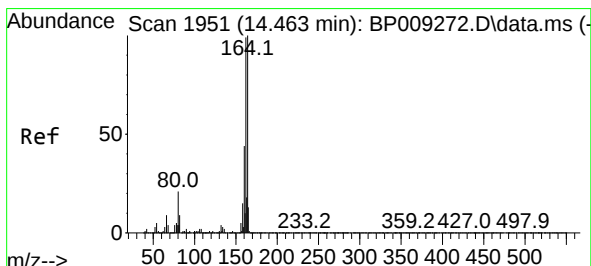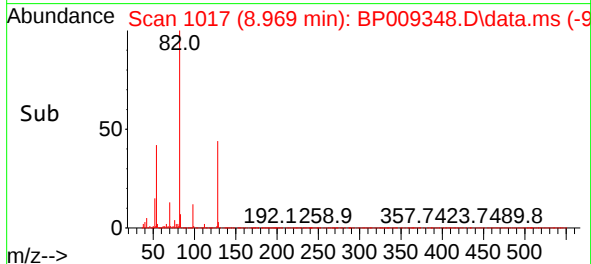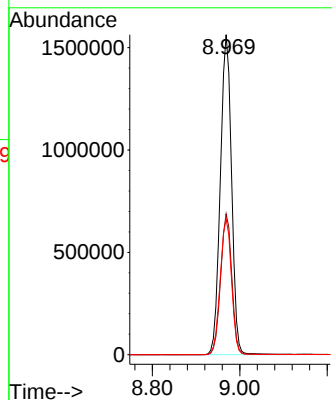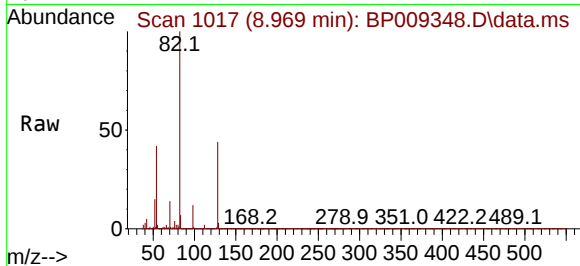

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.457 min Scan# 1950
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16

Tgt Ion:164 Resp: 1303225
Ion Ratio Lower Upper
164 100
162 101.4 79.1 118.7
160 44.6 34.9 52.3


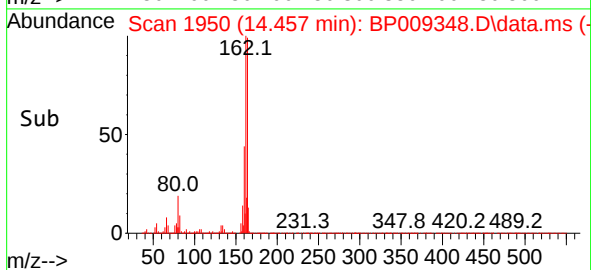
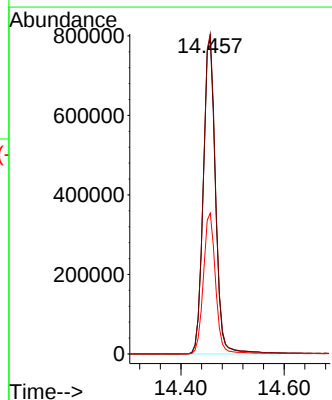
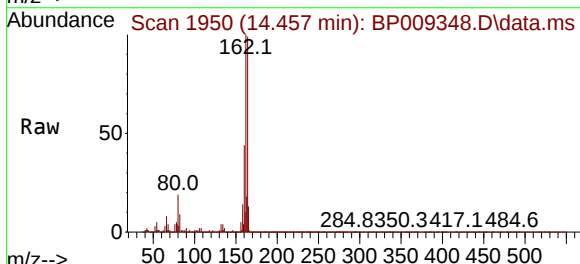


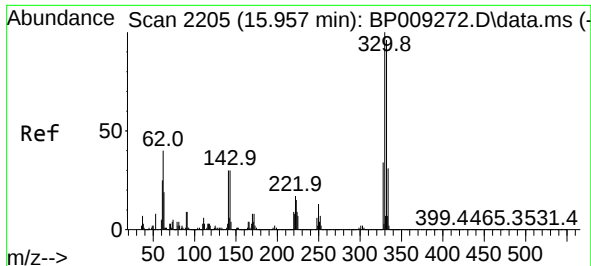

#42
2,4,6-Tribromophenol
Concen: 118.511 ng
RT: 15.951 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16




Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD


Tgt Ion:330 Resp: 1864952
Ion Ratio Lower Upper
330 100
332 97.0 77.0 115.6
141 28.8 27.6 41.4

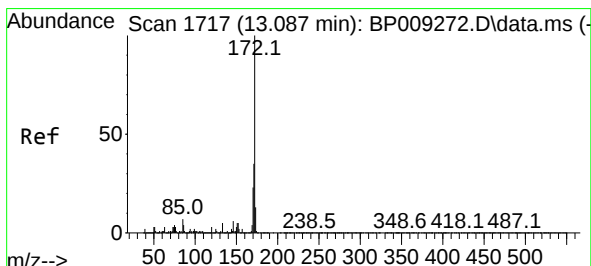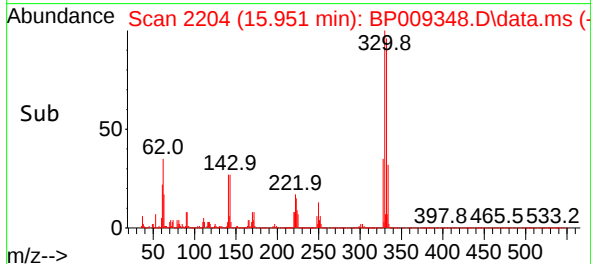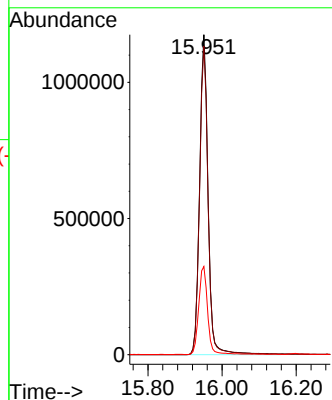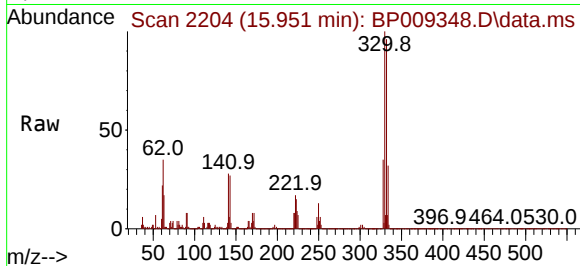

#45
2-Fluorobiphenyl
Concen: 67.435 ng
RT: 13.080 min Scan# 1716
Delta R.T. -0.007 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16

Tgt Ion:172 Resp: 6390527
Ion Ratio Lower Upper
172 100
171 35.5 28.0 42.0
170 23.3 18.6 27.8


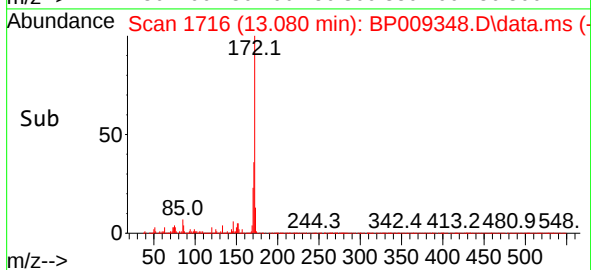
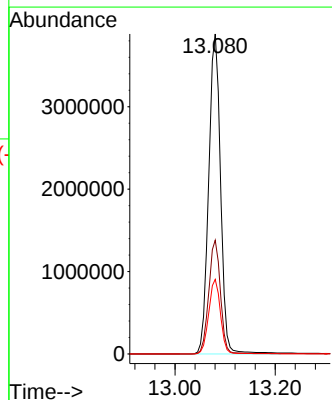
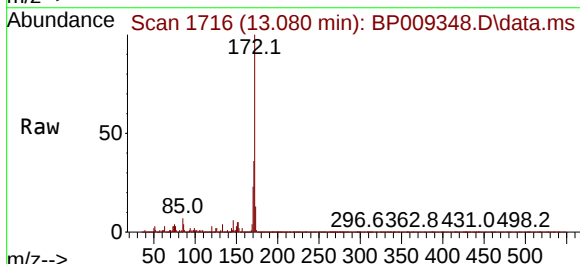


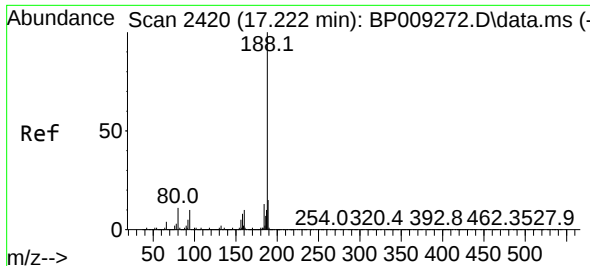

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.215 min Scan# 2419
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16




Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD


Tgt Ion:188 Resp: 2544448
Ion Ratio Lower Upper
188 100
94 8.9 7.9 11.9
80 9.8 8.8 13.2

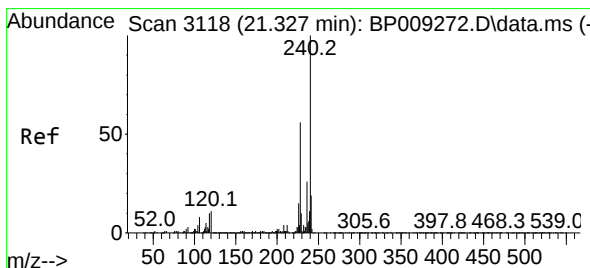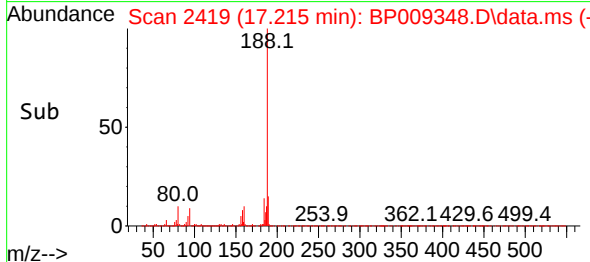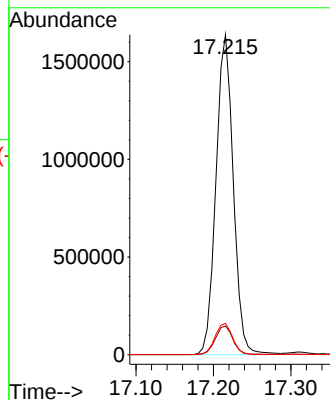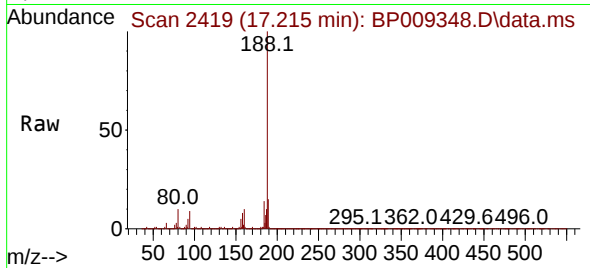

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.321 min Scan# 3117
Delta R.T. -0.006 min
Lab File: BP009348.D
Acq: 10 Mar 2022 17:16

Tgt Ion:240 Resp: 1899172
Ion Ratio Lower Upper
240 100
120 9.5 9.0 13.4
236 25.8 20.6 30.8


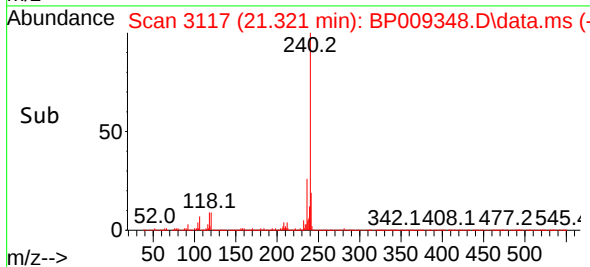
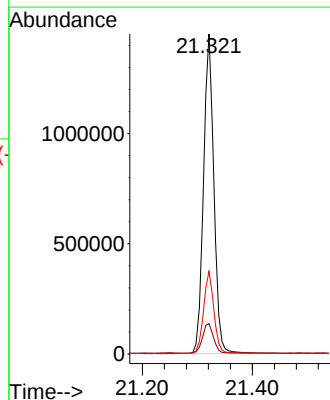
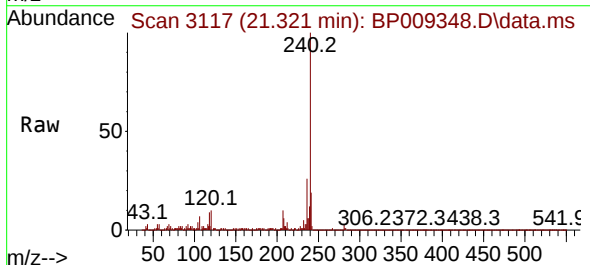


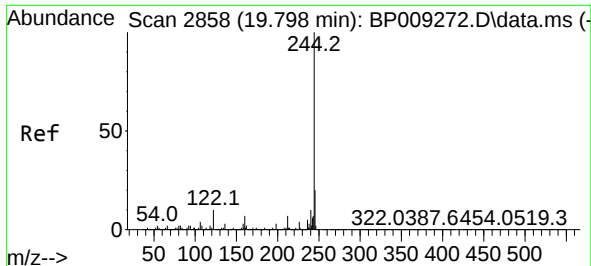

#79
 Terphenyl-d14
 Concen: 79.214 ng
 RT: 19.792 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP009348.D
 Acq: 10 Mar 2022 17:16




Instrument :
 BNA_P
 ClientSampleId :
 CG-B1-030722-0-2-BD


Tgt Ion:244 Resp: 7971994
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 9.1 8.3 12.5

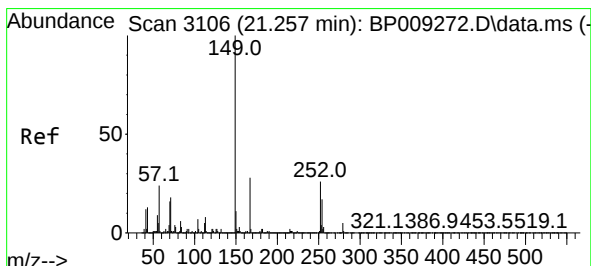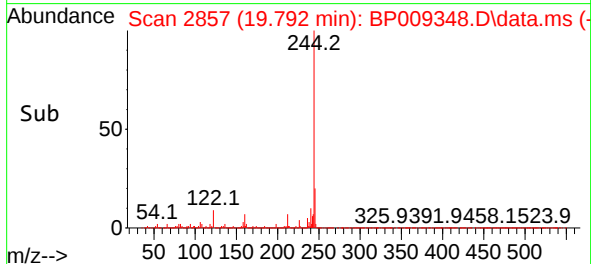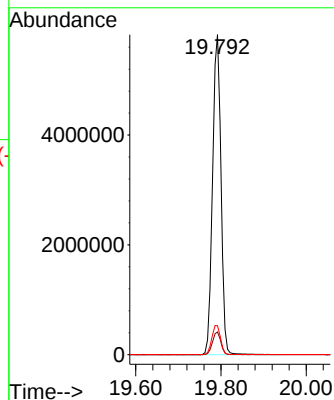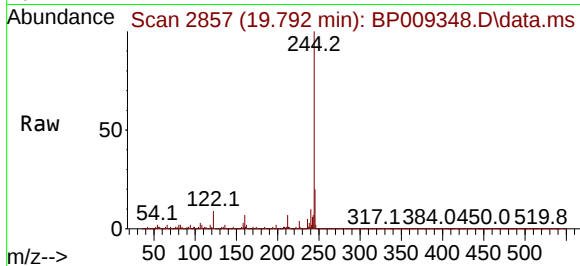

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 53.116 ng
 RT: 21.245 min Scan# 3104
 Delta R.T. -0.012 min
 Lab File: BP009348.D
 Acq: 10 Mar 2022 17:16

Tgt Ion:149 Resp: 3931810
 Ion Ratio Lower Upper
 149 100
 167 28.2 22.6 33.8
 279 4.9 3.8 5.6

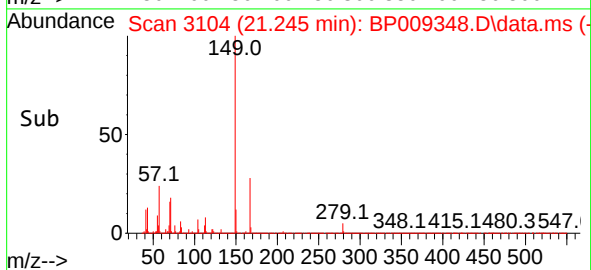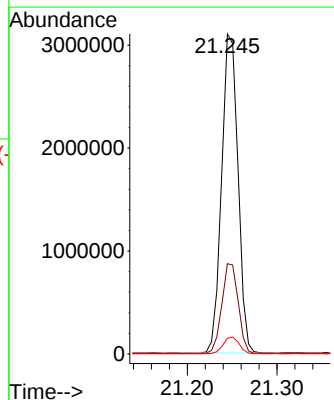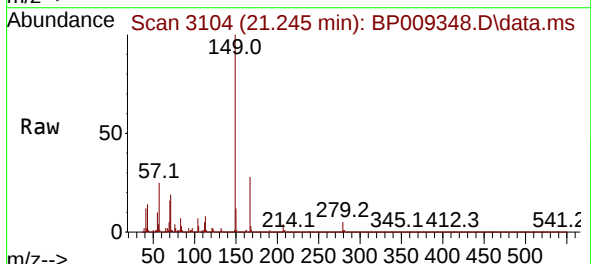

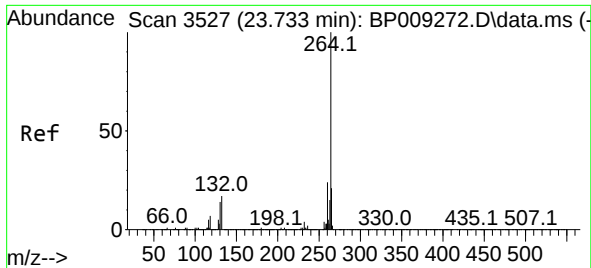

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.727 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP009348.D
 Acq: 10 Mar 2022 17:16

Instrument :
 BNA_P
 ClientSampleId :
 CG-B1-030722-0-2-BD

Tgt Ion:264 Resp: 2067206
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.4 29.0
 265 22.8 17.2 25.8

