

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
 Data File : BP009340.D
 Acq On : 10 Mar 2022 11:52
 Operator : CG/JU
 Sample : PB143199BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143199BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	405	413	426	rBV	6845387	10898683	51.15%	10.690%
2	6.993	673	681	698	rBV	6449128	10977934	51.52%	10.768%
3	7.816	814	821	829	rBV	1274653	2187331	10.26%	2.145%
4	8.969	1007	1017	1027	rBV	4123358	7248957	34.02%	7.110%
5	10.610	1286	1296	1305	rBV	1661369	3036370	14.25%	2.978%
6	13.081	1707	1716	1738	rBV	10837617	17467945	81.98%	17.133%
7	14.457	1942	1950	1971	rBV	2374929	3969632	18.63%	3.894%
8	15.951	2196	2204	2237	rBV	7303247	12305132	57.75%	12.069%
9	17.216	2411	2419	2432	rBV	2832138	4362671	20.47%	4.279%
10	19.792	2851	2857	2871	rVB	15686676	21308659	100.00%	20.901%
11	21.321	3112	3117	3124	rBV	2882208	4040262	18.96%	3.963%
12	23.727	3519	3526	3539	rVB2	1822790	4148792	19.47%	4.069%




Sum of corrected areas: 101952368

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009340.D
Acq On : 10 Mar 2022 11:52
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

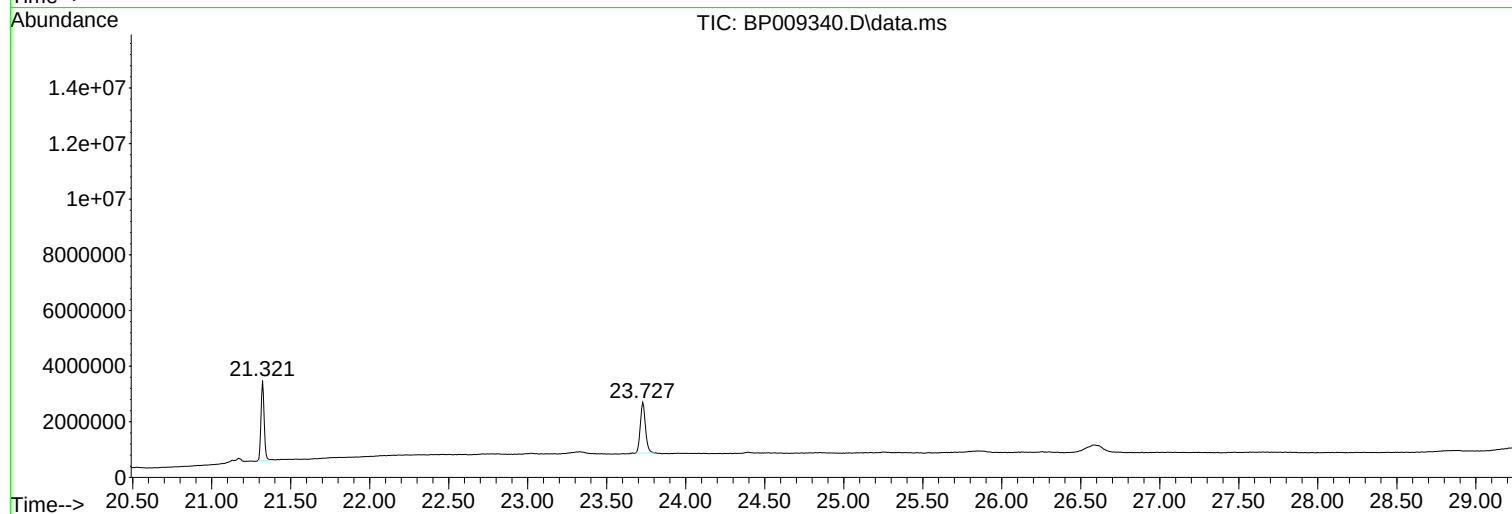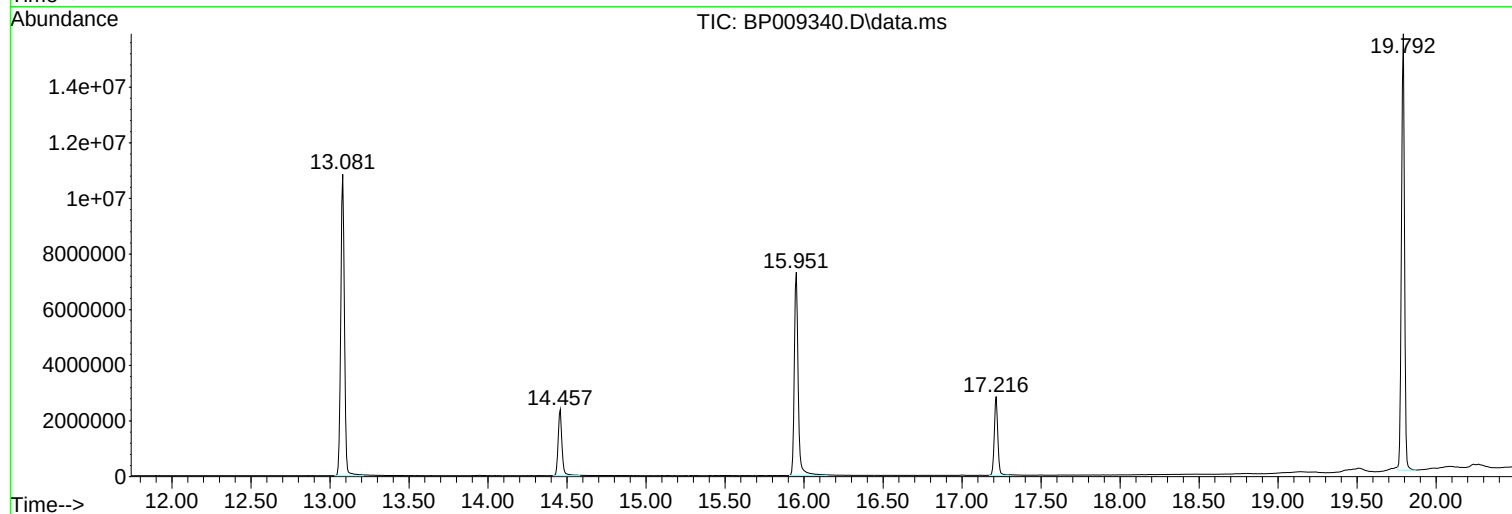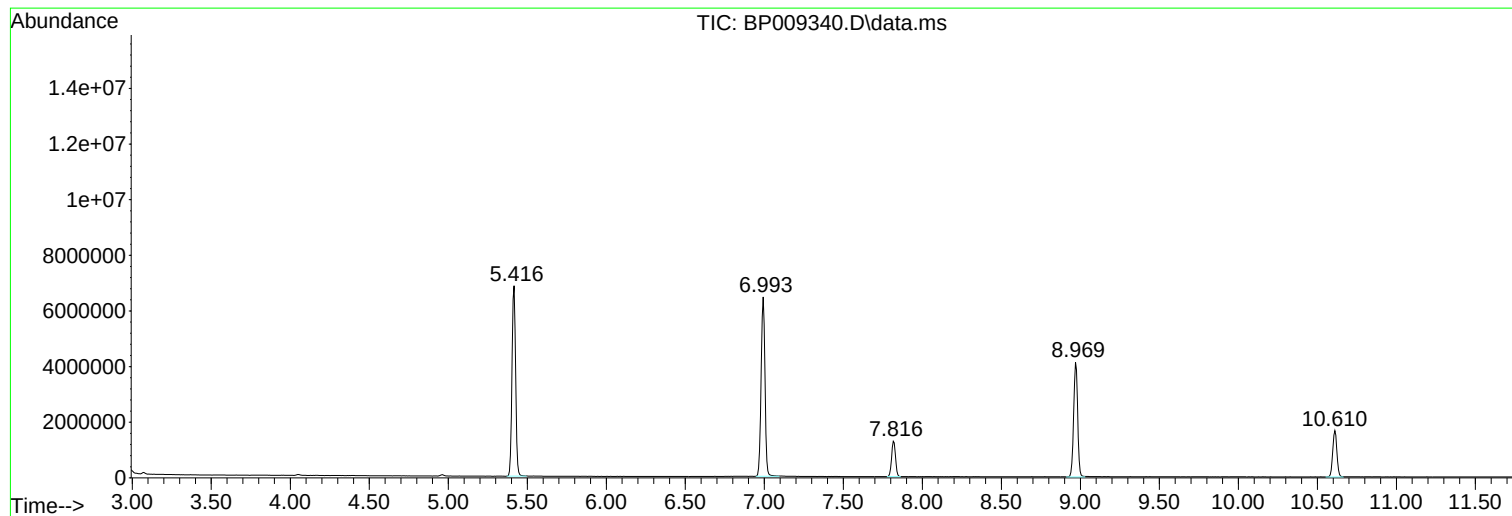

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009340.D
Acq On : 10 Mar 2022 11:52
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009340.D
Acq On : 10 Mar 2022 11:52
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------