

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
 Data File : BP009348.D
 Acq On : 10 Mar 2022 17:16
 Operator : CG/JU
 Sample : N1847-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CG-B1-030722-0-2-BD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	20	rBV	798662	1009653	4.96%	0.719%
2	5.416	405	413	425	rBV	6828809	11142161	54.78%	7.938%
3	6.992	673	681	690	rBV	6800524	11636195	57.21%	8.290%
4	7.816	814	821	828	rBV	1786641	2968220	14.59%	2.115%
5	8.969	1005	1017	1026	rBV	4323031	7657922	37.65%	5.456%
6	10.610	1286	1296	1308	rBV	2357067	4331633	21.30%	3.086%
7	12.057	1535	1542	1549	rBV	256032	412567	2.03%	0.294%
8	13.080	1708	1716	1730	rBV	11014891	17915269	88.08%	12.764%
9	13.298	1747	1753	1762	rVB	551800	805472	3.96%	0.574%
10	13.957	1856	1865	1869	rBV4	103453	263076	1.29%	0.187%
11	14.374	1930	1936	1941	rBV	484533	674258	3.31%	0.480%
12	14.457	1942	1950	1968	rVV	3346949	5600869	27.54%	3.990%
13	15.327	2093	2098	2103	rVB	544393	698904	3.44%	0.498%
14	15.739	2161	2168	2172	rBV	160531	308872	1.52%	0.220%
15	15.951	2197	2204	2223	rBV	8032229	13005044	63.94%	9.266%
16	16.198	2241	2246	2259	rBV	631994	1252349	6.16%	0.892%
17	16.998	2377	2382	2386	rBV	570230	811444	3.99%	0.578%
18	17.051	2387	2391	2401	rVB	239770	414982	2.04%	0.296%
19	17.215	2412	2419	2425	rBV	3896265	6133456	30.15%	4.370%
20	17.515	2465	2470	2479	rVB	900293	1359247	6.68%	0.968%
21	17.739	2504	2508	2513	rVB	570368	711794	3.50%	0.507%
22	18.121	2569	2573	2581	rBV	1578963	2288085	11.25%	1.630%
23	18.415	2618	2623	2627	rBV	507950	655137	3.22%	0.467%
24	19.027	2723	2727	2732	rBV	424627	606655	2.98%	0.432%
25	19.245	2757	2764	2773	rBV2	1090087	2044524	10.05%	1.457%
26	19.362	2780	2784	2795	rBV	390278	730407	3.59%	0.520%
27	19.586	2819	2822	2827	rVB	464045	529620	2.60%	0.377%
28	19.792	2851	2857	2869	rVB	14790725	20340600	100.00%	14.492%
29	21.051	3068	3071	3081	rVB2	677378	1167123	5.74%	0.832%
30	21.245	3100	3104	3111	rVB	9661522	12132430	59.65%	8.644%
31	21.321	3112	3117	3122	rBV	3774409	5126285	25.20%	3.652%
32	23.727	3521	3526	3541	rVB2	2550179	5625021	27.65%	4.008%




Sum of corrected areas: 140359274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009348.D
Acq On : 10 Mar 2022 17:16
Operator : CG/JU
Sample : N1847-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

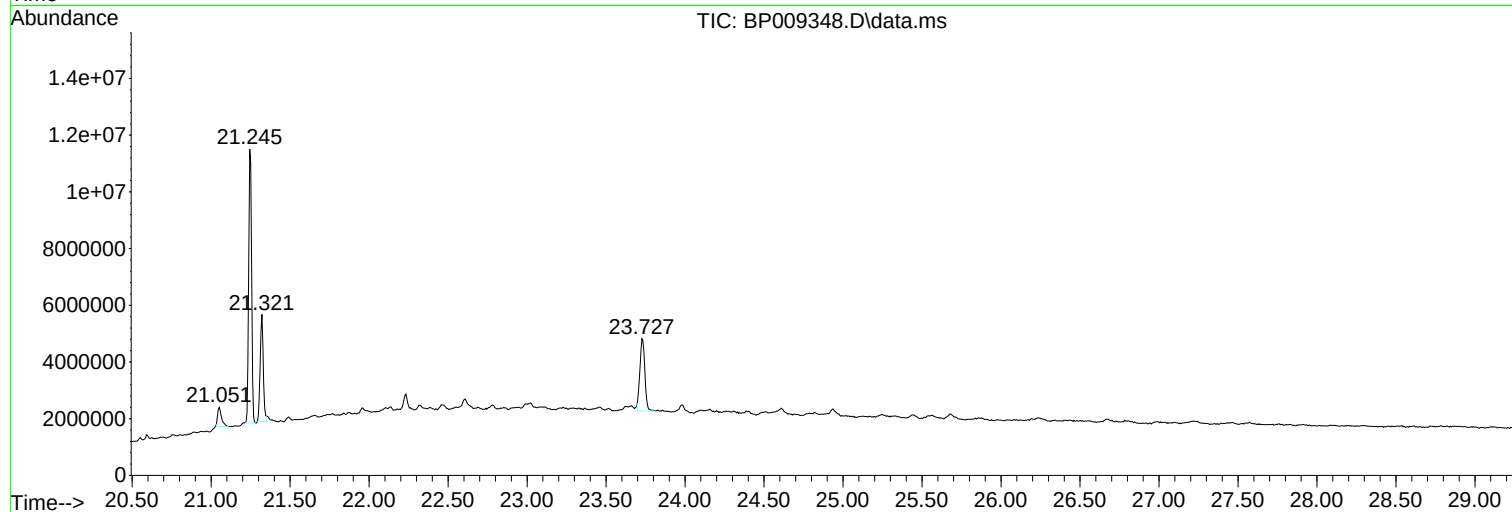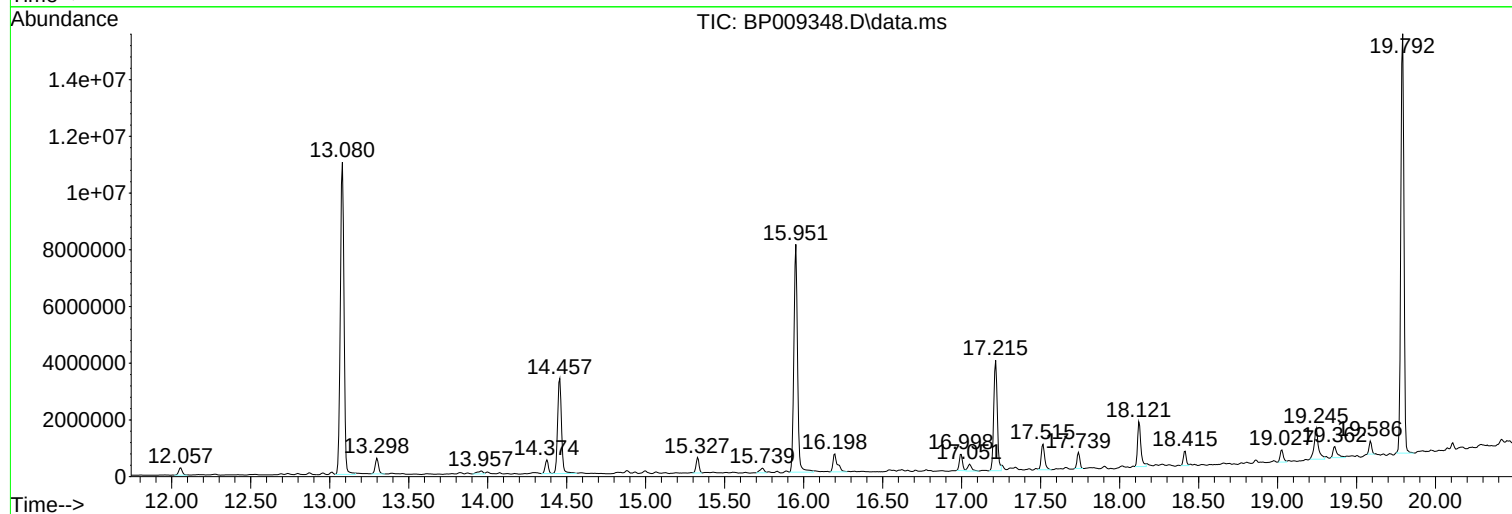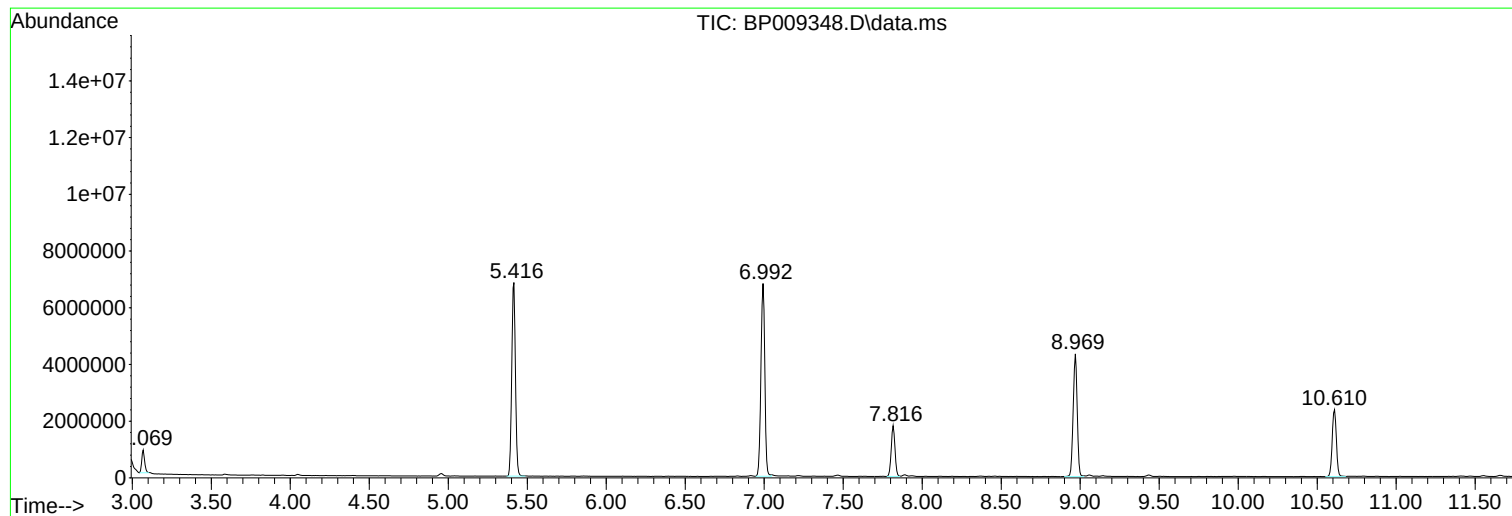

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009348.D
Acq On : 10 Mar 2022 17:16
Operator : CG/JU
Sample : N1847-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009348.D
Acq On : 10 Mar 2022 17:16
Operator : CG/JU
Sample : N1847-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc