

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
 Data File : BP009349.D
 Acq On : 10 Mar 2022 17:50
 Operator : CG/JU
 Sample : N1847-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CG-B1-030722-0-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	20	rBV	609762	803885	5.84%	0.858%
2	5.410	405	412	432	rBV	5431587	8827125	64.16%	9.420%
3	6.992	672	681	700	rBV	5554514	9489830	68.98%	10.128%
4	7.816	813	821	829	rBV	1798278	3016356	21.93%	3.219%
5	8.969	1006	1017	1025	rBV	3494006	6171268	44.86%	6.586%
6	10.610	1287	1296	1305	rBV	2373641	4319994	31.40%	4.610%
7	12.057	1534	1542	1550	rBV	136474	227298	1.65%	0.243%
8	13.080	1708	1716	1732	rBV	8374856	13757204	100.00%	14.682%
9	13.298	1748	1753	1763	rVB	175975	279446	2.03%	0.298%
10	14.457	1942	1950	1970	rBV	3210172	5362492	38.98%	5.723%
11	15.951	2196	2204	2224	rBV	4875759	8101697	58.89%	8.646%
12	17.215	2412	2419	2432	rBV	3483799	5568465	40.48%	5.943%
13	17.515	2466	2470	2478	rVB	82727	140582	1.02%	0.150%
14	17.904	2533	2536	2541	rVB	129096	166573	1.21%	0.178%
15	18.121	2569	2573	2580	rBV3	197887	330408	2.40%	0.353%
16	19.233	2758	2762	2768	rBV	223248	366989	2.67%	0.392%
17	19.586	2819	2822	2825	rBV	188470	223549	1.62%	0.239%
18	19.792	2851	2857	2863	rBV	10770900	13674230	99.40%	14.593%
19	21.051	3068	3071	3077	rBV	500572	716067	5.21%	0.764%
20	21.245	3101	3104	3110	rVB	1477787	1793264	13.04%	1.914%
21	21.321	3112	3117	3123	rBV	3580159	5052585	36.73%	5.392%
22	23.733	3521	3527	3537	rVB2	2496386	5314084	38.63%	5.671%




Sum of corrected areas: 93703391

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009349.D
Acq On : 10 Mar 2022 17:50
Operator : CG/JU
Sample : N1847-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

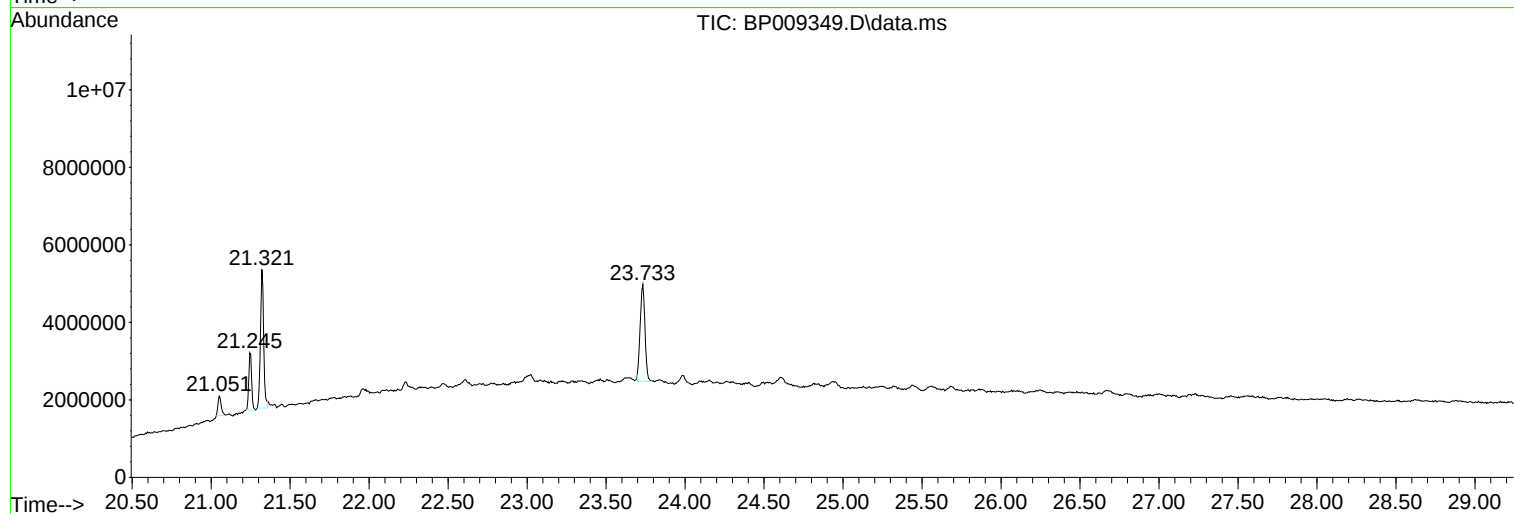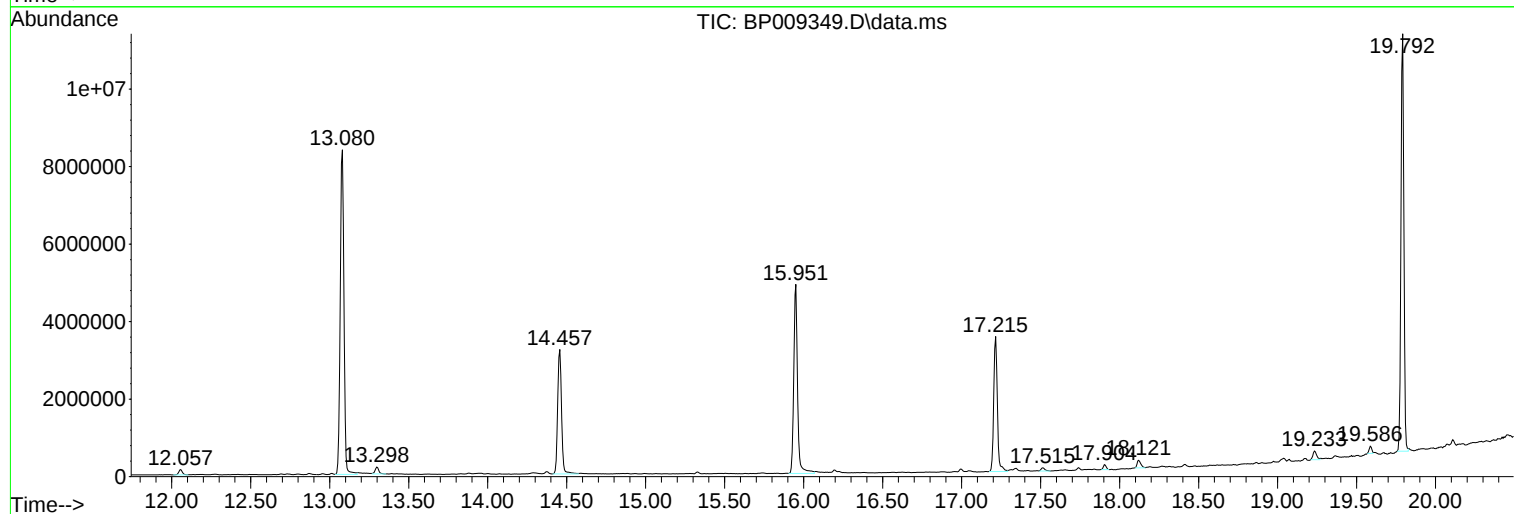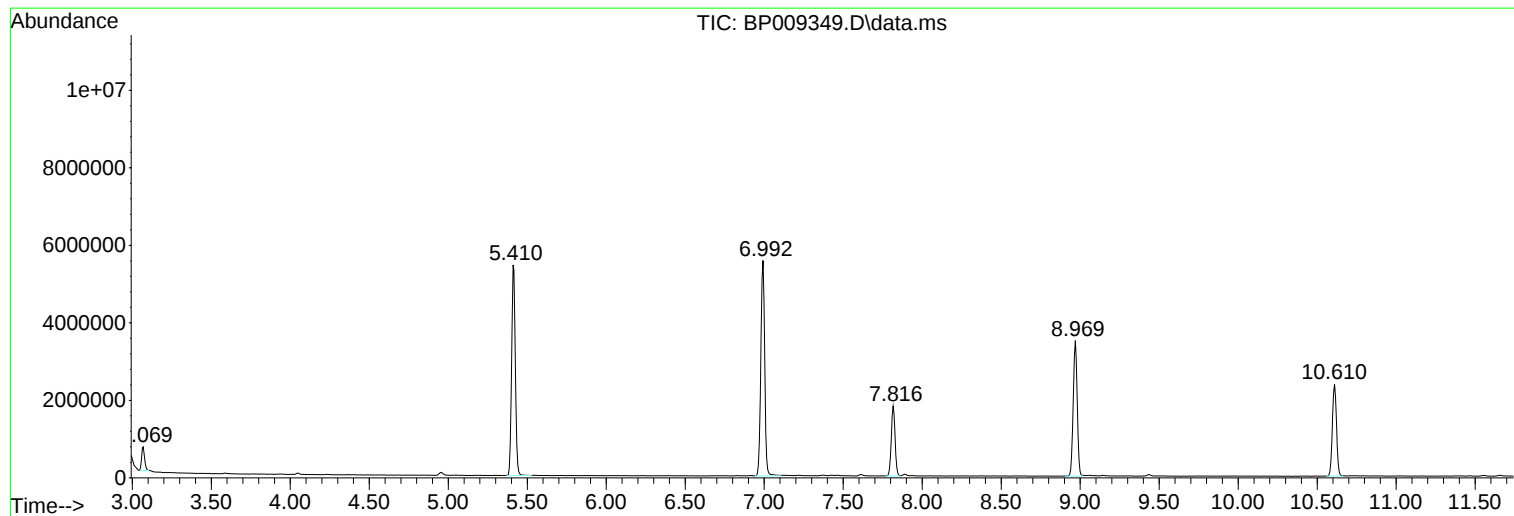

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009349.D
Acq On : 10 Mar 2022 17:50
Operator : CG/JU
Sample : N1847-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009349.D
Acq On : 10 Mar 2022 17:50
Operator : CG/JU
Sample : N1847-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-B1-030722-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------