
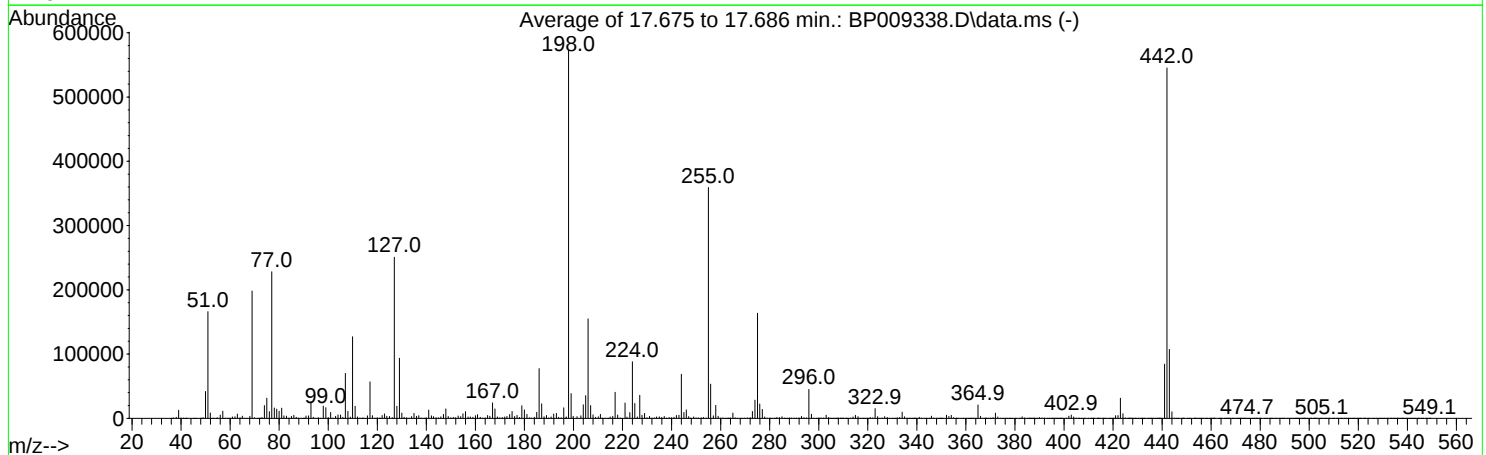


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
 Data File : BP009338.D
 Acq On : 10 Mar 2022 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

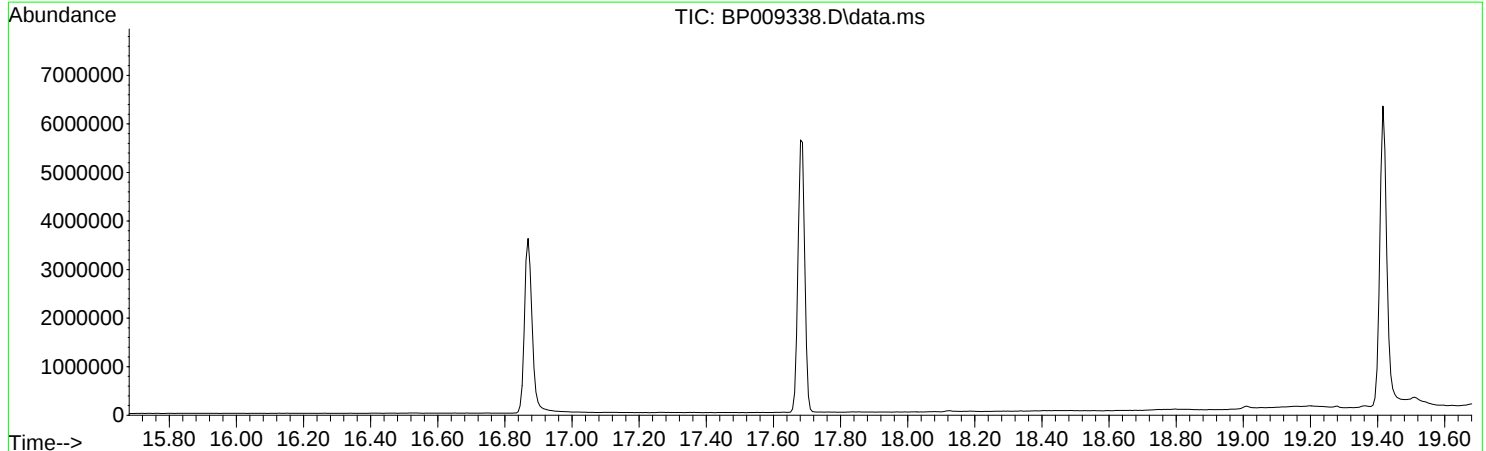

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	166059	PASS
68	69	0.00	2	1.6	3156	PASS
69	198	0.00	100	34.6	198239	PASS
70	69	0.00	2	0.5	952	PASS
127	198	10	80	43.8	250800	PASS
197	198	0.00	2	0.4	2245	PASS
198	198	100	100	100.0	572358	PASS
199	198	5	9	6.7	38530	PASS
275	198	10	60	28.6	163523	PASS
365	198	1	100	3.7	21025	PASS
441	198	0.01	100	14.7	84304	PASS
442	442	100	100	100.0	545195	PASS
443	442	15	24	19.7	107449	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2022	BNA_P	<u>BP009338.D</u>
Compound Name	Response	Retention Time
DDT	1942345	20.633
DDD	43801	20.204
DDE	3908	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47709	1990054	2.40

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009338.D
Acq On : 10 Mar 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 11 06:35:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

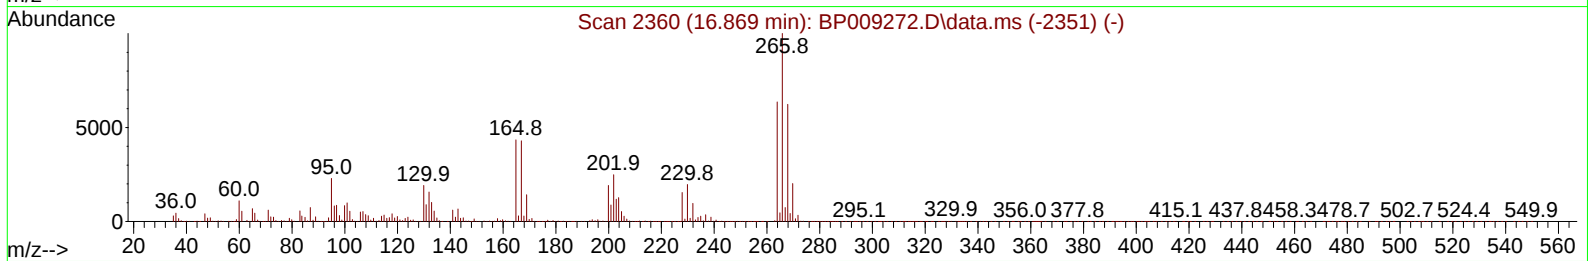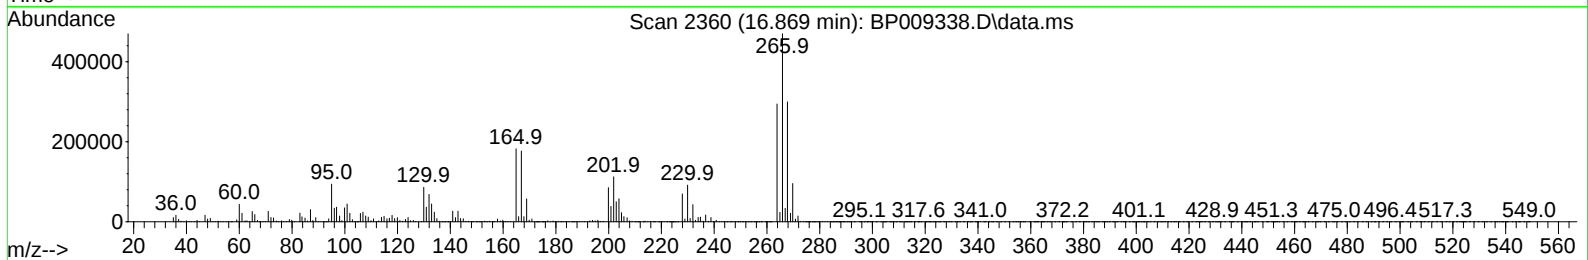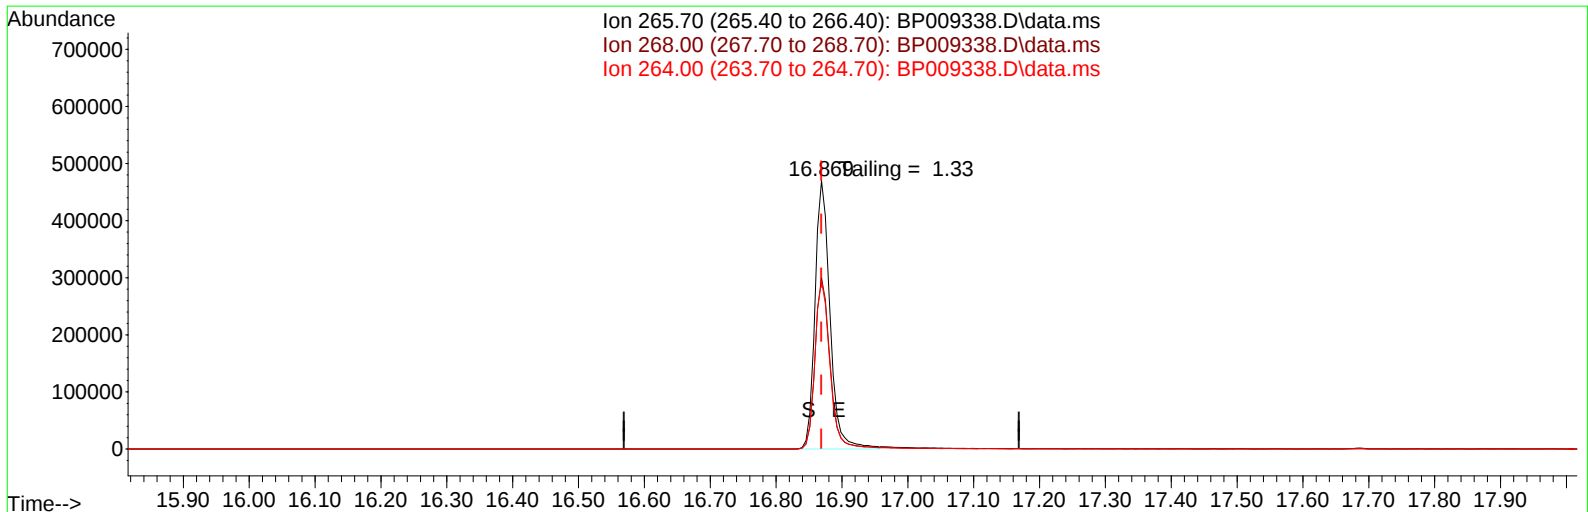

TIC: BP009338.D\data.ms

(70) Pentachlorophenol (C)

16.869min (+ 0.000) 3794868.54 ng




response 751487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.76
264.00	63.60	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031022\
Data File : BP009338.D
Acq On : 10 Mar 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 11 06:35:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

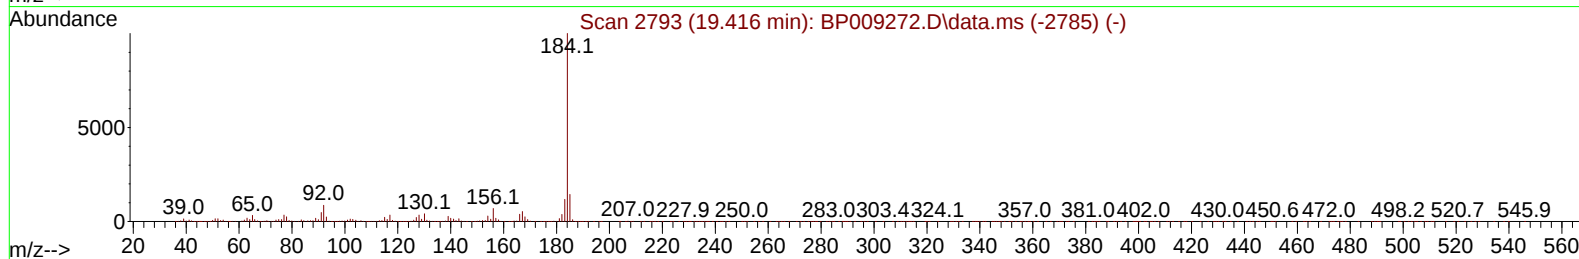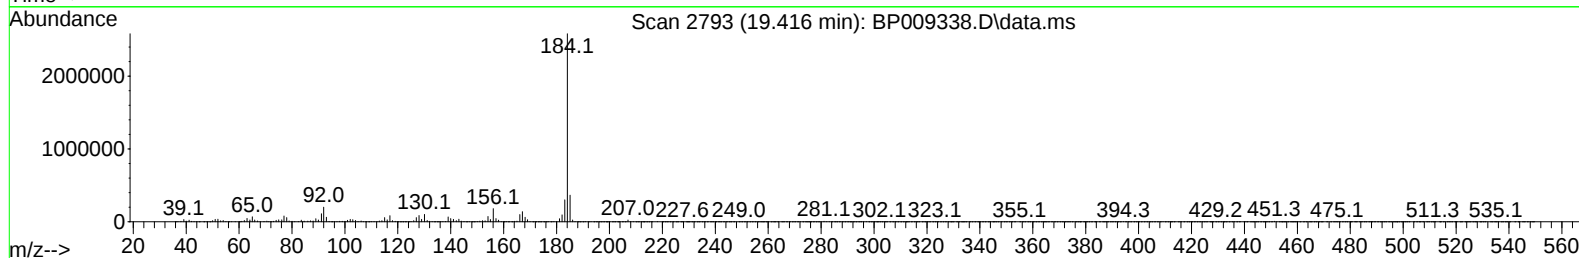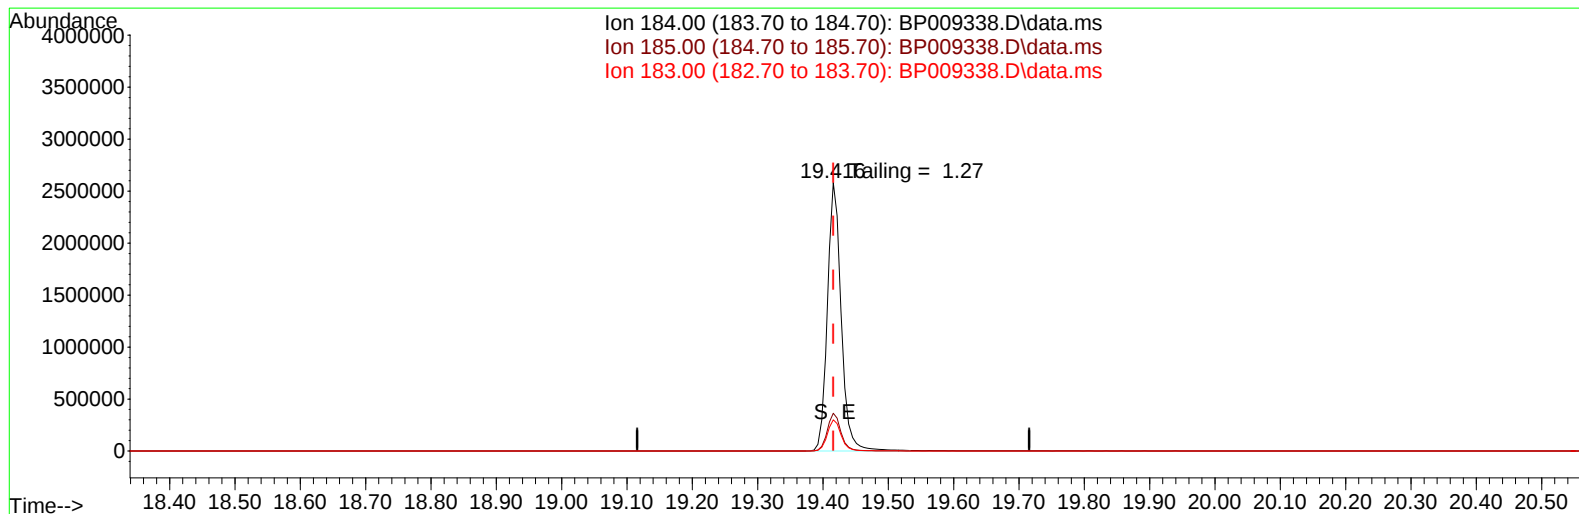

TIC: BP009338.D\data.ms

(77) Benzidine

19.416min (+ 0.000) 460666.03 ng

response 3794652

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.70	11.64
0.00	0.00	0.00