

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014027.D
 Acq On : 10 Mar 2023 13:13
 Operator : CG/JU
 Sample : 01713-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBZZ2

Quant Time: Mar 10 21:29:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	118091	20.000	ng/ul	0.00
20) Naphthalene-d8	10.899	136	524314	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.716	164	389267	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	918011	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1005958	20.000	ng/ul	-0.01
88) Perylene-d12	24.086	264	1026510	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	8417	2.693	ng/uL	0.00
4) Pyridine-d5	3.864	84	53	0.006	ng/ul	0.00
7) Phenol-d5	7.228	99	147201	14.125	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	92741	15.259	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	112078	14.116	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	110126	12.937	ng/ul	-0.01
21) Nitrobenzene-d5	9.252	128	56494	13.504	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	69876	13.953	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	119041	12.633	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	127234	10.203	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	497251	15.052	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	484179	13.835	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	65172	11.195	ng/ul	0.00
60) Fluorene-d10	15.704	176	407769	14.564	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	74138	10.685	ng/ul	-0.01
73) Anthracene-d10	17.569	188	683462	15.336	ng/ul	0.00
81) Pyrene-d10	19.792	212	980042	17.664	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	919568	16.841	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.910	105	20393	1.483	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014027.D
Acq On : 10 Mar 2023 13:13
Operator : CG/JU
Sample : 01713-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ2


Quant Time: Mar 10 21:29:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

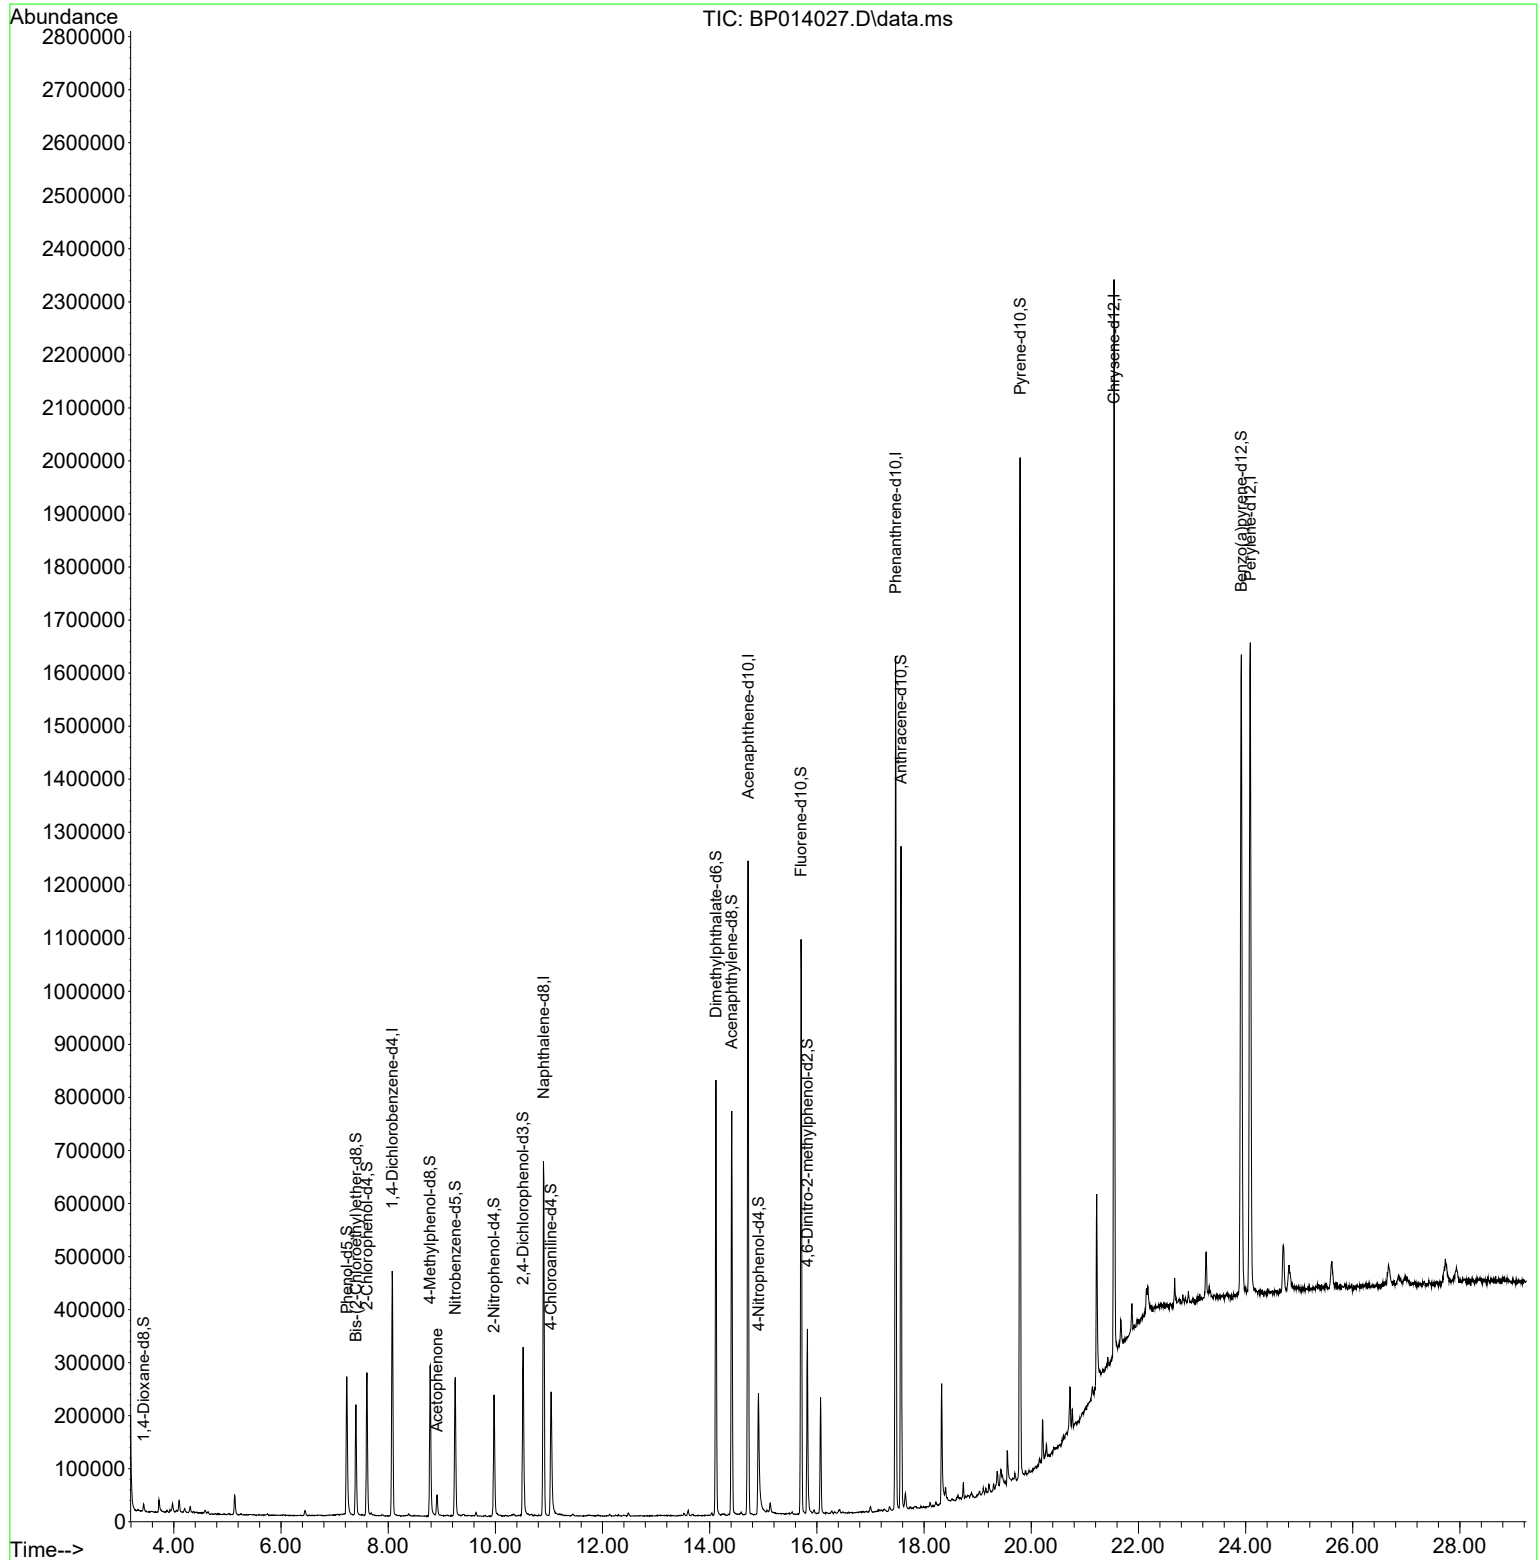

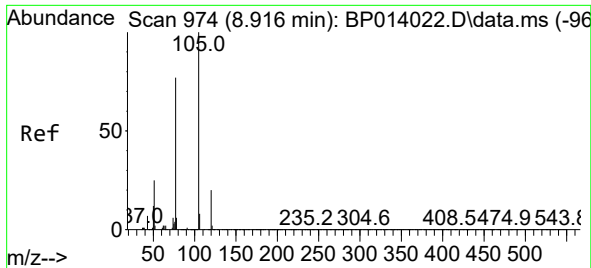

#16
 Acetophenone
 Concen: 1.483 ng/ul
 RT: 8.910 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP014027.D
 Acq: 10 Mar 2023 13:13

Instrument :
 BNA_P
 ClientSampleId :
 DBZZ2

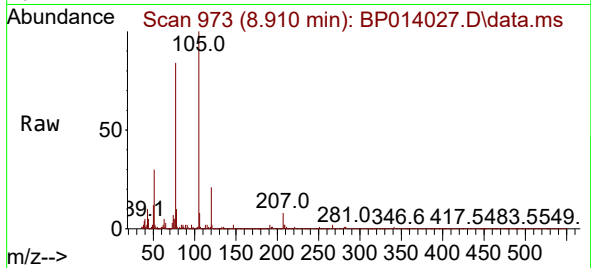

Tgt Ion:105 Resp: 20393
 Ion Ratio Lower Upper
 105 100
 77 84.2 65.4 98.2
 51 30.1 21.8 32.8

